

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL070218\
 Data File : VL032184.D
 Acq On : 2 Jul 2018 16:29
 Operator : SY/AP
 Sample : J3601-11DL 10X
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1


Instrument :
 MSVOA_L
 ClientSampleId :
 OUTDOOR-2DL

Manual Integrations
 APPROVED

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL070218\
Data File : VL032184.D
Acq On : 2 Jul 2018 16:29
Operator : SY/AP
Sample : J3601-11DL 10X
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
OUTDOOR-2DL

Manual Integrations
APPROVED

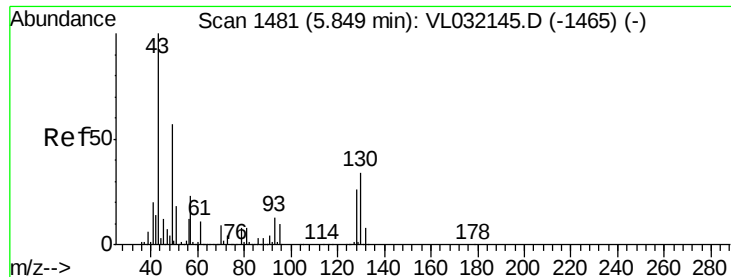


#1

Bromochloromethane

Concen: 10.00 ppbv

RT: 5.84 min Scan# 1479

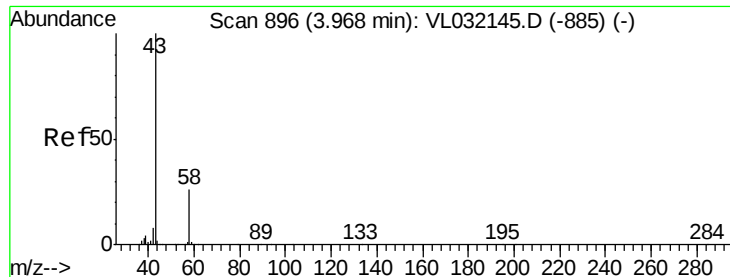


#15

Acetone


Concen: 2.49 ppbv

RT

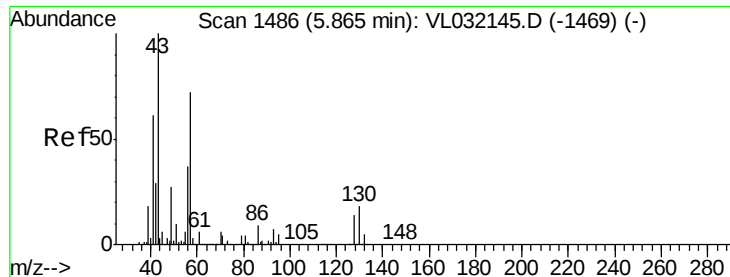


#26
Hexane
Concen: 0.52 ppbv
RT: 5.86 min Scan# 1486
Delta R.T. -0.01 min
Lab File: VL032184.D
Acq: 2 Jul 2018 16:29

Instrument :
MS

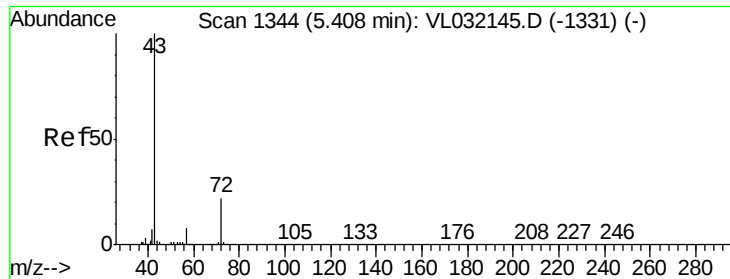


#34
 2-Butanone
 Concen: 0.15 ppbv
 RT: 5.42 min Scan# 1349
 Delta R.T. 0.00 min
 Lab File: VL032184.D
 Acq: 2 Jul 2018 16:29

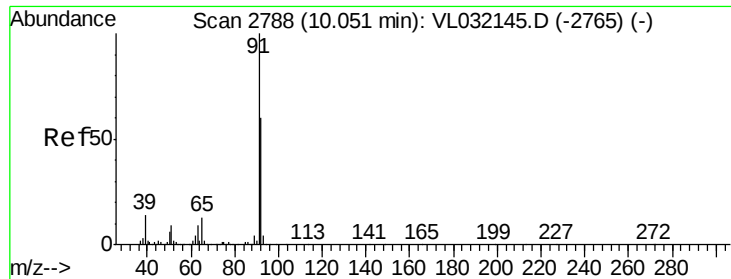

#53


Toluene

Concen: 0.75 ppbv

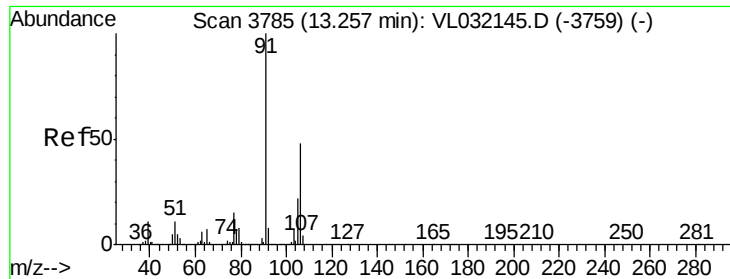

#59
m/p-Xylene
Concen: 0.22 ppbv m
RT: 13.21 min Scan# 3772
Delta R.T. -0.05 min
Lab File: VL032184.D
Acq: 2 Jul 2018 16:29

Instrument :
MSVOA_L
ClientSampleId

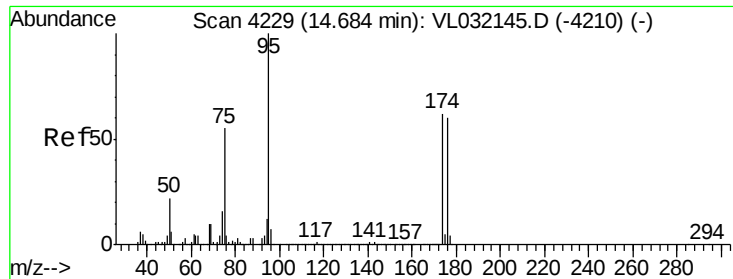

#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.43 ppbv
 RT: 14.68 min Scan# 4227
 Delta R.T. -0.02 min
 Lab File: VL032184.D
 Acq: 2 Jul 201