


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL070218\
Data File : VL032175.D
Acq On : 2 Jul 2018 9:21
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062918AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jun 29 22:27:58 2018
Last Update : Fri Jun 29 22:27:58 2018

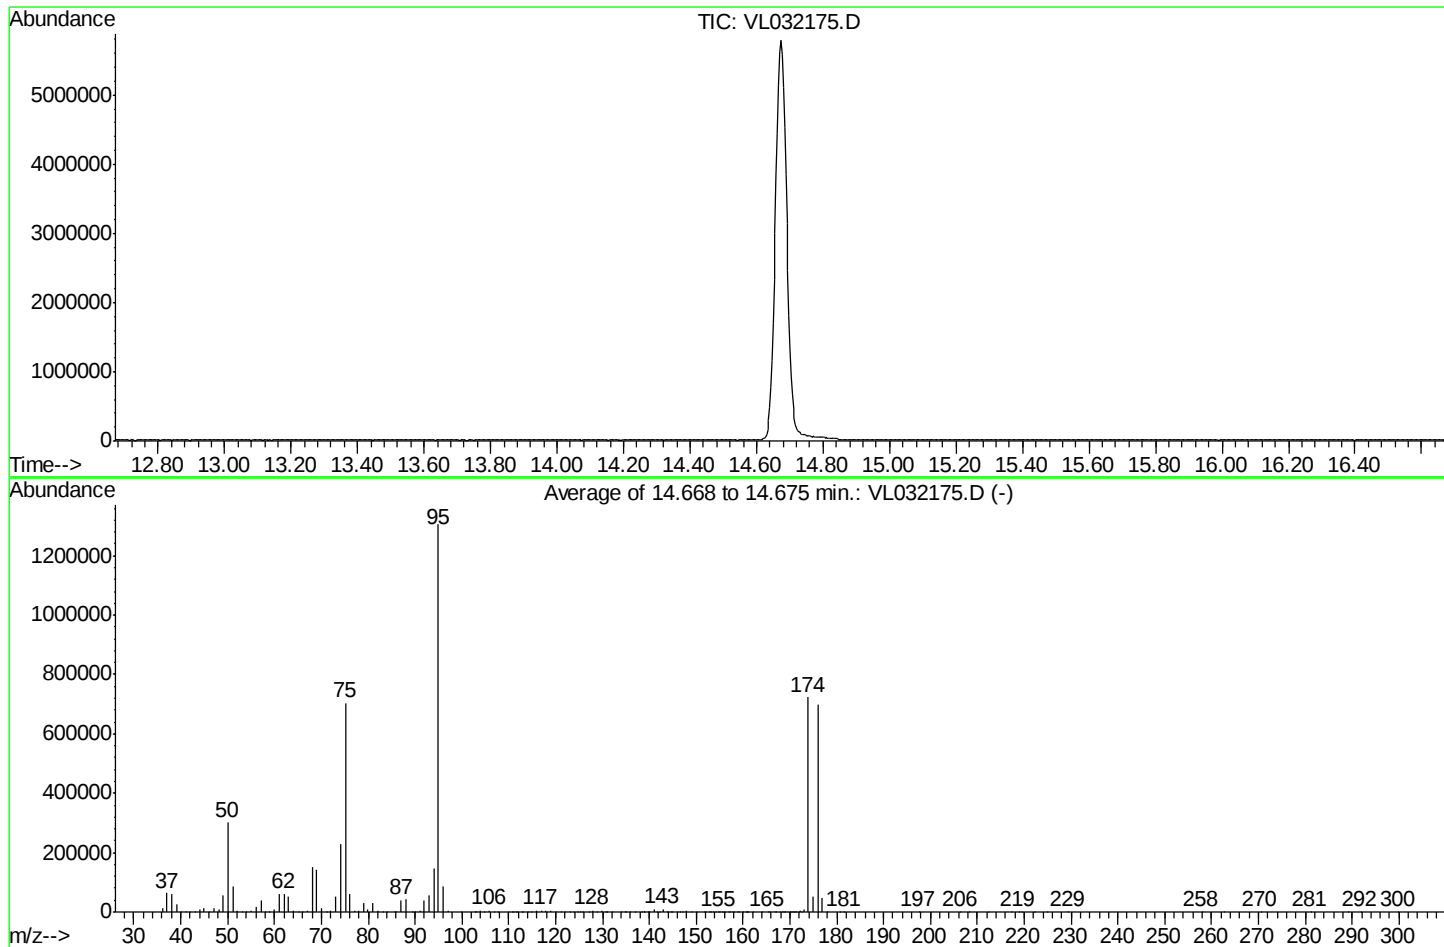

AutoFind: Scans 4224, 4225, 4226; Background Corrected with Scan 4203

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	299925	PASS
75	95	30	66	53.9	704362	PASS
95	95	100	100	100.0	1305600	PASS
96	95	5	9	6.6	86504	PASS
173	174	0.00	2	1.0	7407	PASS
174	95	50	120	55.4	722816	PASS
175	174	4	9	7.1	51389	PASS
176	174	93	101	96.9	700266	PASS
177	176	5	9	6.7	46944	PASS