
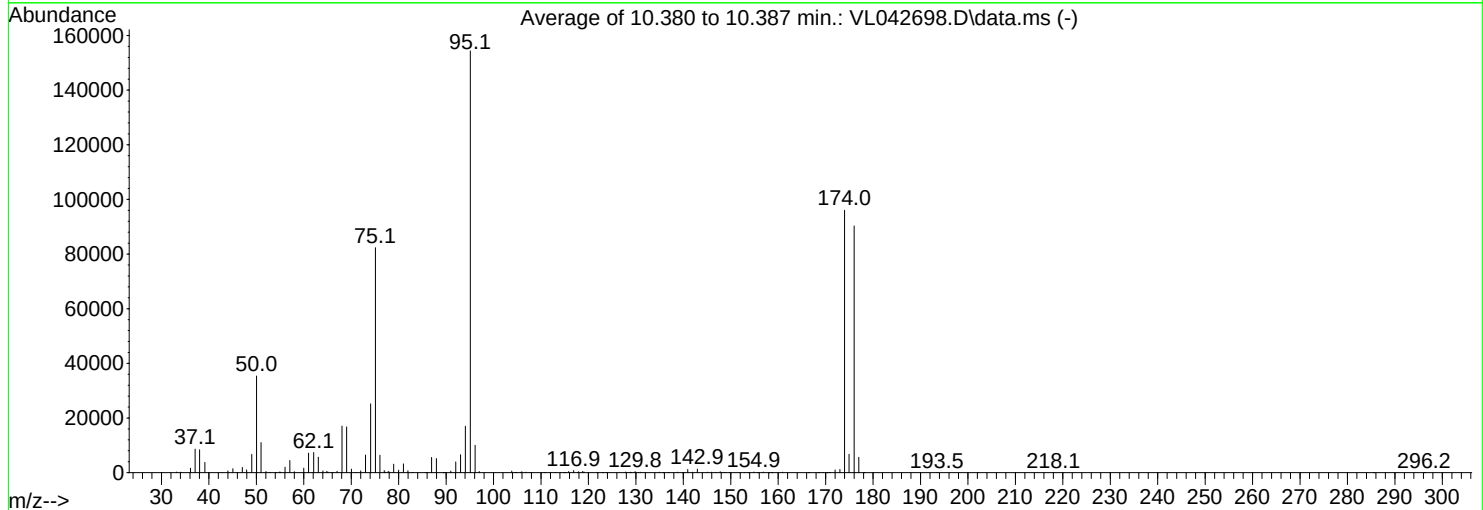


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL070325\
Data File : VL042698.D
Acq On : 03 Jul 2025 07:53
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL070225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jul 03 01:50:16 2025

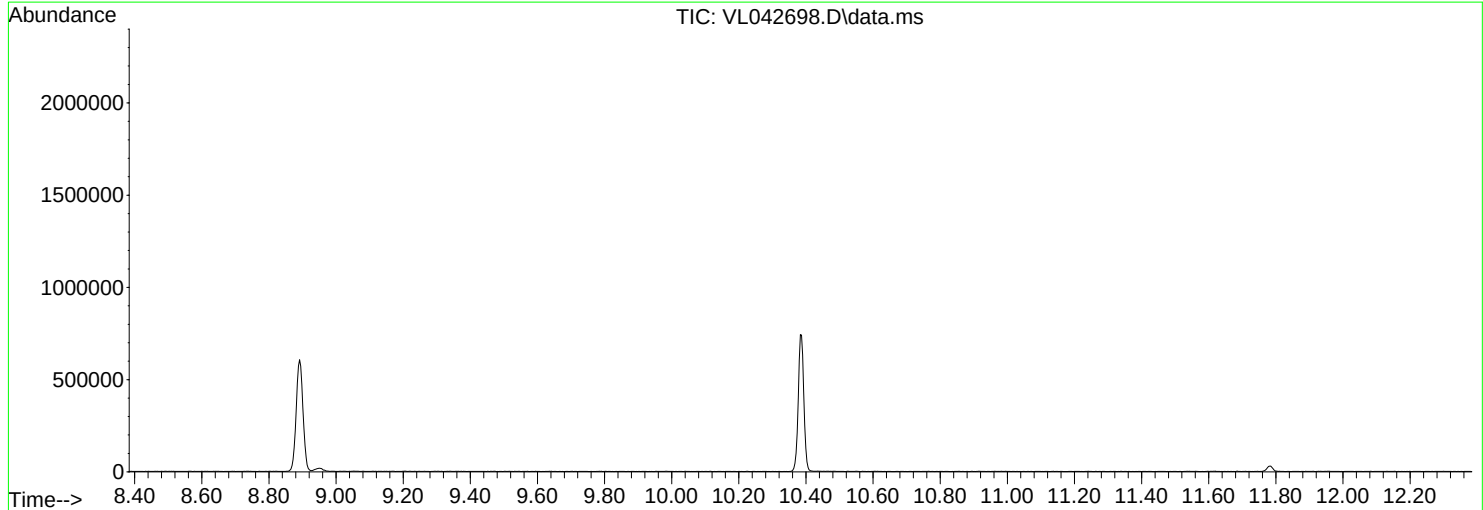

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3168

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.9	35379	PASS
75	95	30	66	53.3	82365	PASS
95	95	100	100	100.0	154389	PASS
96	95	5	9	6.5	10039	PASS
173	174	0.00	2	1.2	1198	PASS
174	95	50	120	62.2	96059	PASS
175	174	4	9	7.0	6756	PASS
176	174	93	101	94.0	90304	PASS
177	176	5	9	6.3	5645	PASS

Average of 10.380 to 10.387 min.: VL042698.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.20	257	47.05	1912	56.05	1977	66.20	71
34.10	167	47.95	998	57.05	4477	67.00	52
36.10	1621	49.05	6702	58.00	355	68.05	1701
37.10	8615	50.05	35379	60.00	1661	69.05	1675
38.05	8393	51.00	11032	61.00	7169	70.05	1317
39.15	3744	52.05	385	62.10	7356	71.10	34
39.95	35	52.90	104	63.05	5686	72.00	666
42.80	47	54.00	87	64.05	665	73.00	6459
44.00	626	54.20	35	64.85	501	74.10	25184
45.05	1482	54.90	247	65.10	238	75.10	82365
46.05	55	55.10	160	65.80	52	76.05	6415

Average of 10.380 to 10.387 min.: VL042698.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.95	796	85.90	96	96.10	10039	110.90	48
77.20	196	86.10	57	97.00	401	112.00	101
77.80	458	86.95	5547	103.85	560	113.00	50
78.00	243	87.95	5141	104.60	40	114.15	40
78.95	3114	89.40	8	104.85	120	114.80	61
80.00	921	89.80	47	105.70	111	115.00	19
81.00	3226	91.00	565	105.95	347	115.85	418
81.95	686	92.05	3942	106.85	185	116.90	779
82.80	79	93.05	6539	107.65	49	117.70	132
83.00	67	94.05	17015	108.10	36	117.95	358
85.60	37	95.10	154389	110.70	88	118.75	410

Average of 10.380 to 10.387 min.: VL042698.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.05	285	131.05	186	145.05	152	153.70	28
121.80	18	134.95	202	145.95	166	154.90	245
123.00	18	135.70	20	146.85	136	155.70	29
123.75	92	136.80	110	147.80	343	156.85	218
127.80	226	137.00	75	148.20	36	158.00	29
128.10	135	138.80	152	148.70	44	158.60	25
128.60	69	139.90	18	148.95	76	158.80	148
128.90	176	140.05	65	149.80	81	160.95	176
129.10	65	140.95	1169	150.00	73	166.40	20
129.85	415	141.90	178	151.90	34	168.50	17
130.60	65	142.95	1282	152.90	93	169.50	72

Average of 10.380 to 10.387 min.: VL042698.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.30	21	202.20	35				
170.80	124	218.10	36				
171.00	65	285.50	23				
172.00	1030	296.20	29				
173.00	1198						
174.00	96059						
174.95	6756						
176.00	90304						
177.00	5645						
178.10	22						
193.50	61						

Instrument :

MSVOA_L

ClientSampleId :

BFB