


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL070518\
 Data File : VL032202.D
 Acq On : 5 Jul 2018 11:38
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062918AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jun 29 22:27:58 2018
 Last Update : Fri Jun 29 22:27:58 2018

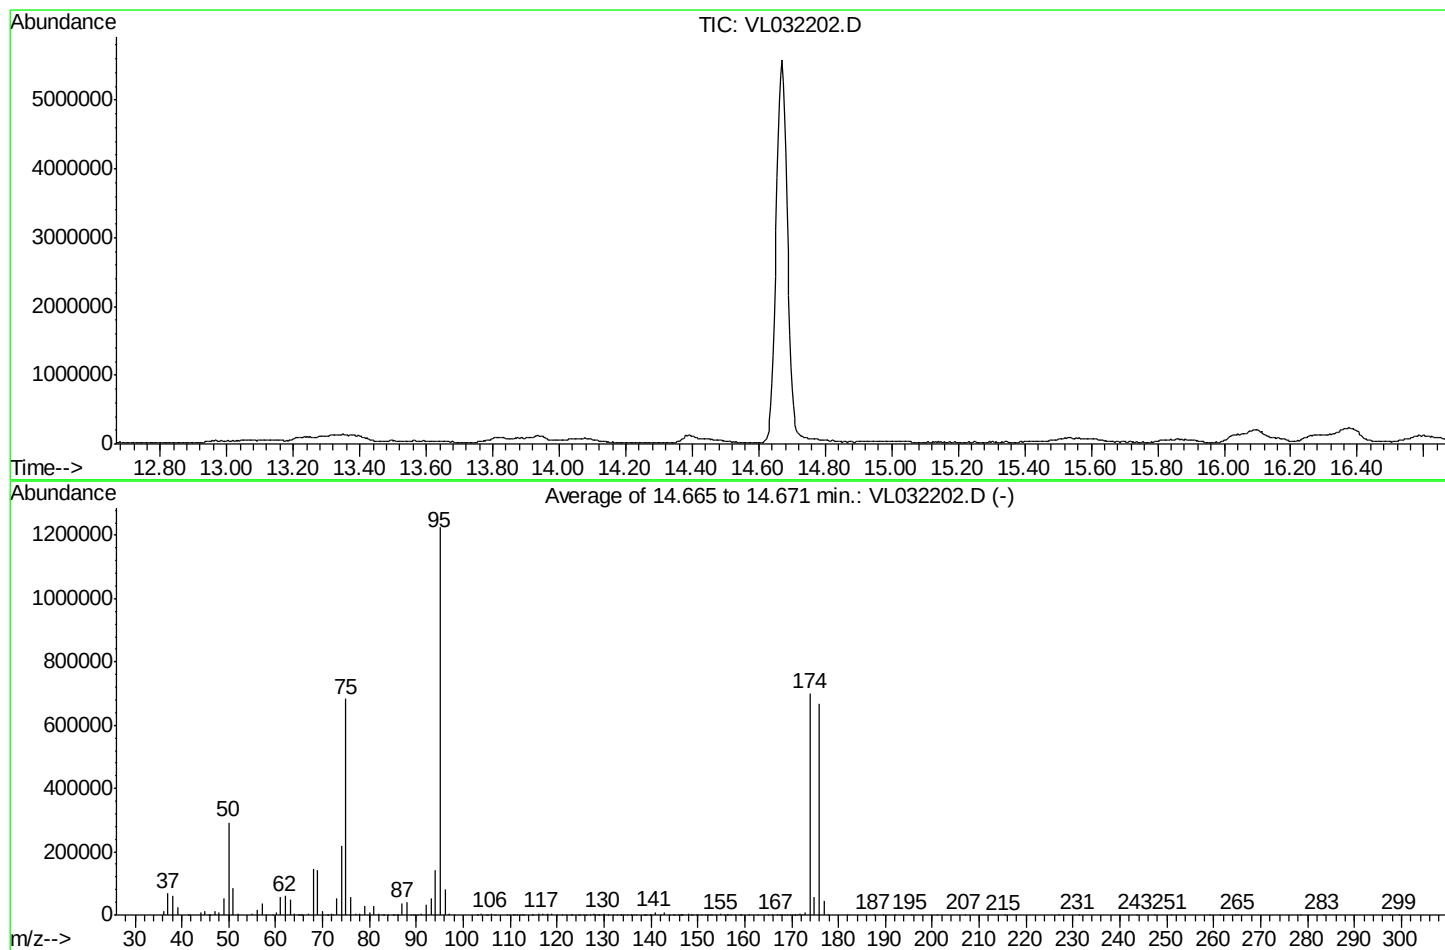

AutoFind: Scans 4223, 4224, 4225; Background Corrected with Scan 4200

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	291392	PASS
75	95	30	66	55.8	683541	PASS
95	95	100	100	100.0	1225386	PASS
96	95	5	9	6.7	81597	PASS
173	174	0.00	2	1.2	8461	PASS
174	95	50	120	57.1	699733	PASS
175	174	4	9	8.0	55680	PASS
176	174	93	101	95.3	667157	PASS
177	176	5	9	6.6	43895	PASS