


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL070820\
 Data File : VL035167.D
 Acq On : 8 Jul 2020 1:21
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL070820AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jul 08 07:05:23 2020
 Last Update : Wed Jul 08 07:05:23 2020

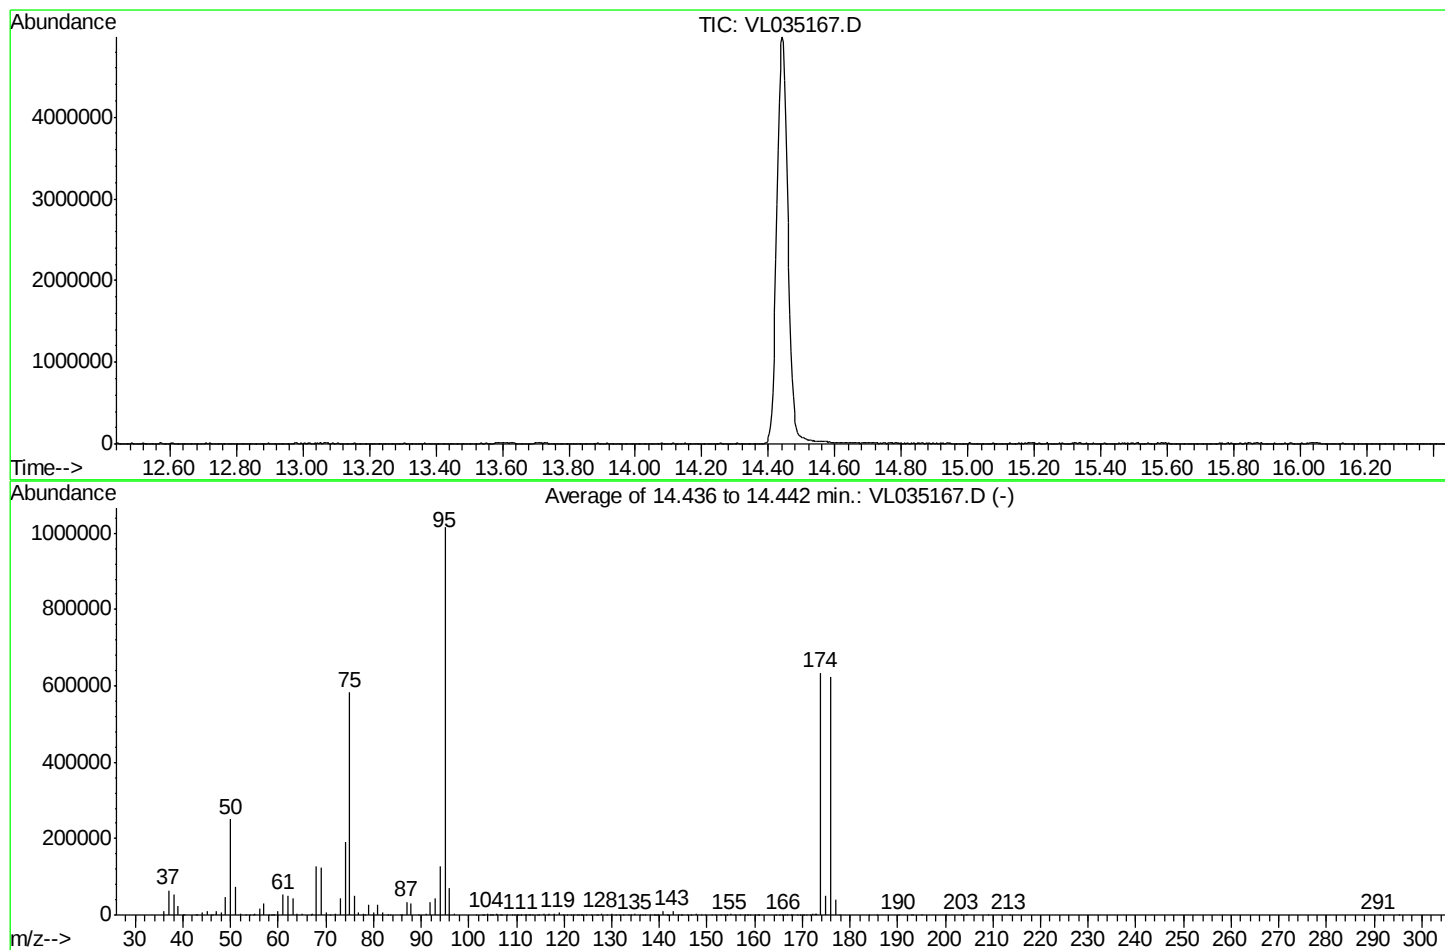

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.7	251050	PASS
75	95	30	66	57.4	583125	PASS
95	95	100	100	100.0	1015360	PASS
96	95	5	9	7.1	72018	PASS
173	174	0.00	2	0.7	4190	PASS
174	95	50	120	62.4	633920	PASS
175	174	4	9	7.7	49032	PASS
176	174	93	101	98.6	624938	PASS
177	176	5	9	6.7	41586	PASS