
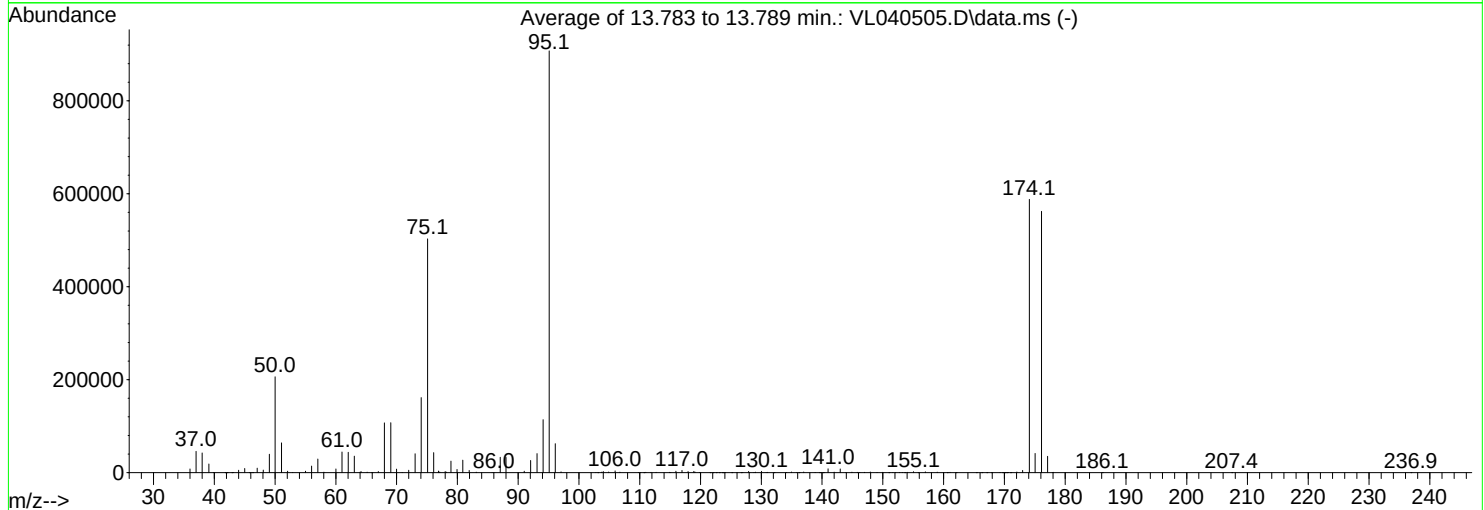


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL071023\
 Data File : VL040505.D
 Acq On : 10 Jul 2023 11:06
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL071023AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Jul 10 16:32:00 2023

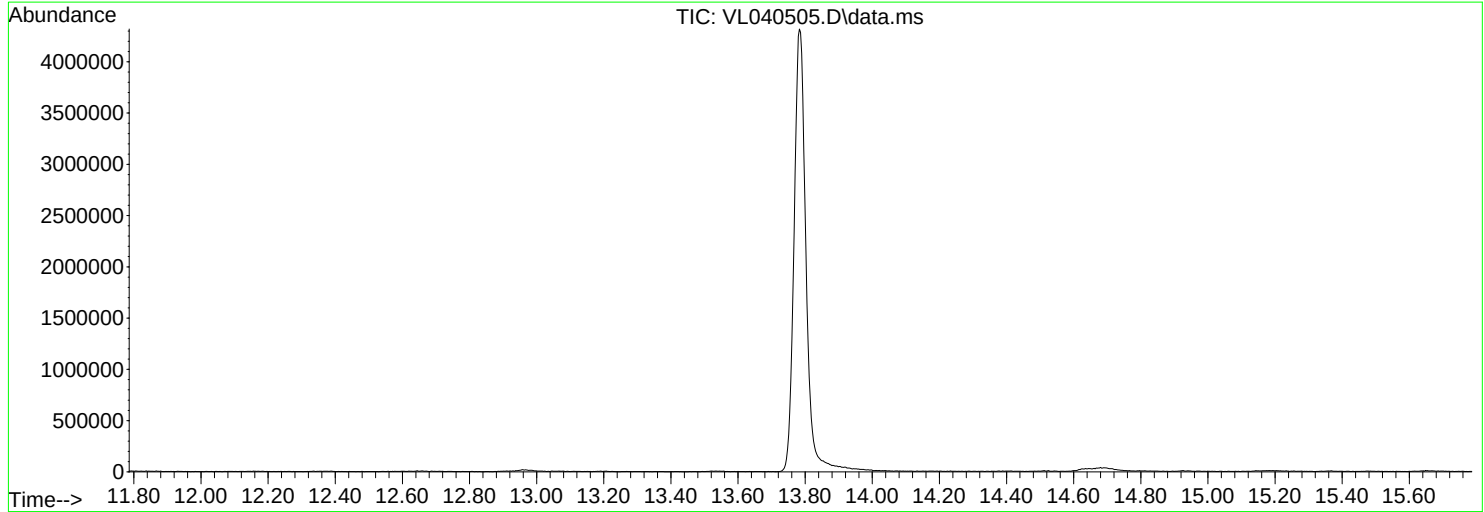

AutoFind: Scans 3477, 3478, 3479; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.7	206336	PASS
75	95	30	66	55.4	503125	PASS
95	95	100	100	100.0	907541	PASS
96	95	5	9	6.9	62472	PASS
173	174	0.00	2	0.8	4902	PASS
174	95	50	120	64.8	587840	PASS
175	174	4	9	7.0	41256	PASS
176	174	93	101	95.6	562027	PASS
177	176	5	9	6.3	35256	PASS

Average of 13.783 to 13.789 min.: VL040505.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7968	45.80	164	56.00	14280	67.00	255
37.00	45939	46.05	540	57.05	29208	68.00	10717
38.00	42432	46.30	136	58.05	943	69.05	10756
39.10	18439	47.05	9814	60.00	8063	70.00	754
39.90	523	48.05	5489	61.00	44549	70.90	432
41.80	126	49.05	39600	62.05	43712	72.00	5140
42.10	83	50.00	206336	63.05	35573	73.05	40765
42.90	142	51.05	63954	64.00	1013	74.05	161643
43.15	276	52.05	3186	64.15	2587	75.10	503125
44.00	5190	52.90	193	65.15	1036	76.10	43037
45.00	9067	55.00	3071	65.90	125	76.90	3448

Average of 13.783 to 13.789 min.: VL040505.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.10	1336	88.00	32683	104.00	2369	115.10	261
78.00	2409	91.00	3120	104.90	1265	115.95	3118
78.20	1023	92.05	26235	105.95	3745	116.95	4760
78.95	24685	93.10	41096	106.75	902	117.95	2602
79.95	7037	94.10	114005	109.80	298	118.90	2684
80.90	26744	95.10	907541	110.15	455	119.10	1271
81.95	4958	96.10	62472	110.70	187	119.85	201
83.10	1018	97.05	1802	111.00	737	121.60	70
85.70	317	102.80	320	111.85	756	122.05	186
86.00	361	103.10	75	112.70	637	122.60	81
87.05	32957	103.75	960	114.90	802	123.10	65

Average of 13.783 to 13.789 min.: VL040505.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.60	154	130.05	2679	139.85	289	149.05	501
123.80	181	130.80	390	140.20	132	150.00	820
124.10	352	131.05	731	141.00	8291	151.00	93
125.15	159	132.10	74	142.00	902	151.65	322
126.00	195	134.15	214	143.00	8042	152.10	212
126.70	63	134.95	1541	143.95	254	152.75	387
126.95	204	135.85	405	144.90	1007	153.20	288
127.90	2301	136.20	75	145.80	561	153.60	168
128.10	647	137.00	1414	146.20	434	154.05	555
128.80	323	138.85	297	147.00	602	155.05	2117
129.05	925	139.60	59	147.95	1504	155.80	110

Average of 13.783 to 13.789 min.: VL040505.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.00	1677	170.10	99	177.90	207		
158.95	912	170.40	173	178.05	730		
160.60	164	170.65	243	186.10	51		
161.05	689	171.00	143	207.40	64		
162.05	165	171.20	266	236.90	62		
165.40	61	172.05	1545				
166.30	74	173.00	4902				
167.10	81	174.10	587840				
167.90	100	175.05	41256				
169.30	231	176.10	562027				
169.70	143	177.10	35256				