

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL071222\
 Data File : VL039455.D
 Acq On : 12 Jul 2022 19:30
 Operator : SY/AP
 Sample : N3660-06 2X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-9

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 07/13/2022
 Supervised By : Mahesh Dadoda 07/13/2022

Quant Time: Jul 13 01:38:51 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 13 11:30:53 2022

QLast Update : Wed Jul 06 02:15:38 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.687	49	1558869	10.000	ppbv	0.04
33) 1,4-Difluorobenzene	7.195	114	4260566	10.000	ppbv	0.04
55) Chlorobenzene-d5	12.105	117	3920614	10.000	ppbv	0.04
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.436	95	2856766	9.822	ppbv	0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.200%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	3.063	85	100231	0.446	ppbv	96
3) Chlorodifluoromethane	3.005	51	36851m	0.186	ppbv	
4) Chloromethane	3.153	50	14959m	0.138	ppbv	
9) Propene	3.028	41	56217m	0.629	ppbv	
10) Heptane	8.140	43	62985	0.301	ppbv	93
11) Trichlorofluoromethane	3.967	101	467801	1.867	ppbv	100
13) Ethanol	3.613	45	518277	100.018	ppbv	73
15) Acetone	3.864	43	1593047	8.638	ppbv	94
17) tert-Butyl alcohol	4.311	59	134706	0.861	ppbv	98
19) Isopropyl Alcohol	3.976	45	112993m	1.149	ppbv	
20) Methylene Chloride	4.362	84	1407538	19.148	ppbv	98
26) Hexane	5.706	57	2567964	16.846	ppbv #	39
27) Carbon Disulfide	4.571	76	221026	1.201	ppbv	96
29) Chloroform	5.771	83	132516	0.500	ppbv	87
30) Cyclohexane	7.147	84	23053m	0.166	ppbv	
32) 1,1,1-Trichloroethane	6.533	97	22998	0.088	ppbv	90
34) 2-Butanone	5.266	43	155344	0.724	ppbv #	89
38) Trichloroethene	7.854	130	43189	0.242	ppbv	92
44) 2,2,4-Trimethylpentane	7.886	57	78964m	0.141	ppbv	
52) Tetrachloroethene	11.243	164	162071	1.221	ppbv	88
53) Toluene	9.822	91	534658	1.406	ppbv	99
58) Ethyl Benzene	12.732	91	244295	0.483	ppbv	94
59) m/p-Xylene	12.982	91	666426m	1.493	ppbv	
60) o-Xylene	13.709	91	311922	0.738	ppbv	100
65) tert-Butylbenzene	16.780	119	65076m	0.109	ppbv	
72) 4-Ethyltoluene	15.857	105	117471m	0.236	ppbv	
73) 1,3,5-Trimethylbenzene	16.018	105	177694	0.389	ppbv	95
74) 1,2,4-Trimethylbenzene	16.780	105	558114	1.105	ppbv #	71
79) Naphthalene	22.217	128	81373m	0.234	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL071222\
Data File : VL039455.D
Acq On : 12 Jul 2022 19:30
Operator : SY/AP
Sample : N3660-06 2X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SG-9

Quant Time: Jul 13 01:38:51 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jul
QLast Update : Wed Jul 06 02:15:38 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

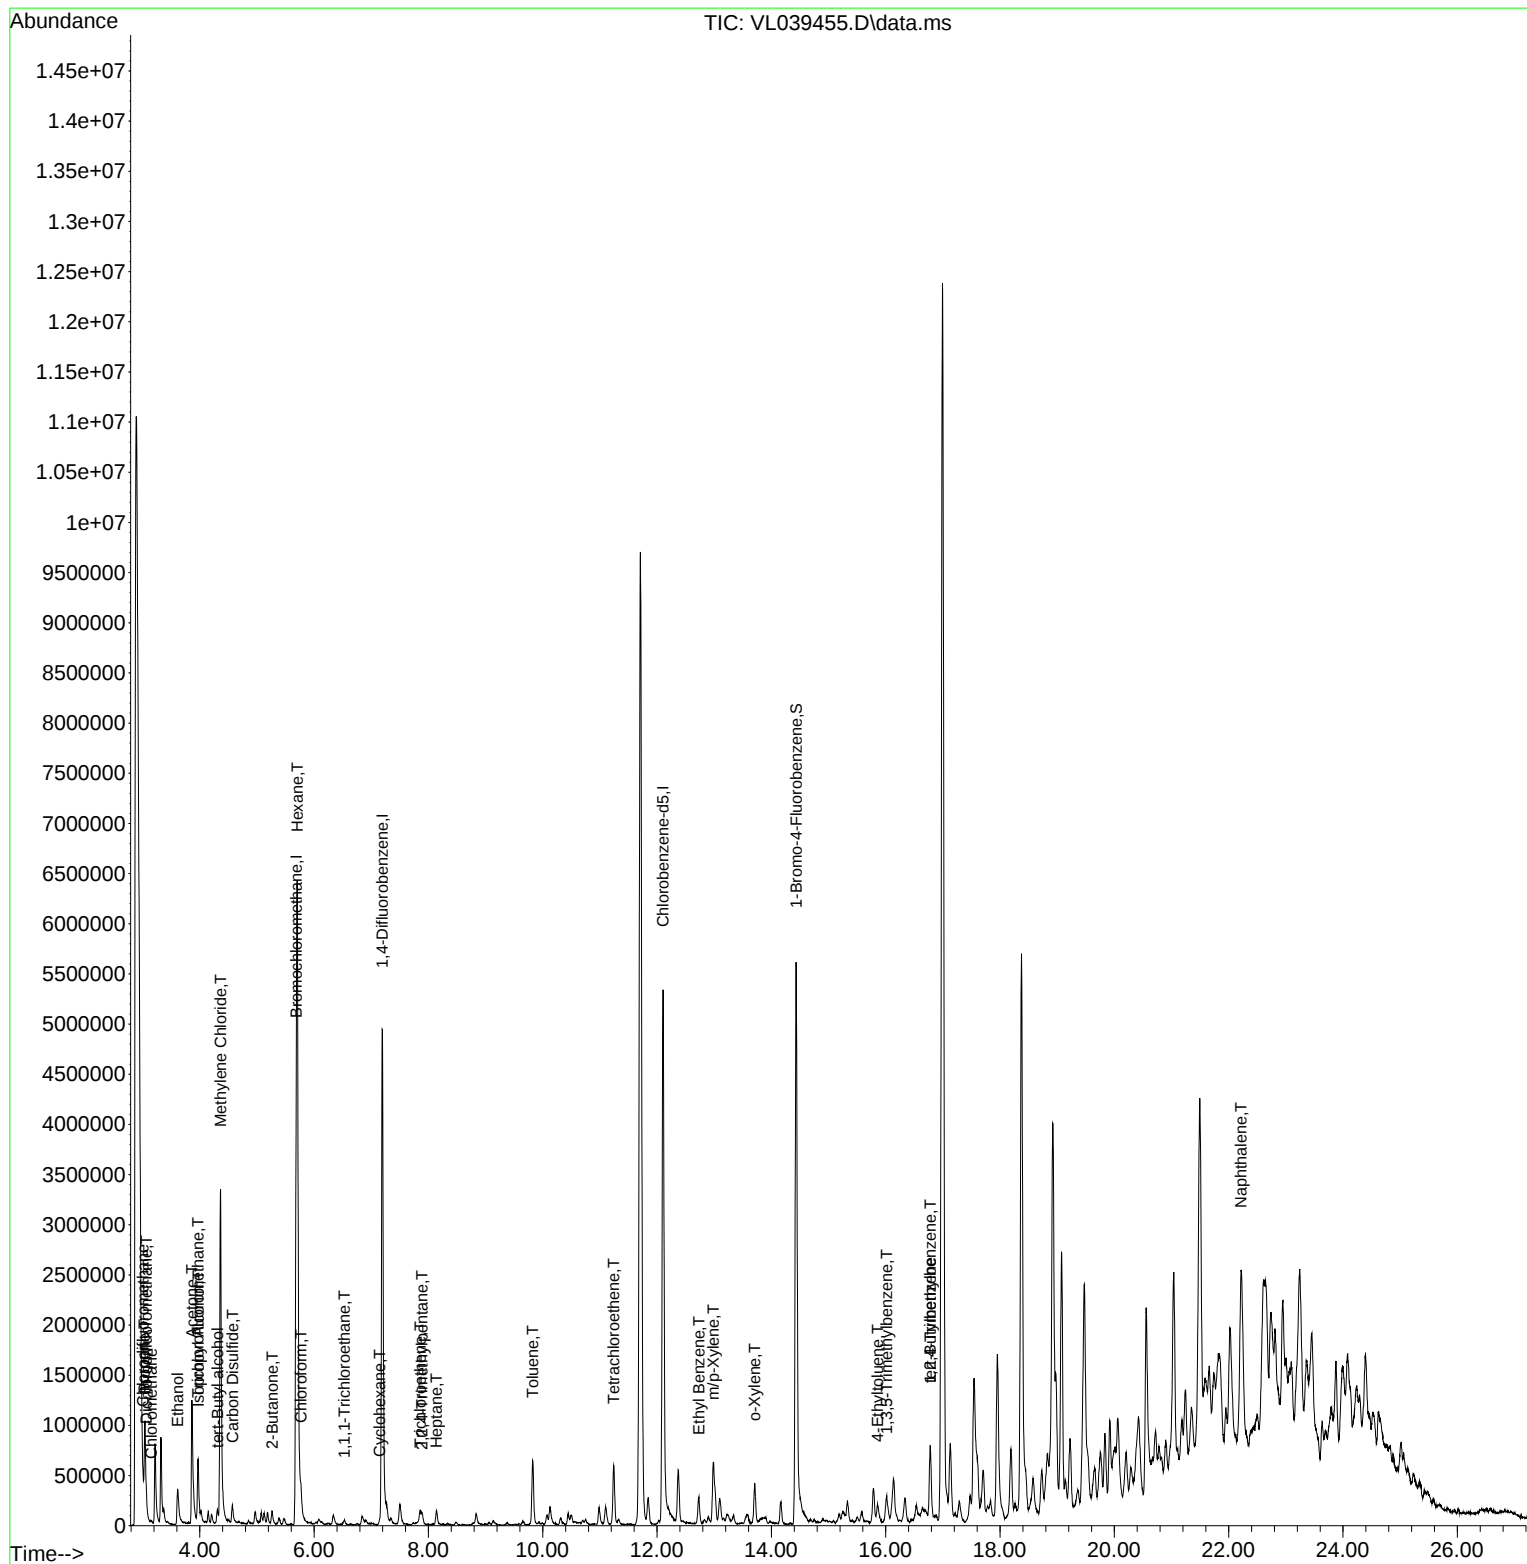







#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.687 min Scan# 90
Delta R.T. 0.035 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

Instrument :
MSVOA_L
ClientSampleId :
SG-9

Tgt Ion: 49 Resp: 155886
Ion Ratio Lower Upper
49 100
128 51.0 26.7 80.0
130 65.5 34.3 102.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

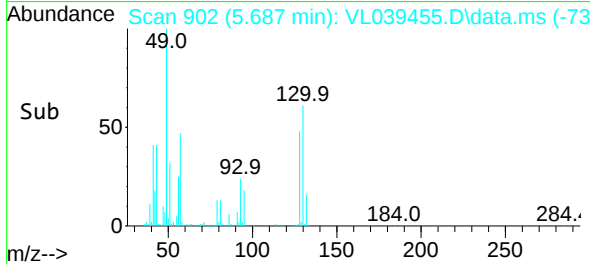

#2
Dichlorodifluoromethane
Concen: 0.446 ppbv
RT: 3.063 min Scan# 86
Delta R.T. 0.022 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30


Tgt Ion: 85 Resp: 100231
Ion Ratio Lower Upper
85 100
87 35.4 26.7 40.1

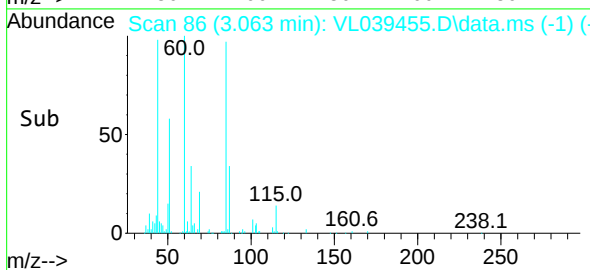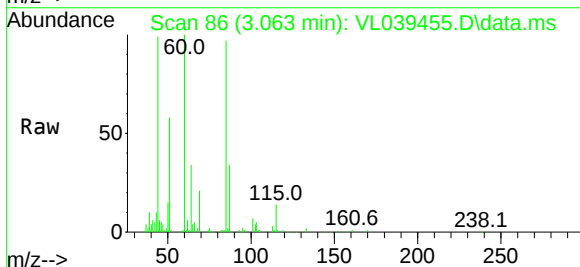



#3
Chlorodifluoromethane
Concen: 0.186 ppbv m
RT: 3.005 min Scan# 60
Delta R.T. 0.026 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9



Tgt Ion: 51 Resp: 3685
Ion Ratio Lower Upper
51 100
67 16.9 15.7 23.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

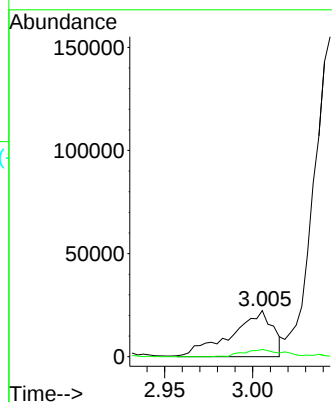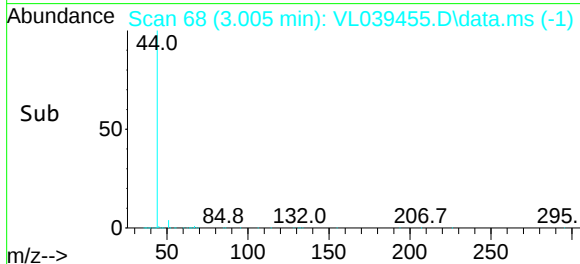

#4
Chloromethane
Concen: 0.138 ppbv m
RT: 3.153 min Scan# 114
Delta R.T. 0.022 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30


Tgt Ion: 50 Resp: 14959
Ion Ratio Lower Upper
50 100
52 34.1 26.5 39.7

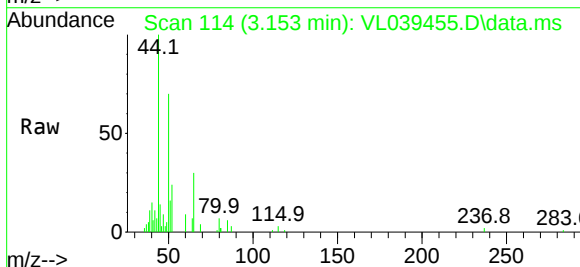

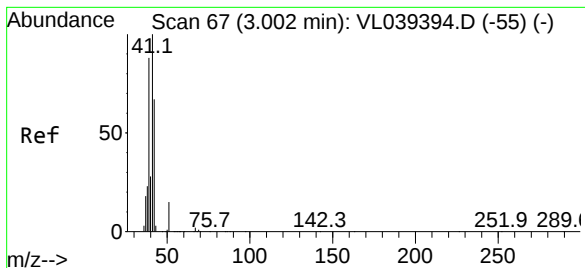

#9
 Propene
 Concen: 0.629 ppbv m
 RT: 3.028 min Scan# 71
 Delta R.T. 0.026 min
 Lab File: VL039455.D
 Acq: 12 Jul 2022 19:30




Instrument :
 MSVOA_L
 ClientSampleId :
 SG-9

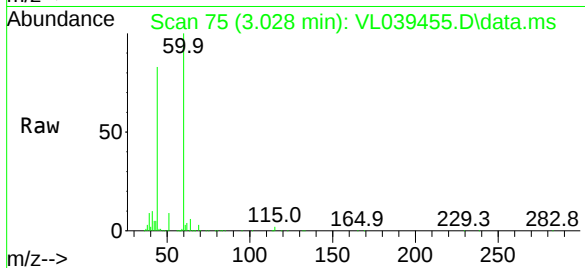

Tgt Ion: 41 Resp: 5621
 Ion Ratio Lower Upper
 41 100
 42 58.7 55.2 82.8




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
 Supervised By :Mahesh Dadoda 07/13/2022

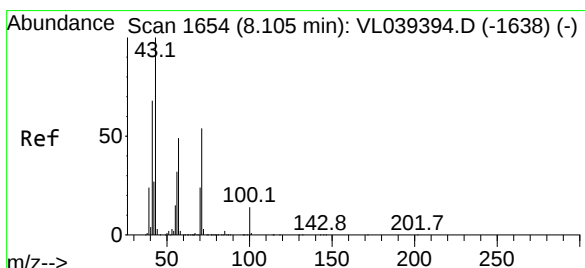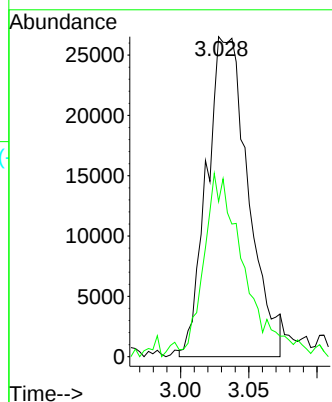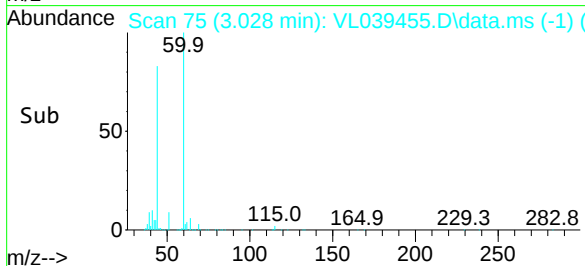

#10
 Heptane
 Concen: 0.301 ppbv
 RT: 8.140 min Scan# 1665
 Delta R.T. 0.035 min
 Lab File: VL039455.D
 Acq: 12 Jul 2022 19:30


Tgt Ion: 43 Resp: 62985
 Ion Ratio Lower Upper
 43 100
 57 55.2 40.5 60.7

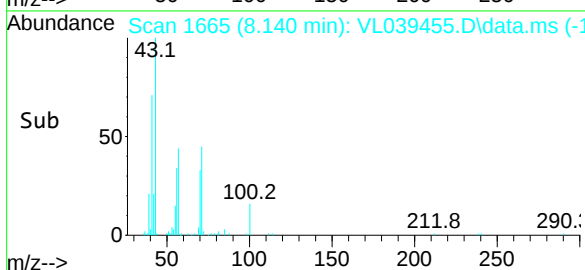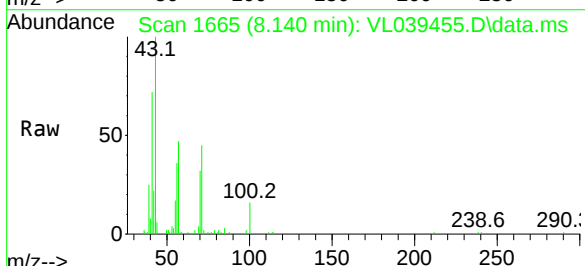



#11
Trichlorofluoromethane
Concen: 1.867 ppbv
RT: 3.967 min Scan# 30
Delta R.T. 0.029 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9




Tgt Ion:101 Resp: 46780
Ion Ratio Lower Upper
101 100
103 64.9 51.8 77.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

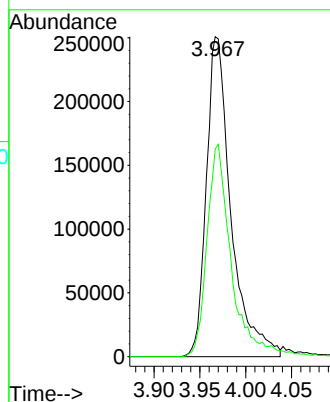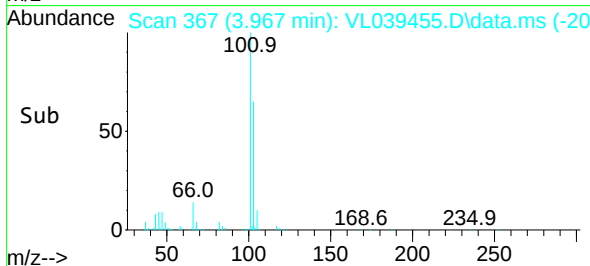


#13
Ethanol
Concen: 100.018 ppbv
RT: 3.613 min Scan# 257
Delta R.T. 0.019 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

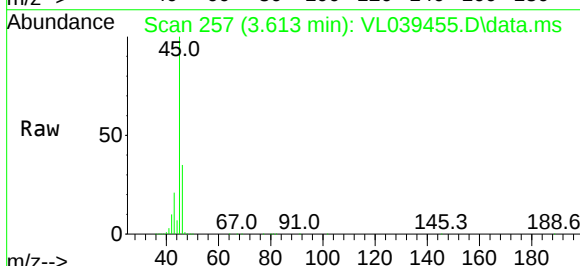


Tgt Ion: 45 Resp: 518277
Ion Ratio Lower Upper
45 100
46 37.1 22.8 91.2

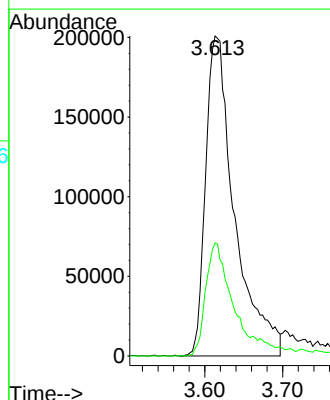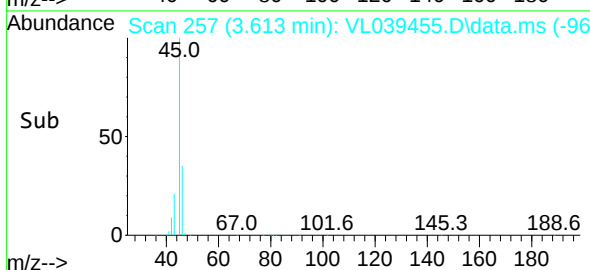

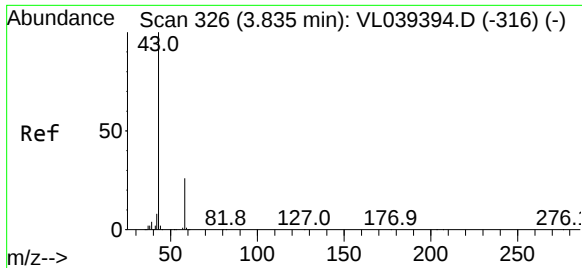

#15
Acetone
Concen: 8.638 ppbv
RT: 3.864 min Scan# 31
Delta R.T. 0.029 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9

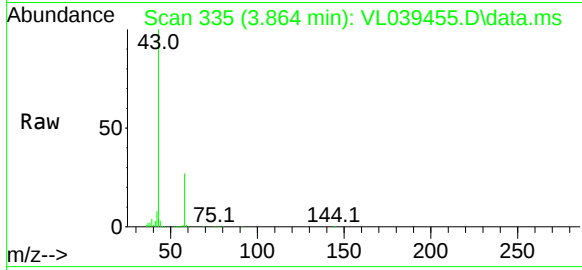

Tgt Ion: 43 Resp: 159304
Ion Ratio Lower Upper
43 100
58 29.6 21.0 31.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

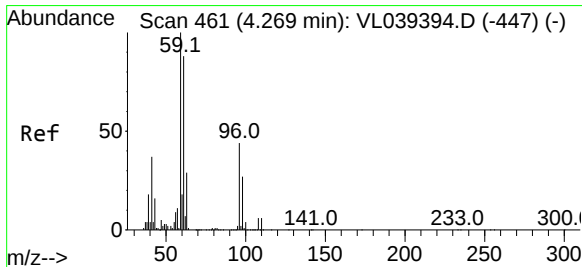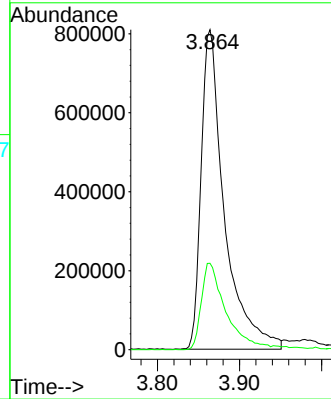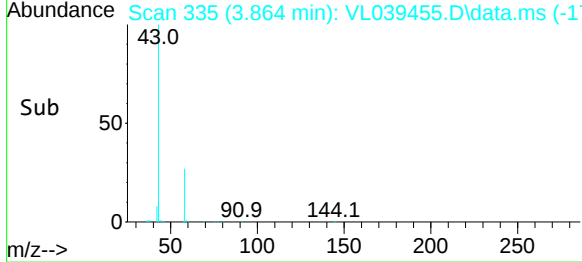

#17
tert-Butyl alcohol
Concen: 0.861 ppbv
RT: 4.311 min Scan# 474
Delta R.T. 0.042 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30


Tgt Ion: 59 Resp: 134706
Ion Ratio Lower Upper
59 100
57 11.5 8.7 13.1

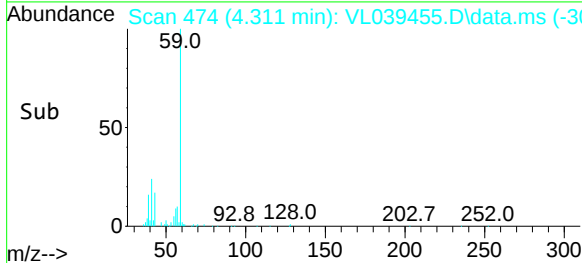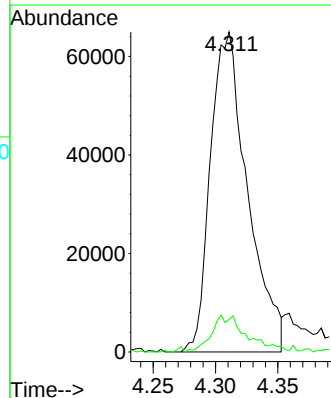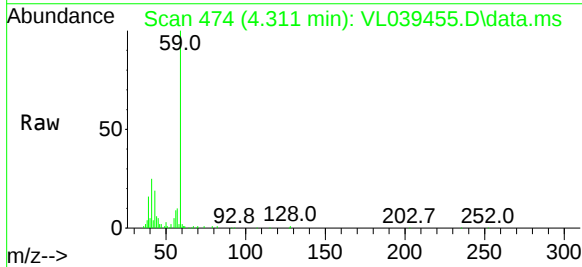



#19
Isopropyl Alcohol
Concen: 1.149 ppbv m
RT: 3.976 min Scan# 31
Delta R.T. 0.029 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9



Tgt Ion: 45 Resp: 11299
Ion Ratio Lower Upper
45 100
58 0.0 3.2 4.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

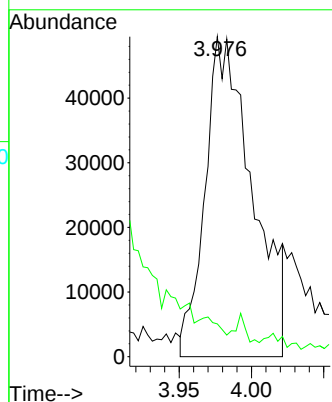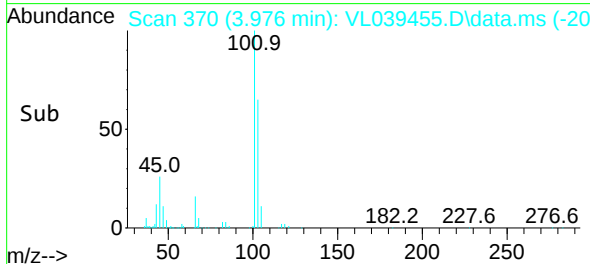

#20
Methylene Chloride
Concen: 19.148 ppbv
RT: 4.362 min Scan# 490
Delta R.T. 0.032 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30


Tgt Ion: 84 Resp: 1407538
Ion Ratio Lower Upper
84 100
49 155.4 123.1 184.7
51 48.1 34.4 51.6
86 63.0 51.1 76.7

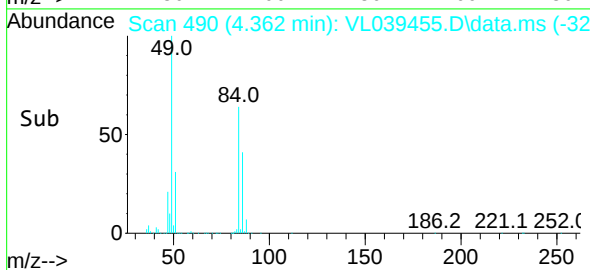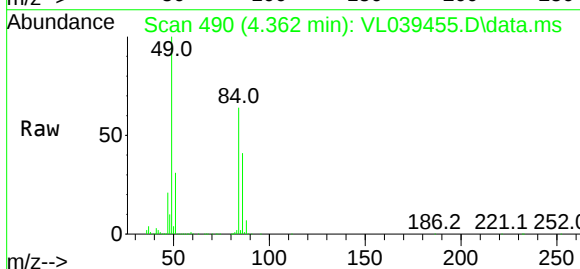

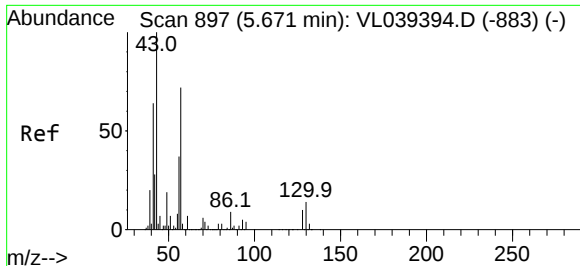

#26
Hexane
Concen: 16.846 ppbv
RT: 5.706 min Scan# 90
Delta R.T. 0.035 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9




Tgt Ion: 57 Resp: 2567964
Ion Ratio Lower Upper
57 100
41 88.2 76.9 115.3
43 76.4 191.0 286.6
56 52.7 43.2 64.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

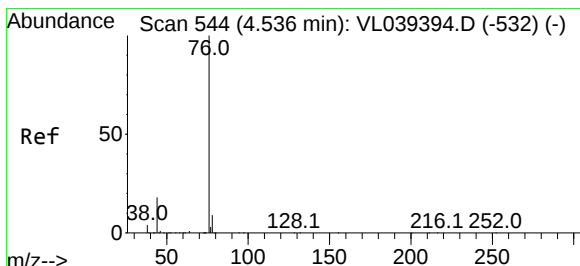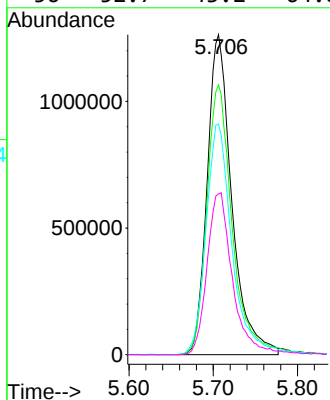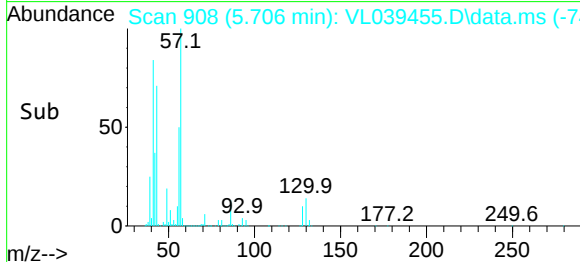


#27
Carbon Disulfide
Concen: 1.201 ppbv
RT: 4.571 min Scan# 555
Delta R.T. 0.035 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

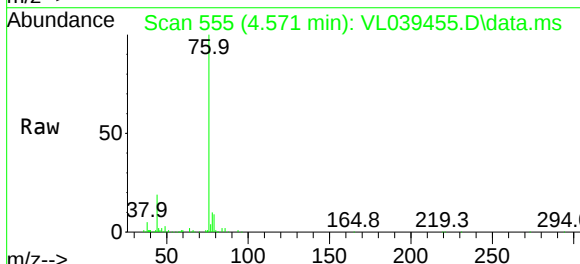

Tgt Ion: 76 Resp: 221026
Ion Ratio Lower Upper
76 100
44 21.0 14.6 21.8
78 10.0 7.8 11.6

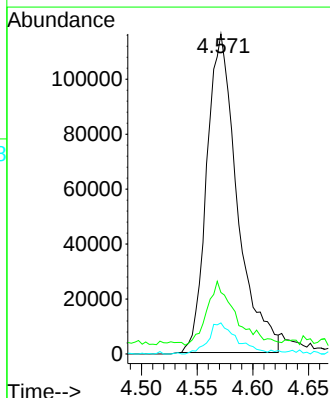







#29
Chloroform
Concen: 0.500 ppbv
RT: 5.771 min Scan# 917
Delta R.T. 0.035 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

Instrument :
MSVOA_L
ClientSampleId :
SG-9

Tgt Ion: 83 Resp: 132510
Ion Ratio Lower Upper
83 100
85 55.7 52.8 79.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

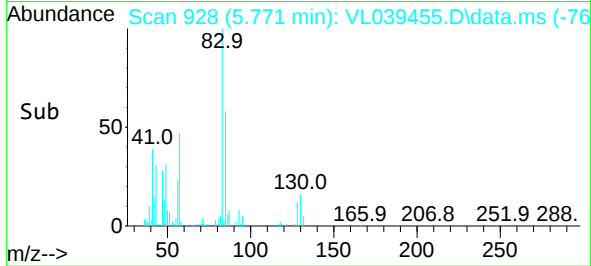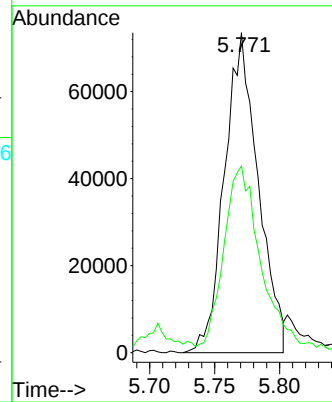

#30
Cyclohexane
Concen: 0.166 ppbv m
RT: 7.147 min Scan# 1356
Delta R.T. 0.035 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30


Tgt Ion: 84 Resp: 23053
Ion Ratio Lower Upper
84 100
56 0.0 107.7 161.5#
41 100.2 67.7 101.5

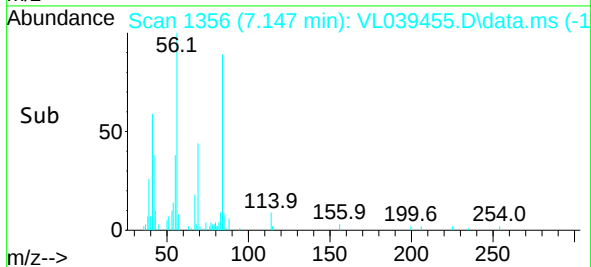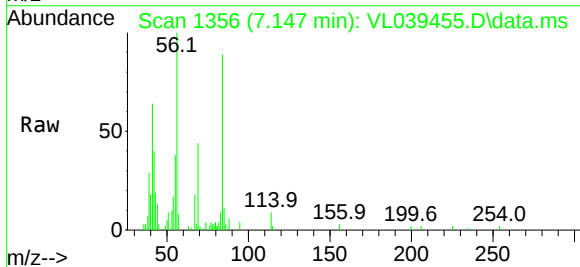

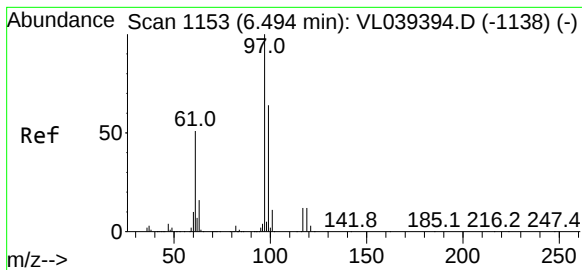

#32
1,1,1-Trichloroethane
Concen: 0.088 ppbv
RT: 6.533 min Scan# 1153
Delta R.T. 0.038 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9

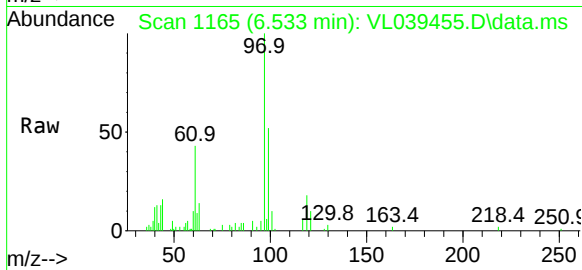


Tgt Ion: 97 Resp: 22998
Ion Ratio Lower Upper
97 100
99 73.7 52.3 78.5
61 58.0 40.9 61.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

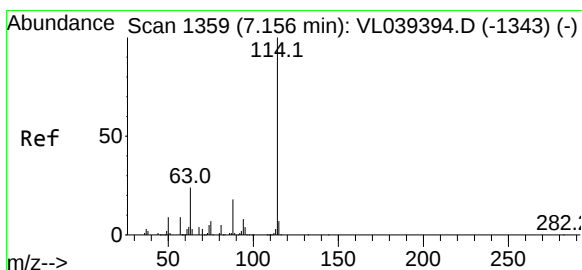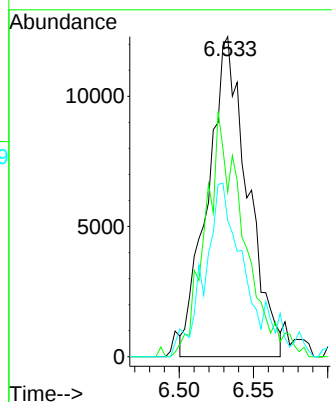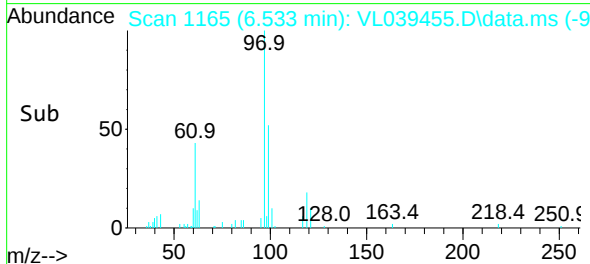


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.195 min Scan# 1371
Delta R.T. 0.038 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

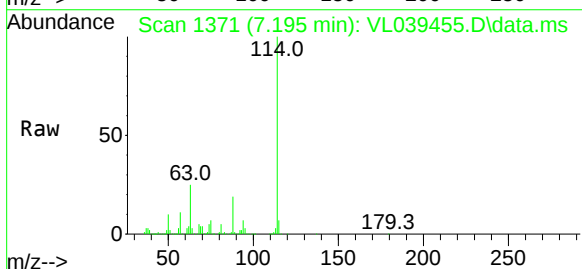


Tgt Ion:114 Resp: 4260566
Ion Ratio Lower Upper
114 100
63 24.8 20.2 30.4
88 18.4 14.5 21.7

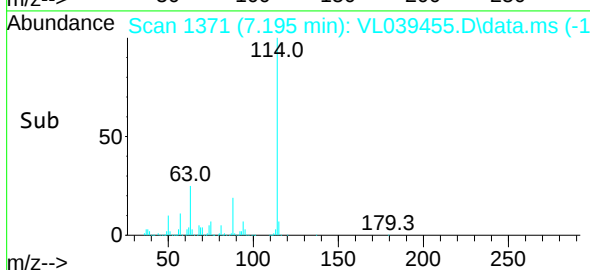

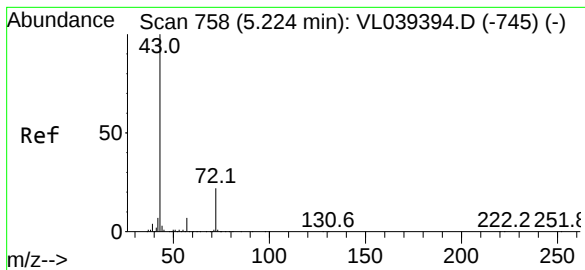

#34
2-Butanone
Concen: 0.724 ppbv
RT: 5.266 min Scan# 71
Delta R.T. 0.042 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9

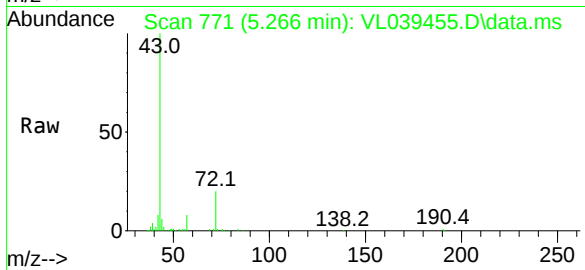

Tgt Ion: 43 Resp: 155344
Ion Ratio Lower Upper
43 100
72 27.8 17.9 26.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

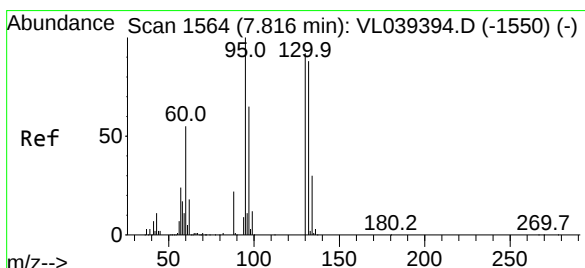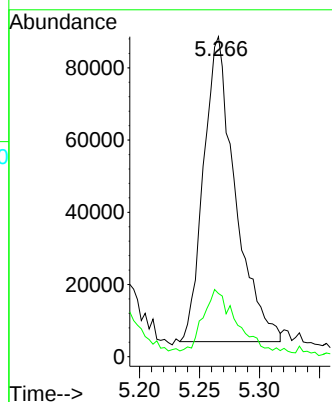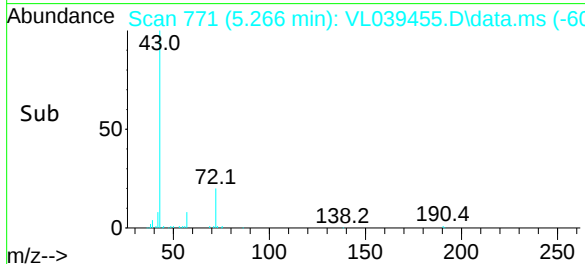

#38
Trichloroethene
Concen: 0.242 ppbv
RT: 7.854 min Scan# 1576
Delta R.T. 0.038 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30


Tgt Ion:130 Resp: 43189
Ion Ratio Lower Upper
130 100
95 97.4 87.3 130.9
132 96.8 76.7 115.1
97 60.6 56.5 84.7

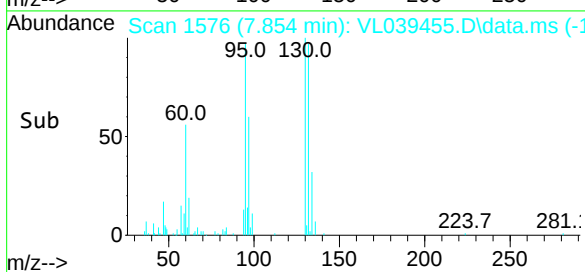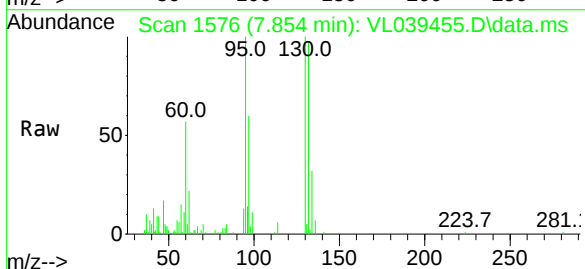



#44
2,2,4-Trimethylpentane
Concen: 0.141 ppbv m
RT: 7.886 min Scan# 1586
Delta R.T. 0.035 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9




Tgt Ion: 57 Resp: 78964
Ion Ratio Lower Upper
57 100
41 50.6 27.4 41.2
56 0.0 24.5 36.7

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

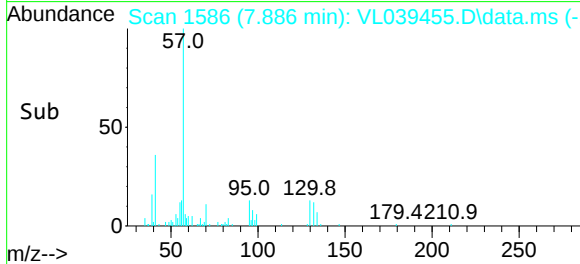


#52
Tetrachloroethene
Concen: 1.221 ppbv
RT: 11.243 min Scan# 2630
Delta R.T. 0.045 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

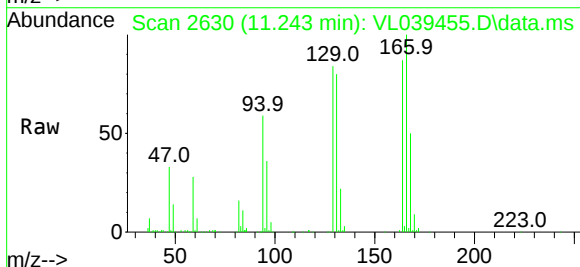


Tgt Ion:164 Resp: 162071
Ion Ratio Lower Upper
164 100
166 113.2 102.2 153.2
129 95.4 85.8 128.8
131 90.7 83.3 124.9

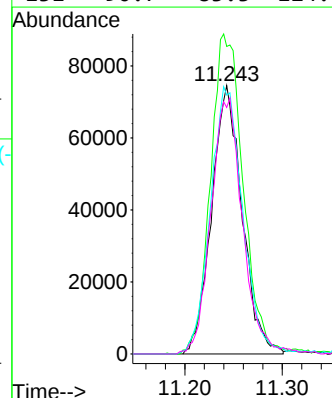



#53
Toluene
Concen: 1.406 ppbv
RT: 9.822 min Scan# 2176
Delta R.T. 0.038 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9




Tgt Ion: 91 Resp: 534658
Ion Ratio Lower Upper
91 100
92 59.3 48.2 72.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

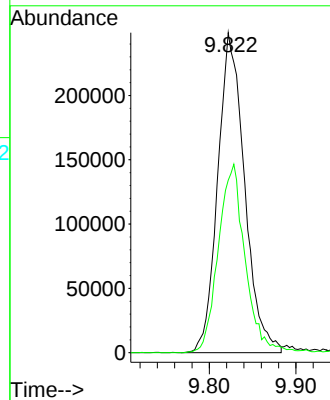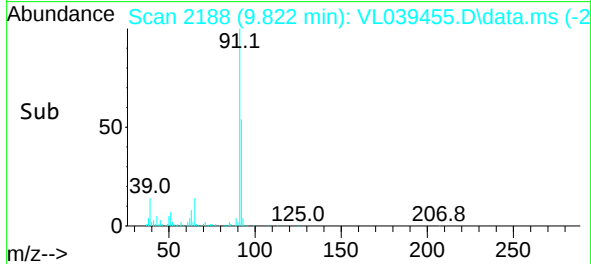


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.105 min Scan# 2898
Delta R.T. 0.038 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

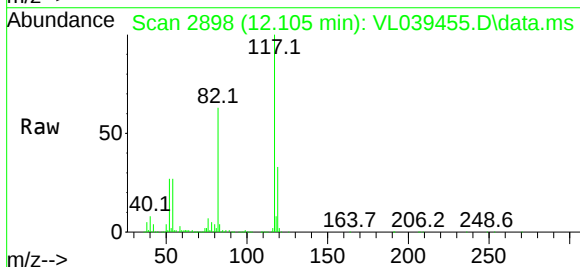


Tgt Ion:117 Resp: 3920614
Ion Ratio Lower Upper
117 100
82 64.6 50.8 76.2
119 33.2 24.1 36.1

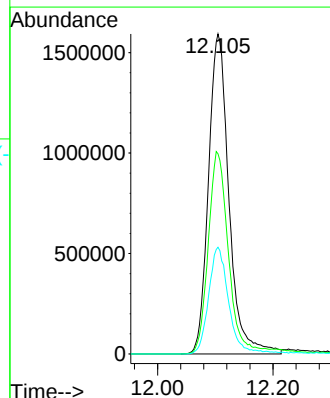



#58
Ethyl Benzene
Concen: 0.483 ppbv
RT: 12.732 min Scan# 3079
Delta R.T. 0.045 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9



Tgt Ion: 91 Resp: 24429
Ion Ratio Lower Upper
91 100
106 28.3 25.4 38.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

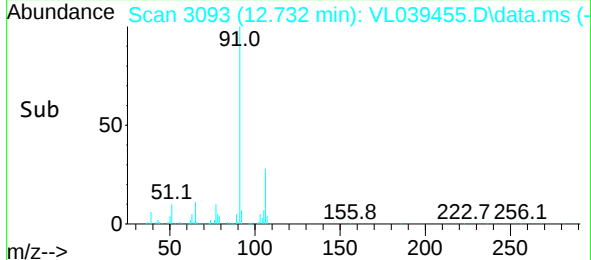

#59
m/p-Xylene
Concen: 1.493 ppbv m
RT: 12.982 min Scan# 3171
Delta R.T. 0.010 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

Tgt Ion: 91 Resp: 666426
Ion Ratio Lower Upper
91 100
106 47.0 35.4 53.2

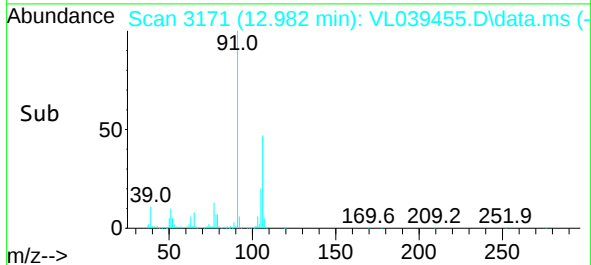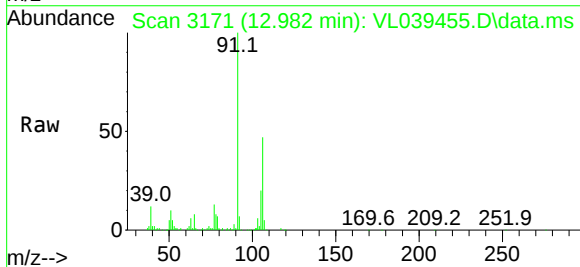







#60
o-Xylene
Concen: 0.738 ppbv
RT: 13.709 min Scan# 31192
Delta R.T. 0.042 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

Instrument :
MSVOA_L
ClientSampleId :
SG-9

Tgt Ion: 91 Resp: 31192
Ion Ratio Lower Upper
91 100
106 45.1 22.4 67.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

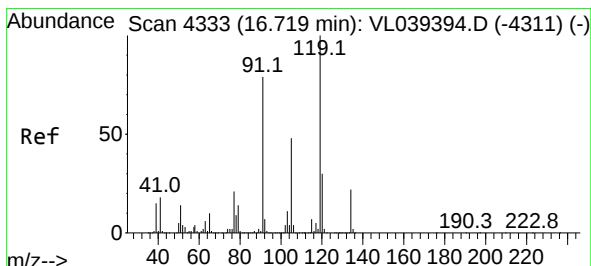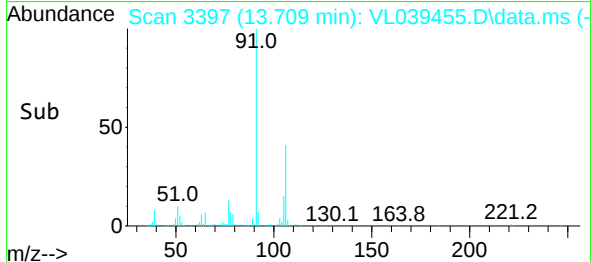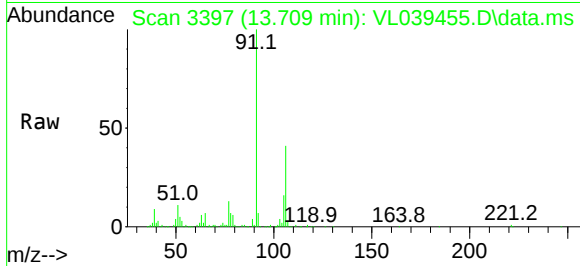

#65
tert-Butylbenzene
Concen: 0.109 ppbv m
RT: 16.780 min Scan# 4352
Delta R.T. 0.061 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30


Tgt Ion:119 Resp: 65076
Ion Ratio Lower Upper
119 100
91 99.5 63.4 95.2#
134 0.0 15.9 23.9#

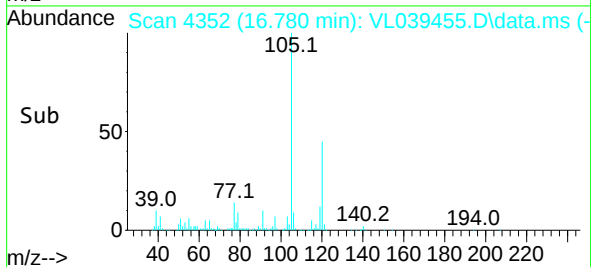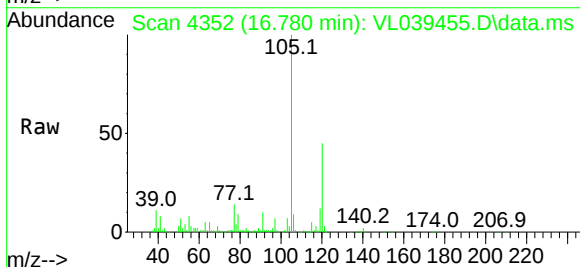

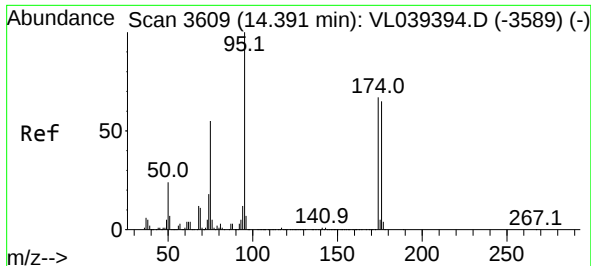

#68
1-Bromo-4-Fluorobenzene
Concen: 9.822 ppbv
RT: 14.436 min Scan# 30
Delta R.T. 0.045 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30




Instrument :
MSVOA_L
ClientSampleId :
SG-9




Tgt Ion: 95 Resp: 285676
Ion Ratio Lower Upper
95 100
174 75.4 55.9 83.9
175 5.8 4.2 6.4

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

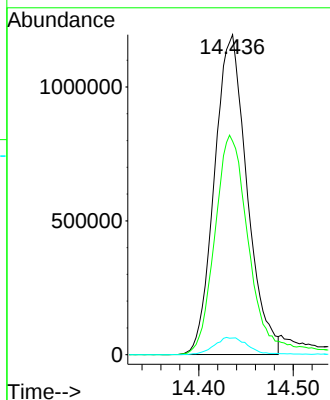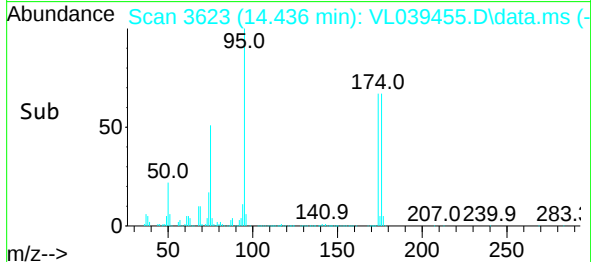


#72
4-Ethyltoluene
Concen: 0.236 ppbv m
RT: 15.857 min Scan# 4065
Delta R.T. 0.042 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

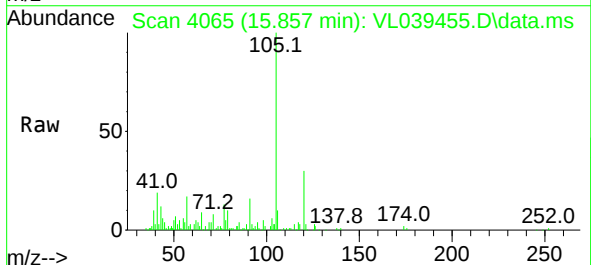

Tgt Ion:105 Resp: 117471
Ion Ratio Lower Upper
105 100
120 28.6 24.2 36.2
91 0.0 10.2 15.4#
77 13.9 11.1 16.7

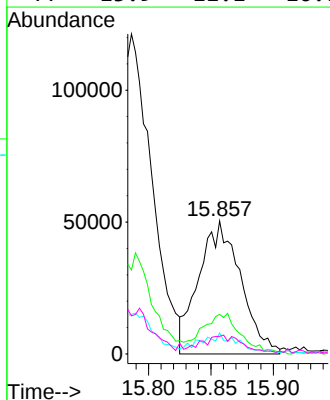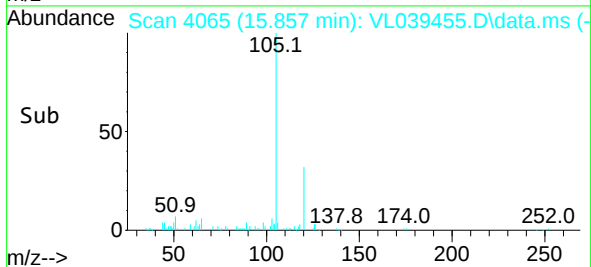



#73

1,3,5-Trimethylbenzene

Concen: 0.389 ppbv

RT: 16.018 min Scan# 4115

Delta R.T. 0.045 min

Lab File: VL039455.D

Acq: 12 Jul 2022 19:30

Instrument :

MSVOA_L

ClientSampleId :

SG-9

Tgt Ion:105 Resp: 177694

Ion Ratio Lower Upper

105 100





120 44.7 38.2 57.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022

Supervised By :Mahesh Dadoda 07/13/2022

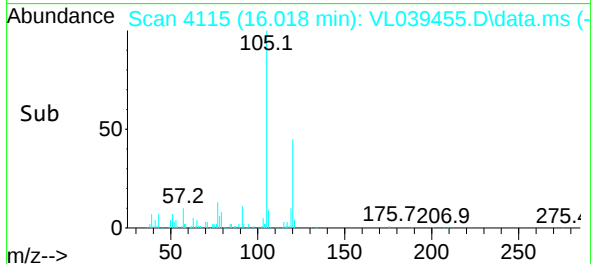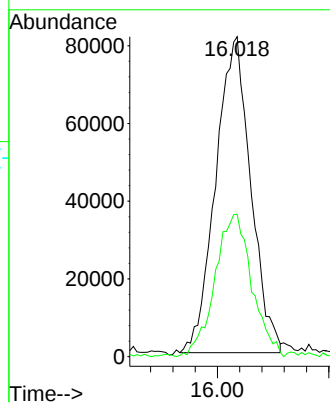

#74

1,2,4-Trimethylbenzene

Concen: 1.105 ppbv

RT: 16.780 min Scan# 4352

Delta R.T. 0.042 min

Lab File: VL039455.D

Acq: 12 Jul 2022 19:30

Tgt Ion:105 Resp: 558114




Ion Ratio Lower Upper


105 100

120 45.1 39.5 59.3

91 9.6 39.2 58.8#


77 13.5 17.2 25.8#

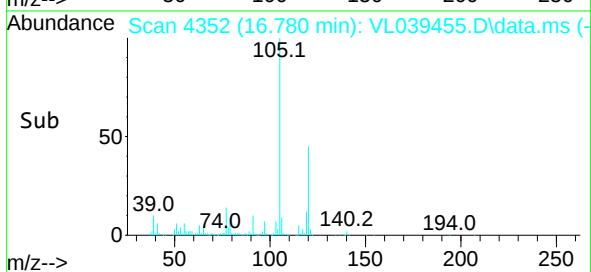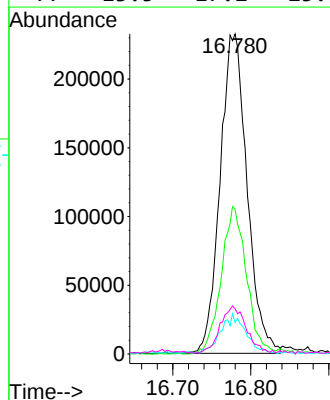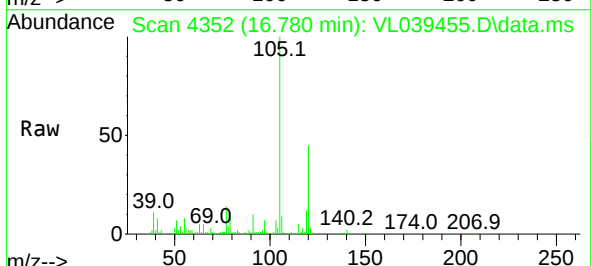

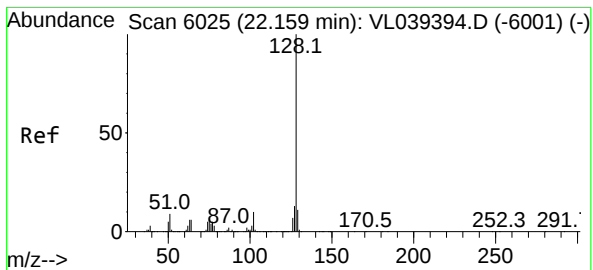

#79
Naphthalene
Concen: 0.234 ppbv m
RT: 22.217 min Scan# 6025
Delta R.T. 0.058 min
Lab File: VL039455.D
Acq: 12 Jul 2022 19:30

Instrument :
MSVOA_L
ClientSampleId :
SG-9



Tgt Ion:128 Resp: 8137
Ion Ratio Lower Upper
128 100
127 20.9 10.6 15.8
129 12.9 8.8 13.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/13/2022
Supervised By :Mahesh Dadoda 07/13/2022

