


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL071222\
 Data File : VL039441.D
 Acq On : 12 Jul 2022 8:06
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 06 02:15:38 2022
 Last Update : Wed Jul 06 02:15:38 2022

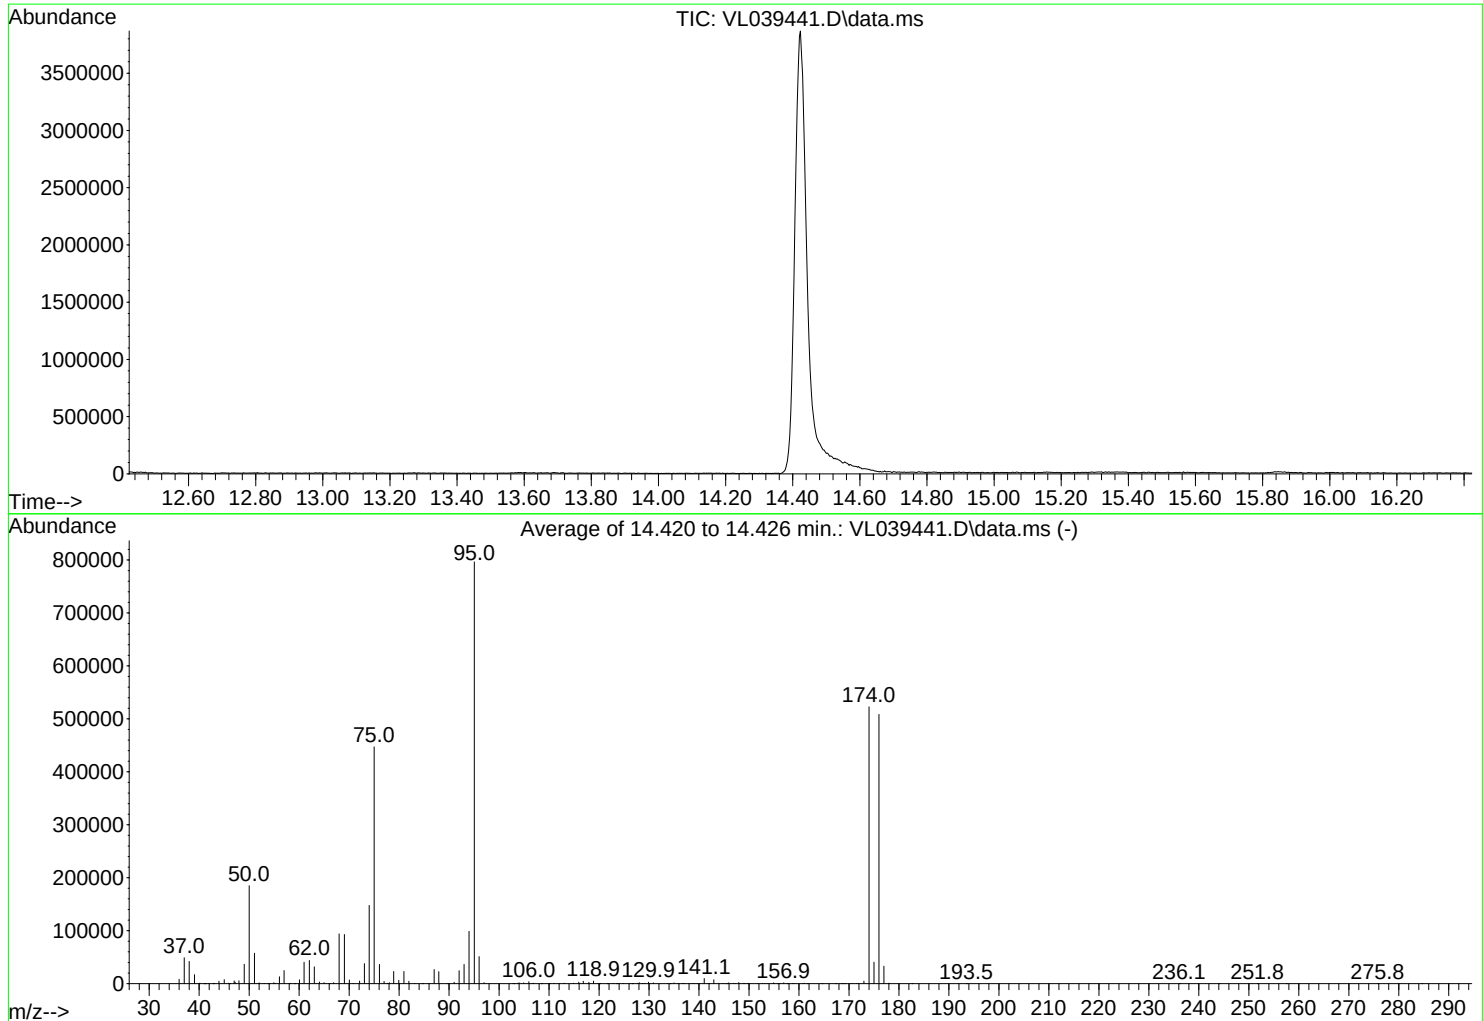

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.2	184960	PASS
75	95	30	66	56.1	447232	PASS
95	95	100	100	100.0	796544	PASS
96	95	5	9	6.4	50944	PASS
173	174	0.00	2	0.9	4945	PASS
174	95	50	120	65.6	522880	PASS
175	174	4	9	7.8	40635	PASS
176	174	93	101	97.3	508523	PASS
177	176	5	9	6.5	32896	PASS

Average of 14.420 to 14.426 min.: VL039441.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8315	43.95	4658	52.05	1310	60.05	7370
37.00	49067	45.00	7619	53.00	396	61.00	40530
38.00	42168	45.90	1044	53.80	74	62.05	4395
39.05	17024	46.10	148	54.05	193	63.05	3186
40.00	341	47.00	5218	54.95	1982	64.05	3095
40.15	893	47.20	2846	55.20	742	65.00	1831
41.00	72	47.95	5555	56.05	13159	66.00	113
41.20	84	49.00	36456	57.00	24923	66.90	1969
41.85	208	50.00	184960	58.05	547	68.00	93957
42.80	62	51.05	57363	58.30	309	69.05	92693
43.05	534	51.90	828	59.10	119	70.05	7026

Average of 14.420 to 14.426 min.: VL039441.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
70.80	412	80.95	22901	94.00	98965	106.95	1057
72.10	4811	81.95	4513	95.05	796544	108.50	79
73.05	37867	83.10	615	96.00	50944	109.80	272
74.00	147691	84.70	64	97.00	1836	110.00	131
75.00	447232	85.95	758	102.80	344	111.00	638
76.05	36315	87.00	26629	103.00	162	112.00	704
77.00	4365	87.95	22640	103.80	956	113.05	773
77.70	679	89.70	101	104.00	1648	114.85	813
78.05	1793	91.00	2604	104.95	1430	115.95	2771
78.90	22963	92.00	24469	105.95	3535	116.85	4605
79.95	6524	93.00	36192	106.60	285	117.95	2422

Average of 14.420 to 14.426 min.: VL039441.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.90	4995	126.60	102	135.80	174	142.95	7286
119.80	63	126.90	438	136.75	606	143.95	545
120.10	88	127.70	722	136.90	397	144.90	434
121.60	105	128.05	1963	137.10	424	145.50	88
121.90	209	128.70	359	138.05	379	145.95	1503
122.80	262	129.00	660	138.75	199	146.95	484
123.50	82	129.90	2701	139.05	274	147.30	200
123.80	232	130.85	1474	139.65	460	147.95	2094
124.00	192	133.70	357	141.05	9686	148.85	436
124.85	378	134.20	85	141.80	216	149.15	660
126.10	323	135.00	1437	142.05	654	149.70	635

Average of 14.420 to 14.426 min.: VL039441.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
150.00	480	158.70	433	171.90	659	244.00	55
151.75	286	159.00	381	173.00	4945	251.75	119
152.65	343	160.80	363	174.00	522880	257.50	70
153.10	333	161.05	1018	175.00	40635	275.80	62
153.80	425	161.70	123	176.00	508523	284.60	55
154.90	1417	164.60	69	177.00	32896		
155.10	420	167.30	51	177.90	359		
155.70	120	168.55	190	178.05	999		
156.20	219	169.10	109	182.60	91		
156.95	1692	170.65	464	193.50	90		
157.65	170	171.50	343	236.10	66		