


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072022\
Data File : VL039509.D
Acq On : 20 Jul 2022 13:54
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jul 06 02:15:38 2022
Last Update : Wed Jul 06 02:15:38 2022

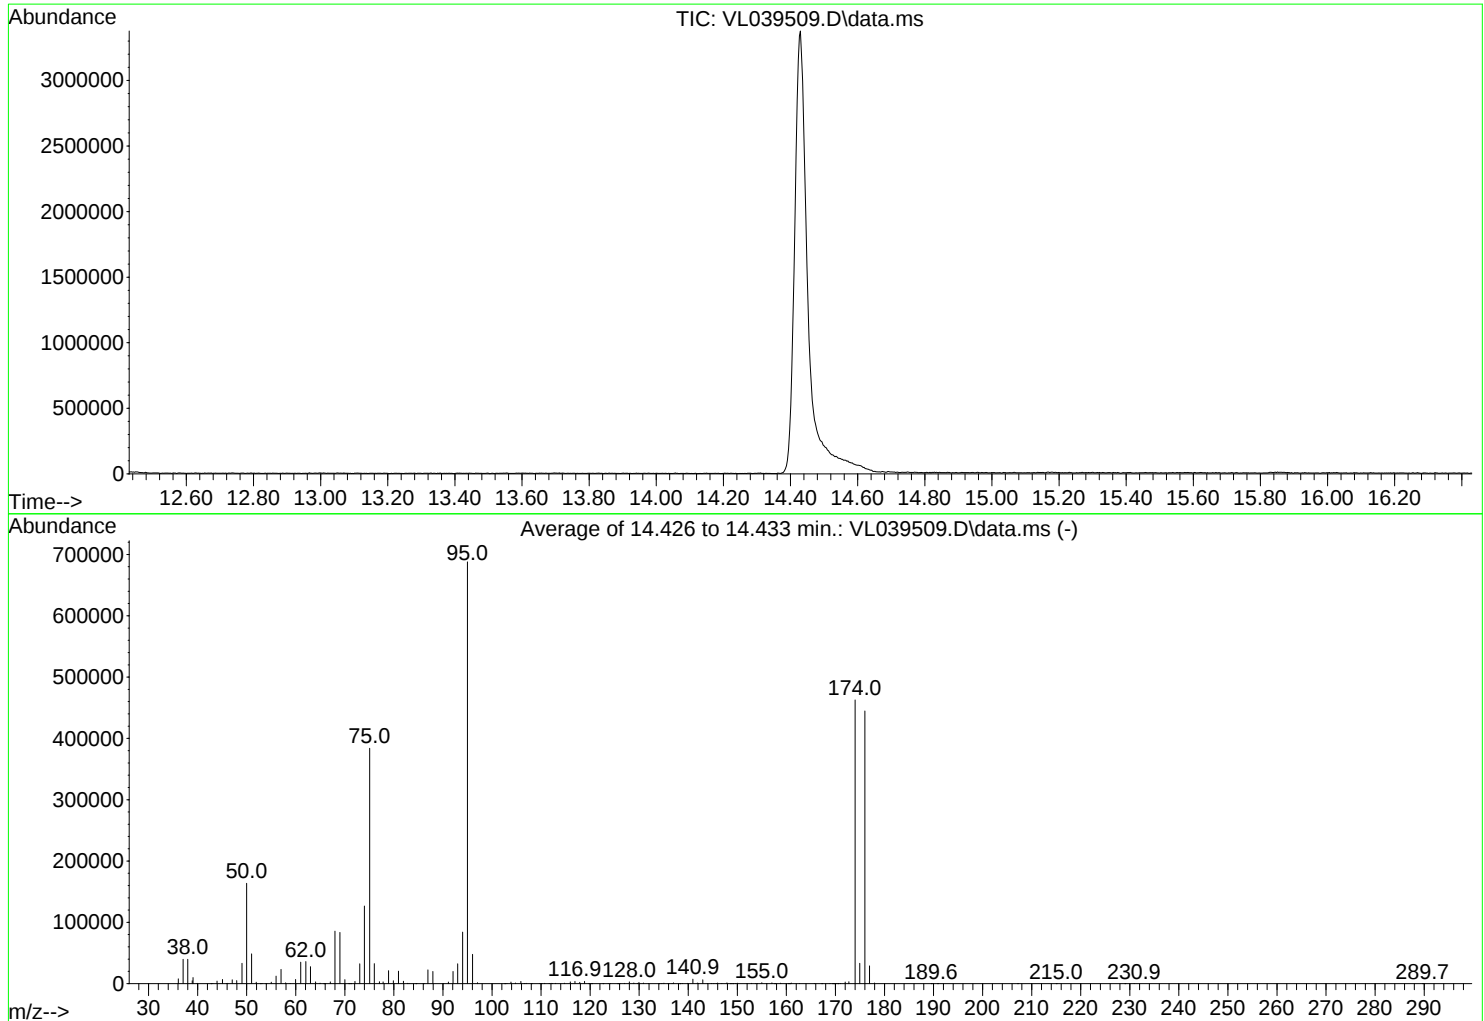

AutoFind: Scans 3620, 3621, 3622; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	163669	PASS
75	95	30	66	55.8	383808	PASS
95	95	100	100	100.0	688021	PASS
96	95	5	9	7.0	47821	PASS
173	174	0.00	2	0.7	3141	PASS
174	95	50	120	67.3	462805	PASS
175	174	4	9	7.1	33040	PASS
176	174	93	101	96.1	444779	PASS
177	176	5	9	6.5	29029	PASS

Average of 14.426 to 14.433 min.: VL039509.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7938	46.15	612	56.00	12213	65.90	64
37.05	39619	47.05	6183	57.00	23227	67.05	302
38.00	39803	47.95	5083	57.95	1365	68.00	8562
38.90	4857	49.05	33240	58.85	260	69.00	8353
39.05	9998	50.00	163669	59.95	6857	70.00	6606
39.90	471	51.00	48587	61.00	35101	70.80	56
42.70	91	51.95	2272	62.05	36035	71.20	82
43.10	218	52.80	112	63.00	27715	72.05	3621
43.95	4079	53.15	296	64.05	3034	73.05	32413
45.05	6694	53.90	61	64.95	911	74.00	126504
45.90	412	55.00	2311	65.70	73	75.05	383808

Average of 14.426 to 14.433 min.: VL039509.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	32621	86.95	22483	103.05	255	112.05	478
77.05	3140	87.95	19960	103.85	2699	112.30	314
77.80	2763	90.10	250	104.80	1028	112.95	571
78.90	21109	91.10	2560	105.90	3656	114.75	704
79.90	4781	92.05	19947	106.60	215	115.95	2792
80.95	20312	93.00	32405	106.95	546	116.90	3780
81.95	3981	94.00	84024	108.00	136	117.90	2107
82.80	564	95.00	688021	109.75	166	118.85	3679
83.10	237	96.05	47821	110.00	55	119.70	62
84.50	115	97.05	1714	110.75	546	120.30	147
86.00	67	102.60	138	111.65	265	122.60	142

Average of 14.426 to 14.433 min.: VL039509.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.70	161	134.00	122	142.10	445	149.60	225
124.10	208	134.60	367	142.95	6317	150.00	689
125.60	54	135.05	788	143.95	311	152.00	350
125.90	116	135.90	131	144.75	240	152.90	651
127.00	416	136.70	310	145.20	377	153.75	411
128.00	2790	137.00	1419	145.70	260	154.10	221
128.90	974	138.30	136	146.00	1052	155.00	1579
129.70	555	138.85	307	146.85	192	156.00	180
129.95	2200	139.90	650	147.90	1444	157.05	1461
130.85	1078	140.95	7268	148.60	133	157.60	55
131.95	169	141.85	1059	149.05	32	158.85	927

Average of 14.426 to 14.433 min.: VL039509.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.40	99	171.00	340	215.00	113		
160.70	135	172.00	2539	229.00	55		
161.00	959	172.75	3141	230.90	188		
162.65	177	174.00	462805	289.70	67		
165.70	223	174.95	33040				
167.20	109	176.00	444779				
168.90	335	176.95	29029				
169.40	145	177.95	1035				
169.70	55	189.55	132				
170.15	391	190.80	115				
170.50	108	207.10	55				