
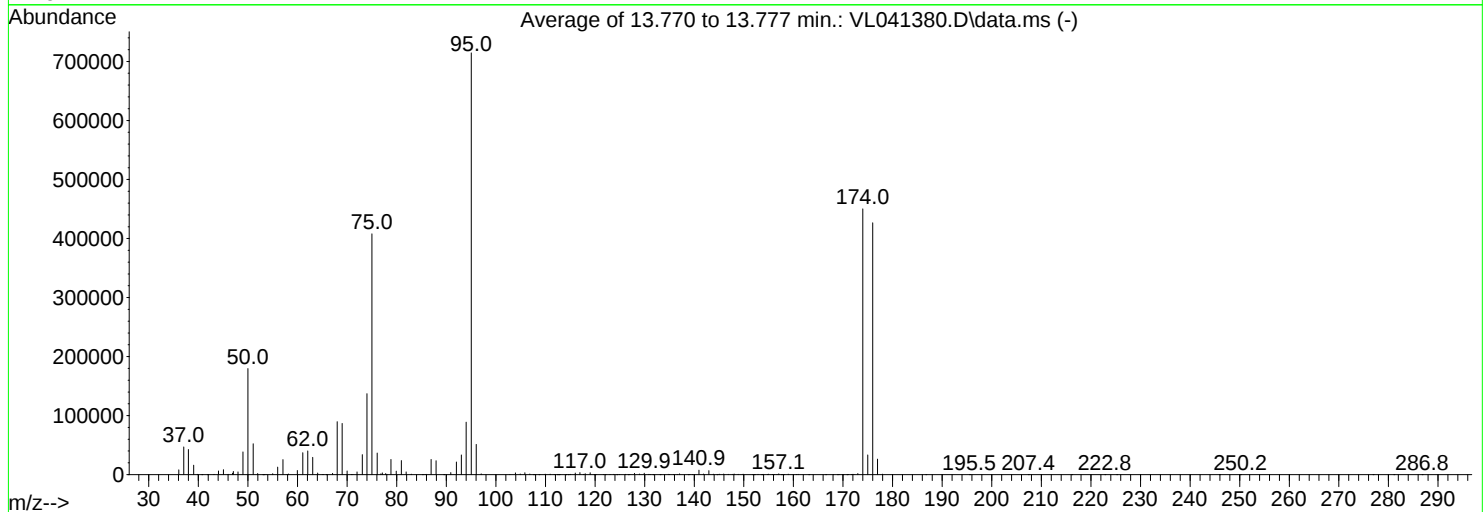


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072224\
Data File : VL041380.D
Acq On : 22 Jul 2024 9:46
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL062624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jul 23 02:50:01 2024

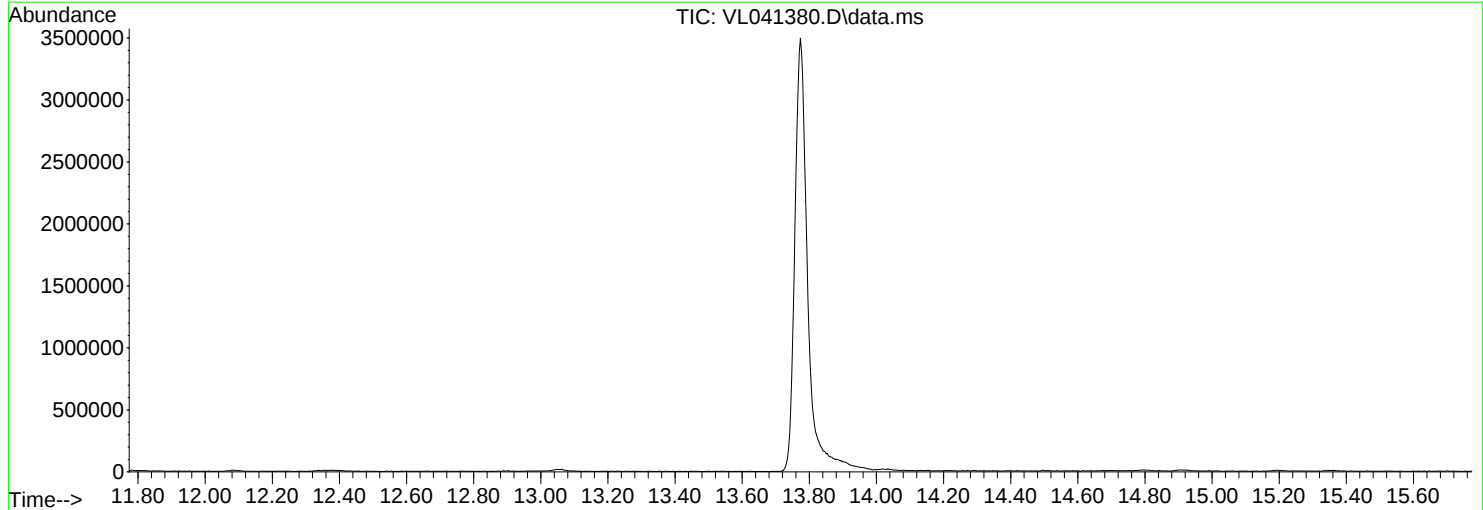

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.2	179797	PASS
75	95	30	66	57.1	408000	PASS
95	95	100	100	100.0	714581	PASS
96	95	5	9	7.2	51389	PASS
173	174	0.00	2	0.4	1847	PASS
174	95	50	120	63.0	450112	PASS
175	174	4	9	7.4	33451	PASS
176	174	93	101	94.8	426603	PASS
177	176	5	9	6.2	26304	PASS

Average of 13.770 to 13.777 min.: VL041380.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8254	46.90	2409	56.00	12862	65.80	111
37.05	46952	47.05	5462	57.05	25424	67.05	205
38.00	42712	48.00	4739	57.90	408	68.00	8978
39.05	16052	49.00	38525	58.15	1000	69.00	8666
39.80	652	50.00	179797	59.95	7085	70.00	6308
40.70	123	51.05	52400	61.05	37067	70.90	167
41.85	139	51.95	2022	62.05	40176	71.15	362
43.15	508	53.00	154	63.05	29179	72.00	4642
44.05	6323	53.20	138	64.05	2847	73.05	33907
45.05	8344	53.65	161	65.00	217	74.00	137173
46.00	667	55.00	1718	65.25	340	75.00	408000

Average of 13.770 to 13.777 min.: VL041380.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	36608	85.70	198	97.05	1295	111.75	313
76.80	1260	85.95	418	102.80	231	112.00	351
77.10	3038	86.95	25845	103.95	2962	112.40	120
77.75	1568	87.95	23491	104.90	1056	112.70	152
78.00	741	89.50	86	105.85	3183	112.95	288
78.85	25677	90.90	3568	106.85	1031	114.10	65
79.90	5970	92.05	21341	107.60	66	114.60	149
80.95	23891	93.05	33315	108.05	228	115.00	614
81.90	4639	94.00	88944	108.70	98	116.00	2753
82.95	766	95.05	714581	109.95	714	116.95	3627
85.20	64	96.05	51389	110.95	708	117.70	689

Average of 13.770 to 13.777 min.: VL041380.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.00	1614	126.70	118	135.00	336	143.85	707
119.00	3312	127.00	255	135.85	225	144.60	97
119.80	61	127.95	2264	136.60	195	145.05	830
120.00	57	128.95	1246	137.05	1255	145.95	1062
121.70	245	129.90	2531	138.80	68	146.85	481
122.00	61	130.85	622	139.10	269	147.80	622
123.00	283	131.10	386	139.70	176	148.05	988
123.80	443	131.70	104	140.00	358	148.85	454
124.40	159	133.10	81	140.95	7527	149.85	732
124.90	237	134.05	204	141.85	1051	151.80	155
126.15	445	134.75	685	142.95	6706	152.10	151

Average of 13.770 to 13.777 min.: VL041380.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.85	463	158.95	902	171.10	331	195.50	93
153.60	133	160.60	208	171.70	368	207.40	54
153.90	561	160.95	426	171.90	439	216.10	91
154.80	268	163.10	106	172.20	444	222.80	97
154.95	900	166.50	110	173.00	1847	225.20	51
155.80	322	168.10	246	174.00	450112	245.90	85
156.10	220	168.90	51	175.00	33451	250.15	126
156.70	241	169.25	323	176.00	426603	276.90	62
157.05	1346	169.90	83	176.95	26304	281.10	81
157.60	53	170.15	358	177.95	732	286.80	149
158.00	66	170.80	116	186.70	61		