


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL072320\
 Data File : VL035222.D
 Acq On : 23 Jul 2020 8:40
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL070820AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jul 08 07:05:23 2020
 Last Update : Wed Jul 08 07:05:23 2020

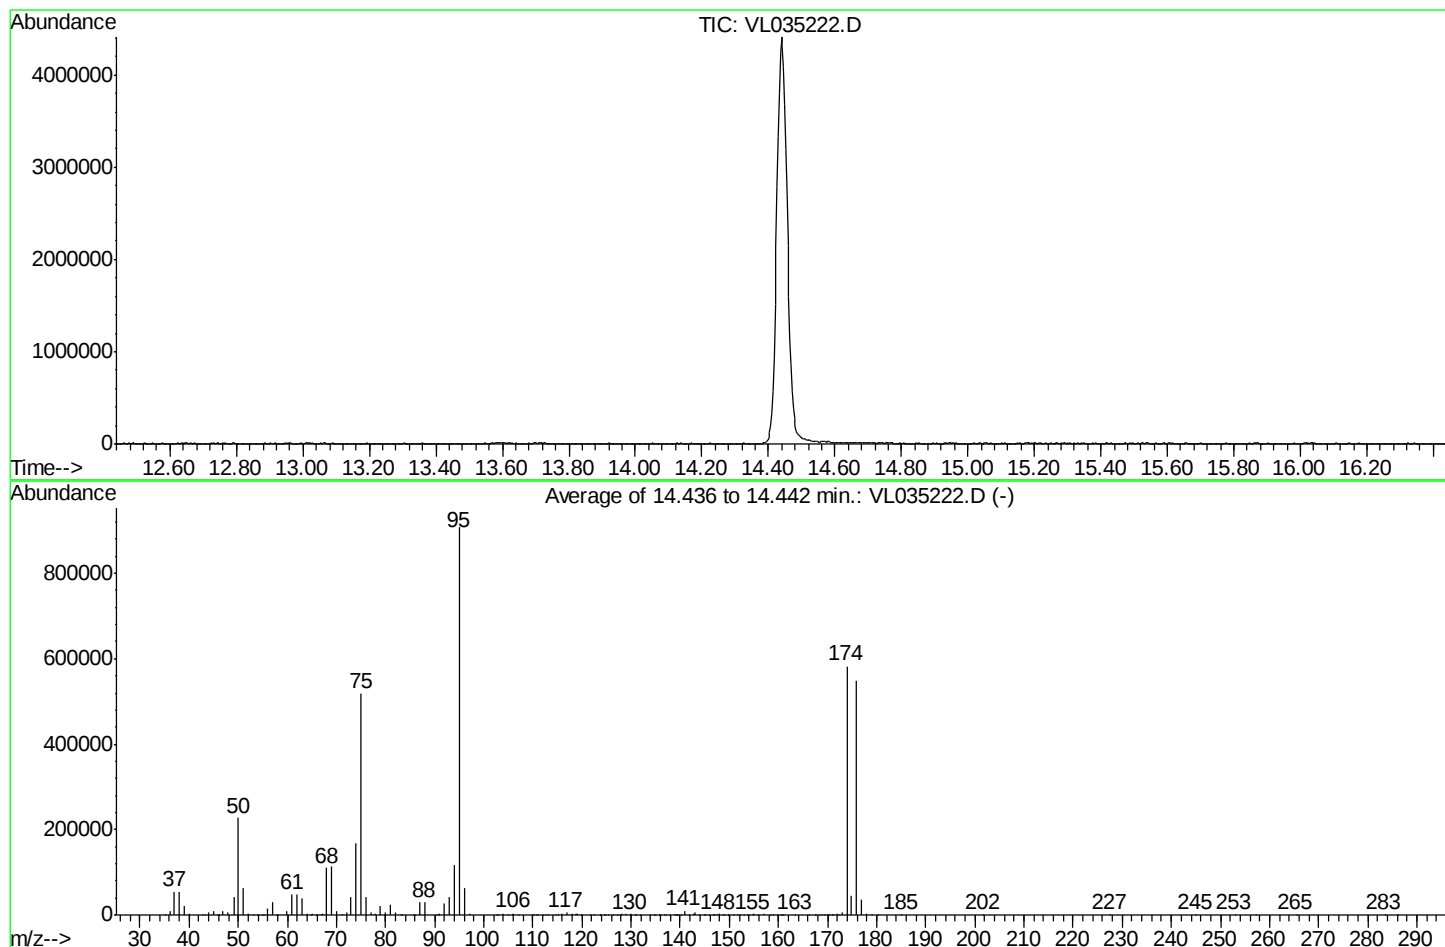

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	226538	PASS
75	95	30	66	57.1	517888	PASS
95	95	100	100	100.0	907669	PASS
96	95	5	9	6.8	62168	PASS
173	174	0.00	2	1.1	6346	PASS
174	95	50	120	64.2	582613	PASS
175	174	4	9	7.8	45613	PASS
176	174	93	101	94.4	549698	PASS
177	176	5	9	6.8	37250	PASS