

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072325\
 Data File : VL042754.D
 Acq On : 23 Jul 2025 13:00
 Operator : SY/MD
 Sample : VSTDICC0.1
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.1

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 07/24/2025
 Supervised By : Mahesh Dadoda 07/24/2025

Quant Time: Jul 24 05:01:17 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072325AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Jul 24 04:55:41 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	152358	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.953	114	438604	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.879	117	393042	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.374	95	298283	9.583	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.800%
Target Compounds						
					Qvalue	
5) Vinyl Chloride	1.583	62	837	0.104	ppbv #	60
32) 1,1,1-Trichloroethane	3.363	97	3550	0.108	ppbv	96
35) Carbon Tetrachloride	3.758	117	3035m	0.093	ppbv	
38) Trichloroethene	4.555	130	2207m	0.110	ppbv	
52) Tetrachloroethene	8.222	164	1852m	0.107	ppbv	
54) 1,2-Dibromoethane	7.665	107	2184m	0.094	ppbv	
63) 1,1,2,2-Tetrachloroethane	9.963	83	3084m	0.095	ppbv	
79) Naphthalene	13.514	128	2509	0.475	ppbv #	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072325\
Data File : VL042754.D
Acq On : 23 Jul 2025 13:00
Operator : SY/MD
Sample : VSTDICC0.1
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/24/2025
Supervised By :Mahesh Dadoda 07/24/2025


Quant Time: Jul 24 05:01:17 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072325AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Thu Jul 24 04:55:41 2025
Response via : Initial Calibration

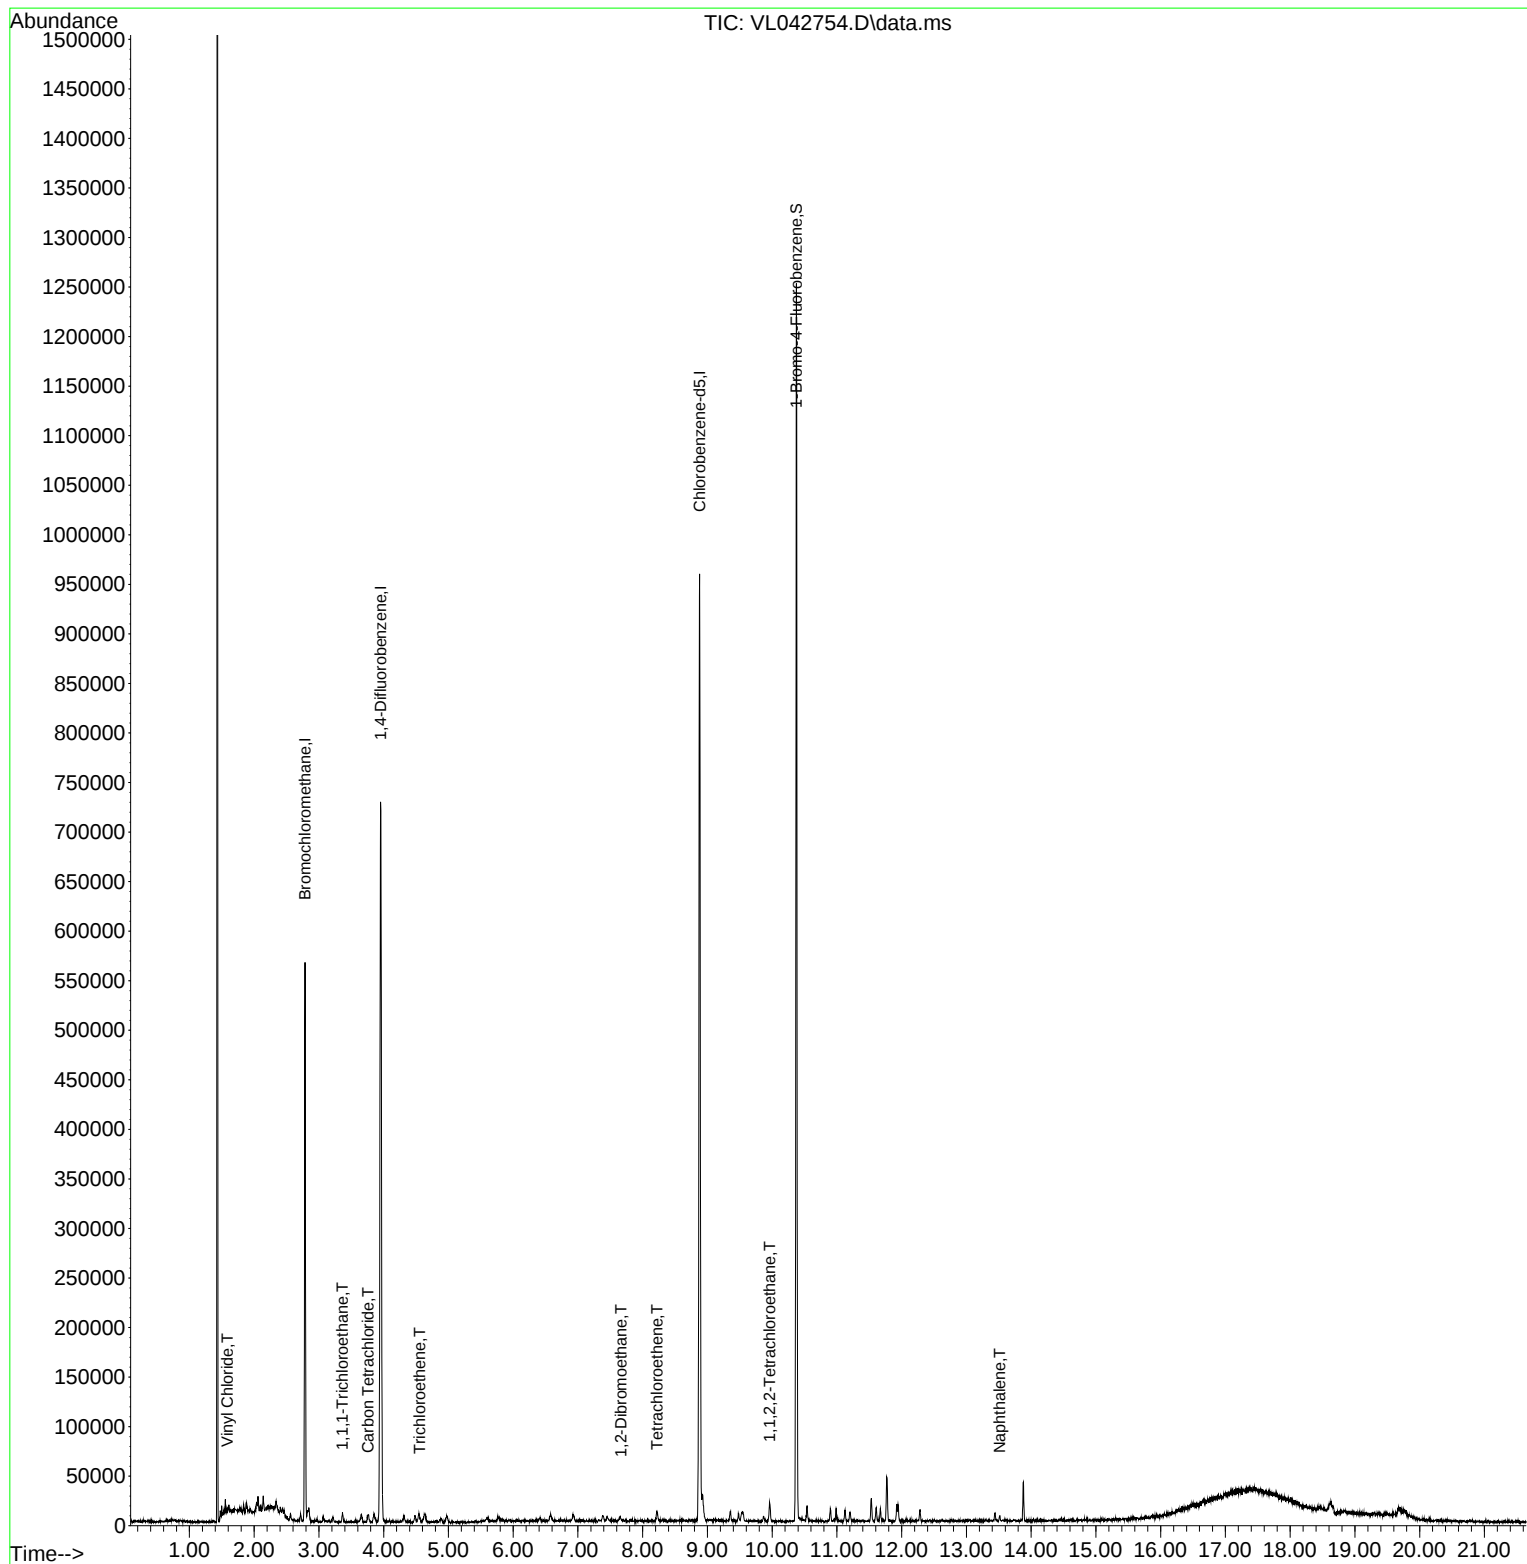

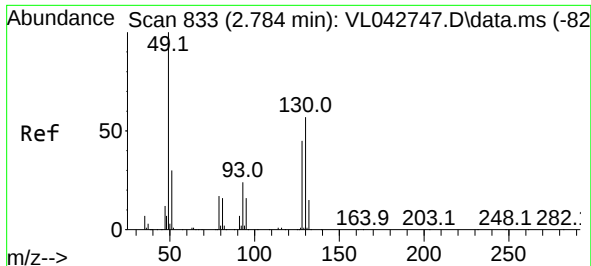

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.784 min Scan# 833
Delta R.T. 0.000 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00




Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.1

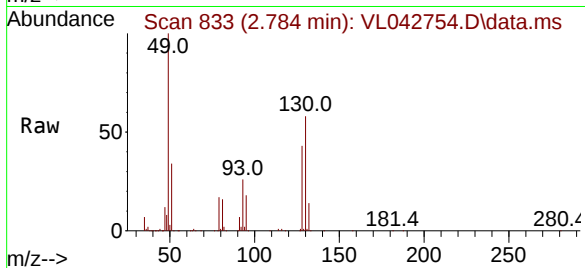

Tgt Ion: 49 Resp: 152358
Ion Ratio Lower Upper
49 100
128 46.3 23.6 71.0
130 60.6 30.3 90.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/24/2025
Supervised By :Mahesh Dadoda 07/24/2025

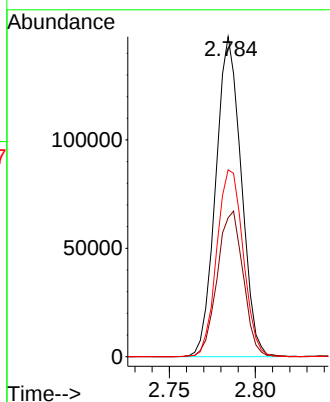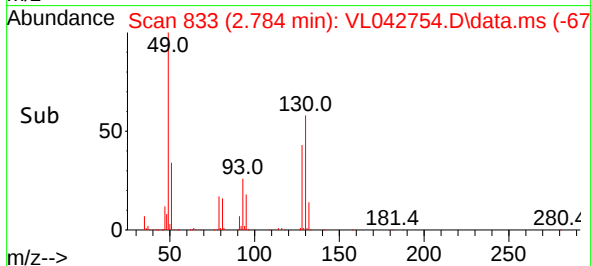

#5
Vinyl Chloride
Concen: 0.104 ppbv
RT: 1.583 min Scan# 462
Delta R.T. 0.004 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00


Tgt Ion: 62 Resp: 837
Ion Ratio Lower Upper
62 100
64 8.9 24.5 36.7#

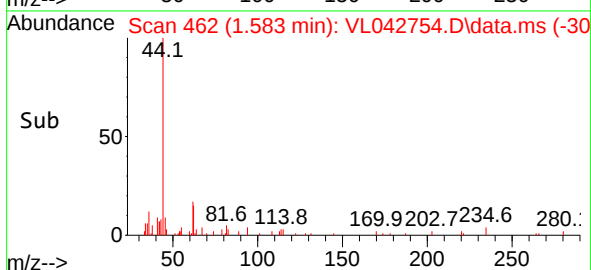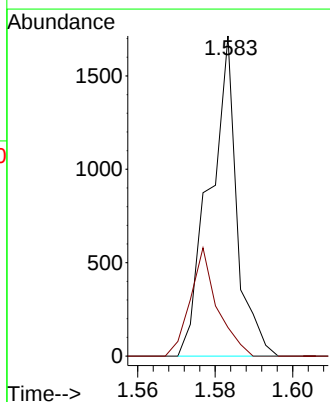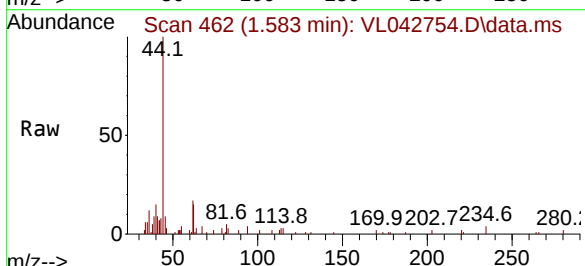

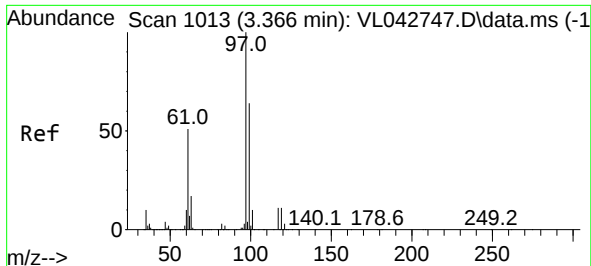

#32
 1,1,1-Trichloroethane
 Concen: 0.108 ppbv
 RT: 3.363 min Scan# 1012
 Delta R.T. -0.003 min
 Lab File: VL042754.D
 Acq: 23 Jul 2025 13:00




Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDIC0.1



Tgt Ion: 97 Resp: 3550
 Ion Ratio Lower Upper
 97 100
 99 59.4 51.0 76.6
 61 50.4 40.9 61.3




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 07/24/2025
 Supervised By :Mahesh Dadoda 07/24/2025

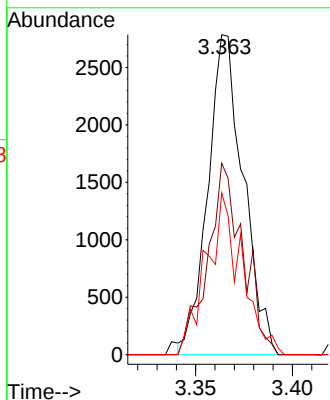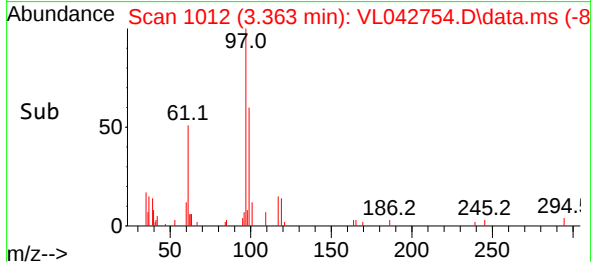

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 3.953 min Scan# 1194
 Delta R.T. -0.003 min
 Lab File: VL042754.D
 Acq: 23 Jul 2025 13:00


Tgt Ion:114 Resp: 438604
 Ion Ratio Lower Upper
 114 100
 63 25.8 20.5 30.7
 88 17.8 14.0 21.0

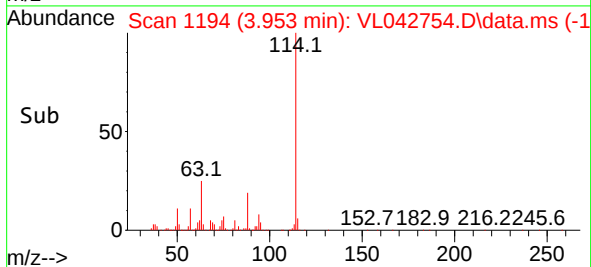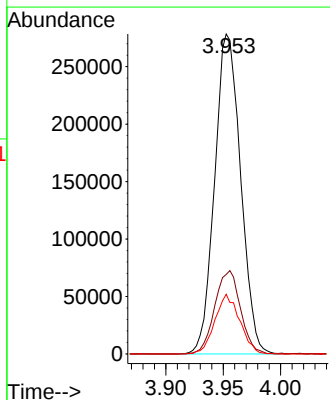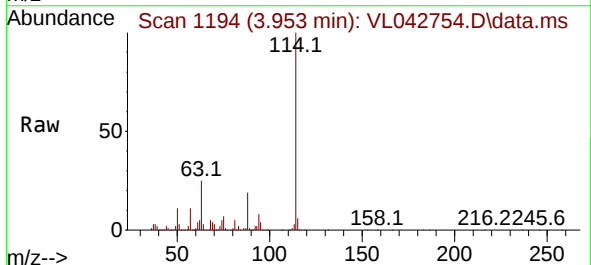



#35
Carbon Tetrachloride
Concen: 0.093 ppbv m
RT: 3.758 min Scan# 1134
Delta R.T. 0.000 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00




Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.1



Tgt Ion:117 Resp: 3038
Ion Ratio Lower Upper
117 100
119 56.3 77.1 115.7#
121 38.3 25.5 38.3#




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/24/2025
Supervised By :Mahesh Dadoda 07/24/2025

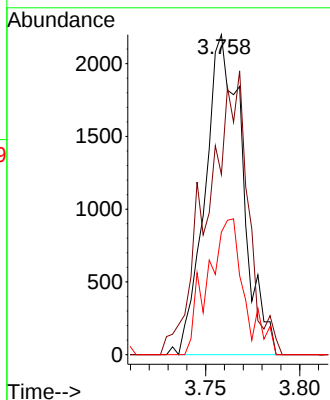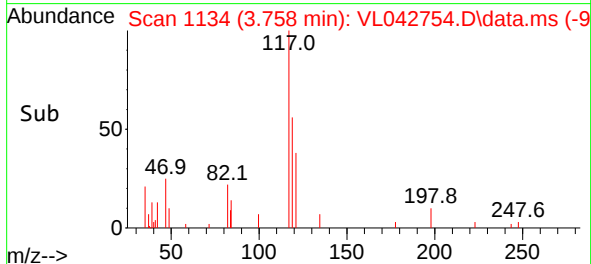

#38
Trichloroethene
Concen: 0.110 ppbv m
RT: 4.555 min Scan# 1380
Delta R.T. 0.010 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00


Tgt Ion:130 Resp: 2207
Ion Ratio Lower Upper
130 100
95 56.4 85.4 128.2#
132 49.9 78.2 117.2#
97 43.1 54.8 82.2#

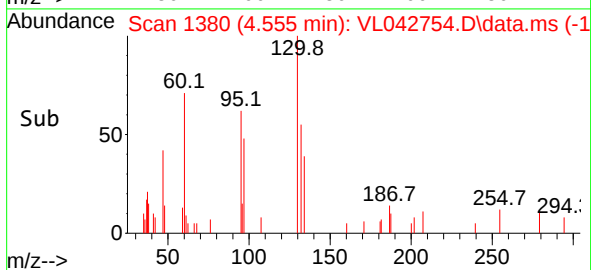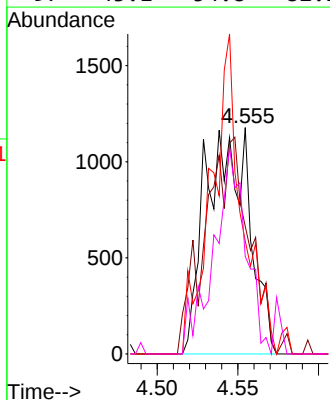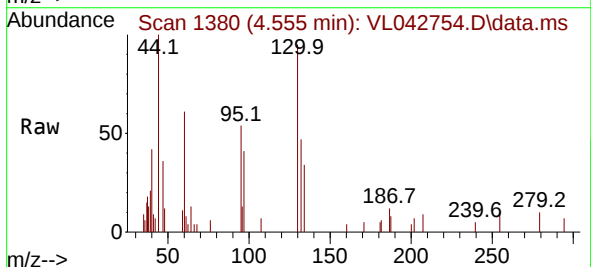

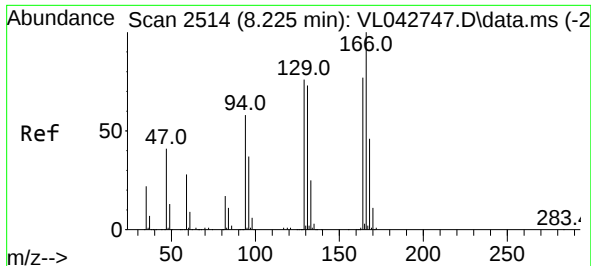

#52
Tetrachloroethene
Concen: 0.107 ppbv m
RT: 8.222 min Scan# 2185
Delta R.T. -0.003 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00




Instrument :
MSVOA_L
ClientSampleId :
VSTDIC0.1



Tgt Ion:164 Resp: 185
Ion Ratio Lower Upper
164 100
166 84.0 104.0 156.0
129 64.3 79.2 118.8
131 52.7 76.2 114.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/24/2025
Supervised By :Mahesh Dadoda 07/24/2025

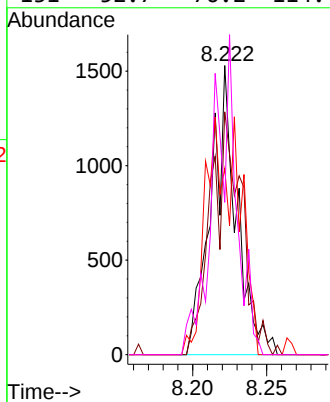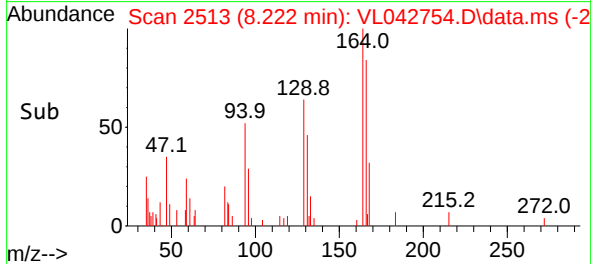

#54
1,2-Dibromoethane
Concen: 0.094 ppbv m
RT: 7.665 min Scan# 2341
Delta R.T. 0.016 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00

Tgt Ion:107 Resp: 2184
Ion Ratio Lower Upper
107 100
109 85.2 72.7 109.1

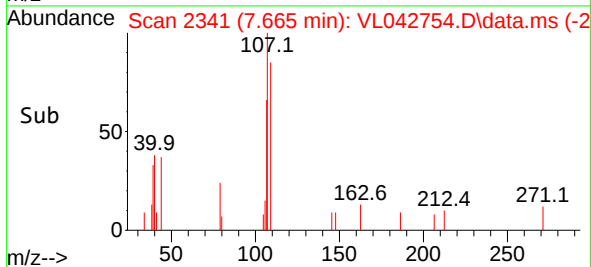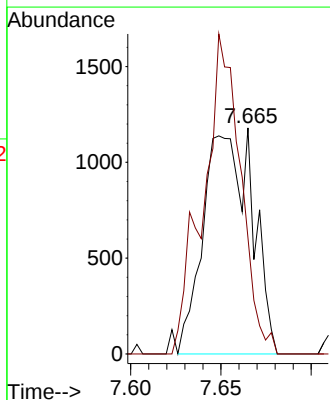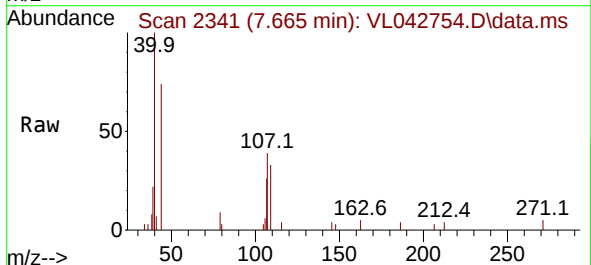







#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.879 min Scan# 2716
Delta R.T. 0.000 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00

Instrument :
MSVOA_1
ClientSampleId :
VSTDIC0.1

Tgt Ion: 117 Resp: 39304
Ion Ratio Lower Upper
117 100
82 63.6 53.3 79.9
119 31.7 25.8 38.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/24/2025
Supervised By :Mahesh Dadoda 07/24/2025

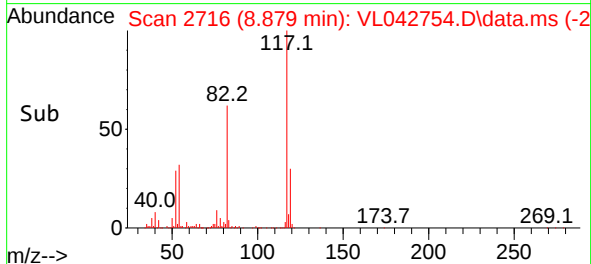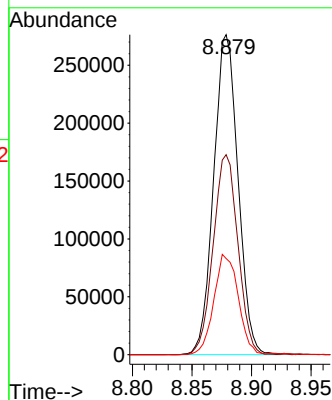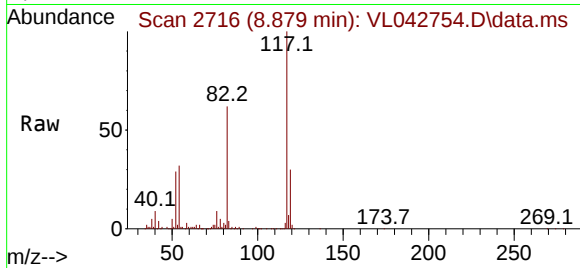

#63
1,1,2,2-Tetrachloroethane
Concen: 0.095 ppbv m
RT: 9.963 min Scan# 3051
Delta R.T. 0.000 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00


Tgt Ion: 83 Resp: 3084
Ion Ratio Lower Upper
83 100
131 10.9 5.0 15.0
85 70.7 32.6 97.7

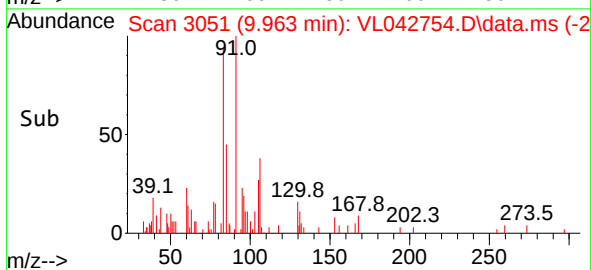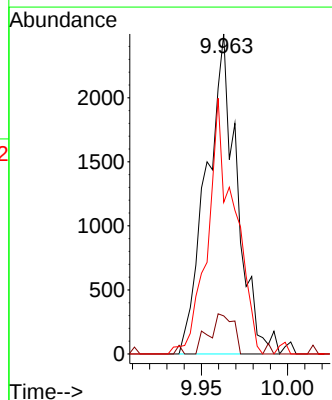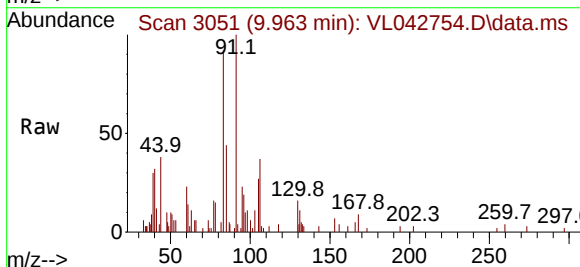

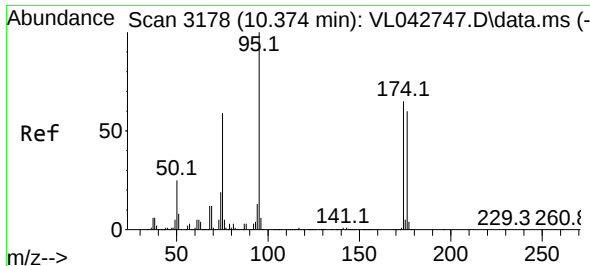

#68
1-Bromo-4-Fluorobenzene
Concen: 9.583 ppbv
RT: 10.374 min Scan# 3178
Delta R.T. 0.000 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00




Instrument :
MSVOA_L
ClientSampleId :
VSTDIC0.1

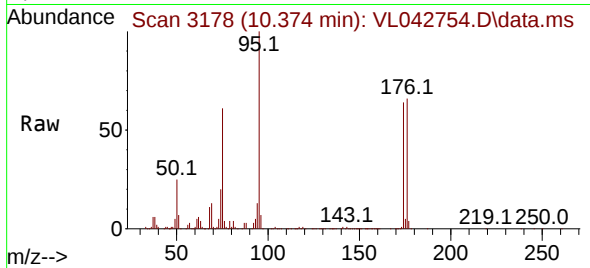


Tgt Ion: 95 Resp: 29828
Ion Ratio Lower Upper
95 100
174 65.8 53.8 80.6
175 5.0 4.0 6.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/24/2025
Supervised By :Mahesh Dadoda 07/24/2025

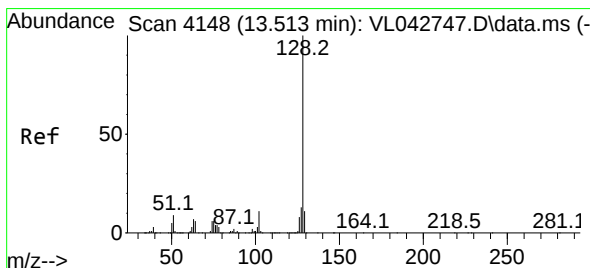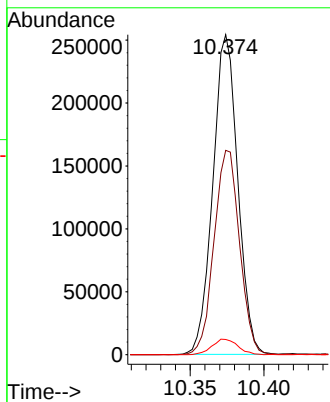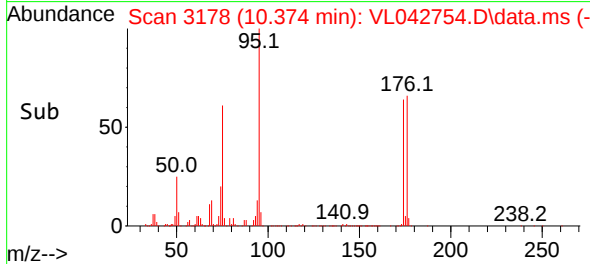

#79
Naphthalene
Concen: 0.475 ppbv
RT: 13.514 min Scan# 4148
Delta R.T. 0.000 min
Lab File: VL042754.D
Acq: 23 Jul 2025 13:00

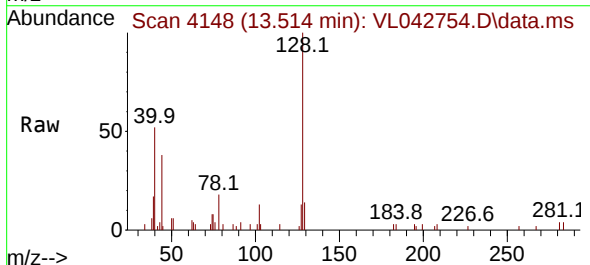

Tgt Ion:128 Resp: 2509
Ion Ratio Lower Upper
128 100
127 12.9 10.5 15.7
129 13.7 8.6 13.0#

