


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072522\
Data File : VL039518.D
Acq On : 25 Jul 2022 11:32
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jul 06 02:15:38 2022
Last Update : Wed Jul 06 02:15:38 2022

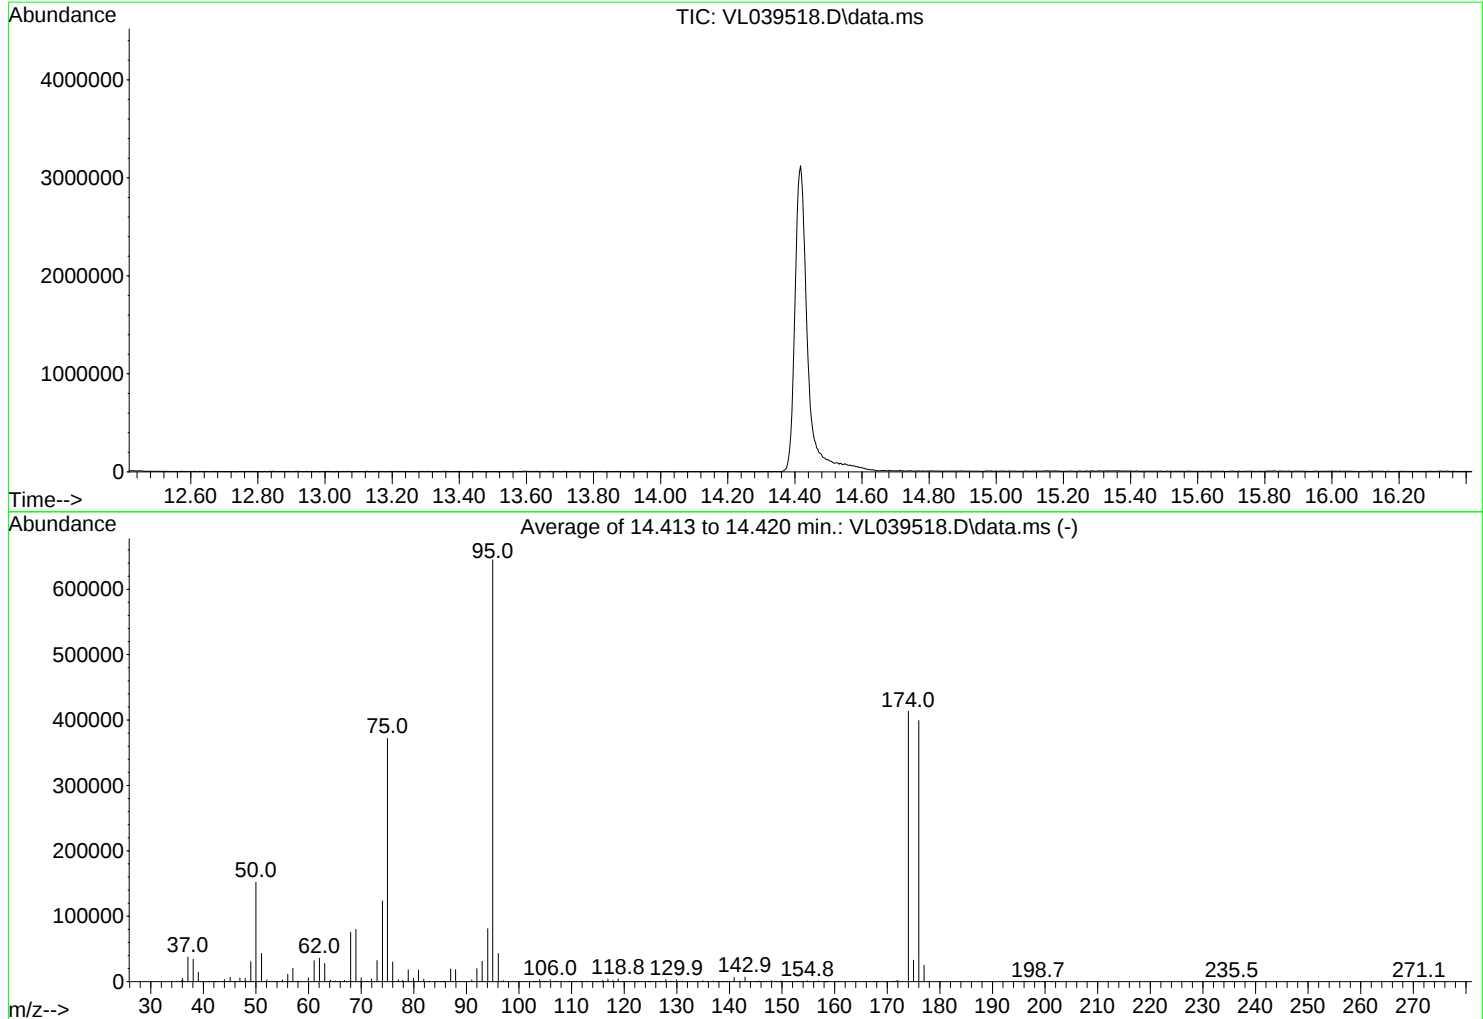

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	152000	PASS
75	95	30	66	57.7	371968	PASS
95	95	100	100	100.0	644949	PASS
96	95	5	9	6.7	42949	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	64.1	413163	PASS
175	174	4	9	8.0	32856	PASS
176	174	93	101	96.6	399275	PASS
177	176	5	9	6.3	25160	PASS

Average of 14.413 to 14.420 min.: VL039518.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	1974	44.00	3247	53.90	113	65.15	102
36.05	4846	45.10	6316	55.05	2377	65.85	31
37.05	37725	45.90	314	56.05	11347	66.85	193
38.05	34243	46.30	230	57.00	20632	67.20	48
39.05	14427	46.95	5547	57.95	928	68.00	75616
39.90	475	47.95	4818	59.95	5807	69.00	80061
41.00	79	49.00	30688	61.05	32189	70.00	5897
41.60	179	50.00	152000	62.05	35717	71.10	257
42.10	71	51.05	43435	63.05	27795	71.95	4201
42.70	205	52.05	2596	64.15	2446	73.00	32440
43.10	187	53.50	162	65.00	486	74.05	123424

Average of 14.413 to 14.420 min.: VL039518.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	371968	85.60	136	102.70	155	110.90	319
76.00	30216	85.90	394	103.10	80	111.80	703
77.05	2894	87.00	19400	103.90	3027	112.85	841
77.90	2032	87.95	18288	104.70	129	114.75	543
78.95	18043	91.00	2809	105.00	588	115.10	316
79.95	4900	92.00	19741	105.20	449	115.80	736
80.90	17611	93.00	31117	105.95	2696	115.95	1607
81.90	3706	94.05	81043	106.95	813	116.90	3851
82.95	747	95.00	644949	109.50	275	117.80	1524
84.05	122	96.05	42949	109.90	98	118.00	1041
85.00	138	97.00	1392	110.25	272	118.85	4103

Average of 14.413 to 14.420 min.: VL039518.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.80	203	128.90	713	139.50	129	147.00	747
120.05	162	129.10	421	139.95	461	147.95	1628
121.85	117	129.95	2767	140.90	6466	148.95	294
122.50	136	131.00	772	141.95	1004	149.55	128
122.95	377	133.90	58	142.95	7221	149.95	1185
123.90	383	134.95	1509	144.05	386	151.70	317
124.60	90	135.90	294	144.75	282	151.90	74
124.90	107	136.90	1034	145.10	130	152.95	571
125.90	275	137.70	145	145.40	310	153.60	111
126.90	112	138.60	225	145.75	906	154.05	265
127.90	3178	138.90	155	146.30	89	154.85	1558

Average of 14.413 to 14.420 min.: VL039518.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.00	125	169.95	533	201.20	73		
156.95	1235	171.00	171	233.90	68		
158.10	65	171.25	815	235.50	119		
158.40	145	171.85	1961	271.10	50		
158.80	615	172.10	656				
160.70	512	174.00	413163				
161.00	305	175.00	32856				
166.55	186	176.00	399275				
167.40	56	177.00	25160				
168.10	90	178.00	860				
169.20	249	198.70	117				