
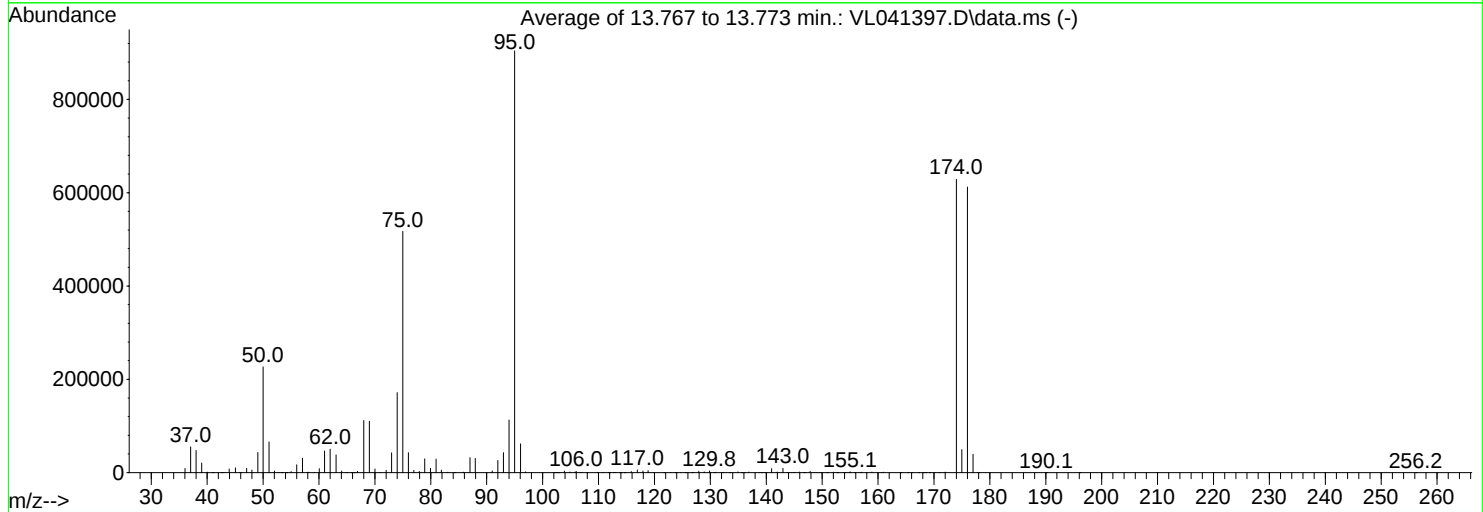


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072524\
Data File : VL041397.D
Acq On : 25 Jul 2024 12:29
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Jul 26 07:31:14 2024

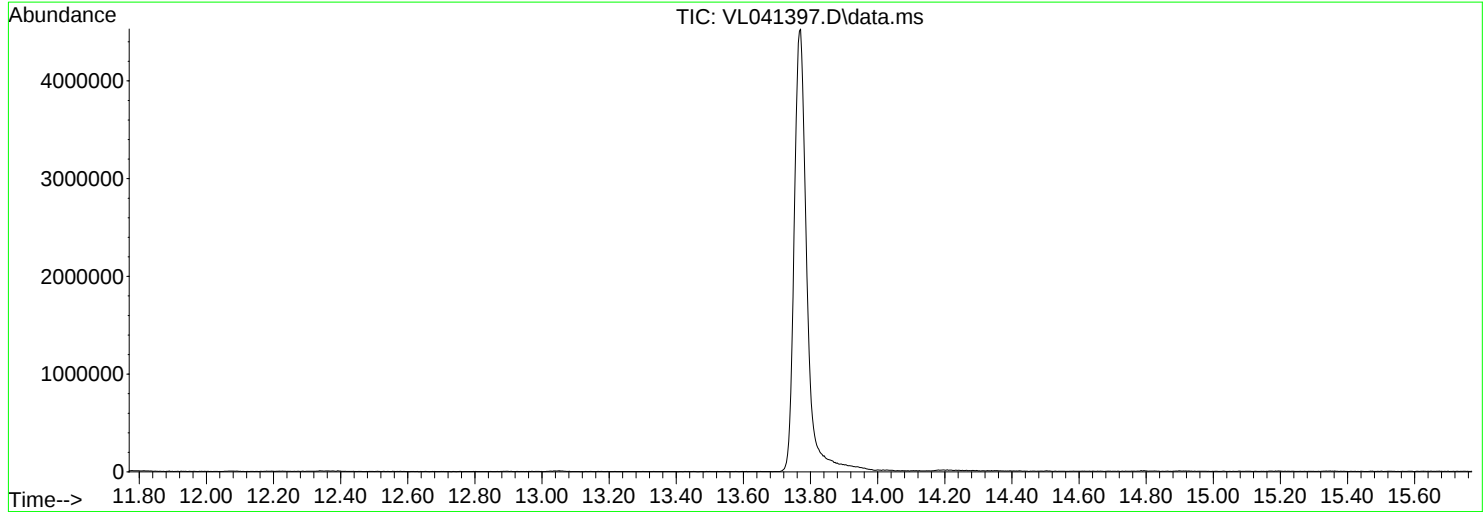

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	25.1	226560	PASS
75	95	30	66	57.2	517099	PASS
95	95	100	100	100.0	904149	PASS
96	95	5	9	6.8	61827	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.5	628715	PASS
175	174	4	9	7.9	49563	PASS
176	174	93	101	97.4	612373	PASS
177	176	5	9	6.5	39536	PASS

Average of 13.767 to 13.773 min.: VL041397.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8938	46.20	747	56.00	16676	65.05	551
37.05	55184	47.05	9213	57.05	31064	65.80	81
38.00	47675	48.00	5580	57.90	369	66.30	10
39.00	20752	49.05	43096	58.10	1087	66.90	288
40.05	1048	50.00	226560	59.15	203	68.00	111861
41.00	138	51.05	66029	60.05	8699	69.00	110240
42.60	79	52.05	3388	61.00	46269	70.00	8026
43.00	328	52.80	214	62.00	50419	71.00	223
43.95	7790	53.30	58	63.05	38069	72.00	5052
45.05	10433	54.20	58	64.05	3478	73.00	42536
45.85	541	55.00	2439	64.80	240	74.00	171456

Average of 13.767 to 13.773 min.: VL041397.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	517099	87.00	32264	102.80	91	111.80	547
76.00	42749	87.95	30379	103.10	218	112.00	141
76.95	4771	91.00	3867	103.90	3349	112.70	384
77.95	2880	92.00	26149	104.90	1227	112.90	196
78.90	29461	93.00	42979	105.80	1264	113.10	362
79.95	9176	94.00	112992	106.00	2940	113.80	59
80.95	29333	95.00	904149	106.75	574	114.05	127
81.90	5623	96.05	61827	107.05	687	114.60	138
83.05	1031	96.95	1813	107.90	66	114.95	806
84.20	64	102.10	66	109.80	728	115.85	2516
85.85	912	102.50	68	110.85	786	116.95	5823

Average of 13.767 to 13.773 min.: VL041397.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.95	3451	127.00	452	136.90	1559	144.60	239
118.85	4375	127.95	2876	138.85	234	144.85	493
119.95	282	128.90	1703	139.10	68	145.10	546
121.70	129	129.85	3746	139.60	225	145.95	1224
122.95	288	130.80	427	139.80	304	146.70	187
123.70	104	130.95	691	140.10	626	147.05	598
124.05	549	132.20	91	140.95	8524	147.85	2732
124.70	240	133.50	69	141.95	1362	148.65	388
125.50	164	134.95	1826	143.00	9411	149.05	445
126.00	241	135.60	142	143.80	496	149.60	257
126.70	122	136.00	66	144.10	250	149.85	681

Average of 13.767 to 13.773 min.: VL041397.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
150.90	76	157.90	234	170.15	220	190.10	76
152.05	986	158.90	1386	170.90	340	196.10	56
152.70	159	160.60	208	171.20	248	256.20	100
152.95	643	161.00	1037	171.80	759		
153.80	503	164.10	70	172.05	974		
154.10	102	165.30	83	174.00	628715		
154.90	627	166.00	133	175.00	49563		
155.05	1691	167.30	75	176.00	612373		
155.85	163	168.10	83	177.00	39536		
156.80	419	168.55	131	177.85	738		
157.10	1211	169.20	88	178.10	340		