


Data Path : W:\HPCHEM1\MSVOA_L\Data\VL072715\
Data File : VL025748.D
Acq On : 27 Jul 2015 10:32
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL070715AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jul 08 02:22:55 2015
Last Update : Wed Jul 08 02:22:55 2015

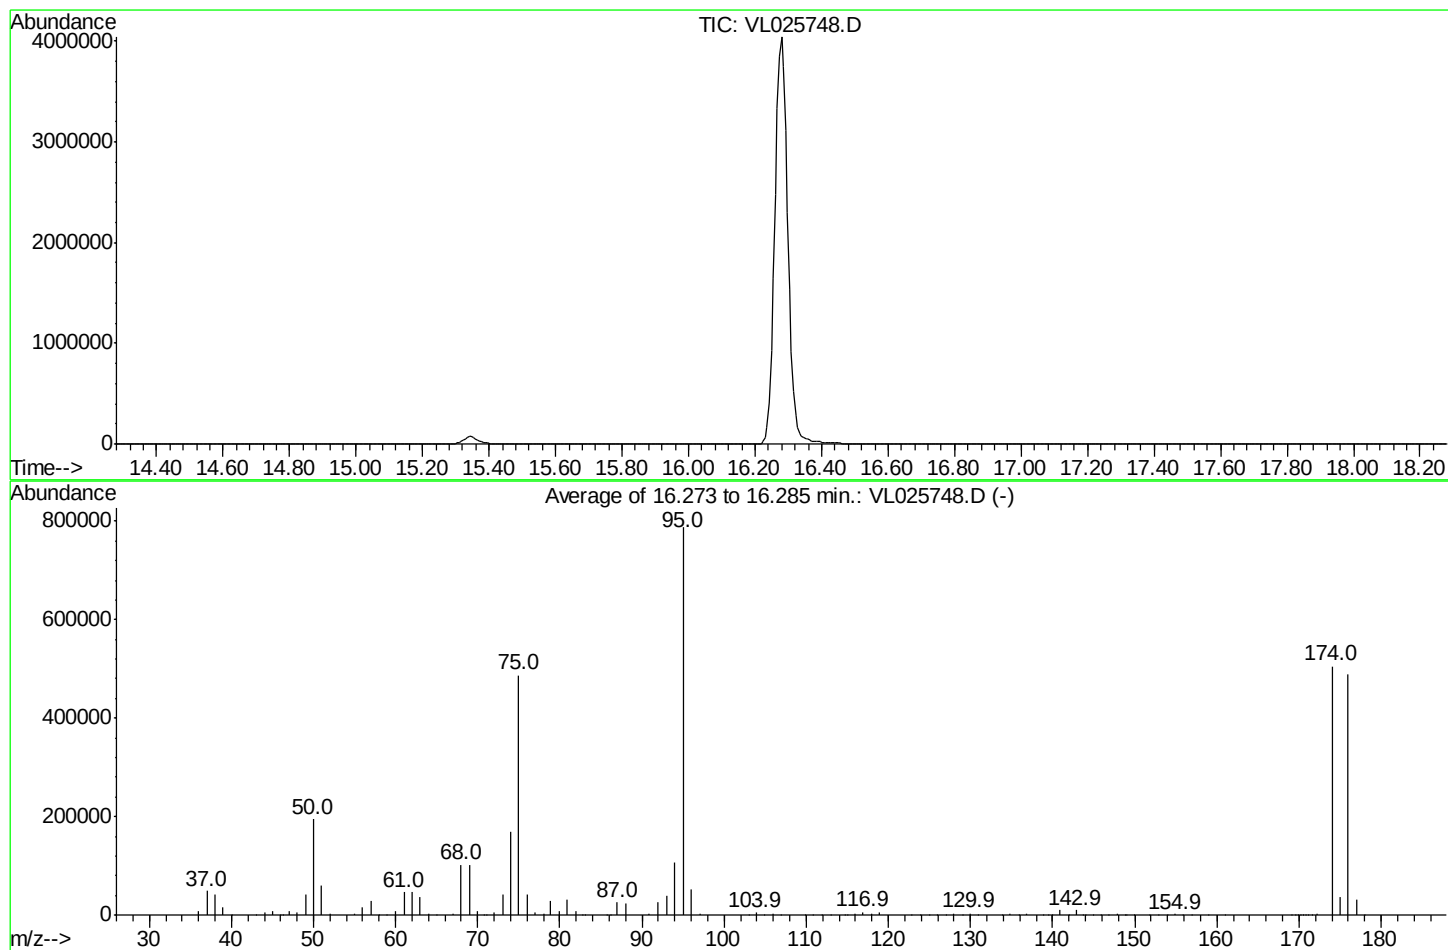

AutoFind: Scans 2163, 2164, 2165; Background Corrected with Scan 2148

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	194922	PASS
75	95	30	66	61.8	486954	PASS
95	95	100	100	100.0	787562	PASS
96	95	5	9	6.6	51850	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	64.2	505344	PASS
175	174	4	9	7.4	37344	PASS
176	174	93	101	96.6	487936	PASS
177	176	5	9	6.2	30352	PASS