


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL072718\
 Data File : VL032308.D
 Acq On : 26 Jul 2018 23:16
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL072718AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jul 27 07:05:37 2018
 Last Update : Fri Jul 27 07:05:37 2018

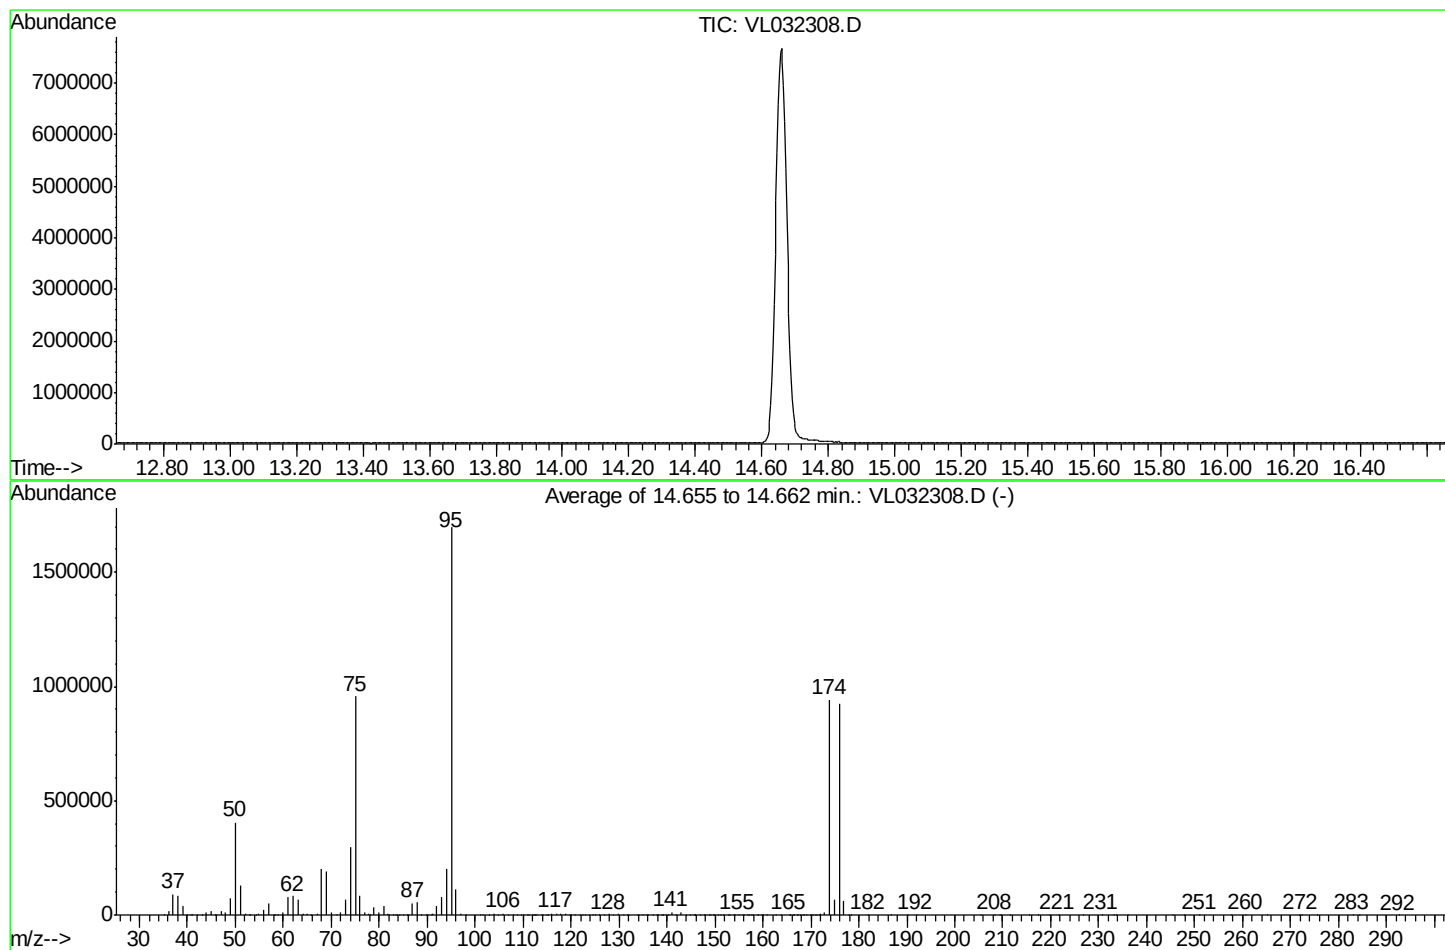

AutoFind: Scans 4220, 4221, 4222; Background Corrected with Scan 4191

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	405632	PASS
75	95	30	66	56.4	956928	PASS
95	95	100	100	100.0	1696597	PASS
96	95	5	9	6.7	113592	PASS
173	174	0.00	2	0.9	8876	PASS
174	95	50	120	55.6	943765	PASS
175	174	4	9	7.4	69962	PASS
176	174	93	101	97.7	921898	PASS
177	176	5	9	6.6	60434	PASS