


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL072920\
 Data File : VL035232.D
 Acq On : 29 Jul 2020 1:27
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL072920AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jul 29 07:14:29 2020
 Last Update : Wed Jul 29 07:14:29 2020

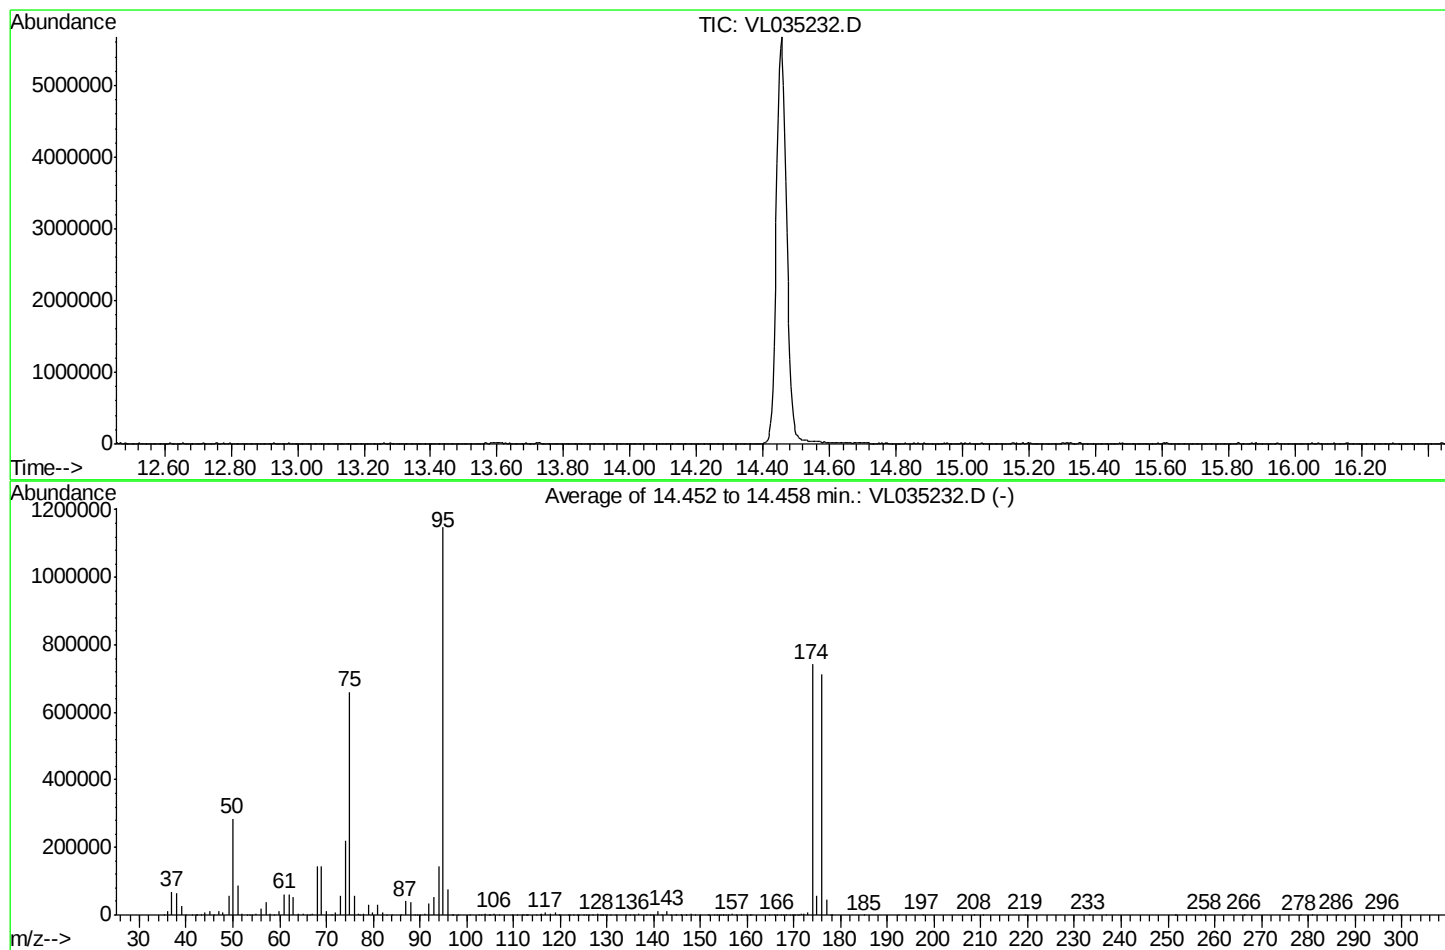

AutoFind: Scans 3628, 3629, 3630; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	285909	PASS
75	95	30	66	57.5	660053	PASS
95	95	100	100	100.0	1147904	PASS
96	95	5	9	6.7	76520	PASS
173	174	0.00	2	0.9	6999	PASS
174	95	50	120	64.6	741973	PASS
175	174	4	9	7.7	57069	PASS
176	174	93	101	96.1	712981	PASS
177	176	5	9	6.4	45626	PASS