

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072924\
 Data File : VL041440.D
 Acq On : 29 Jul 2024 22:28
 Operator : SY/MD
 Sample : P3342-05DL 10X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-03

Quant Time: Jul 30 02:55:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Jul 30 02:42:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	5.192	49	1063656	10.000	ppbv	0.01
33) 1,4-Difluorobenzene	6.652	114	2876090	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.465	117	2629445	10.000	ppbv	# 0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.773	95	2029848	10.031	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	= 100.300%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.729	85	64093	0.350	ppbv	100
3) Chlorodifluoromethane	2.655	51	93082	0.735	ppbv #	73
4) Chloromethane	2.813	50	52126	0.774	ppbv	94
9) Propene	2.874	41	344167	5.917	ppbv	93
10) Heptane	7.584	43	66025	0.505	ppbv	95
11) Trichlorofluoromethane	3.565	101	37781	0.232	ppbv	90
12) 1,1,2-Trichlorotrifluo...	4.070	101	4692	0.040	ppbv #	47
13) Ethanol	3.237	45	531648	102.261	ppbv	92
15) Acetone	3.465	43	2841708	23.514	ppbv	94
16) 1,3-Butadiene	2.970	39	11844	0.183	ppbv #	10
19) Isopropyl Alcohol	3.581	45	247059	3.497	ppbv #	93
20) Methylene Chloride	3.931	84	49108	1.090	ppbv	93
21) Allyl Chloride	3.957	41	7709	0.097	ppbv #	1
23) Vinyl Acetate	4.610	43	142846	1.548	ppbv #	18
25) Ethyl Acetate	5.211	43	233732	0.974	ppbv #	91
26) Hexane	5.214	57	200061	2.009	ppbv #	55
27) Carbon Disulfide	4.121	76	8377	0.072	ppbv #	41
29) Chloroform	5.279	83	20209	0.124	ppbv	96
30) Cyclohexane	6.603	84	7702	0.095	ppbv #	1
34) 2-Butanone	4.787	43	220229	1.583	ppbv	97
36) Benzene	6.369	78	146707	0.698	ppbv	99
37) 1,2-Dichloroethane	5.809	62	55817	0.475	ppbv #	95
39) 1,2-Dichloropropane	6.652	63	704909	8.761	ppbv #	25
41) Tetrahydrofuran	5.565	42	138999	1.747	ppbv	98
44) 2,2,4-Trimethylpentane	7.330	57	99643	0.284	ppbv #	76
53) Toluene	9.221	91	914590	3.907	ppbv	100
58) Ethyl Benzene	12.085	91	50791	0.168	ppbv	95
59) m/p-Xylene	12.343	91	220628	0.843	ppbv	95
60) o-Xylene	13.056	91	80261	0.324	ppbv	98
61) Styrene	12.899	104	24438	0.219	ppbv #	50
69) p-Isopropyltoluene	16.998	119	26925	0.069	ppbv #	87
71) 2-Chlorotoluene	14.915	91	10194	0.037	ppbv #	45
74) 1,2,4-Trimethylbenzene	16.105	105	38298	0.131	ppbv #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072924\
Data File : VL041440.D
Acq On : 29 Jul 2024 22:28
Operator : SY/MD
Sample : P3342-05DL 10X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03

Quant Time: Jul 30 02:55:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Jul 30 02:42:20 2024
Response via : Initial Calibration




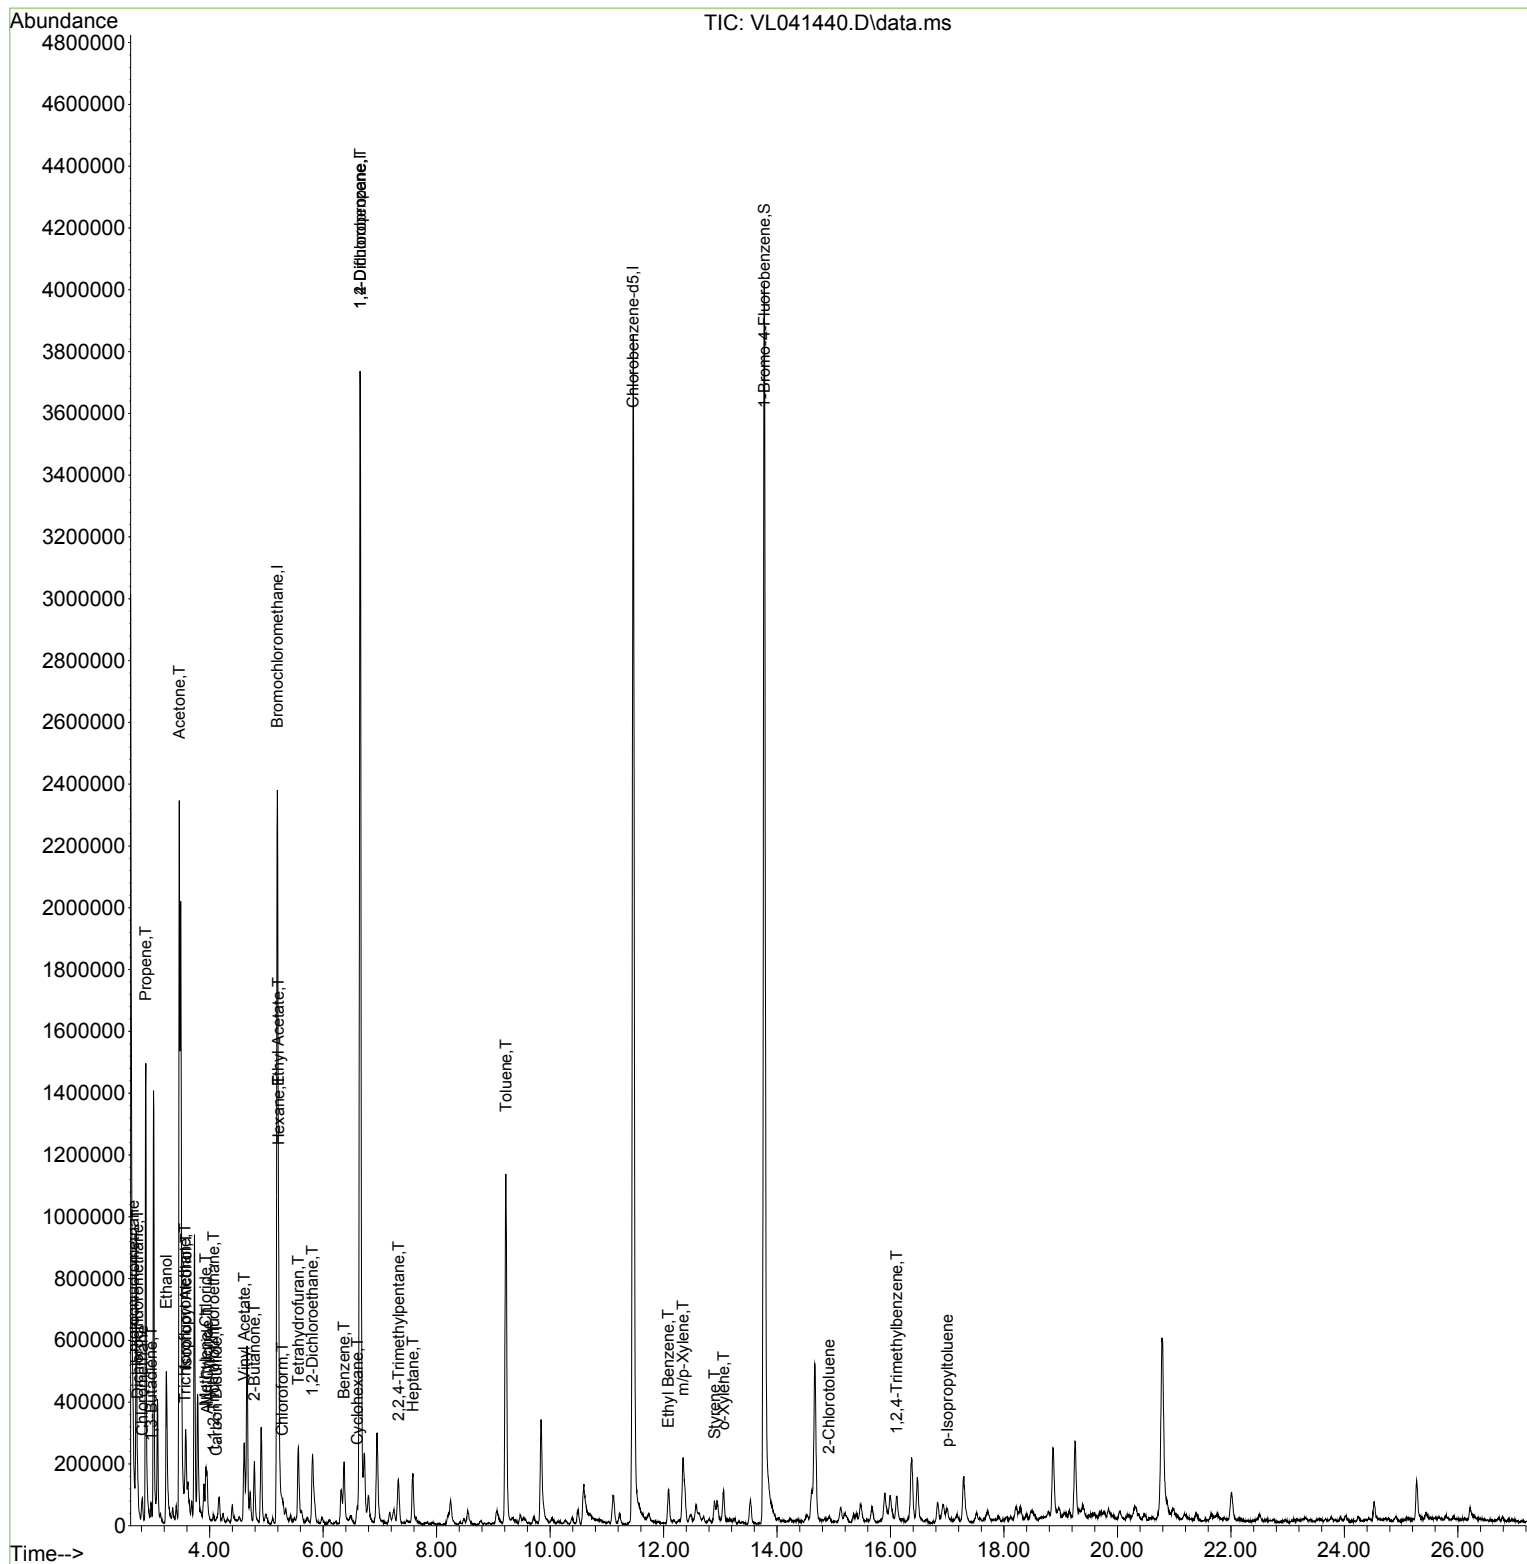




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.192 min Scan# 80
Delta R.T. 0.013 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03


Tgt Ion: 49 Resp: 1063656
Ion Ratio Lower Upper
49 100
128 46.8 23.8 71.4
130 60.2 30.8 92.4

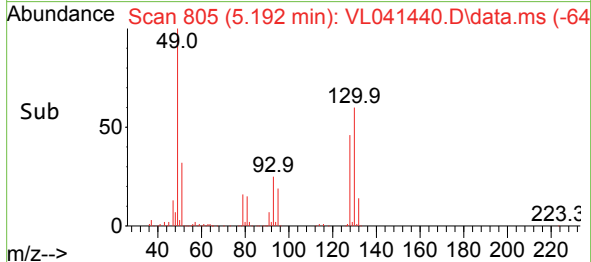

#2
Dichlorodifluoromethane
Concen: 0.350 ppbv
RT: 2.729 min Scan# 39
Delta R.T. 0.019 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Tgt Ion: 85 Resp: 64093
Ion Ratio Lower Upper
85 100
87 32.4 26.0 39.0




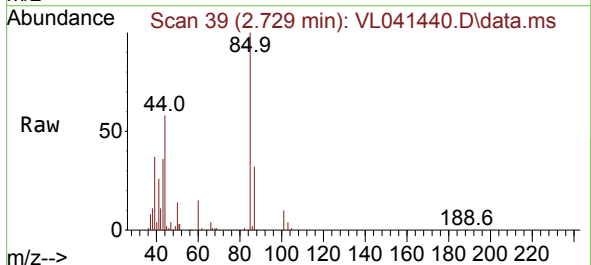


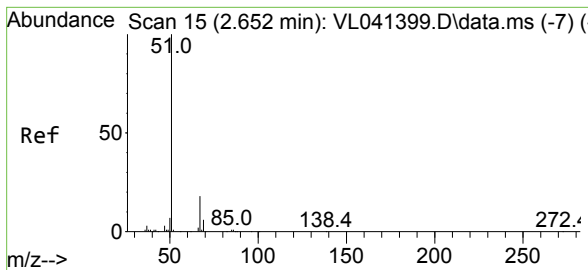

#3
Chlorodifluoromethane
Concen: 0.735 ppbv
RT: 2.655 min Scan# 1
Delta R.T. 0.000 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03


Tgt Ion: 51 Resp: 93082
Ion Ratio Lower Upper
51 100
67 6.0 14.5 21.7#

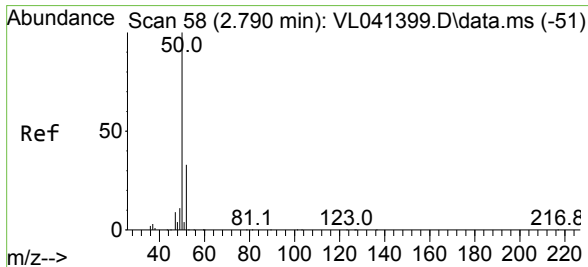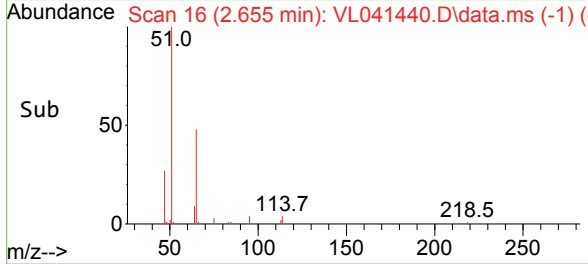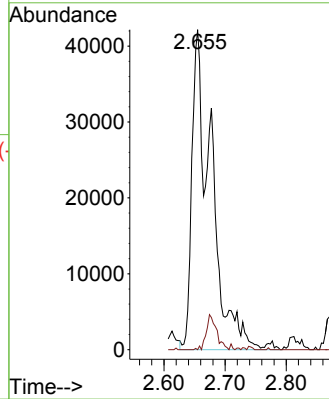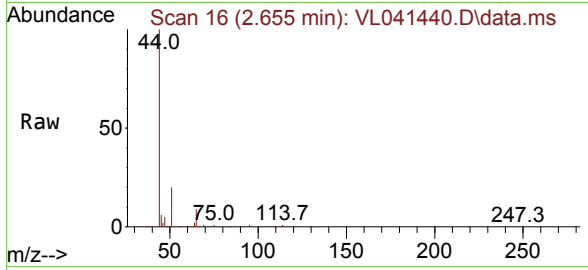

#4
Chloromethane
Concen: 0.774 ppbv
RT: 2.813 min Scan# 65
Delta R.T. 0.019 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Tgt Ion: 50 Resp: 52126
Ion Ratio Lower Upper
50 100
52 35.8 26.1 39.1


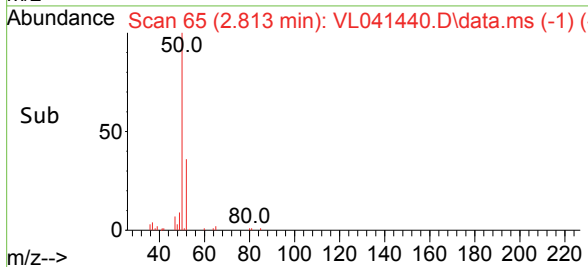
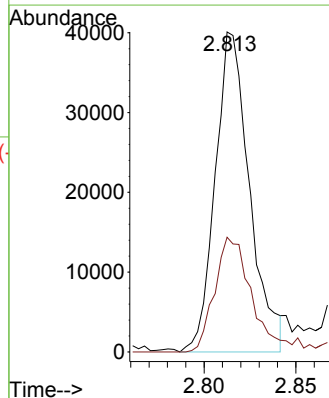
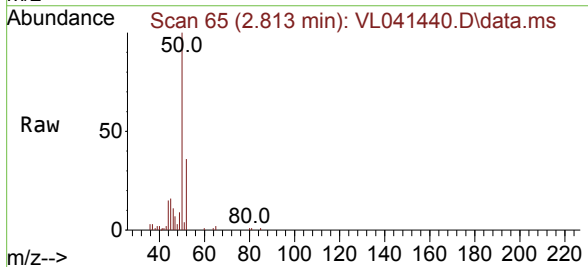


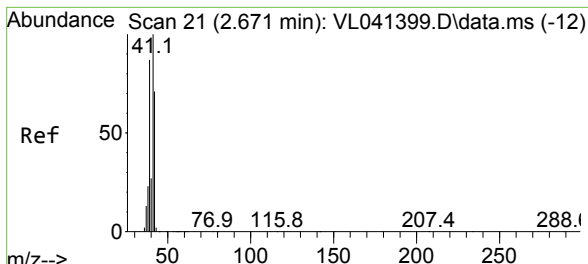

#9
 Propene
 Concen: 5.917 ppbv
 RT: 2.874 min Scan# 84
 Delta R.T. 0.203 min
 Lab File: VL041440.D
 Acq: 29 Jul 2024 22:28




Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-03


Tgt Ion: 41 Resp: 344167
 Ion Ratio Lower Upper
 41 100
 42 75.7 55.9 83.9

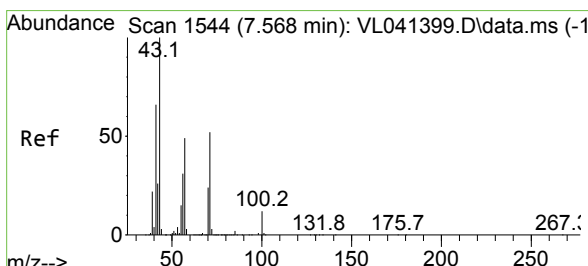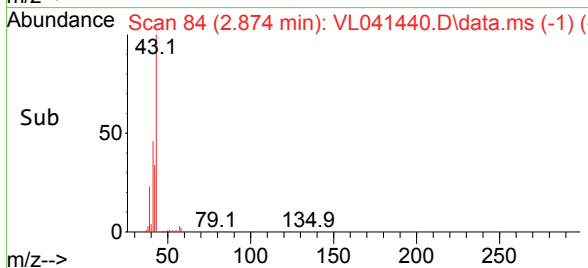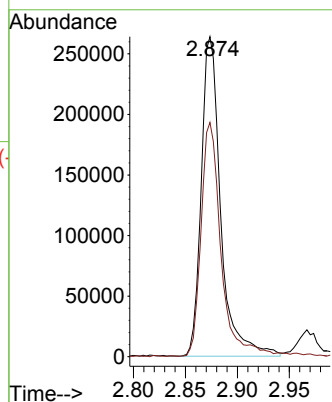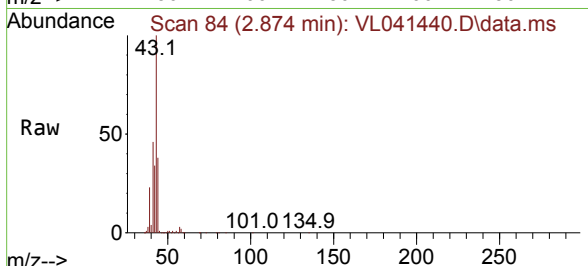

#10
 Heptane
 Concen: 0.505 ppbv
 RT: 7.584 min Scan# 1549
 Delta R.T. 0.013 min
 Lab File: VL041440.D
 Acq: 29 Jul 2024 22:28

Tgt Ion: 43 Resp: 66025
 Ion Ratio Lower Upper
 43 100
 57 54.2 40.5 60.7


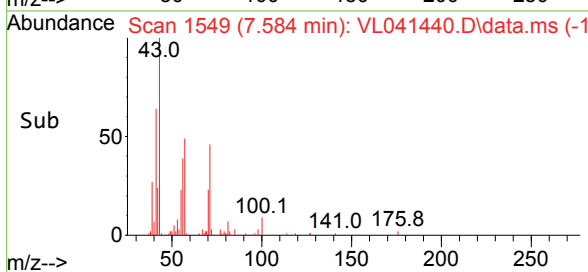
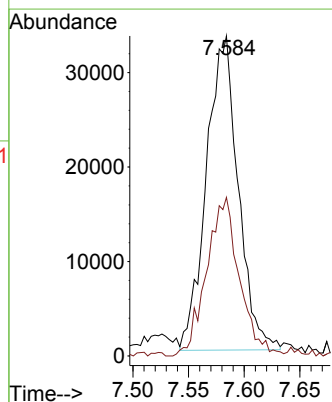
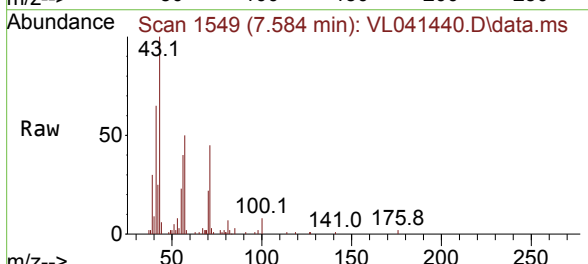




#11
 Trichlorofluoromethane
 Concen: 0.232 ppbv
 RT: 3.565 min Scan# 292
 Delta R.T. 0.019 min
 Lab File: VL041440.D
 Acq: 29 Jul 2024 22:28




Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-03


Tgt Ion:101 Resp: 37781
 Ion Ratio Lower Upper
 101 100
 103 57.6 52.6 79.0

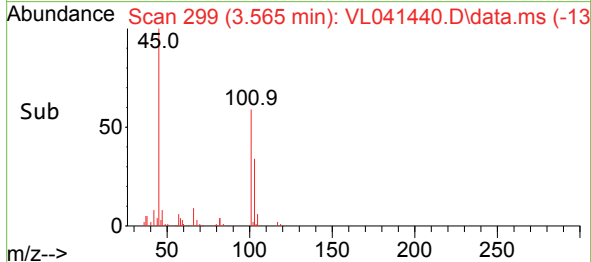

#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.040 ppbv
 RT: 4.070 min Scan# 456
 Delta R.T. 0.019 min
 Lab File: VL041440.D
 Acq: 29 Jul 2024 22:28

Tgt Ion:101 Resp: 4692
 Ion Ratio Lower Upper
 101 100
 151 119.0 59.4 89.2#


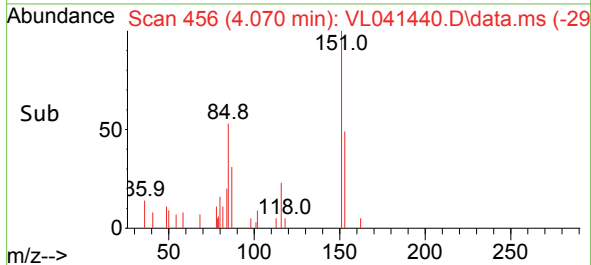






#13
Ethanol
Concen: 102.261 ppbv
RT: 3.237 min Scan# 197
Delta R.T. 0.010 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03


Tgt Ion: 45 Resp: 531648
Ion Ratio Lower Upper
45 100
46 37.7 13.4 53.4

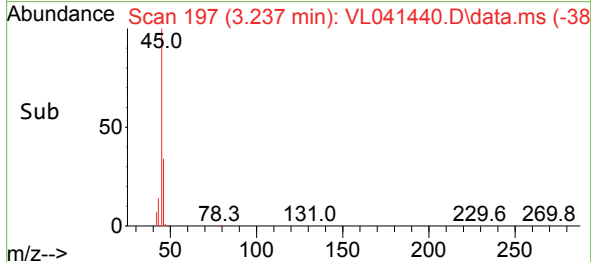

#15
Acetone
Concen: 23.514 ppbv
RT: 3.465 min Scan# 268
Delta R.T. 0.013 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Tgt Ion: 43 Resp: 2841708
Ion Ratio Lower Upper
43 100
58 23.9 21.4 32.2




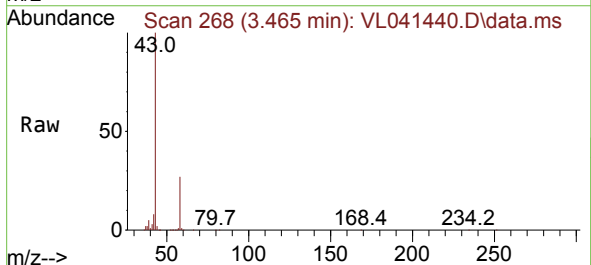




#16
1,3-Butadiene
Concen: 0.183 ppbv
RT: 2.970 min Scan# 11
Delta R.T. 0.003 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03


Tgt Ion: 39 Resp: 11844
Ion Ratio Lower Upper
39 100
54 0.0 62.5 93.7#

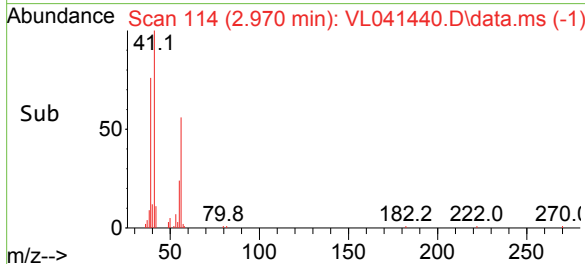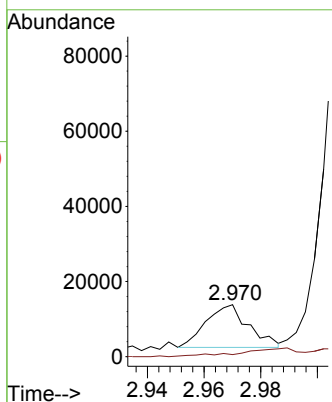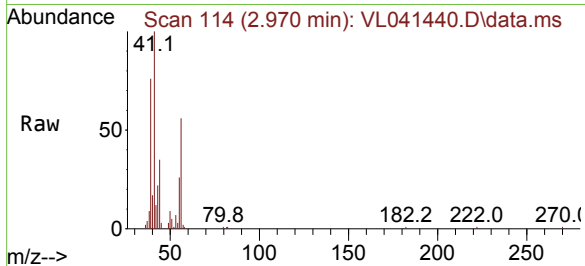

#19
Isopropyl Alcohol
Concen: 3.497 ppbv
RT: 3.581 min Scan# 304
Delta R.T. 0.019 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Tgt Ion: 45 Resp: 247059
Ion Ratio Lower Upper
45 100
58 0.0 1.9 2.9#

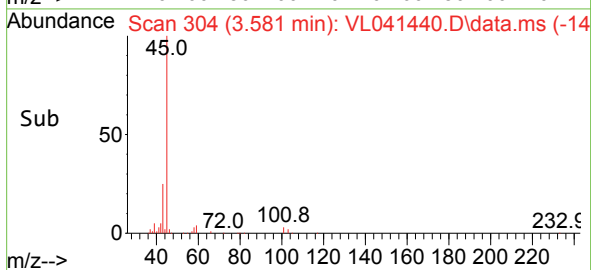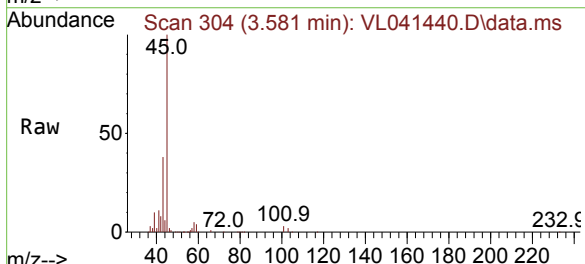







#20
Methylene Chloride
Concen: 1.090 ppbv
RT: 3.931 min Scan# 413
Delta R.T. 0.013 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03

Tgt Ion: 84 Resp: 49108




Ion	Ratio	Lower	Upper
84	100		
49	163.4	126.6	190.0
51	40.6	38.6	58.0
86	55.9	53.0	79.4

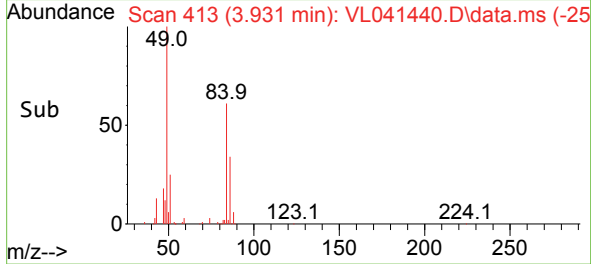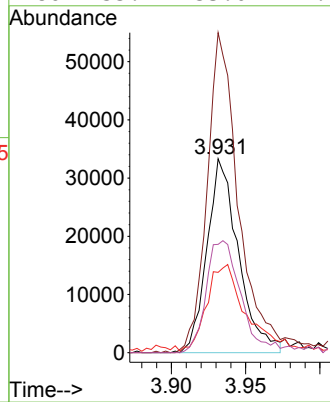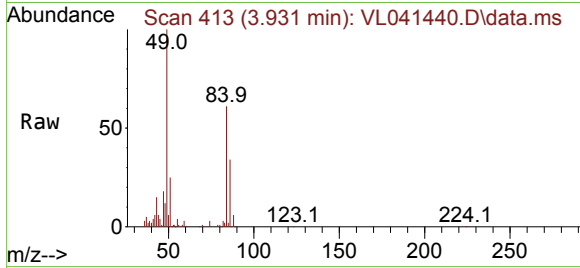


#21
Allyl Chloride
Concen: 0.097 ppbv
RT: 3.957 min Scan# 421
Delta R.T. -0.022 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Tgt Ion: 41 Resp: 7709

Ion	Ratio	Lower	Upper
41	100		
76	0.0	23.7	35.5#
39	324.4	64.3	96.5#

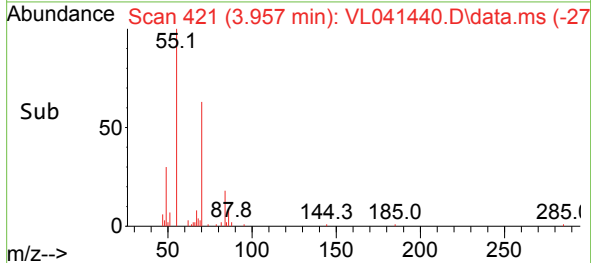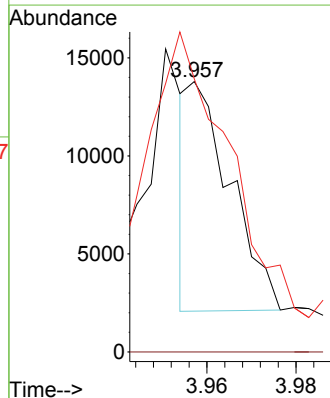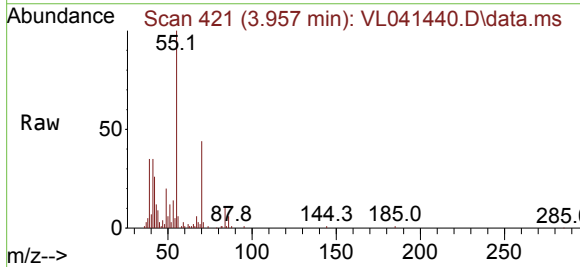







#23
 Vinyl Acetate
 Concen: 1.548 ppbv
 RT: 4.610 min Scan# 61
 Delta R.T. -0.003 min
 Lab File: VL041440.D
 Acq: 29 Jul 2024 22:28

Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-03

Tgt Ion: 43 Resp: 142846




Ion	Ratio	Lower	Upper
43	100		
86	4.6	4.6	6.8
42	70.1	7.9	11.9#
44	0.6	4.2	6.4#

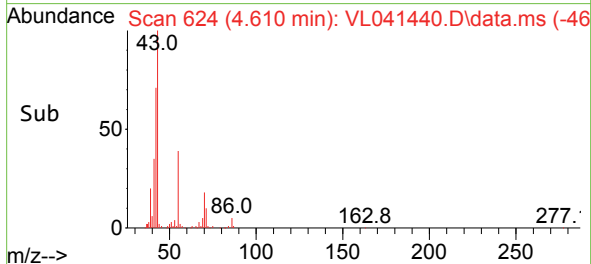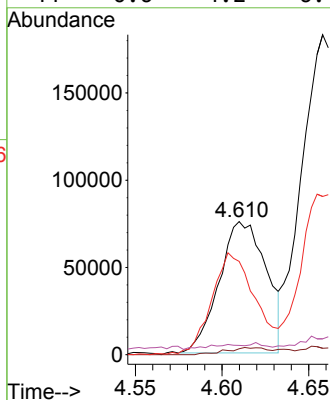


#25
 Ethyl Acetate
 Concen: 0.974 ppbv
 RT: 5.211 min Scan# 811
 Delta R.T. 0.019 min
 Lab File: VL041440.D
 Acq: 29 Jul 2024 22:28

Tgt Ion: 43 Resp: 233732

Ion	Ratio	Lower	Upper
43	100		
45	14.6	8.5	12.7#
61	6.6	8.0	12.0#
70	5.6	5.9	8.9#


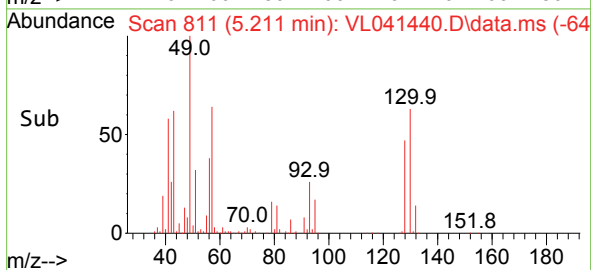
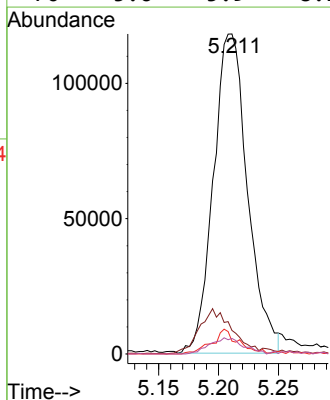





#26
Hexane
Concen: 2.009 ppbv
RT: 5.214 min Scan# 812
Delta R.T. 0.016 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03


Tgt Ion: 57 Resp: 200061
Ion Ratio Lower Upper
57 100
41 97.3 74.0 111.0
43 124.8 193.6 290.4#
56 57.2 43.1 64.7

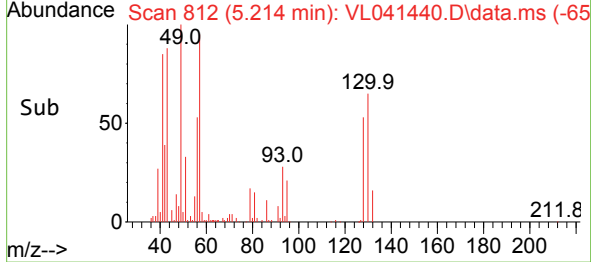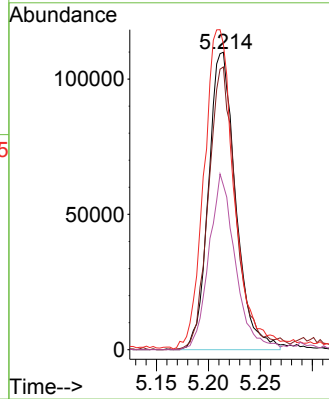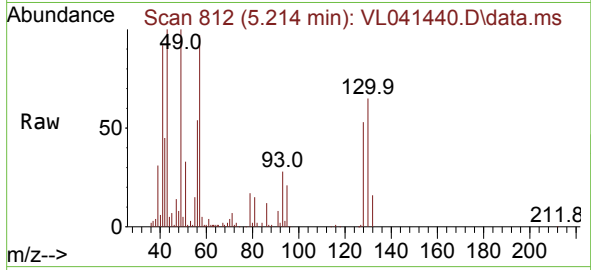

#27
Carbon Disulfide
Concen: 0.072 ppbv
RT: 4.121 min Scan# 472
Delta R.T. 0.013 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Tgt Ion: 76 Resp: 8377
Ion Ratio Lower Upper
76 100
44 53.7 15.6 23.4#
78 0.0 7.7 11.5#

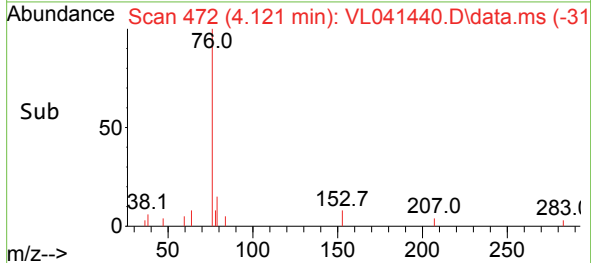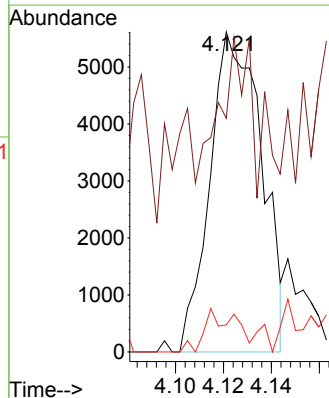



#29

Chloroform

Concen: 0.124 ppbv

RT: 5.279 min Scan# 81

Delta R.T. 0.016 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28

Instrument :

MSVOA_L

ClientSampleId :





ACVI-IA-03

Tgt Ion: 83 Resp: 20209

Ion Ratio Lower Upper

83 100

85 63.3 53.1 79.7

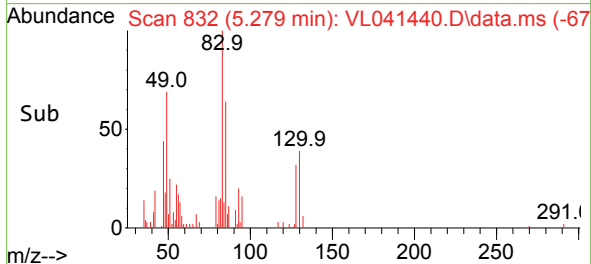

#30

Cyclohexane

Concen: 0.095 ppbv

RT: 6.603 min Scan# 1244

Delta R.T. 0.010 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28




Tgt Ion: 84 Resp: 7702


Ion Ratio Lower Upper

84 100

56 0.0 111.2 166.8#

41 220.7 70.3 105.5#

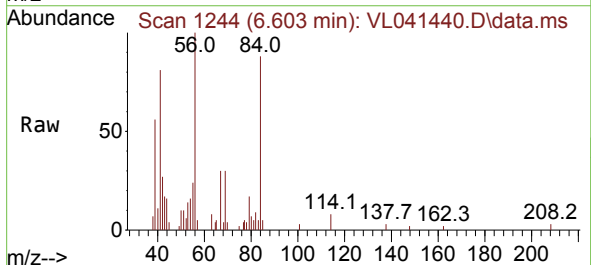



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.652 min Scan# 1

Delta R.T. 0.006 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28

Instrument :

MSVOA_L

ClientSampleId :

ACVI-IA-03





Tgt Ion:114 Resp: 2876090

Ion Ratio Lower Upper

114 100

63 25.2 20.3 30.5

88 18.0 14.3 21.5



#34

2-Butanone

Concen: 1.583 ppbv

RT: 4.787 min Scan# 679

Delta R.T. 0.013 min

Lab File: VL041440.D




Acq: 29 Jul 2024 22:28


Tgt Ion: 43 Resp: 220229

Ion Ratio Lower Upper

43 100

72 23.0 17.3 25.9


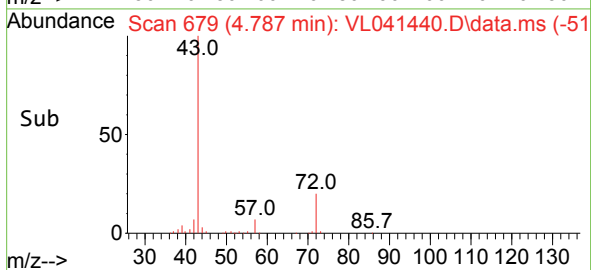






#36
Benzene
Concen: 0.698 ppbv
RT: 6.369 min Scan# 1168
Delta R.T. 0.010 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03


Tgt Ion: 78 Resp: 146707
Ion Ratio Lower Upper
78 100
77 22.2 18.1 27.1
50 18.4 15.5 23.3

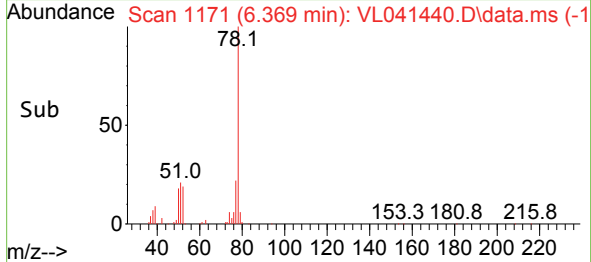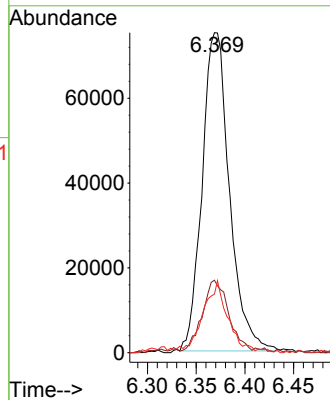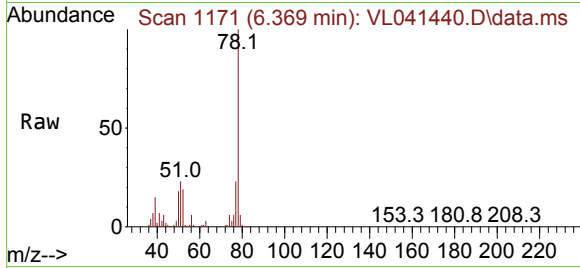

#37
1,2-Dichloroethane
Concen: 0.475 ppbv
RT: 5.809 min Scan# 997
Delta R.T. 0.013 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Tgt Ion: 62 Resp: 55817
Ion Ratio Lower Upper
62 100
98 7.8 5.0 7.4#

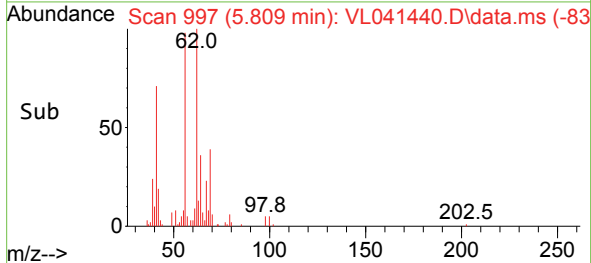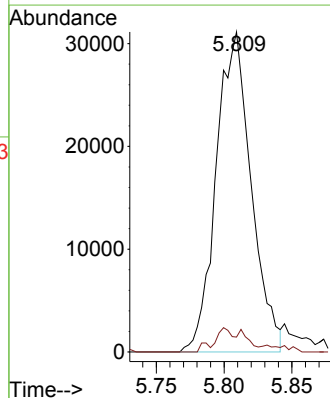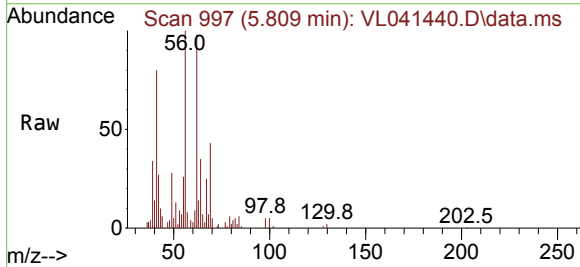



#39

1,2-Dichloropropane

Concen: 8.761 ppbv

RT: 6.652 min Scan# 11

Delta R.T. -0.412 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28

Instrument :

MSVOA_L

ClientSampleId :

ACVI-IA-03





Tgt Ion: 63 Resp: 704909

Ion Ratio Lower Upper

63 100

41 0.0 58.3 87.5#

62 18.0 53.9 80.9#

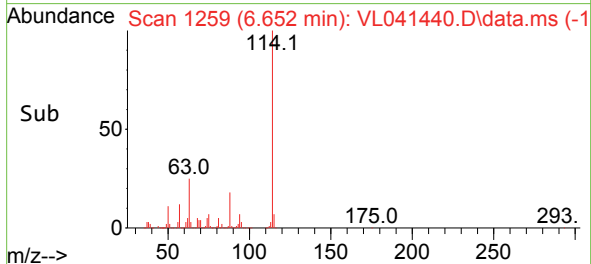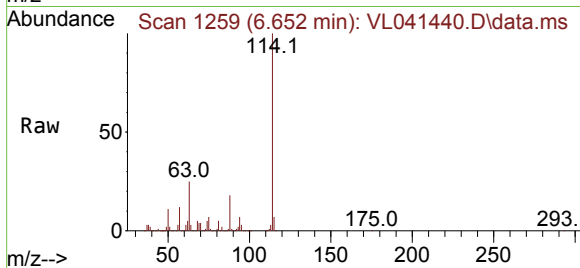

#41

Tetrahydrofuran

Concen: 1.747 ppbv

RT: 5.565 min Scan# 921

Delta R.T. 0.019 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28




Tgt Ion: 42 Resp: 138999


Ion Ratio Lower Upper

42 100

72 37.9 31.2 46.8

71 36.9 30.5 45.7


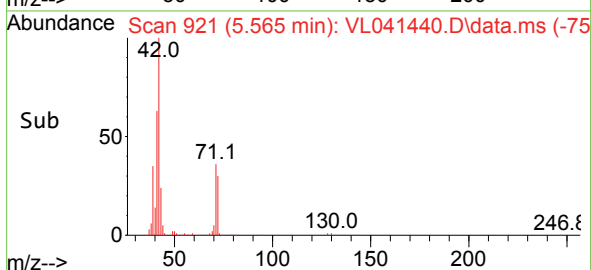

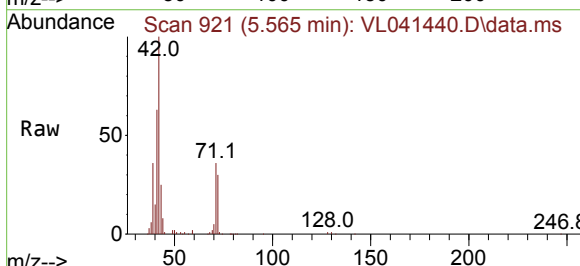




#44
2,2,4-Trimethylpentane
Concen: 0.284 ppbv
RT: 7.330 min Scan# 1466
Delta R.T. 0.013 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03


Tgt Ion: 57 Resp: 99643
Ion Ratio Lower Upper
57 100
41 49.9 27.0 40.6#
56 42.7 25.2 37.8#

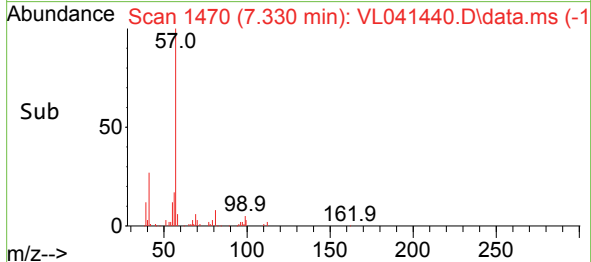

#53
Toluene
Concen: 3.907 ppbv
RT: 9.221 min Scan# 2058
Delta R.T. 0.003 min
Lab File: VL041440.D
Acq: 29 Jul 2024 22:28

Tgt Ion: 91 Resp: 914590
Ion Ratio Lower Upper
91 100
92 61.0 48.7 73.1

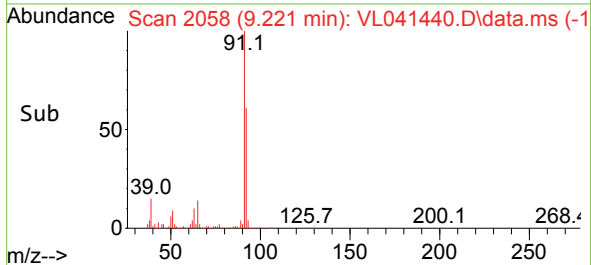



#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 11.465 min Scan# 2756

Delta R.T. 0.000 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28

Instrument :

MSVOA_L

ClientSampleId :

ACVI-IA-03





Tgt Ion:117 Resp: 2629445

Ion Ratio Lower Upper

117 100

82 64.7 51.0 76.6

119 33.1 45.2 67.8#

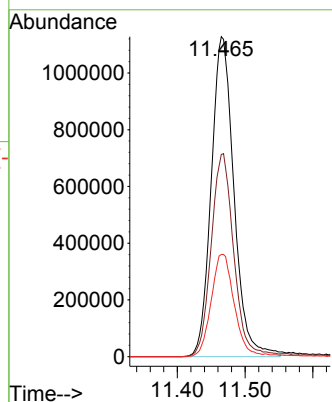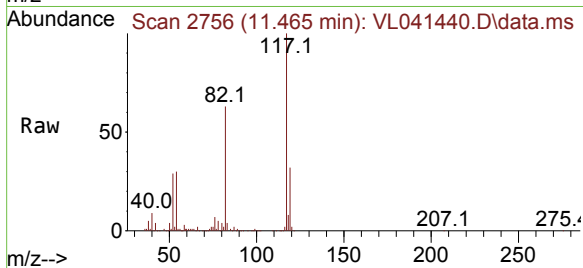

#58

Ethyl Benzene

Concen: 0.168 ppbv

RT: 12.085 min Scan# 2949

Delta R.T. 0.000 min

Lab File: VL041440.D




Acq: 29 Jul 2024 22:28


Tgt Ion: 91 Resp: 50791

Ion Ratio Lower Upper

91 100

106 29.3 25.8 38.8

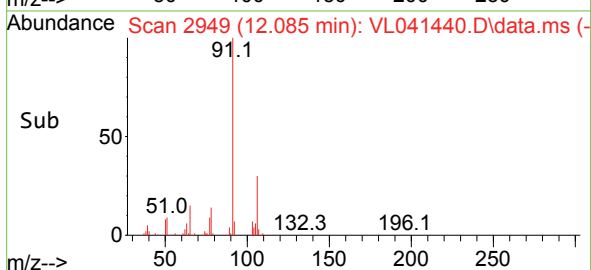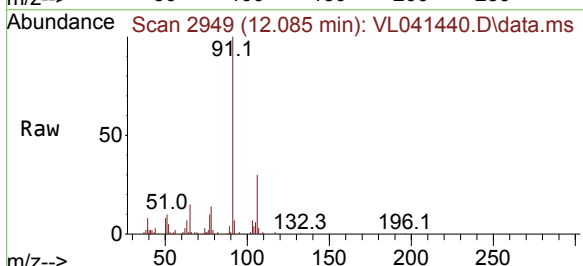



#59

m/p-Xylene

Concen: 0.843 ppbv

RT: 12.343 min Scan# 3037

Delta R.T. -0.026 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28

Instrument :

MSVOA_L

ClientSampleId :





ACVI-IA-03

Tgt Ion: 91 Resp: 220628

Ion Ratio Lower Upper

91 100

106 48.5 36.3 54.5

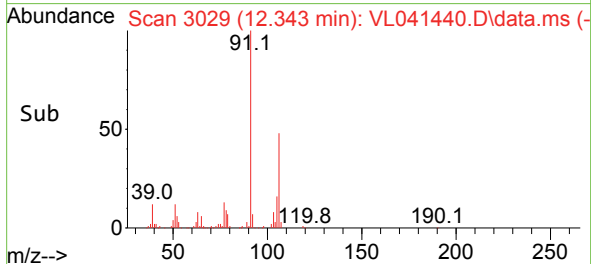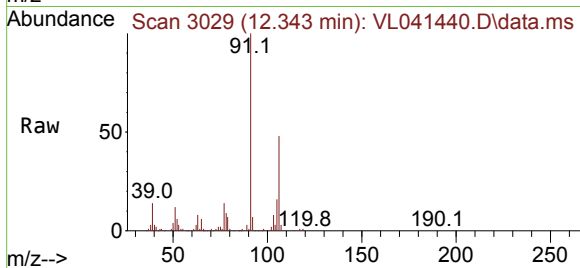

#60

o-Xylene

Concen: 0.324 ppbv

RT: 13.056 min Scan# 3251

Delta R.T. 0.000 min

Lab File: VL041440.D




Acq: 29 Jul 2024 22:28


Tgt Ion: 91 Resp: 80261

Ion Ratio Lower Upper

91 100

106 44.7 23.1 69.3

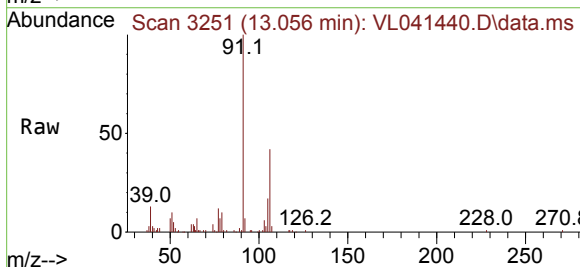

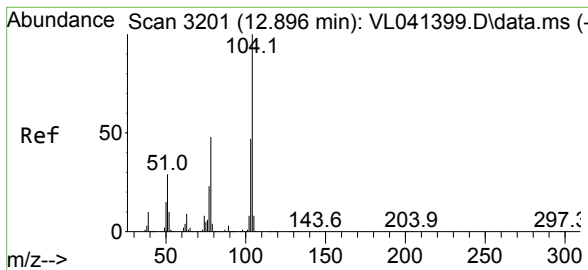

#61

Styrene

Concen: 0.219 ppbv

RT: 12.899 min Scan# 31

Delta R.T. 0.003 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28

Instrument :

MSVOA_L

ClientSampleId :

ACVI-IA-03





Tgt Ion:104 Resp: 24438

Ion Ratio Lower Upper

104 100

78 86.4 40.8 61.2#

103 81.0 38.2 57.4#

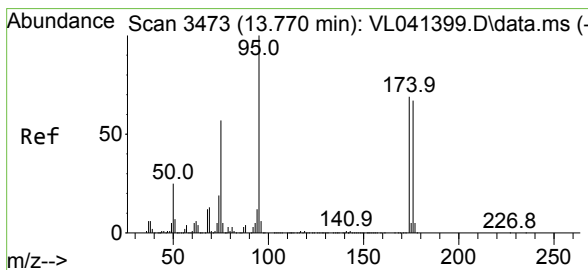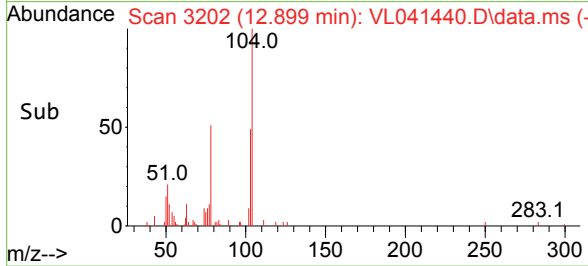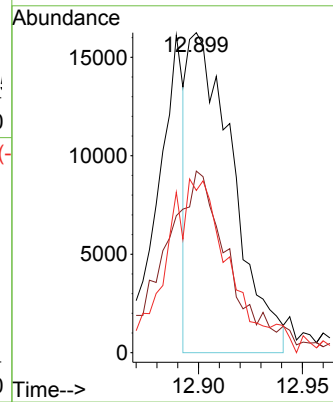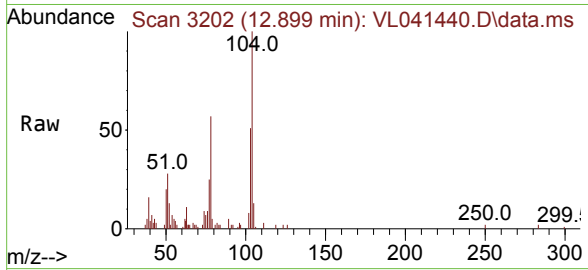

#68

1-Bromo-4-Fluorobenzene

Concen: 10.031 ppbv

RT: 13.773 min Scan# 3474

Delta R.T. 0.000 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28




Tgt Ion: 95 Resp: 2029848


Ion Ratio Lower Upper

95 100

174 71.7 56.3 84.5

175 5.2 4.0 6.0

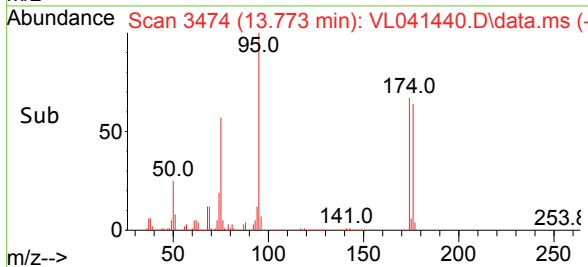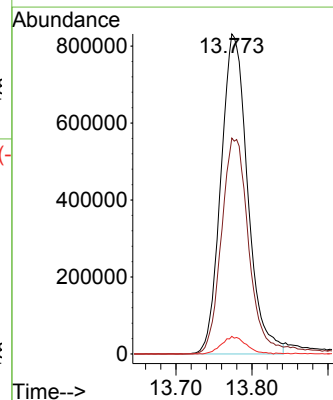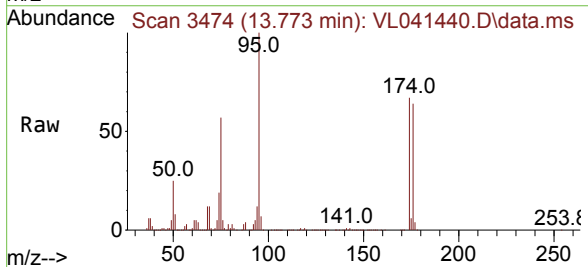



#69

p-Isopropyltoluene

Concen: 0.069 ppbv

RT: 16.998 min Scan# 4474

Delta R.T. 0.003 min

Lab File: VL041440.D

Acq: 29 Jul 2024 22:28

Instrument :

MSVOA_L

ClientSampleId :

ACVI-IA-03





Tgt Ion:119 Resp: 26925

Ion Ratio Lower Upper

119 100

134 28.8 20.5 30.7

91 39.4 23.2 34.8#

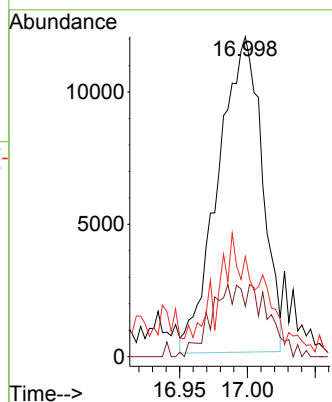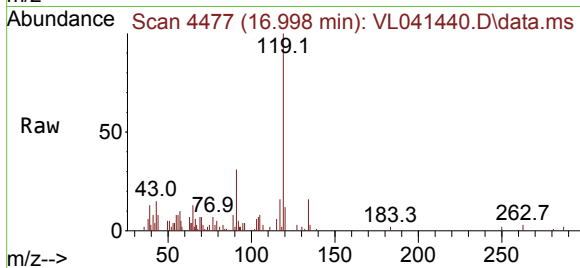

#71

2-Chlorotoluene

Concen: 0.037 ppbv

RT: 14.915 min Scan# 3829

Delta R.T. 0.116 min

Lab File: VL041440.D




Acq: 29 Jul 2024 22:28


Tgt Ion: 91 Resp: 10194

Ion Ratio Lower Upper

91 100


126 1.0 12.7 50.9#

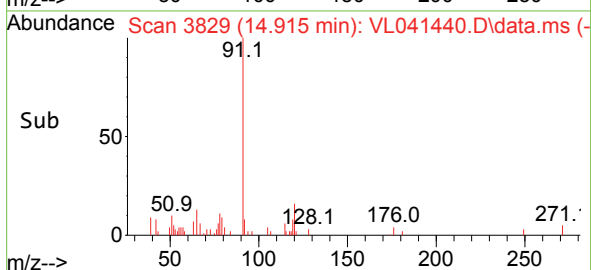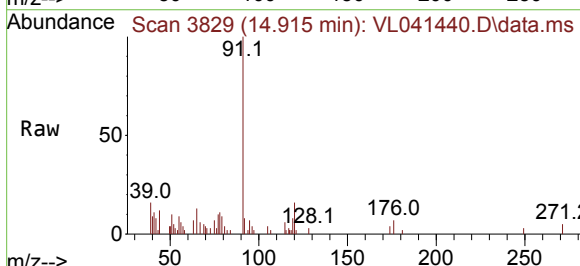

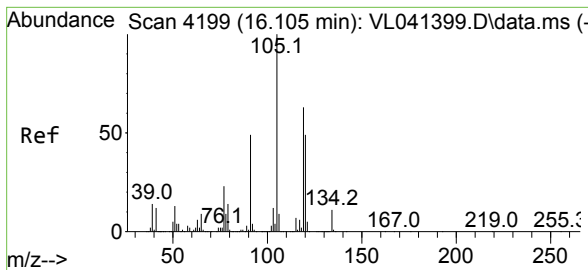

#74
 1,2,4-Trimethylbenzene
 Concen: 0.131 ppbv
 RT: 16.105 min Scan# 4199
 Delta R.T. -0.003 min
 Lab File: VL041440.D
 Acq: 29 Jul 2024 22:28

Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-03

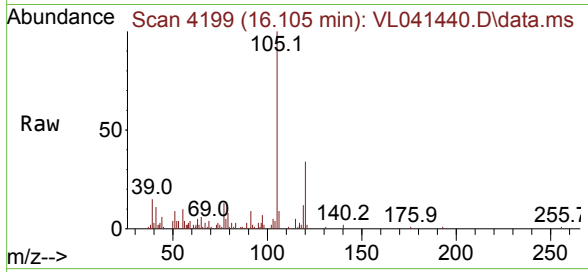

Tgt Ion:	105	Resp:	38298
Ion	Ratio	Lower	Upper
105	100		
120	33.8	39.5	59.3#
91	6.4	39.8	59.8#
77	13.2	18.2	27.4#

