

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072924\
 Data File : VL041437.D
 Acq On : 29 Jul 2024 20:25
 Operator : SY/MD
 Sample : P3342-05
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-02

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Quant Time: Jul 30 02:53:56 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 2

QLast Update : Tue Jul 30 02:42:20 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.192	49	1076480	10.000	ppbv	0.01
33) 1,4-Difluorobenzene	6.655	114	2910344	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.468	117	2719407	10.000	ppbv	# 0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.780	95	2118775	10.124	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.200%
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	2.729	85	100689	0.544	ppbv	99
4) Chloromethane	2.812	50	48192	0.707	ppbv	97
9) Propene	2.706	41	166921m	2.835	ppbv	
10) Heptane	7.584	43	296798	2.244	ppbv	96
11) Trichlorofluoromethane	3.565	101	34892	0.212	ppbv	93
13) Ethanol	3.246	45	6703312	1274.007	ppbv	94
15) Acetone	3.468	43	1251458	10.232	ppbv #	46
19) Isopropyl Alcohol	3.584	45	1948237	27.246	ppbv #	98
20) Methylene Chloride	3.935	84	264591	5.801	ppbv	98
26) Hexane	5.214	57	1436668	14.253	ppbv #	49
27) Carbon Disulfide	4.127	76	21963	0.186	ppbv #	57
29) Chloroform	5.272	83	22953	0.140	ppbv	90
30) Cyclohexane	6.603	84	142408	1.735	ppbv	94
34) 2-Butanone	4.787	43	241339	1.714	ppbv	97
35) Carbon Tetrachloride	6.494	117	9230m	0.057	ppbv	
36) Benzene	6.372	78	763233	3.589	ppbv	99
43) Methyl Methacrylate	7.475	69	52871	0.693	ppbv #	75
44) 2,2,4-Trimethylpentane	7.330	57	833248	2.346	ppbv #	82
52) Tetrachloroethene	10.622	164	10630m	0.129	ppbv	
53) Toluene	9.220	91	3004756	12.685	ppbv	99
58) Ethyl Benzene	12.092	91	860980	2.747	ppbv	97
59) m/p-Xylene	12.343	91	1237086	4.572	ppbv	97
60) o-Xylene	13.056	91	470594	1.839	ppbv	100
61) Styrene	12.896	104	460062	3.984	ppbv	99
62) Isopropylbenzene	14.034	105	36321m	0.093	ppbv	
64) n-propylbenzene	14.918	120	11103m	0.109	ppbv	
72) 4-Ethyltoluene	15.195	105	58992m	0.196	ppbv	
73) 1,3,5-Trimethylbenzene	15.355	105	44497m	0.171	ppbv	
74) 1,2,4-Trimethylbenzene	16.108	105	168842	0.559	ppbv #	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072924\
Data File : VL041437.D
Acq On : 29 Jul 2024 20:25
Operator : SY/MD
Sample : P3342-05
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02

Quant Time: Jul 30 02:53:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jul 30 02:42:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

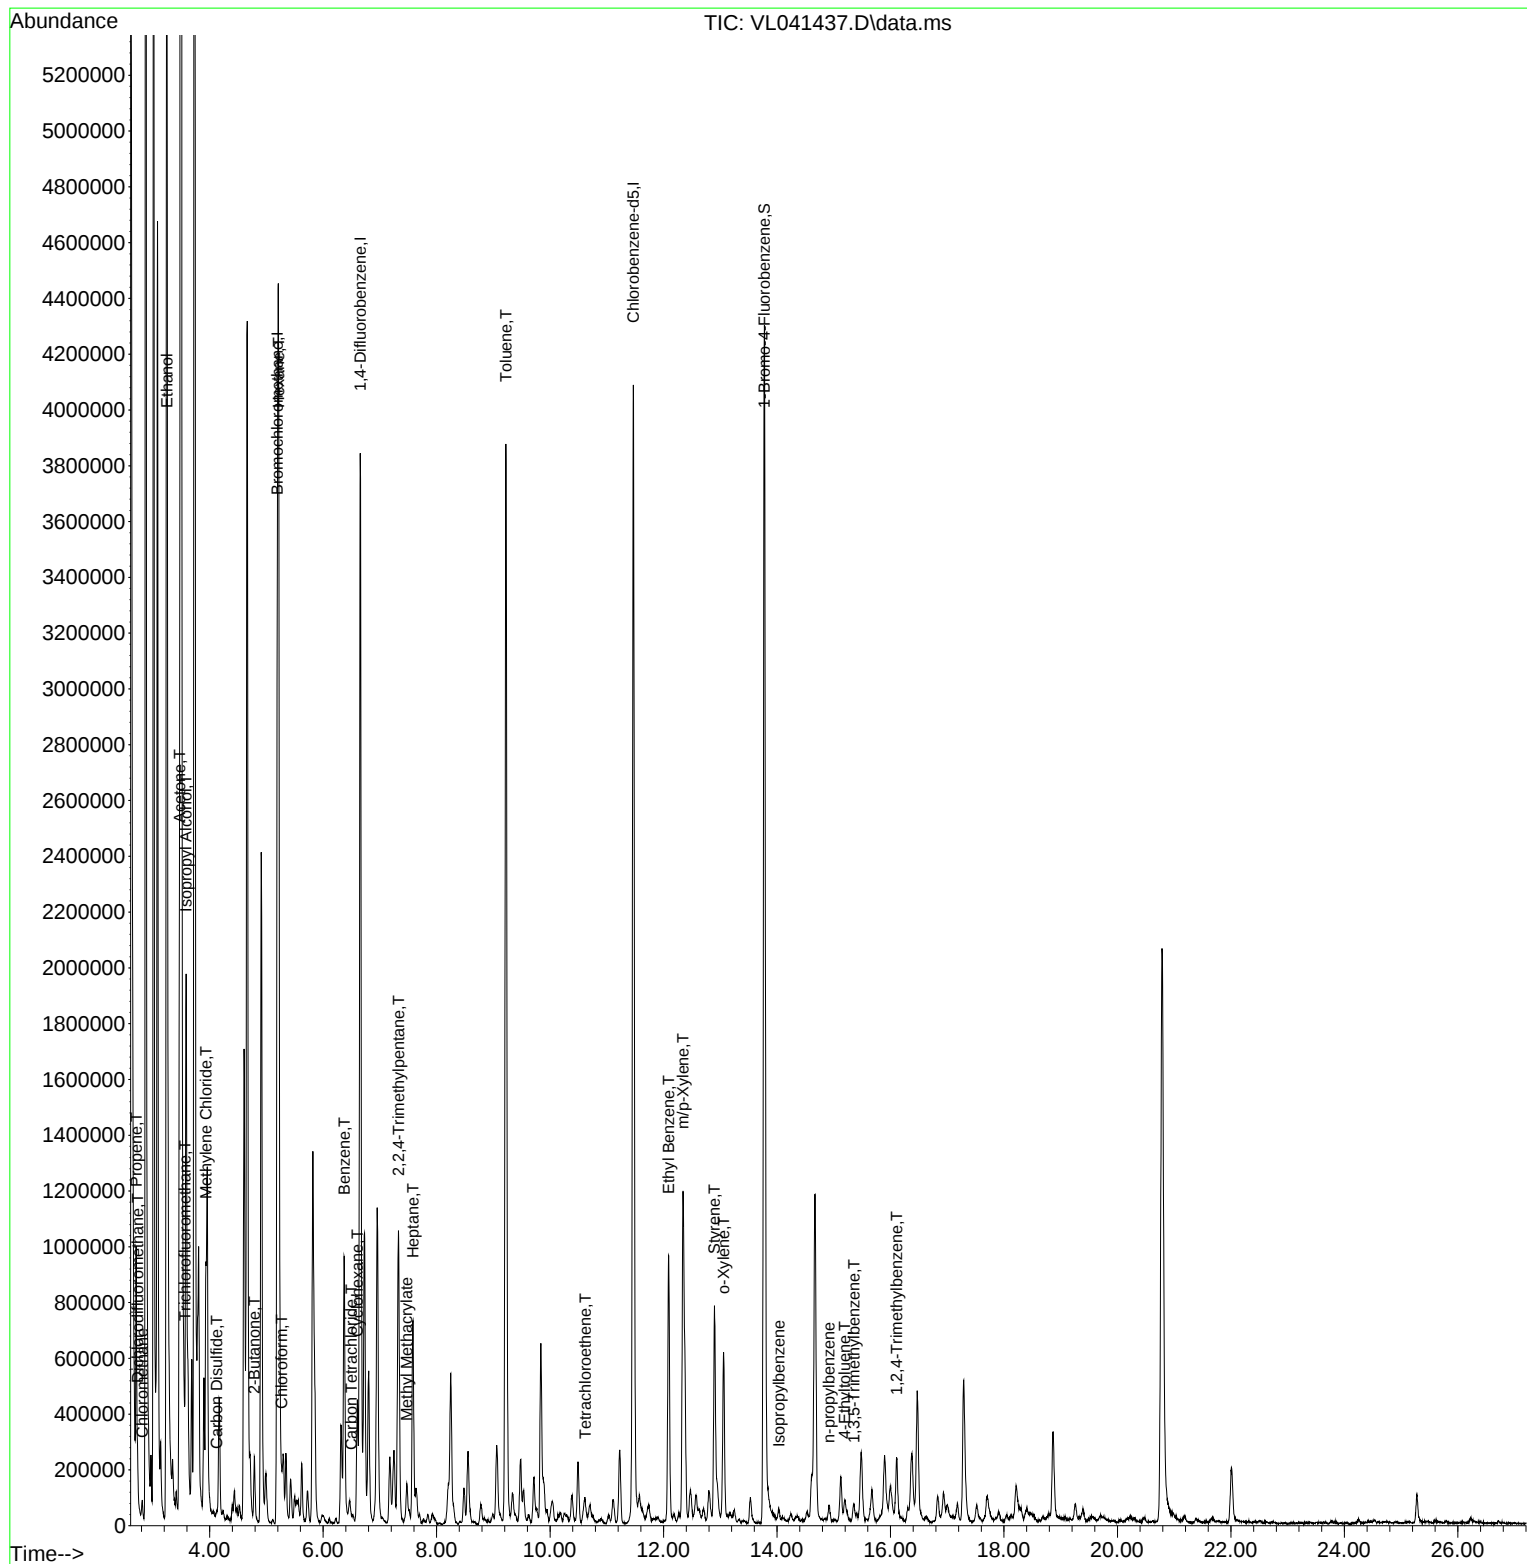



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.192 min Scan# 80
Delta R.T. 0.013 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02




Tgt Ion: 49 Resp: 1076480
Ion Ratio Lower Upper
49 100
128 47.0 23.8 71.4
130 61.0 30.8 92.4

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

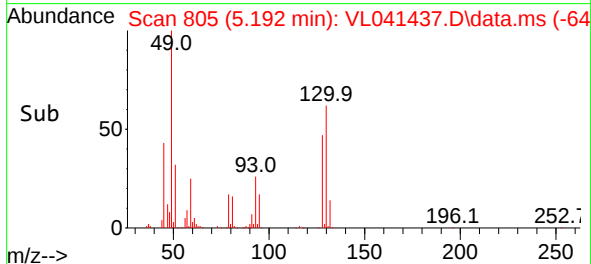


#2
Dichlorodifluoromethane
Concen: 0.544 ppbv
RT: 2.729 min Scan# 39
Delta R.T. 0.019 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Tgt Ion: 85 Resp: 100689
Ion Ratio Lower Upper
85 100
87 33.2 26.0 39.0

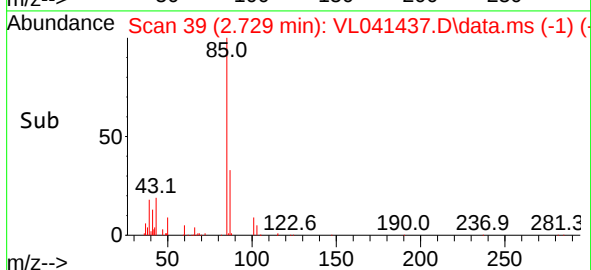

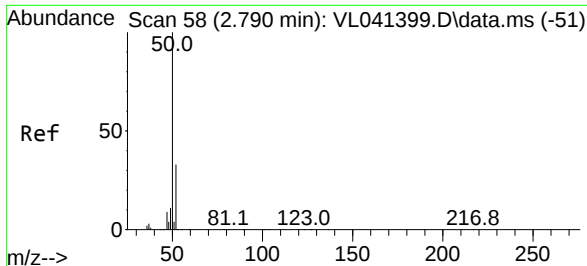

#4
Chloromethane
Concen: 0.707 ppbv
RT: 2.812 min Scan# 61
Delta R.T. 0.019 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02

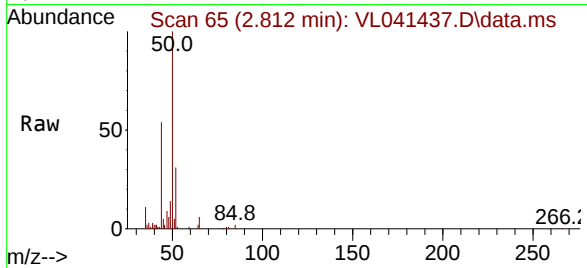

Tgt Ion: 50 Resp: 48192
Ion Ratio Lower Upper
50 100
52 30.9 26.1 39.1




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

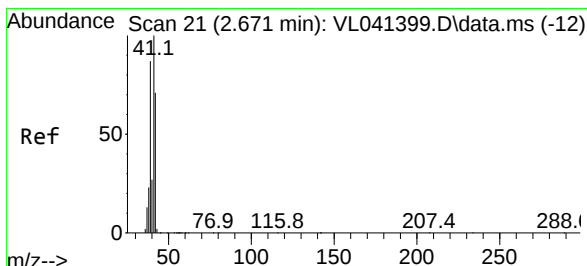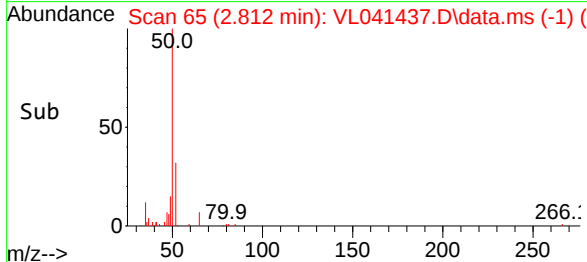

#9
Propene
Concen: 2.835 ppbv m
RT: 2.706 min Scan# 32
Delta R.T. 0.035 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25


Tgt Ion: 41 Resp: 166921
Ion Ratio Lower Upper
41 100
42 1383.3 55.9 83.9#

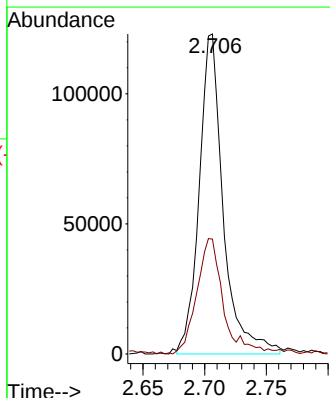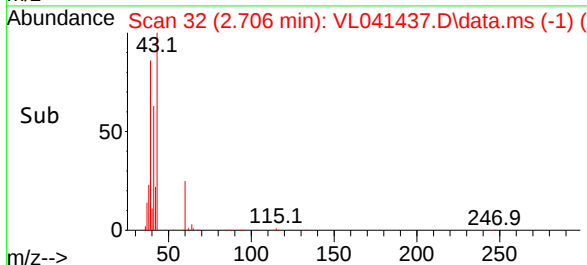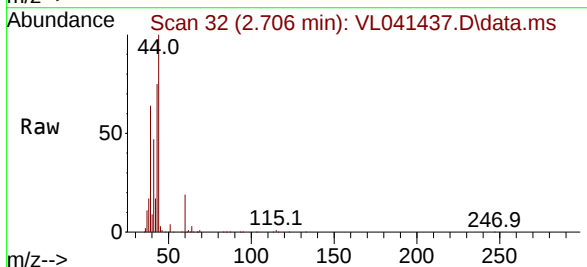



#10
Heptane
Concen: 2.244 ppbv
RT: 7.584 min Scan# 11
Delta R.T. 0.013 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02



Tgt Ion: 43 Resp: 296798
Ion Ratio Lower Upper
43 100
57 53.7 40.5 60.7




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

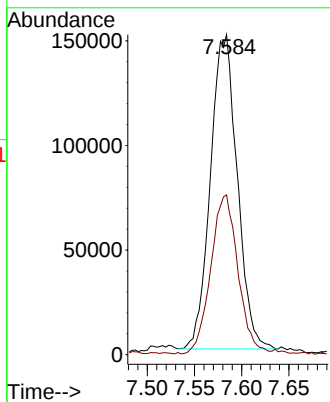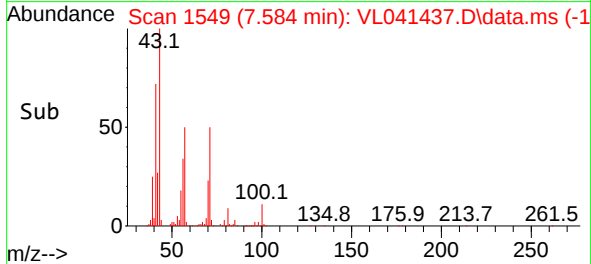

#11
Trichlorofluoromethane
Concen: 0.212 ppbv
RT: 3.565 min Scan# 299
Delta R.T. 0.019 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25


Tgt Ion:101 Resp: 34892
Ion Ratio Lower Upper
101 100
103 60.5 52.6 79.0

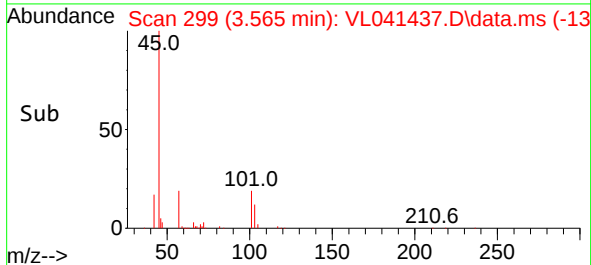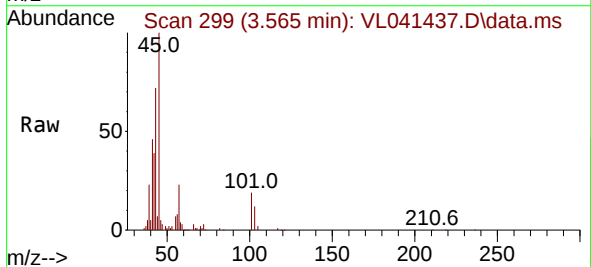



#13
Ethanol
Concen: 1274.007 ppbv
RT: 3.246 min Scan# 200
Delta R.T. 0.019 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02




Tgt Ion: 45 Resp: 6703312
Ion Ratio Lower Upper
45 100
46 36.7 13.4 53.4

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

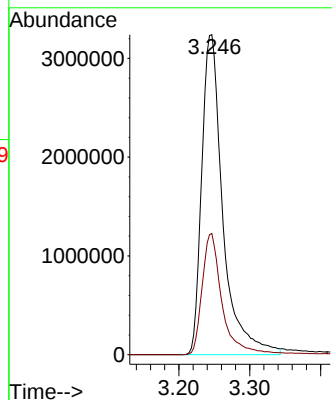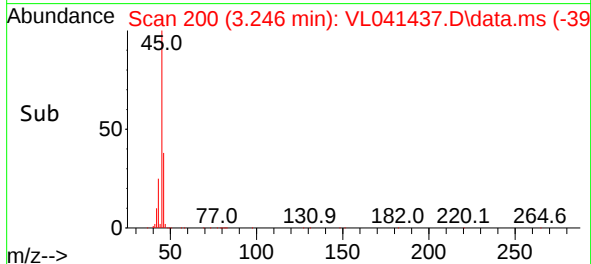


#15
Acetone
Concen: 10.232 ppbv
RT: 3.468 min Scan# 269
Delta R.T. 0.016 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25

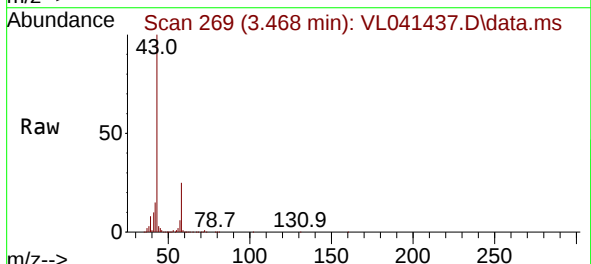


Tgt Ion: 43 Resp: 1251458
Ion Ratio Lower Upper
43 100
58 54.8 21.4 32.2#

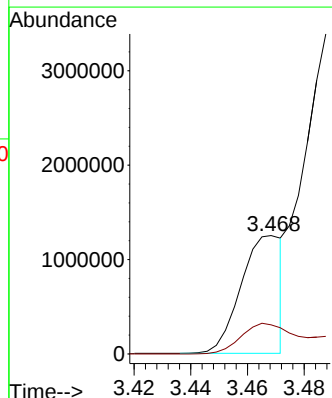



#19
Isopropyl Alcohol
Concen: 27.246 ppbv
RT: 3.584 min Scan# 305
Delta R.T. 0.022 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02

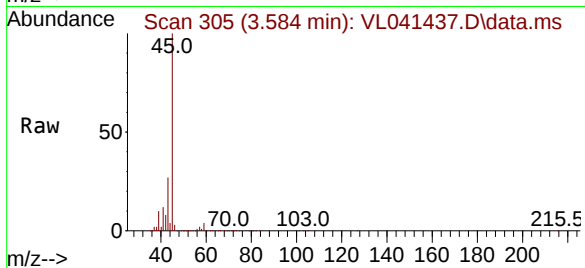


Tgt Ion: 45 Resp: 194823
Ion Ratio Lower Upper
45 100
58 1.7 1.9 2.9

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

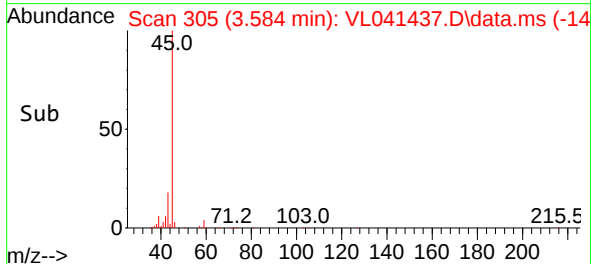


#20
Methylene Chloride
Concen: 5.801 ppbv
RT: 3.935 min Scan# 414
Delta R.T. 0.016 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25

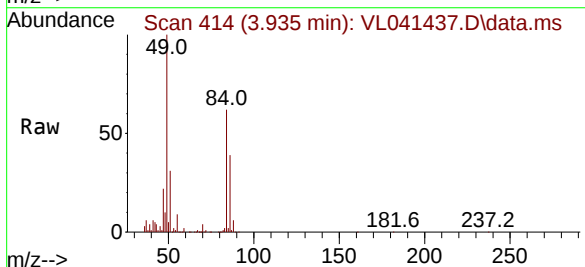


Tgt Ion: 84 Resp: 264591
Ion Ratio Lower Upper
84 100
49 159.6 126.6 190.0
51 47.8 38.6 58.0
86 62.3 53.0 79.4

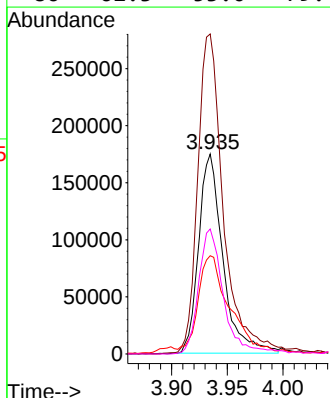



#26
Hexane
Concen: 14.253 ppbv
RT: 5.214 min Scan# 812
Delta R.T. 0.016 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02

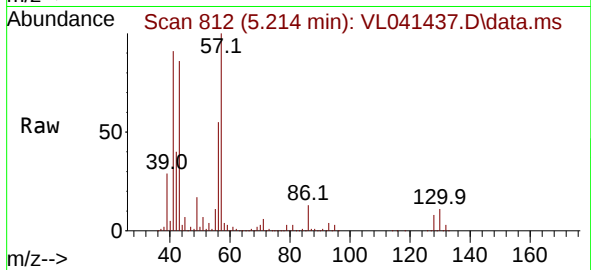


Tgt Ion: 57 Resp: 143666
Ion Ratio Lower Upper
57 100
41 92.7 74.0 111.0
43 102.9 193.6 290.4
56 54.0 43.1 64.7

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

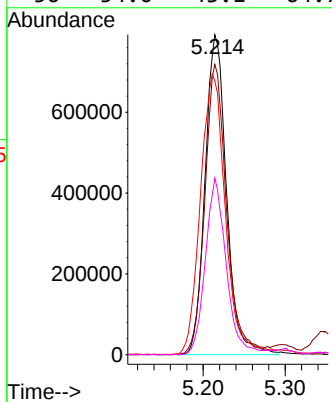


#27
Carbon Disulfide
Concen: 0.186 ppbv
RT: 4.127 min Scan# 474
Delta R.T. 0.019 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25

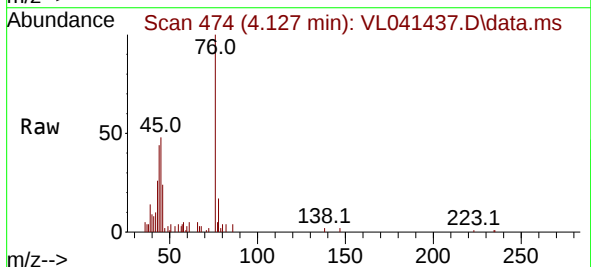

Tgt Ion: 76 Resp: 21963
Ion Ratio Lower Upper
76 100
44 45.3 15.6 23.4#
78 14.7 7.7 11.5#

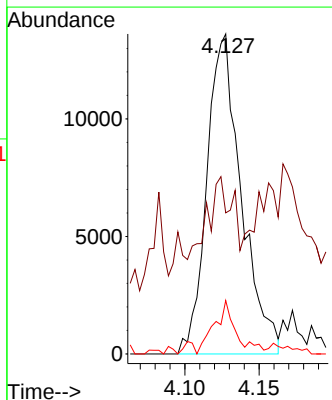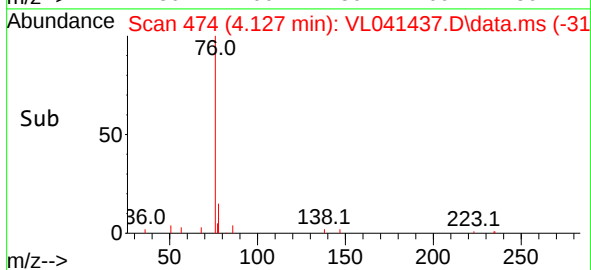







#29
Chloroform
Concen: 0.140 ppbv
RT: 5.272 min Scan# 81
Delta R.T. 0.010 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25

Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02

Tgt Ion: 83 Resp: 2295
Ion Ratio Lower Upper
83 100
85 58.6 53.1 79.7




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

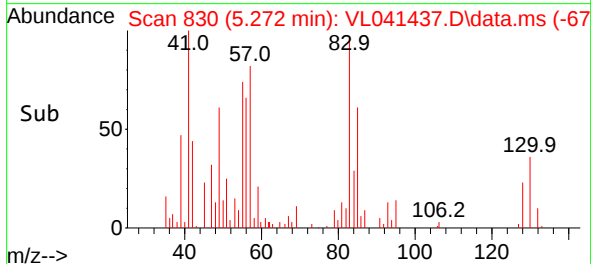

#30
Cyclohexane
Concen: 1.735 ppbv
RT: 6.603 min Scan# 1244
Delta R.T. 0.010 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25

Tgt Ion: 84 Resp: 142408
Ion Ratio Lower Upper
84 100
56 127.5 111.2 166.8
41 88.3 70.3 105.5

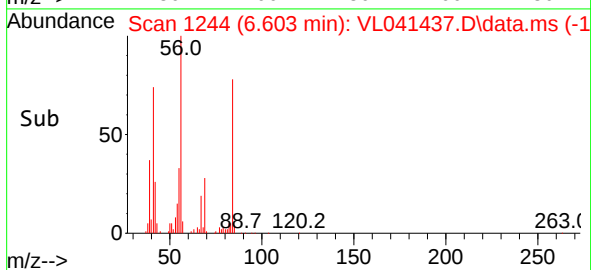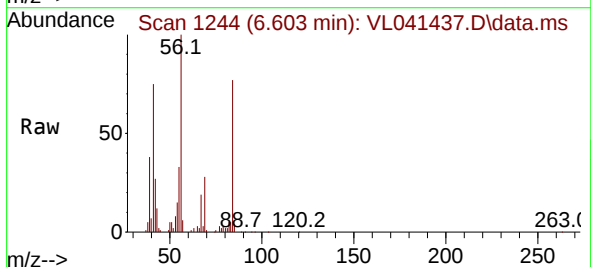



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.655 min Scan# 1

Delta R.T. 0.010 min

Lab File: VL041437.D

Acq: 29 Jul 2024 20:25

Instrument :

MSVOA_L

ClientSampleId :

ACVI-IA-02

Tgt Ion:114 Resp: 291034

Ion Ratio Lower Upper

114 100

63 25.2 20.3 30.5





88 17.9 14.3 21.5

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024

Supervised By :Semsettin Yesilyurt 07/30/2024

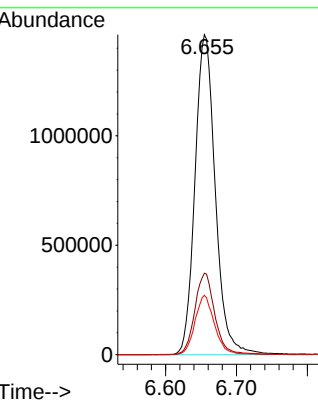

#34

2-Butanone

Concen: 1.714 ppbv

RT: 4.787 min Scan# 679

Delta R.T. 0.013 min

Lab File: VL041437.D




Acq: 29 Jul 2024 20:25


Tgt Ion: 43 Resp: 241339

Ion Ratio Lower Upper

43 100

72 23.0 17.3 25.9

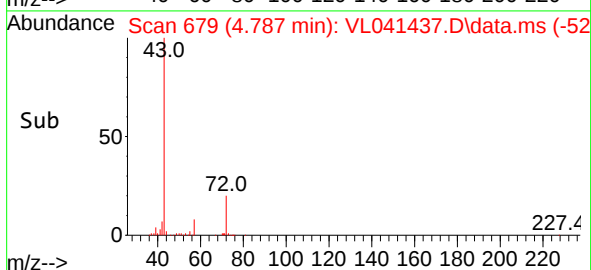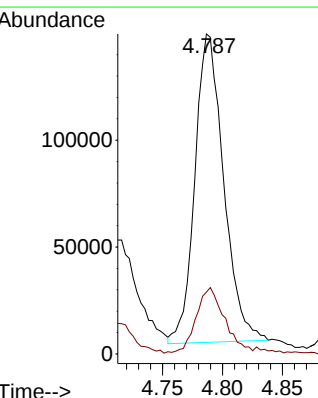



#35

Carbon Tetrachloride

Concen: 0.057 ppbv

RT: 6.494 min Scan# 1172

Delta R.T. 0.010 min

Lab File: VL041437.D

Acq: 29 Jul 2024 20:25

Instrument :

MSVOA_L

ClientSampleId :





ACVI-IA-02

Tgt Ion:	117	Resp:	9230
Ion	Ratio	Lower	Upper
117	100		
119	99.0	76.6	115.0
121	38.9	25.1	37.7

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

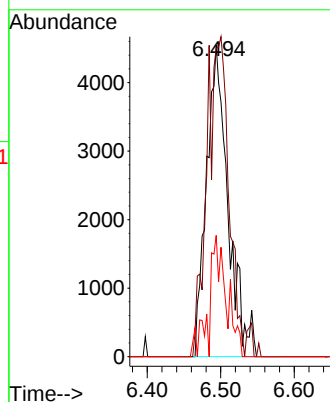

#36

Benzene

Concen: 3.589 ppbv




RT: 6.372 min Scan# 1172


Delta R.T. 0.013 min

Lab File: VL041437.D

Acq: 29 Jul 2024 20:25


Tgt Ion:	78	Resp:	763233
Ion	Ratio	Lower	Upper
78	100		
77	22.6	18.1	27.1
50	18.9	15.5	23.3

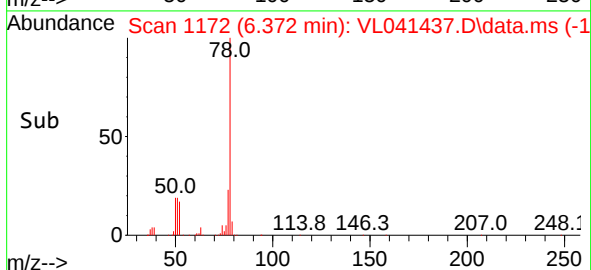



#43
Methyl Methacrylate
Concen: 0.693 ppbv
RT: 7.475 min Scan# 1512
Delta R.T. 0.010 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02



Tgt Ion: 69 Resp: 5287
Ion Ratio Lower Upper
69 100
41 187.8 118.7 178.1
100 33.8 27.0 40.4




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

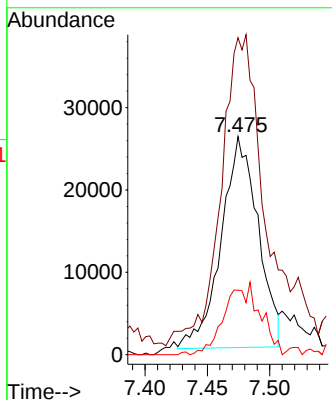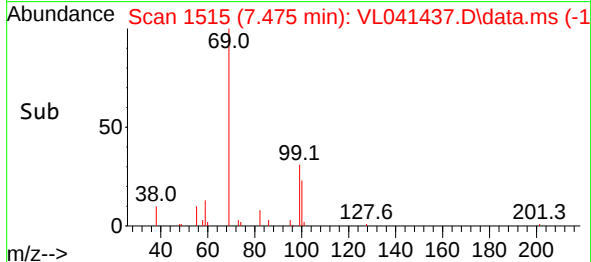

#44
2,2,4-Trimethylpentane
Concen: 2.346 ppbv
RT: 7.330 min Scan# 1470
Delta R.T. 0.013 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25


Tgt Ion: 57 Resp: 833248
Ion Ratio Lower Upper
57 100
41 43.2 27.0 40.6#
56 42.0 25.2 37.8#

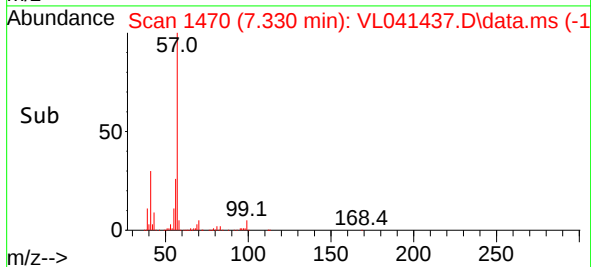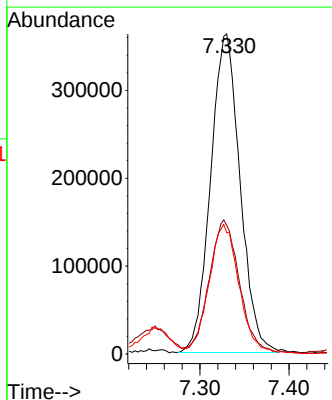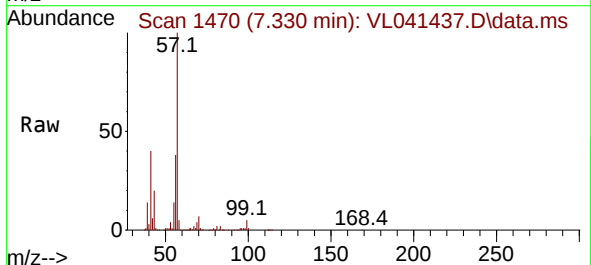



#52
Tetrachloroethene
Concen: 0.129 ppbv m
RT: 10.622 min Scan# 2491
Delta R.T. 0.013 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02



Tgt Ion:164 Resp: 10630
Ion Ratio Lower Upper
164 100
166 116.1 101.1 151.7
129 118.8 81.7 122.5
131 122.3 76.2 114.4#




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

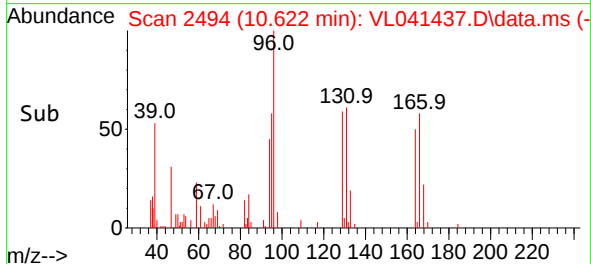

#53
Toluene
Concen: 12.685 ppbv
RT: 9.220 min Scan# 2058
Delta R.T. 0.003 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25


Tgt Ion: 91 Resp: 3004756
Ion Ratio Lower Upper
91 100
92 61.3 48.7 73.1

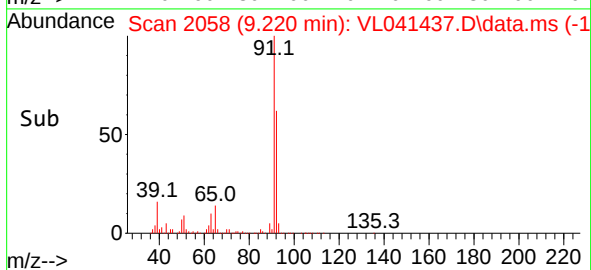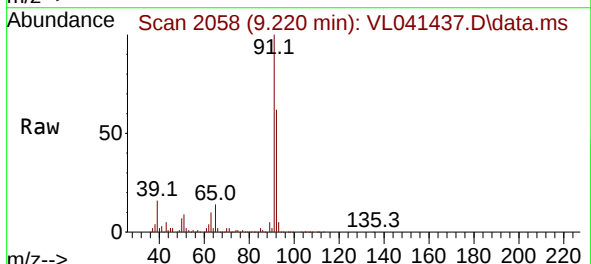

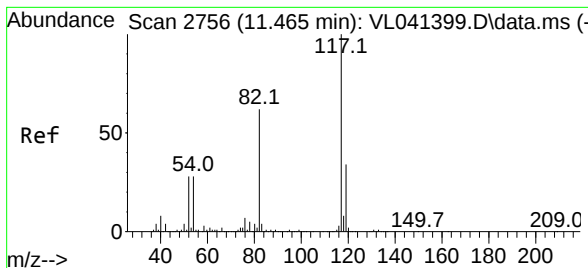

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.468 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02

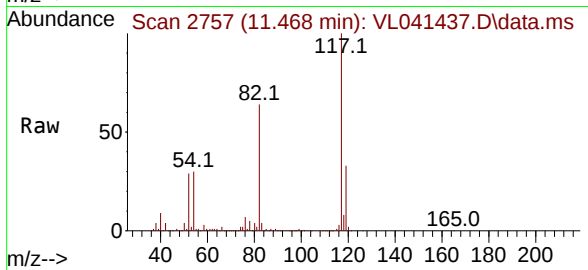


Tgt Ion: 117 Resp: 271940
Ion Ratio Lower Upper
117 100
82 63.1 51.0 76.6
119 32.6 45.2 67.8

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

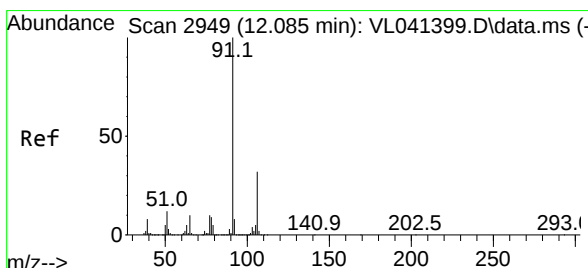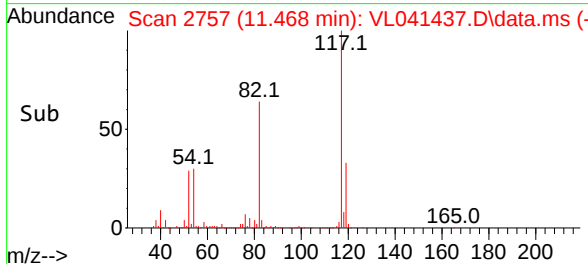


#58
Ethyl Benzene
Concen: 2.747 ppbv
RT: 12.092 min Scan# 2951
Delta R.T. 0.006 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25

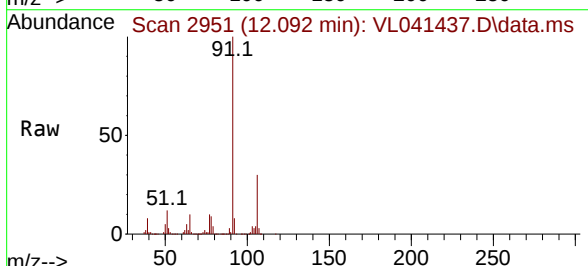

Tgt Ion: 91 Resp: 860980
Ion Ratio Lower Upper
91 100
106 30.5 25.8 38.8

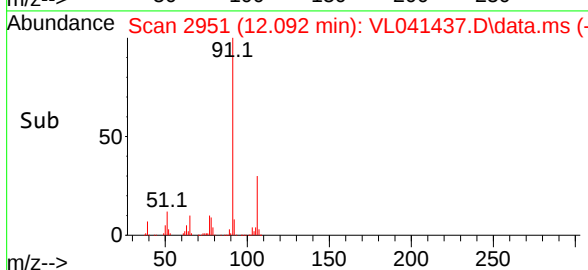







#59
m/p-Xylene
Concen: 4.572 ppbv
RT: 12.343 min Scan# 3037
Delta R.T. -0.026 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25

Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02

Tgt Ion: 91 Resp: 1237080
Ion Ratio Lower Upper
91 100
106 47.4 36.3 54.5




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

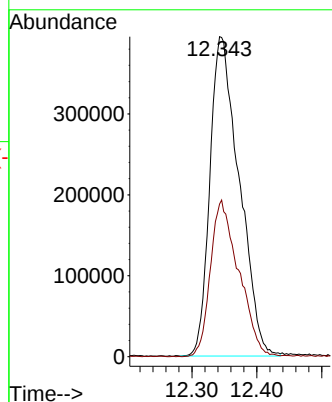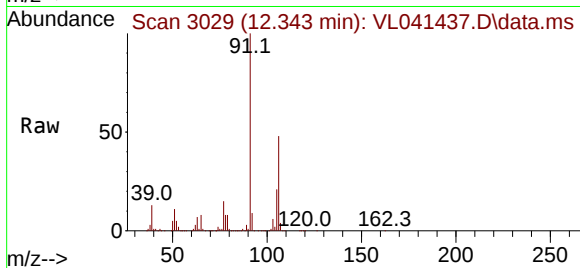

#60
o-Xylene
Concen: 1.839 ppbv
RT: 13.056 min Scan# 3251
Delta R.T. -0.000 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25

Tgt Ion: 91 Resp: 470594
Ion Ratio Lower Upper
91 100
106 46.3 23.1 69.3

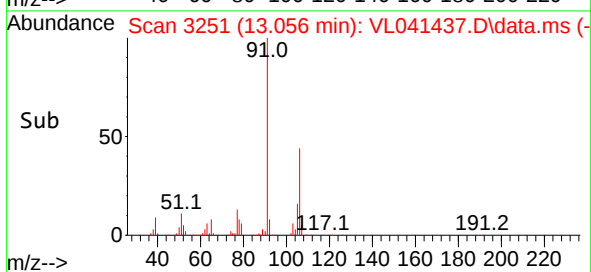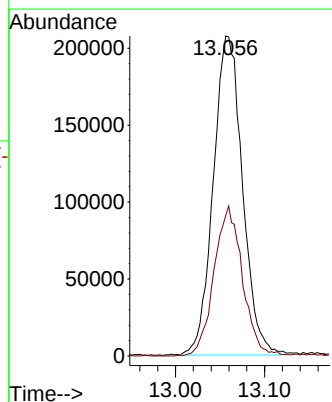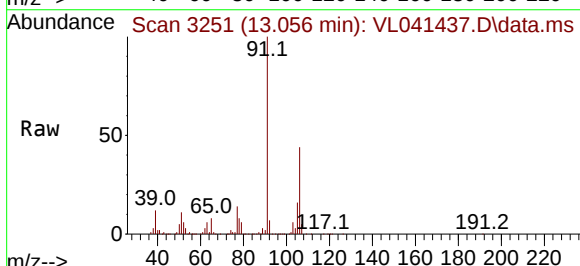



#61

Styrene

Concen: 3.984 ppbv

RT: 12.896 min Scan# 31

Delta R.T. -0.000 min

Lab File: VL041437.D

Acq: 29 Jul 2024 20:25

Instrument :

MSVOA_L

ClientSampleId :





ACVI-IA-02

Tgt Ion:104 Resp: 460062
 Ion Ratio Lower Upper
 104 100
 78 50.3 40.8 61.2
 103 46.5 38.2 57.4

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

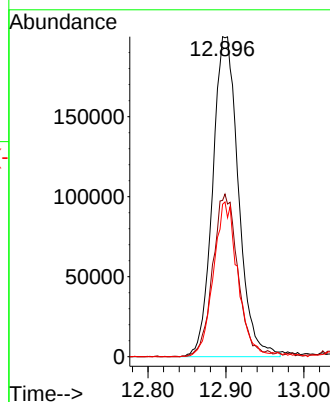

#62

Isopropylbenzene

Concen: 0.093 ppbv m




RT: 14.034 min Scan# 3555


Delta R.T. 0.006 min

Lab File: VL041437.D

Acq: 29 Jul 2024 20:25


Tgt Ion:105 Resp: 36321
 Ion Ratio Lower Upper
 105 100
 120 0.0 21.0 31.4#

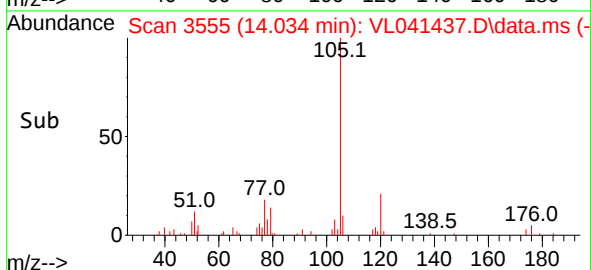



#64
n-propylbenzene
Concen: 0.109 ppbv m
RT: 14.918 min Scan# 3828
Delta R.T. 0.003 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02



Tgt Ion:120 Resp: 1110
Ion Ratio Lower Upper
120 100
91 514.5 361.4 542.0




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

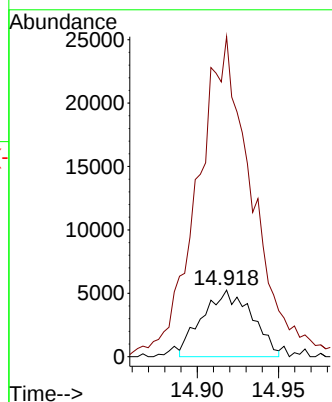

#68
1-Bromo-4-Fluorobenzene
Concen: 10.124 ppbv
RT: 13.780 min Scan# 3476
Delta R.T. 0.006 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25


Tgt Ion: 95 Resp: 2118775
Ion Ratio Lower Upper
95 100
174 69.2 56.3 84.5
175 5.1 4.0 6.0

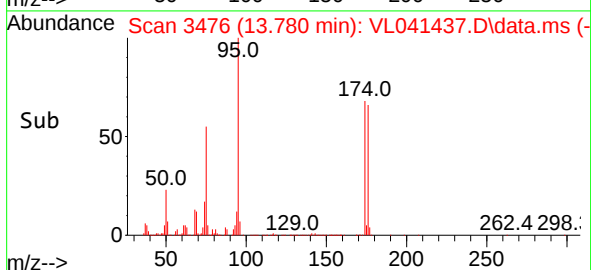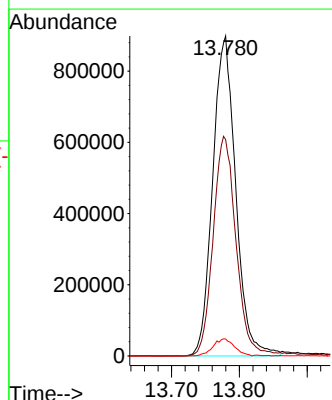

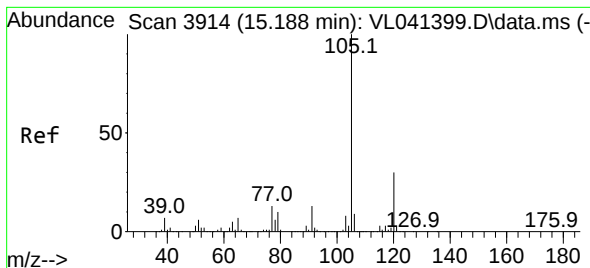

#72
4-Ethyltoluene
Concen: 0.196 ppbv m
RT: 15.195 min Scan# 3916
Delta R.T. 0.003 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-02

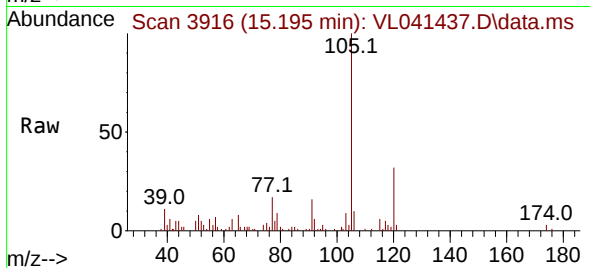

Tgt Ion:105 Resp: 58992
Ion Ratio Lower Upper
105 100
120 29.6 24.2 36.2
91 21.6 10.4 15.6
77 14.6 11.0 16.4




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

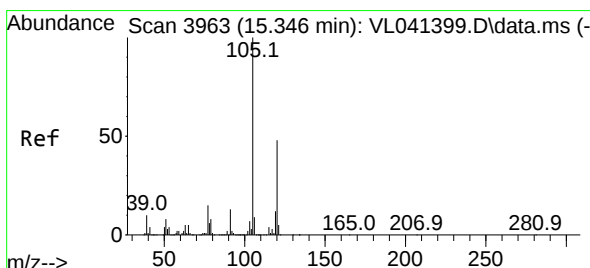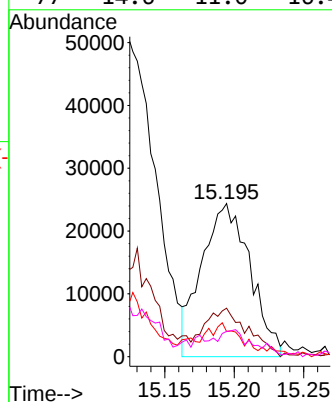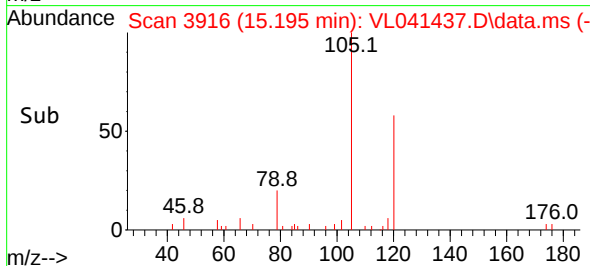

#73
1,3,5-Trimethylbenzene
Concen: 0.171 ppbv m
RT: 15.355 min Scan# 3966
Delta R.T. 0.006 min
Lab File: VL041437.D
Acq: 29 Jul 2024 20:25


Tgt Ion:105 Resp: 44497
Ion Ratio Lower Upper
105 100
120 37.8 38.6 57.8#

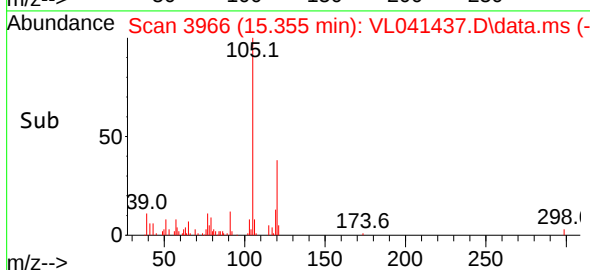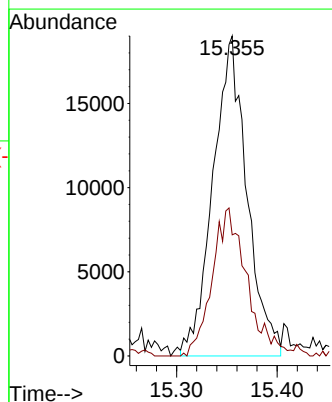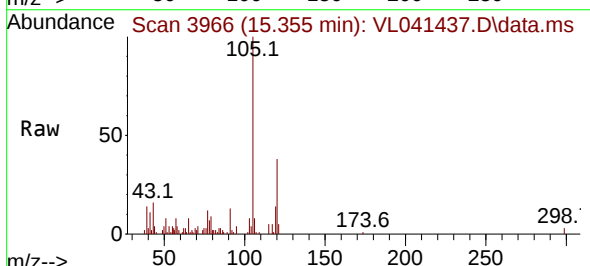



#74
 1,2,4-Trimethylbenzene
 Concen: 0.559 ppbv
 RT: 16.108 min Scan# 4199
 Delta R.T. -0.000 min
 Lab File: VL041437.D
 Acq: 29 Jul 2024 20:25

Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-02



Tgt Ion:	105	Resp:	16884
Ion Ratio	Lower	Upper	
105	100		
120	39.9	39.5	59.3
91	11.7	39.8	59.8
77	12.5	18.2	27.4

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

