

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072924\
 Data File : VL041442.D
 Acq On : 29 Jul 2024 23:49
 Operator : SY/MD
 Sample : P3342-07
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-03D

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Quant Time: Jul 30 02:56:14 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 2

QLast Update : Tue Jul 30 02:42:20 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.195	49	1082784	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	6.658	114	2875417	10.000	ppbv	0.01
55) Chlorobenzene-d5	11.468	117	2694025	10.000	ppbv	# 0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.777	95	2124478	10.247	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.500%
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	2.732	85	105549	0.567	ppbv	93
4) Chloromethane	2.819	50	53297	0.777	ppbv	95
10) Heptane	7.578	43	453144	3.406	ppbv	99
11) Trichlorofluoromethane	3.571	101	37327	0.226	ppbv	98
13) Ethanol	3.250	45	2462622	465.312	ppbv	97
15) Acetone	3.472	43	1607741	13.068	ppbv	# 43
19) Isopropyl Alcohol	3.591	45	2664788	37.050	ppbv	99
20) Methylene Chloride	3.938	84	909107	19.816	ppbv	99
26) Hexane	5.218	57	2280287	22.491	ppbv	# 51
27) Carbon Disulfide	4.128	76	28759	0.242	ppbv	# 67
29) Chloroform	5.282	83	26208m	0.158	ppbv	
30) Cyclohexane	6.607	84	181583	2.199	ppbv	91
34) 2-Butanone	4.790	43	388536	2.793	ppbv	95
35) Carbon Tetrachloride	6.494	117	9492m	0.060	ppbv	
36) Benzene	6.372	78	980012	4.664	ppbv	98
41) Tetrahydrofuran	5.562	42	127295	1.600	ppbv	93
44) 2,2,4-Trimethylpentane	7.327	57	1210107	3.448	ppbv	# 85
52) Tetrachloroethene	10.616	164	12861m	0.158	ppbv	
53) Toluene	9.224	91	4673657	19.970	ppbv	99
58) Ethyl Benzene	12.089	91	944505	3.042	ppbv	100
59) m/p-Xylene	12.343	91	1819188	6.787	ppbv	97
60) o-Xylene	13.057	91	675630	2.664	ppbv	99
61) Styrene	12.896	104	488871	4.273	ppbv	99
62) Isopropylbenzene	14.031	105	45276m	0.117	ppbv	
64) n-propylbenzene	14.912	120	17809m	0.177	ppbv	
69) p-Isopropyltoluene	16.999	119	34322m	0.086	ppbv	
72) 4-Ethyltoluene	15.195	105	92609m	0.310	ppbv	
73) 1,3,5-Trimethylbenzene	15.349	105	64146m	0.249	ppbv	
74) 1,2,4-Trimethylbenzene	16.108	105	257902	0.863	ppbv	# 70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072924\
Data File : VL041442.D
Acq On : 29 Jul 2024 23:49
Operator : SY/MD
Sample : P3342-07
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D

Quant Time: Jul 30 02:56:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jul 30 02:42:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Mahesh Dadoda 07/30/2024
Supervised By : Semsettin Yesilyurt 07/30/2024

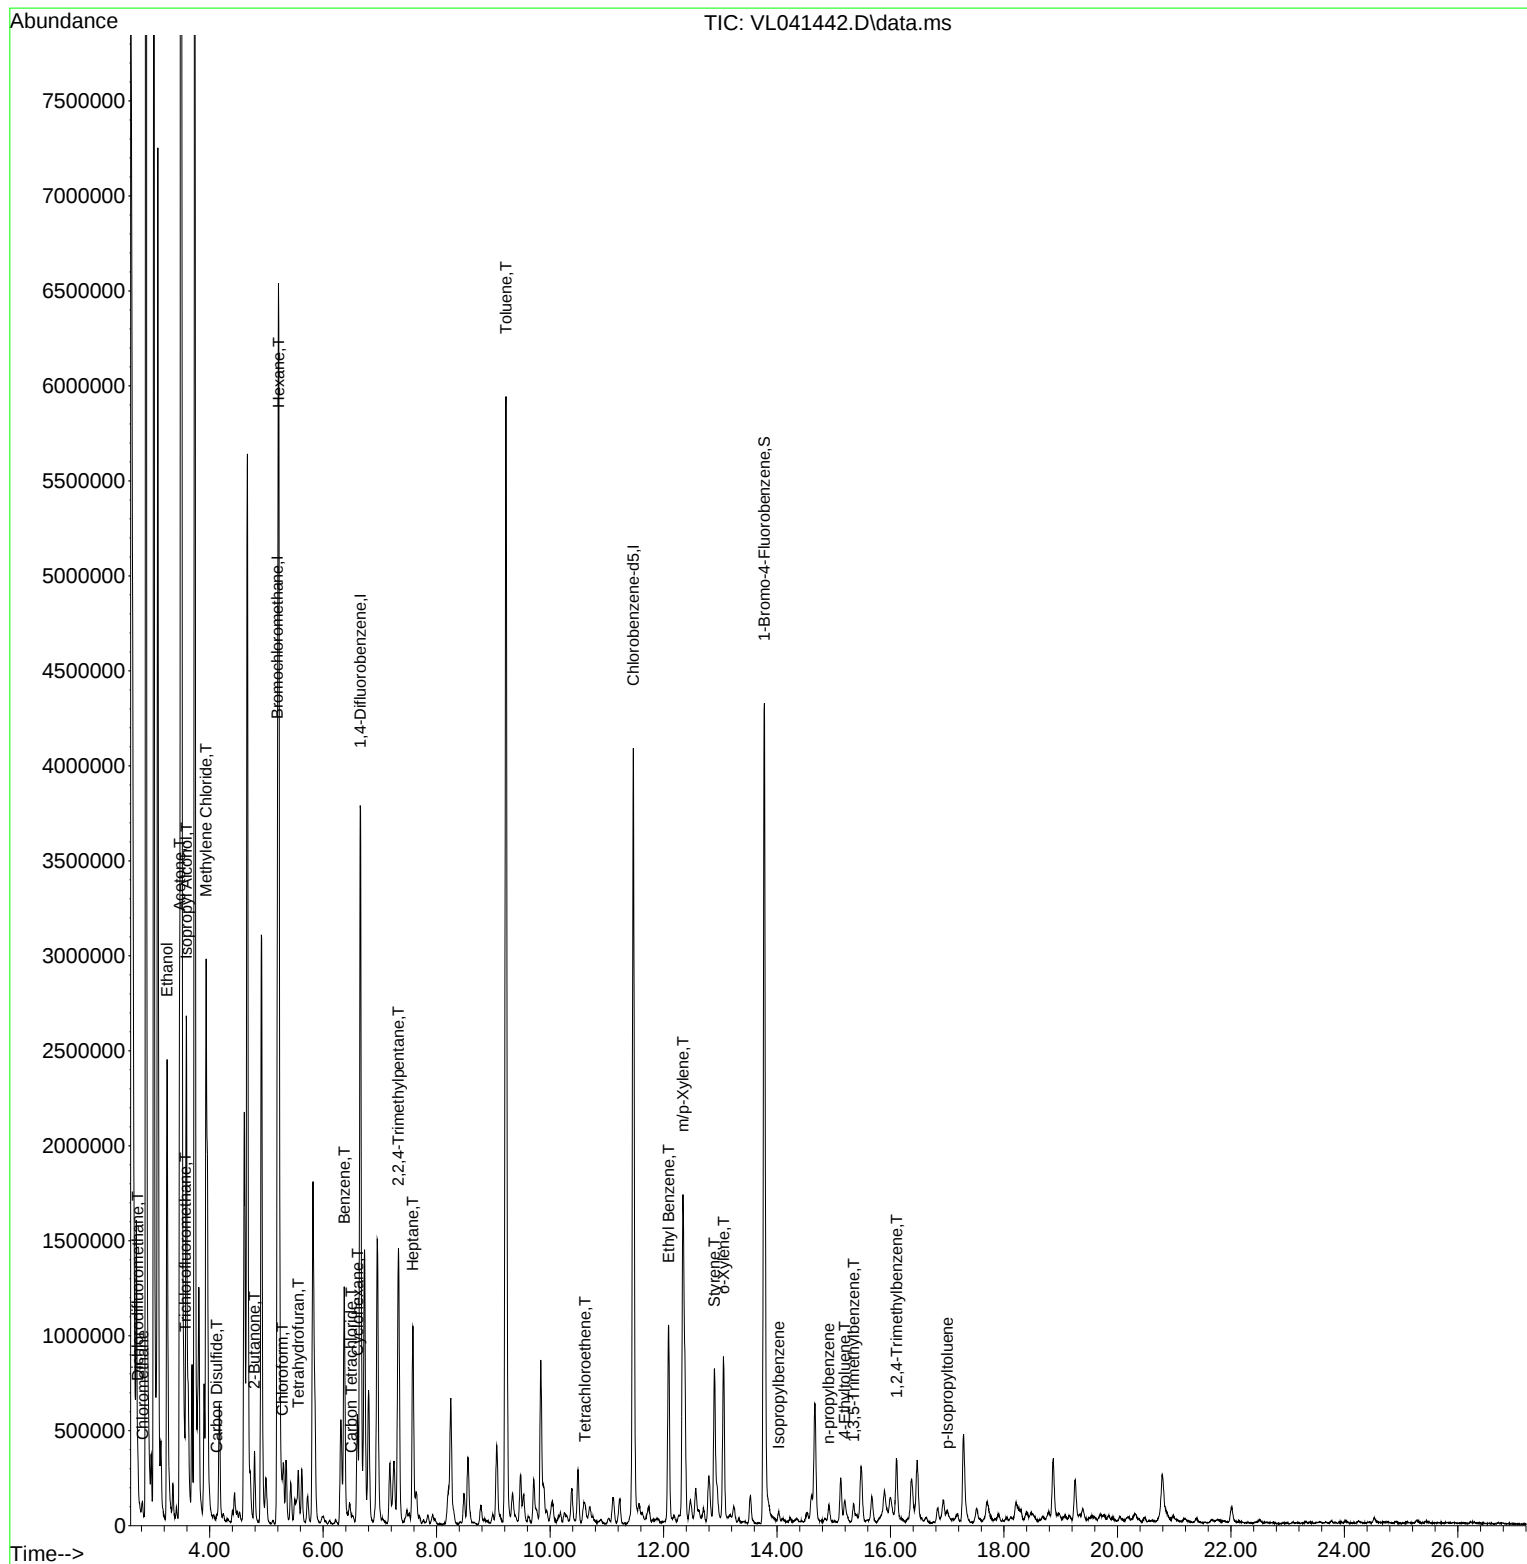







#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.195 min Scan# 80
Delta R.T. 0.016 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49

Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D

Tgt Ion: 49 Resp: 1082784
Ion Ratio Lower Upper
49 100
128 46.5 23.8 71.4
130 59.3 30.8 92.4




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

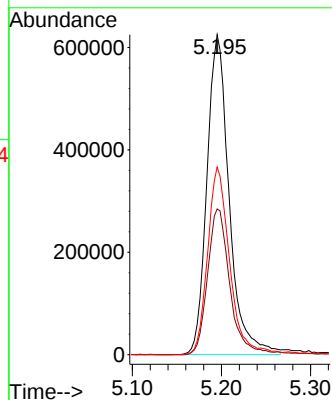

#2
Dichlorodifluoromethane
Concen: 0.567 ppbv
RT: 2.732 min Scan# 40
Delta R.T. 0.023 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion: 85 Resp: 105549
Ion Ratio Lower Upper
85 100
87 28.6 26.0 39.0

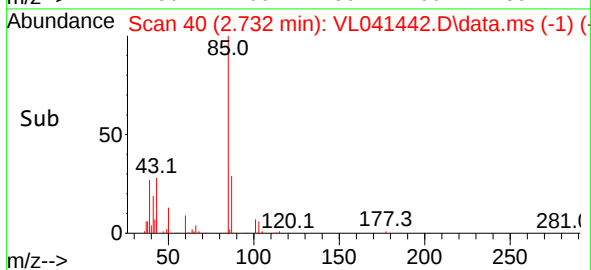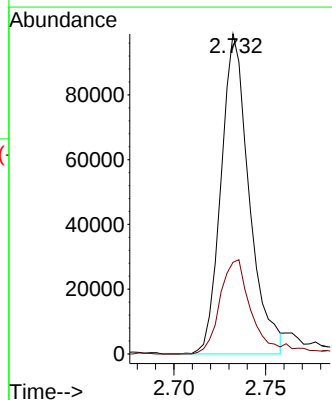

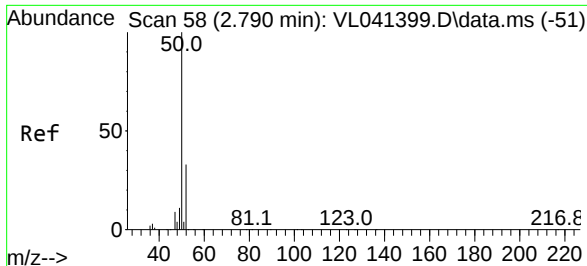

#4
Chloromethane
Concen: 0.777 ppbv
RT: 2.819 min Scan# 61
Delta R.T. 0.026 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D

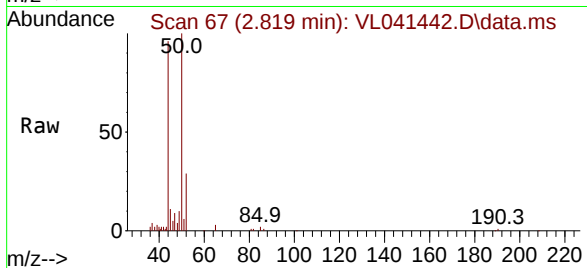

Tgt Ion: 50 Resp: 5329
Ion Ratio Lower Upper
50 100
52 29.6 26.1 39.1




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

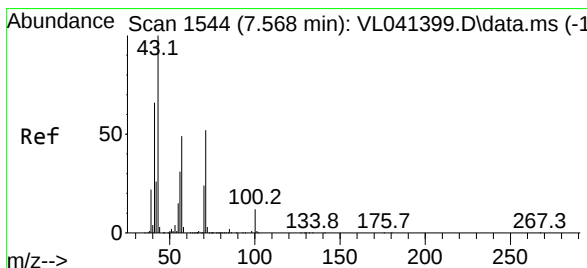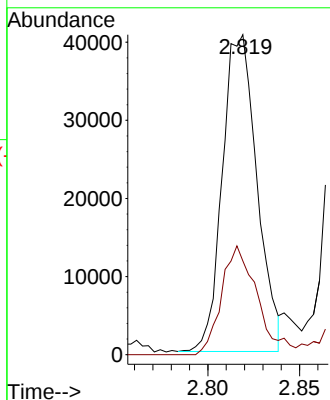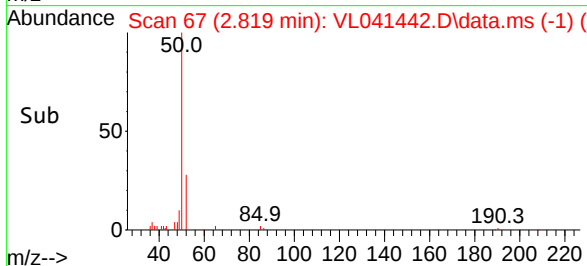

#10
Heptane
Concen: 3.406 ppbv
RT: 7.578 min Scan# 1547
Delta R.T. 0.007 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion: 43 Resp: 453144
Ion Ratio Lower Upper
43 100
57 50.1 40.5 60.7

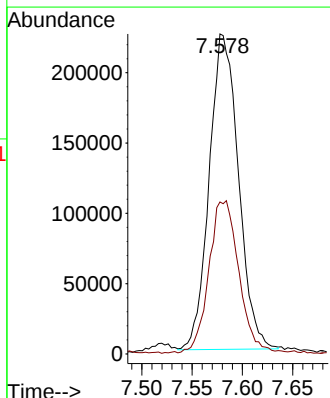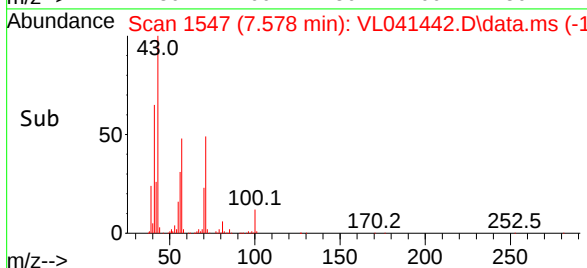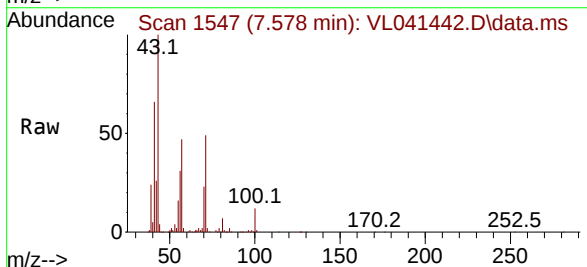



#11
Trichlorofluoromethane
Concen: 0.226 ppbv
RT: 3.571 min Scan# 301
Delta R.T. 0.026 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D



Tgt Ion:101 Resp: 3732
Ion Ratio Lower Upper
101 100
103 64.2 52.6 79.0




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

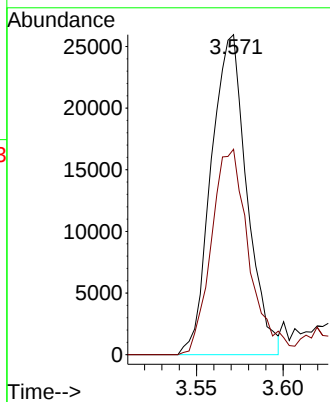

#13
Ethanol
Concen: 465.312 ppbv
RT: 3.250 min Scan# 201
Delta R.T. 0.023 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion: 45 Resp: 2462622
Ion Ratio Lower Upper
45 100
46 35.4 13.4 53.4

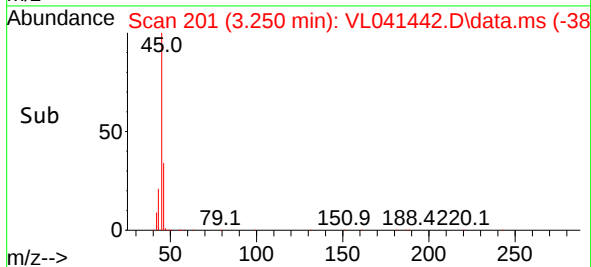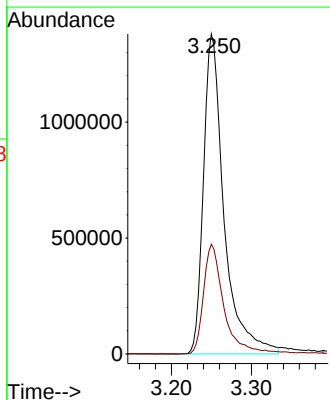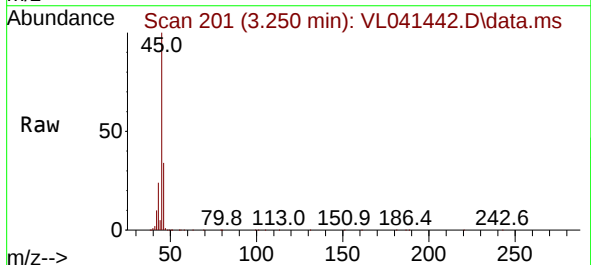



#15
Acetone
Concen: 13.068 ppbv
RT: 3.472 min Scan# 21
Delta R.T. 0.019 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D




Tgt Ion: 43 Resp: 160774
Ion Ratio Lower Upper
43 100
58 56.4 21.4 32.2

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

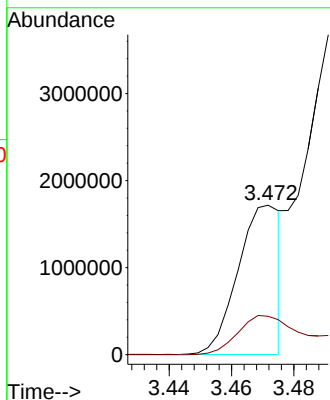


#19
Isopropyl Alcohol
Concen: 37.050 ppbv
RT: 3.591 min Scan# 307
Delta R.T. 0.029 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Tgt Ion: 45 Resp: 2664788
Ion Ratio Lower Upper
45 100
58 2.0 1.9 2.9

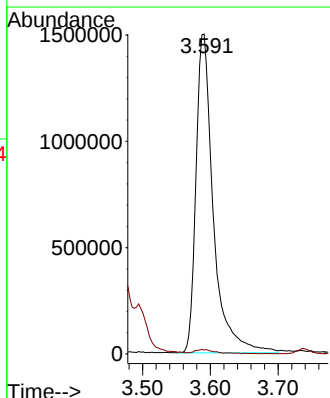



#20
Methylene Chloride
Concen: 19.816 ppbv
RT: 3.938 min Scan# 415
Delta R.T. 0.019 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D



Tgt Ion: 84 Resp: 909107
Ion Ratio Lower Upper
84 100
49 158.9 126.6 190.0
51 49.5 38.6 58.0
86 63.7 53.0 79.4




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

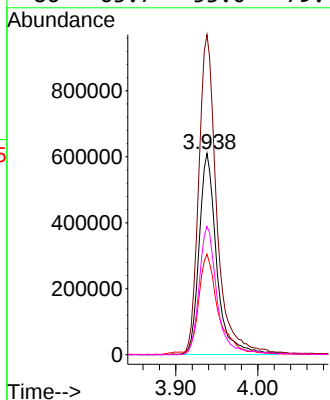

#26
Hexane
Concen: 22.491 ppbv
RT: 5.218 min Scan# 813
Delta R.T. 0.019 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion: 57 Resp: 2280287
Ion Ratio Lower Upper
57 100
41 92.3 74.0 111.0
43 106.7 193.6 290.4#
56 54.0 43.1 64.7

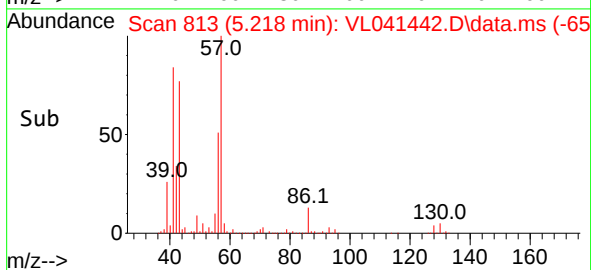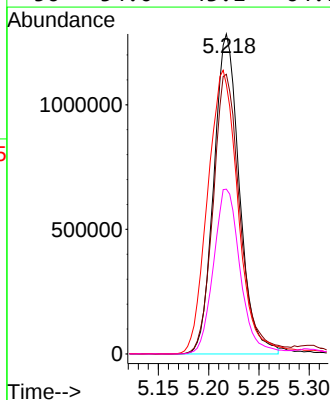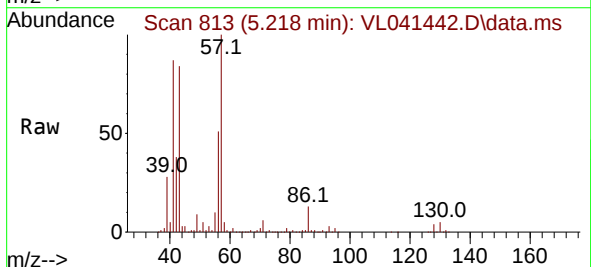



#27
Carbon Disulfide
Concen: 0.242 ppbv
RT: 4.128 min Scan# 41
Delta R.T. 0.019 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D



Tgt Ion: 76 Resp: 2875
Ion Ratio Lower Upper
76 100
44 38.9 15.6 23.4
78 14.3 7.7 11.5




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

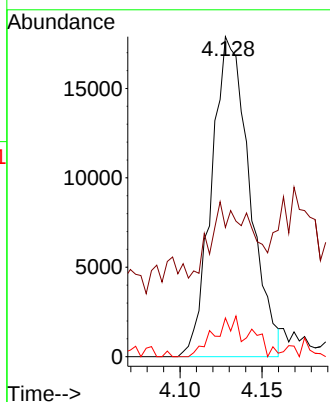

#29
Chloroform
Concen: 0.158 ppbv m
RT: 5.282 min Scan# 833
Delta R.T. 0.019 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion: 83 Resp: 26208
Ion Ratio Lower Upper
83 100
85 66.2 53.1 79.7

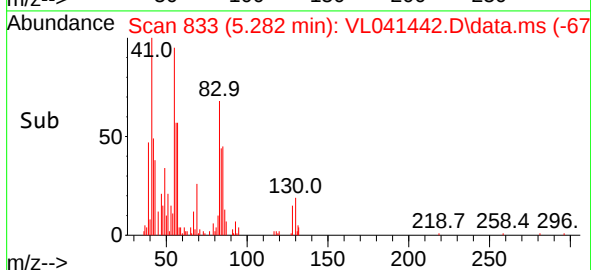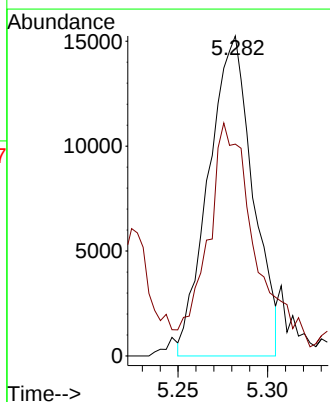



#30
Cyclohexane
Concen: 2.199 ppbv
RT: 6.607 min Scan# 1245
Delta R.T. 0.013 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D




Tgt Ion: 84 Resp: 18158
Ion Ratio Lower Upper
84 100
56 126.8 111.2 166.8
41 94.7 70.3 105.5

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

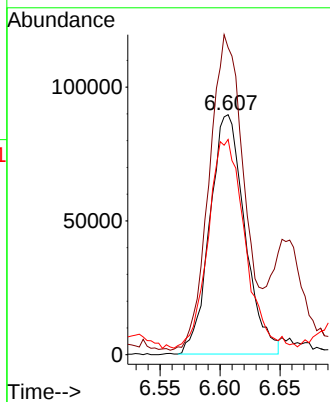


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.658 min Scan# 1261
Delta R.T. 0.013 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49

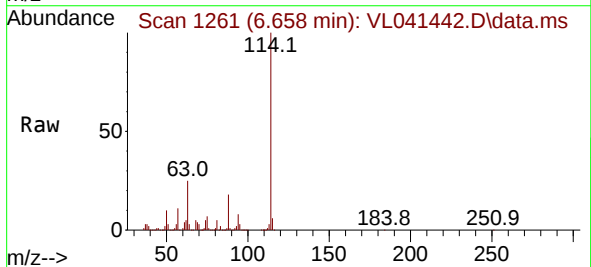


Tgt Ion:114 Resp: 2875417
Ion Ratio Lower Upper
114 100
63 25.2 20.3 30.5
88 18.0 14.3 21.5

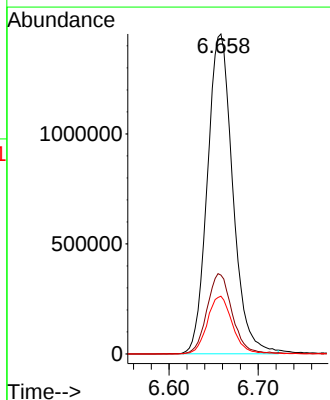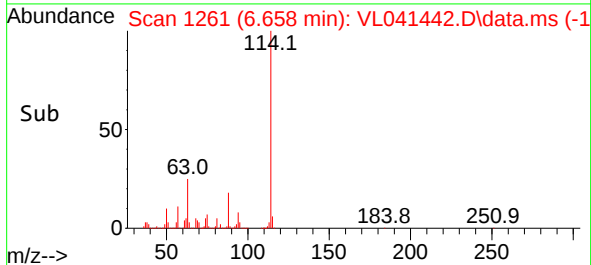



#34
2-Butanone
Concen: 2.793 ppbv
RT: 4.790 min Scan# 61
Delta R.T. 0.016 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D



Tgt Ion: 43 Resp: 388530
Ion Ratio Lower Upper
43 100
72 23.8 17.3 25.9




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

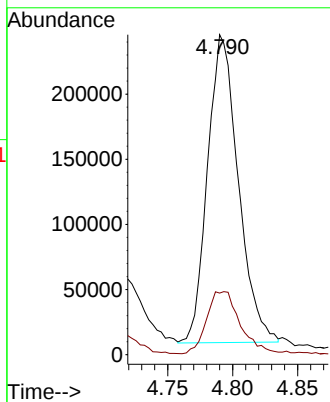

#35
Carbon Tetrachloride
Concen: 0.060 ppbv m
RT: 6.494 min Scan# 1210
Delta R.T. 0.010 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion:117 Resp: 9492
Ion Ratio Lower Upper
117 100
119 96.9 76.6 115.0
121 25.5 25.1 37.7

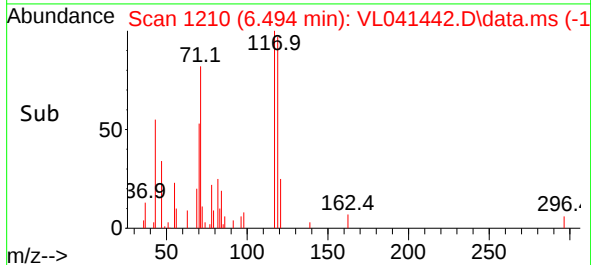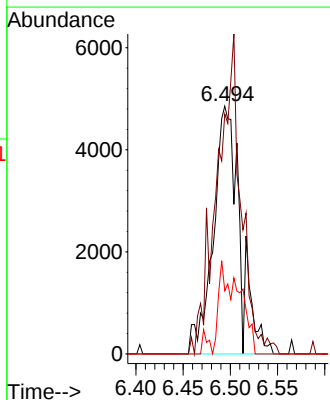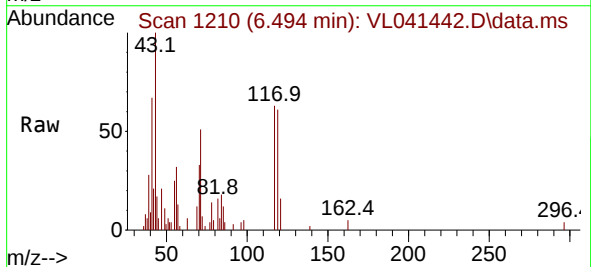



#36
Benzene
Concen: 4.664 ppbv
RT: 6.372 min Scan# 1168
Delta R.T. 0.013 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D




Tgt Ion: 78 Resp: 98001
Ion Ratio Lower Upper
78 100
77 23.5 18.1 27.1
50 20.3 15.5 23.3

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

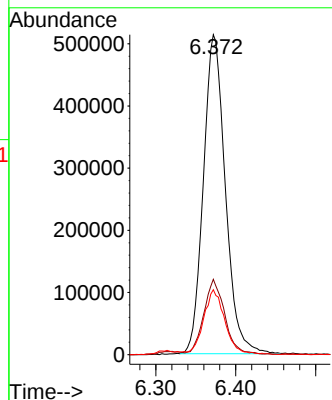


#41
Tetrahydrofuran
Concen: 1.600 ppbv
RT: 5.562 min Scan# 920
Delta R.T. 0.016 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Tgt Ion: 42 Resp: 127295
Ion Ratio Lower Upper
42 100
72 45.8 31.2 46.8
71 40.0 30.5 45.7

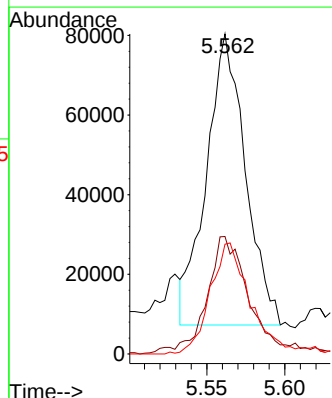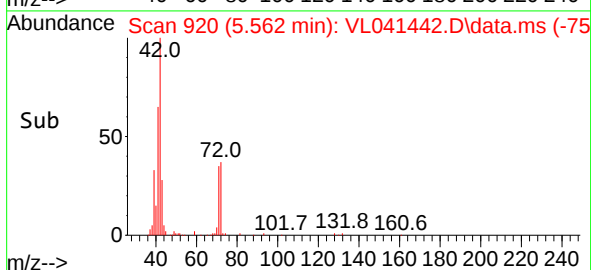

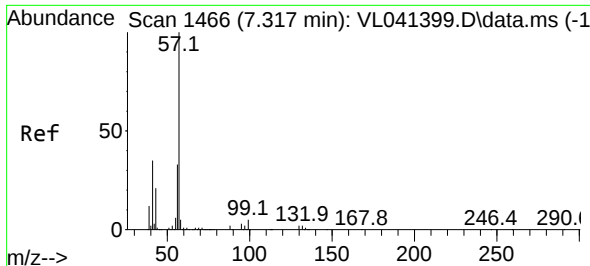

#44
2,2,4-Trimethylpentane
Concen: 3.448 ppbv
RT: 7.327 min Scan# 1466
Delta R.T. 0.010 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D



Tgt Ion: 57 Resp: 121010
Ion Ratio Lower Upper
57 100
41 41.3 27.0 40.6
56 40.8 25.2 37.8




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

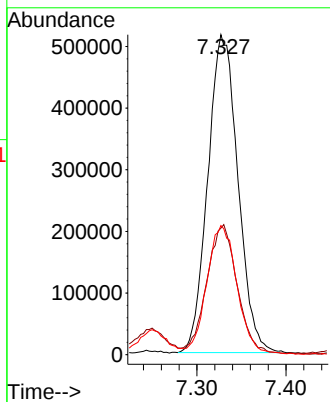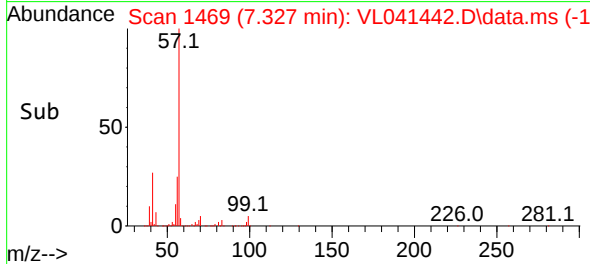

#52
Tetrachloroethene
Concen: 0.158 ppbv m
RT: 10.616 min Scan# 2492
Delta R.T. 0.007 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion:164 Resp: 12861
Ion Ratio Lower Upper
164 100
166 119.8 101.1 151.7
129 81.1 81.7 122.5#
131 92.9 76.2 114.4

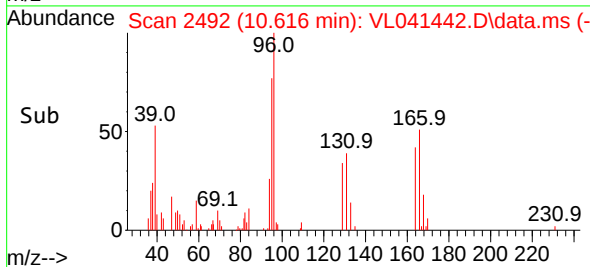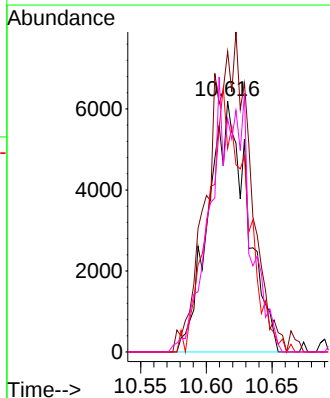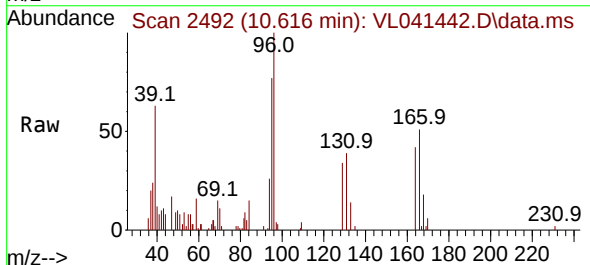



#53
Toluene
Concen: 19.970 ppbv
RT: 9.224 min Scan# 2056
Delta R.T. 0.007 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D




Tgt Ion: 91 Resp: 467365
Ion Ratio Lower Upper
91 100
92 61.8 48.7 73.1

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

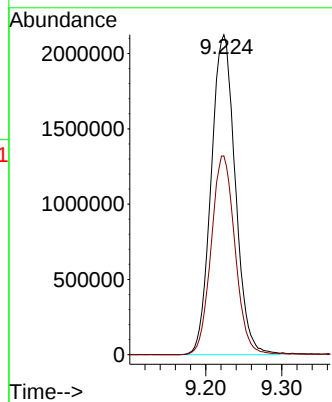


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.468 min Scan# 2757
Delta R.T. 0.003 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49

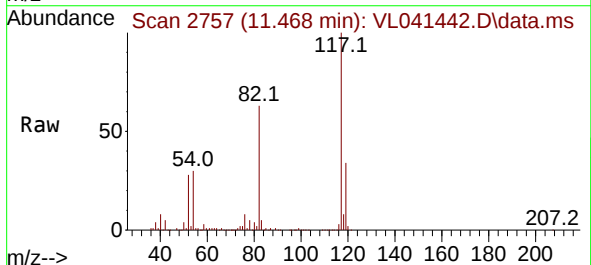

Tgt Ion:117 Resp: 2694025
Ion Ratio Lower Upper
117 100
82 62.7 51.0 76.6
119 32.8 45.2 67.8#

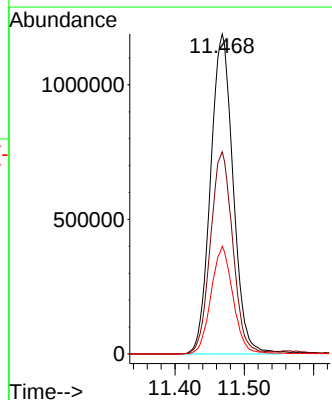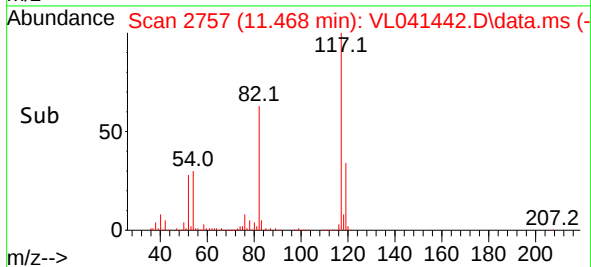







#58
Ethyl Benzene
Concen: 3.042 ppbv
RT: 12.089 min Scan# 2949
Delta R.T. 0.003 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49

Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D

Tgt Ion: 91 Resp: 944509
Ion Ratio Lower Upper
91 100
106 32.1 25.8 38.8




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

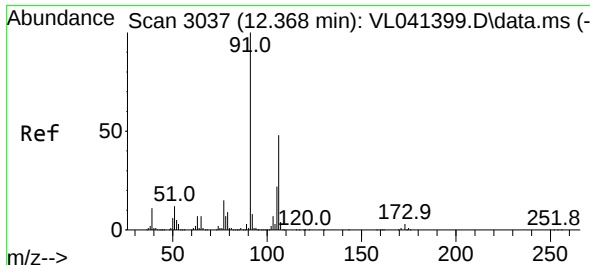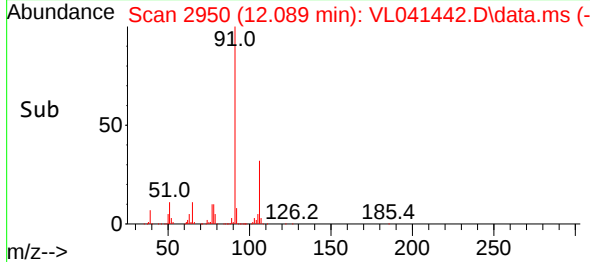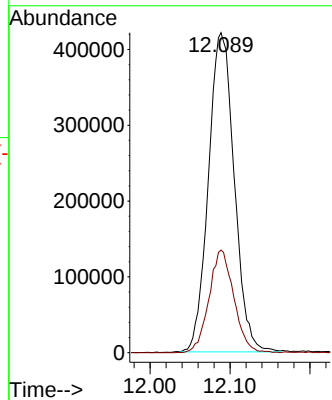

#59
m/p-Xylene
Concen: 6.787 ppbv
RT: 12.343 min Scan# 3029
Delta R.T. -0.026 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49

Tgt Ion: 91 Resp: 1819188
Ion Ratio Lower Upper
91 100
106 47.4 36.3 54.5

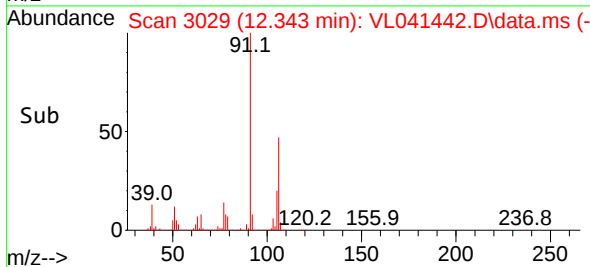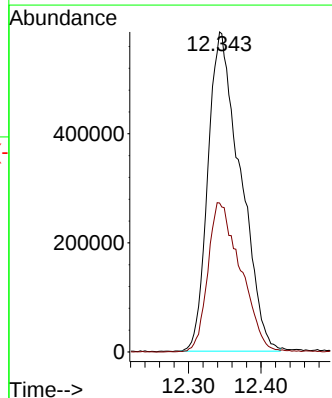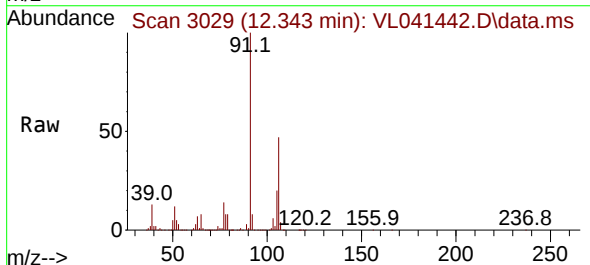







#60
o-Xylene
Concen: 2.664 ppbv
RT: 13.057 min Scan# 3250
Delta R.T. 0.000 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49

Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D

Tgt Ion: 91 Resp: 675630
Ion Ratio Lower Upper
91 100
106 45.6 23.1 69.3




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

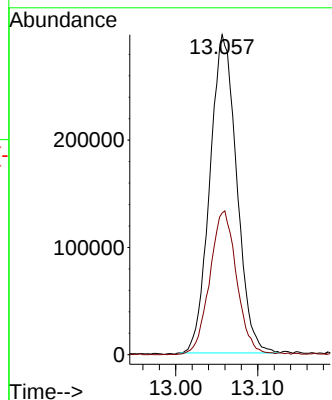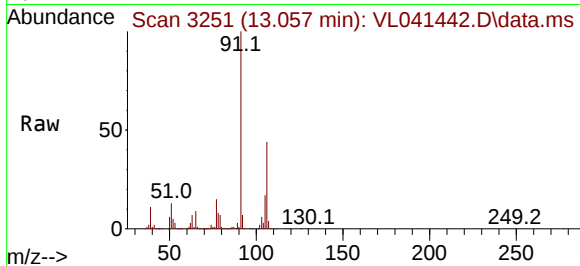

#61
Styrene
Concen: 4.273 ppbv
RT: 12.896 min Scan# 3201
Delta R.T. 0.000 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion:104 Resp: 488871
Ion Ratio Lower Upper
104 100
78 51.7 40.8 61.2
103 47.5 38.2 57.4

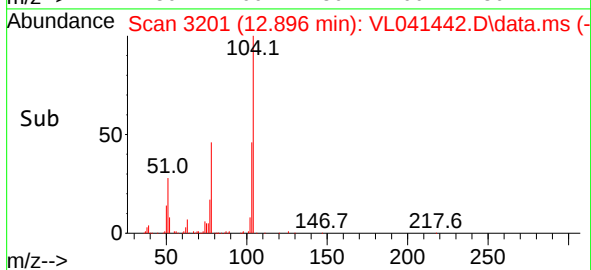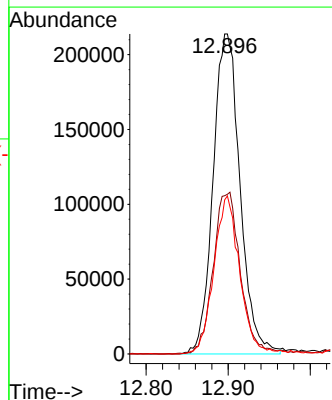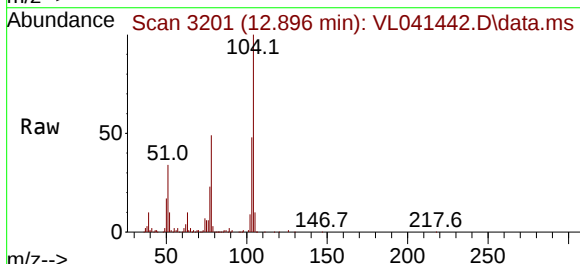

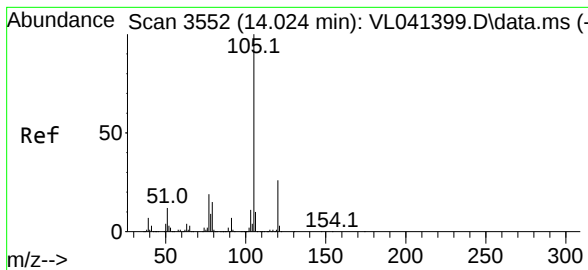

#62
Isopropylbenzene
Concen: 0.117 ppbv m
RT: 14.031 min Scan# 3554
Delta R.T. 0.003 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D

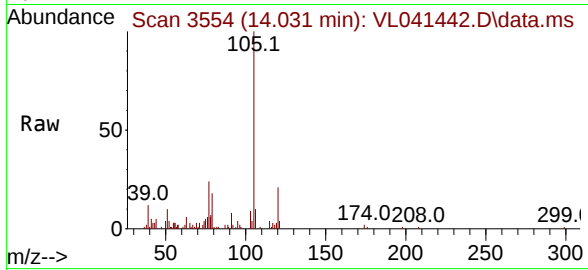


Tgt Ion:105 Resp: 45270
Ion Ratio Lower Upper
105 100
120 25.9 21.0 31.4

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

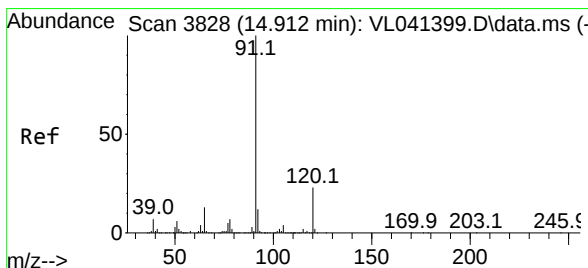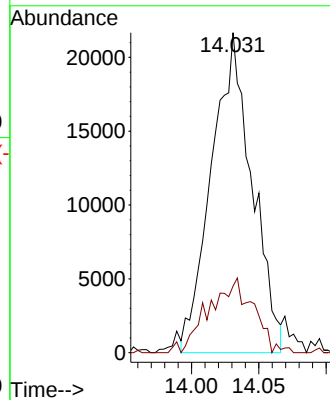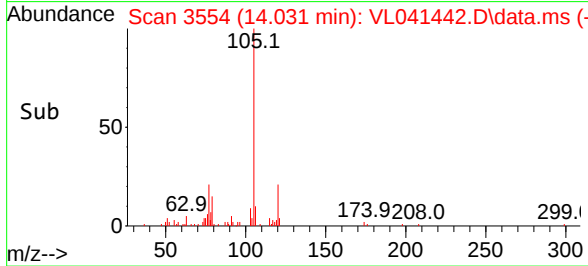


#64
n-propylbenzene
Concen: 0.177 ppbv m
RT: 14.912 min Scan# 3828
Delta R.T. -0.003 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49

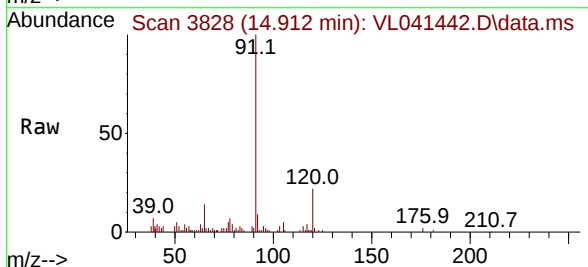


Tgt Ion:120 Resp: 17809
Ion Ratio Lower Upper
120 100
91 490.2 361.4 542.0

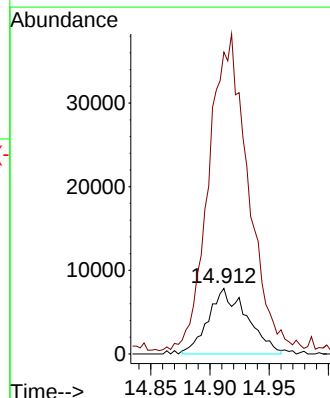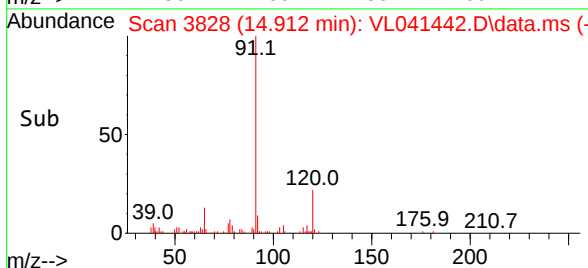



#68
1-Bromo-4-Fluorobenzene
Concen: 10.247 ppbv
RT: 13.777 min Scan# 3475
Delta R.T. 0.003 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D



Tgt Ion: 95 Resp: 2124478
Ion Ratio Lower Upper
95 100
174 69.6 56.3 84.5
175 5.2 4.0 6.0




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

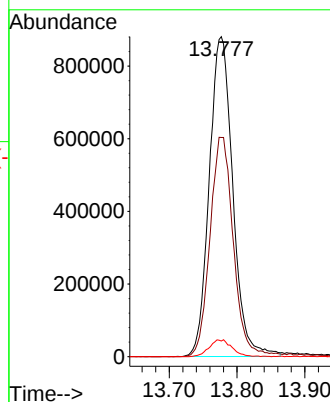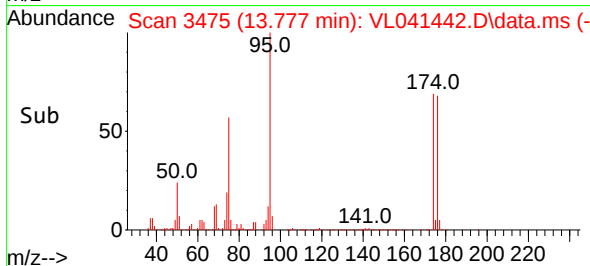

#69
p-Isopropyltoluene
Concen: 0.086 ppbv m
RT: 16.999 min Scan# 4477
Delta R.T. 0.003 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49


Tgt Ion:119 Resp: 34322
Ion Ratio Lower Upper
119 100
134 28.3 20.5 30.7
91 36.8 23.2 34.8#

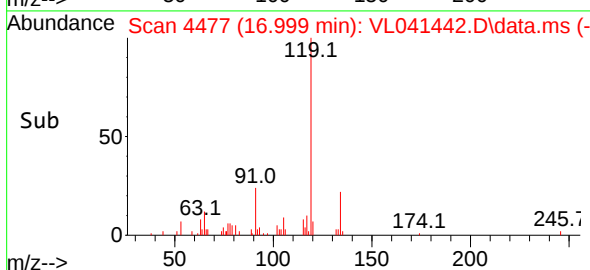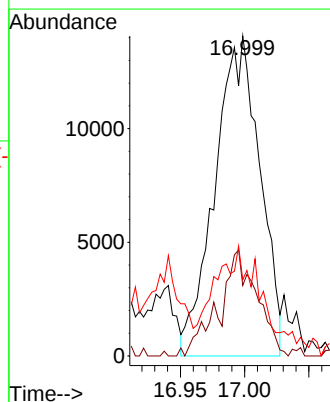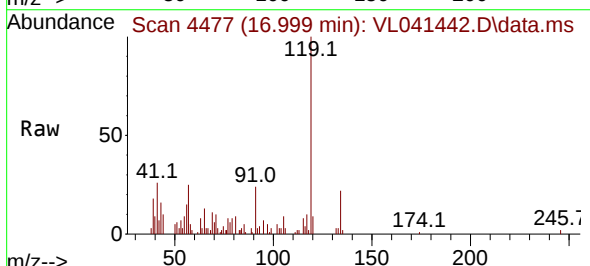



#72
4-Ethyltoluene
Concen: 0.310 ppbv m
RT: 15.195 min Scan# 3916
Delta R.T. 0.003 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49




Instrument :
MSVOA_L
ClientSampleId :
ACVI-IA-03D




Tgt Ion:105 Resp: 92609
Ion Ratio Lower Upper
105 100
120 29.3 24.2 36.2
91 14.3 10.4 15.6
77 14.1 11.0 16.4

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

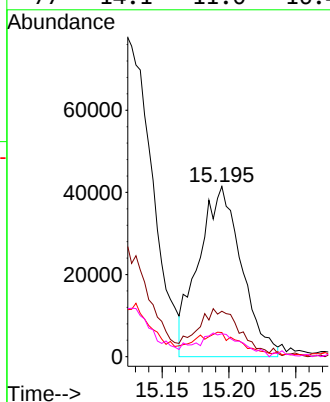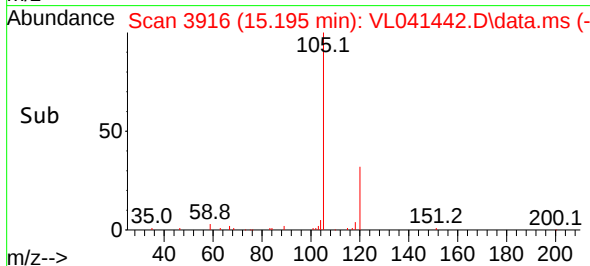


#73
1,3,5-Trimethylbenzene
Concen: 0.249 ppbv m
RT: 15.349 min Scan# 3964
Delta R.T. 0.000 min
Lab File: VL041442.D
Acq: 29 Jul 2024 23:49

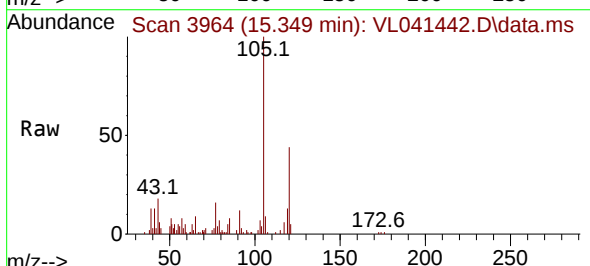


Tgt Ion:105 Resp: 64146
Ion Ratio Lower Upper
105 100
120 44.5 38.6 57.8

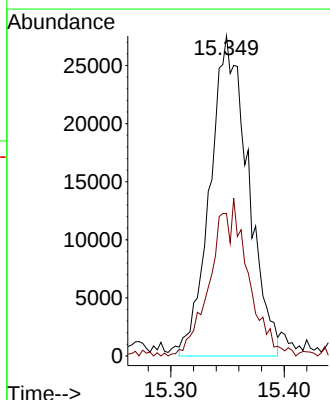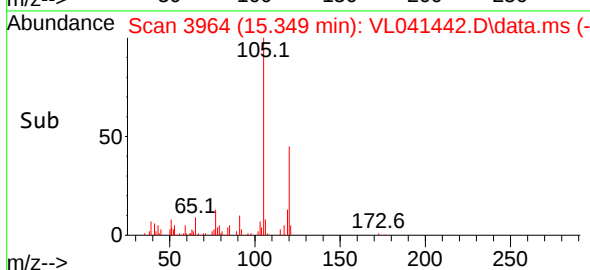

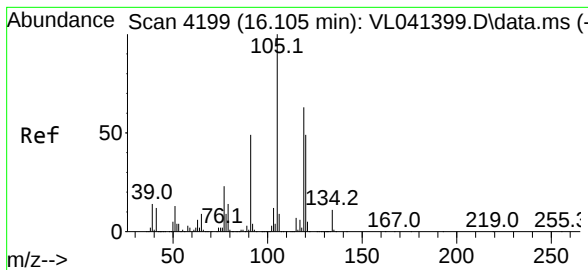

#74
 1,2,4-Trimethylbenzene
 Concen: 0.863 ppbv
 RT: 16.108 min Scan# 4199
 Delta R.T. 0.000 min
 Lab File: VL041442.D
 Acq: 29 Jul 2024 23:49

Instrument :
 MSVOA_L
 ClientSampleId :
 ACVI-IA-03D

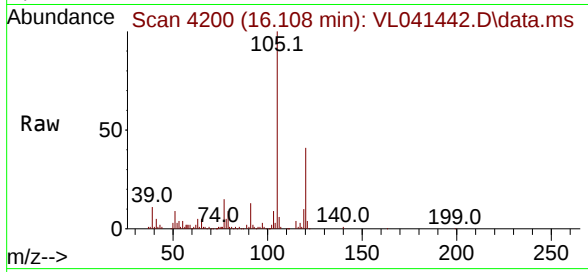

Tgt Ion:	105	Resp:	25790
Ion	Ratio	Lower	Upper
105	100		
120	40.9	39.5	59.3
91	12.4	39.8	59.8
77	14.6	18.2	27.4

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

