
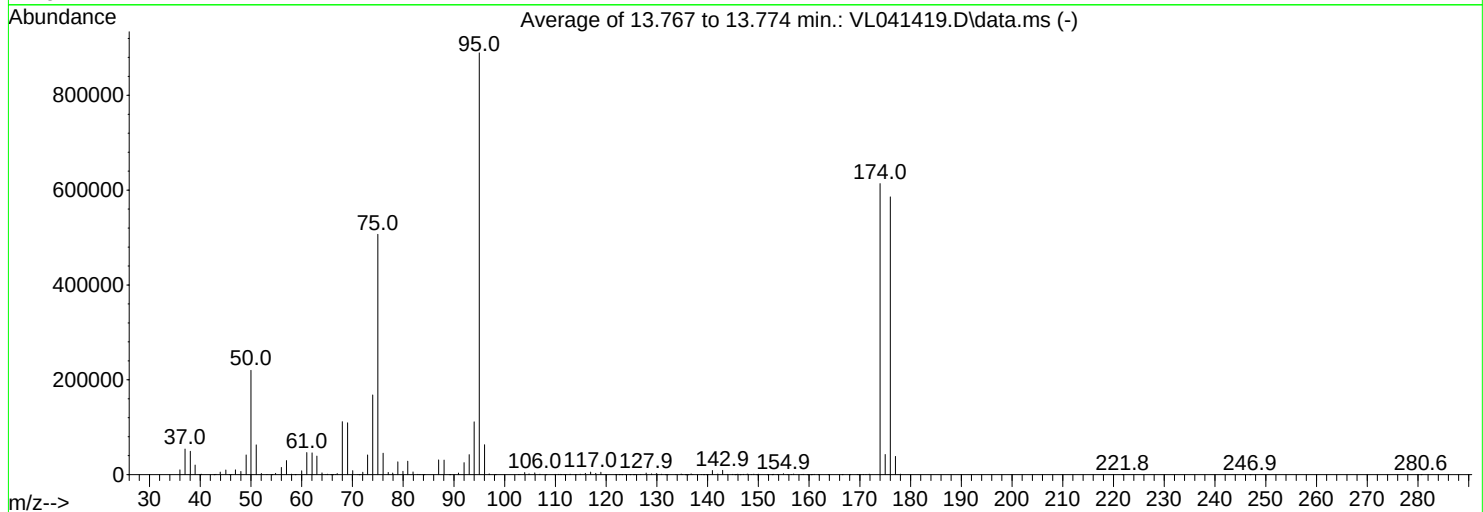


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072924\
Data File : VL041419.D
Acq On : 29 Jul 2024 7:38
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jul 30 02:42:20 2024

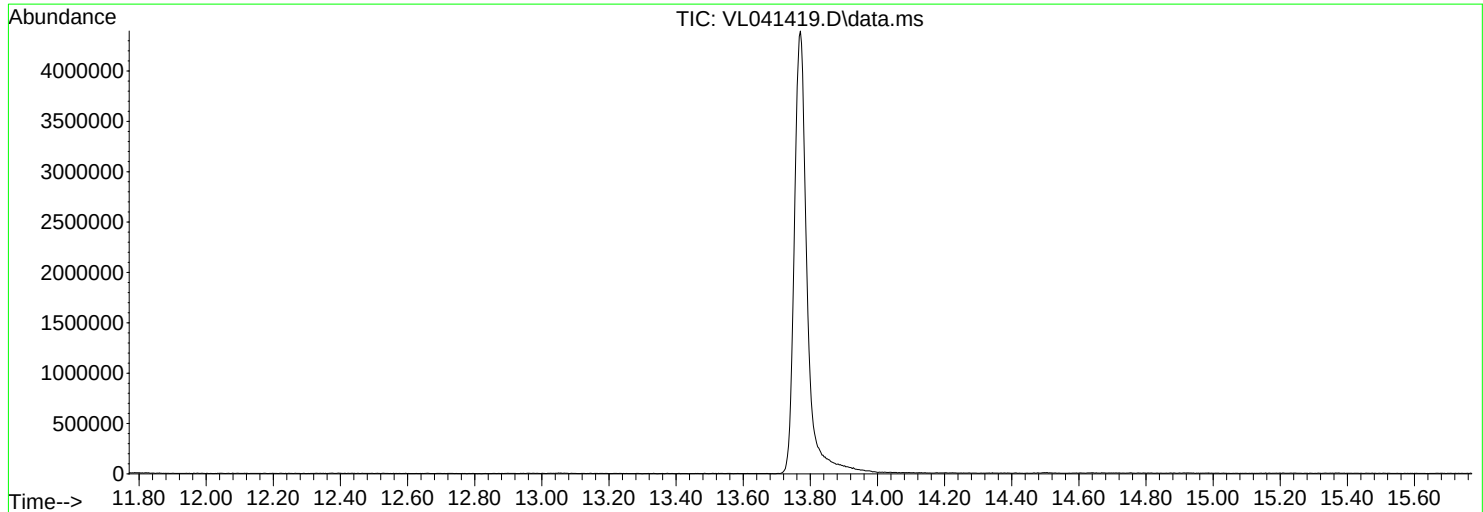

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.7	220053	PASS
75	95	30	66	57.0	506709	PASS
95	95	100	100	100.0	889557	PASS
96	95	5	9	7.1	63101	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.0	613909	PASS
175	174	4	9	7.0	42677	PASS
176	174	93	101	95.4	585728	PASS
177	176	5	9	6.6	38629	PASS

Average of 13.767 to 13.774 min.: VL041419.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	10042	46.10	391	57.00	29568	66.10	91
37.00	53971	46.95	10268	58.00	1163	66.70	51
38.05	49413	48.00	6924	58.70	82	67.00	248
39.00	20436	49.05	41421	60.00	8042	68.00	11171
39.90	113	50.00	220053	61.00	46440	69.05	109397
40.20	960	51.05	62859	62.05	46072	70.05	8294
42.70	178	52.05	2508	63.00	39016	71.05	194
43.10	624	53.15	251	64.00	3744	71.30	98
43.95	5565	54.10	143	64.80	267	72.05	5175
45.05	9778	54.85	2850	65.10	977	73.00	41571
45.80	199	56.00	15329	65.75	186	74.00	168021

Average of 13.767 to 13.774 min.: VL041419.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	506709	84.10	115	98.15	164	111.20	225
76.05	45163	87.00	30955	102.75	285	111.70	239
77.05	4668	88.05	30560	103.00	268	111.90	462
77.95	3444	89.15	140	103.95	4430	112.10	339
78.95	26917	90.90	3299	104.80	1565	112.90	867
79.95	6999	92.00	25315	105.95	3849	113.90	107
80.90	28365	93.00	42232	106.95	970	114.90	938
81.95	5664	94.00	111496	108.10	53	115.90	2870
82.90	823	95.00	889557	109.95	644	116.95	5376
83.30	255	96.05	63101	110.65	579	117.95	2849
83.90	99	96.95	1723	110.95	673	118.95	5140

Average of 13.767 to 13.774 min.: VL041419.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.80	218	129.90	2290	136.75	1544	145.40	164
121.90	127	130.10	896	137.10	306	145.70	397
122.60	68	130.95	1209	138.75	202	145.95	931
123.10	115	131.70	60	139.20	132	146.40	100
123.80	456	132.00	67	139.80	148	147.05	632
124.70	84	133.75	336	140.05	444	147.80	1317
125.40	72	134.80	1245	140.95	8663	148.00	747
125.85	518	135.00	519	142.00	1464	148.60	194
126.80	303	135.60	66	142.95	9102	149.10	932
127.90	3463	135.80	140	143.95	699	149.70	97
128.95	1562	136.10	111	144.90	596	150.00	873

Average of 13.767 to 13.774 min.: VL041419.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
151.80	128	158.95	672	170.05	376	280.60	65
152.00	429	159.70	108	170.70	276		
152.70	160	160.40	94	171.20	464		
152.95	612	160.70	268	171.85	1148		
153.75	454	161.00	601	174.00	613909		
154.95	1993	161.80	56	175.00	42677		
155.70	203	163.80	67	176.00	585728		
155.90	268	166.50	74	177.00	38629		
156.50	248	168.00	154	178.05	1105		
156.95	1431	169.50	304	221.80	71		
158.60	308	169.80	53	246.90	139		