
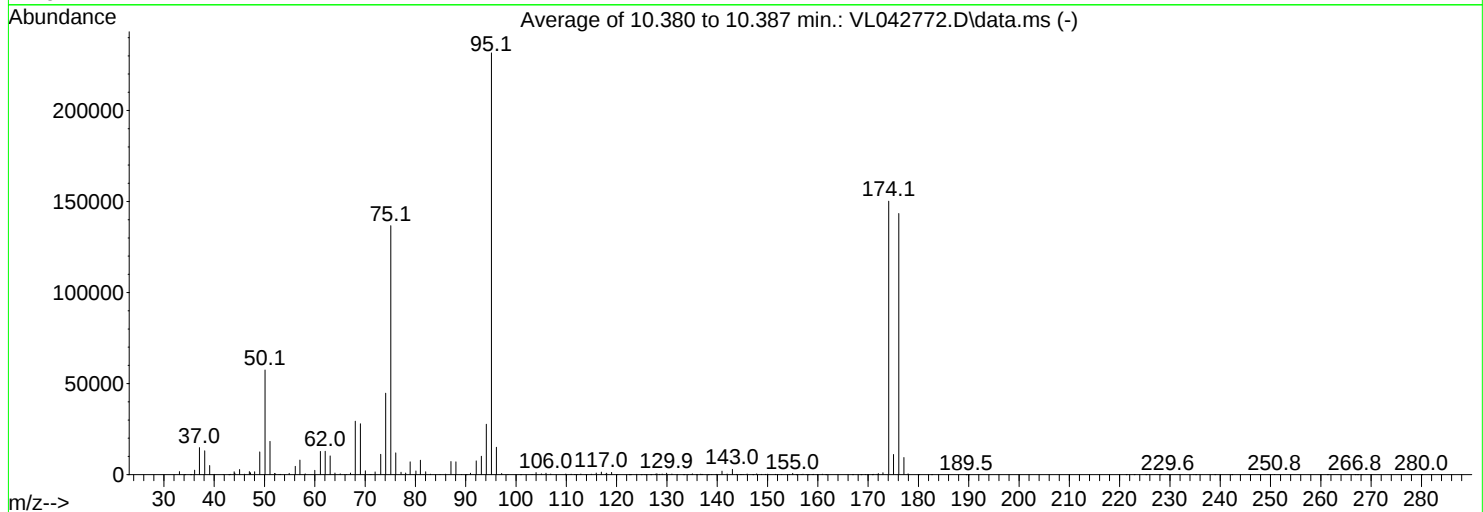


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072925\
Data File : VL042772.D
Acq On : 29 Jul 2025 07:37
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jul 24 05:24:41 2025

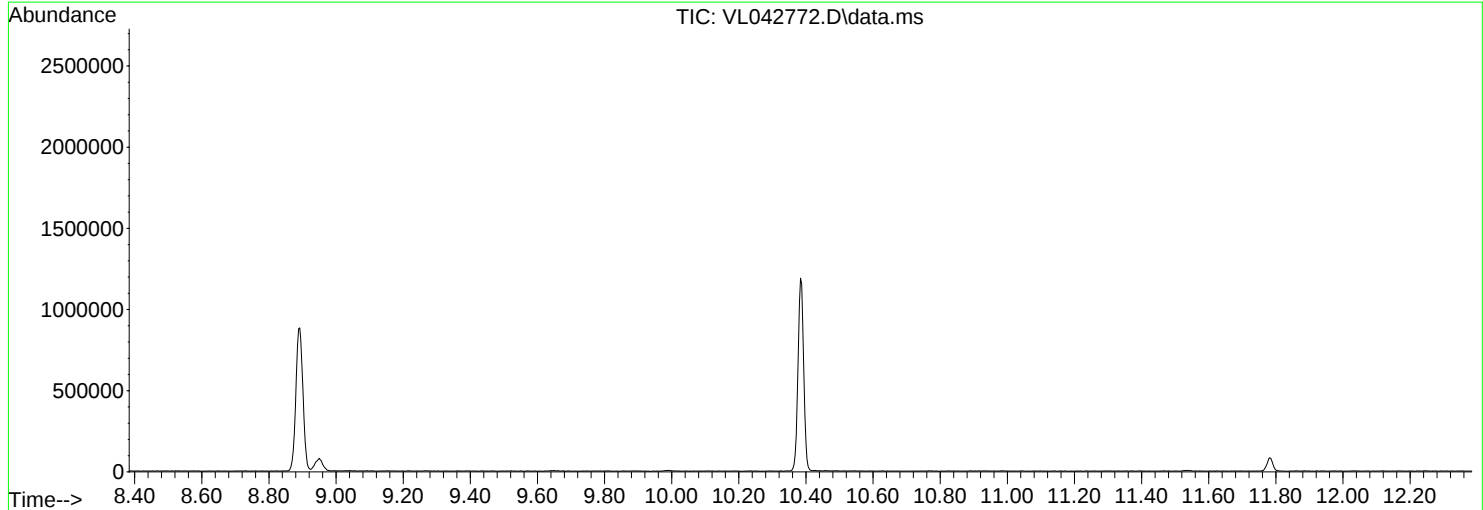

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	57437	PASS
75	95	30	66	59.0	136723	PASS
95	95	100	100	100.0	231659	PASS
96	95	5	9	6.5	15049	PASS
173	174	0.00	2	0.7	1083	PASS
174	95	50	120	64.8	150165	PASS
175	174	4	9	7.4	11110	PASS
176	174	93	101	95.5	143419	PASS
177	176	5	9	6.5	9388	PASS

Average of 10.380 to 10.387 min.: VL042772.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1698	43.95	1598	52.20	473	64.00	85
34.10	34	44.10	843	52.90	91	65.05	42
35.30	42	45.05	2802	53.20	182	65.95	12
36.10	2492	46.05	267	54.90	738	66.30	5
37.05	14881	47.00	1640	56.10	4541	67.10	896
38.10	13066	47.20	1067	57.05	8003	68.05	29365
39.10	5020	48.05	1559	58.10	407	69.05	27941
40.00	185	49.05	12441	60.00	2377	70.05	2074
41.80	82	50.10	57437	61.10	12758	71.00	104
42.90	20	51.10	18251	62.05	12840	71.20	63
43.20	155	52.00	689	63.05	10324	72.00	1464

Average of 10.380 to 10.387 min.: VL042772.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.10	11121	84.90	73	96.10	15049	111.65	116
74.10	44709	86.00	283	97.15	641	111.90	134
75.10	136723	87.05	7186	98.40	54	112.15	114
76.10	11943	88.05	7066	100.90	18	112.90	344
77.15	1295	89.15	50	103.20	81	113.90	22
78.05	848	90.10	18	104.00	1181	114.95	296
78.95	7013	90.95	828	105.05	452	115.95	889
80.10	1995	92.10	7551	105.95	806	116.95	1369
81.00	7928	93.10	10114	106.90	393	117.80	292
82.05	1622	94.10	27651	109.90	343	118.00	782
83.00	241	95.10	231659	110.95	294	119.00	1229

Average of 10.380 to 10.387 min.: VL042772.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
120.10	105	129.05	348	137.10	144	145.95	322
122.50	29	129.95	778	138.20	18	147.10	39
122.75	39	131.00	346	138.90	105	147.85	437
123.95	196	132.10	72	139.80	200	148.80	168
124.90	46	133.30	24	140.95	1972	149.60	143
125.50	114	134.25	80	141.95	385	150.05	247
125.80	22	134.80	137	143.00	2934	151.60	172
126.80	46	135.05	406	143.80	188	152.00	103
127.70	280	135.90	22	144.60	130	152.80	115
128.00	551	136.65	245	144.85	102	154.00	88
128.50	140	136.90	157	145.15	50	154.30	70

Average of 10.380 to 10.387 min.: VL042772.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.00	672	161.60	40	175.05	11110	228.10	24
155.70	29	166.90	42	176.10	143419	229.60	77
156.00	133	168.60	20	177.10	9388	234.75	66
156.70	92	169.45	64	177.95	468	235.10	41
157.05	299	169.90	45	180.00	27	238.90	18
157.80	55	170.80	33	182.60	22	242.30	22
158.10	31	171.00	219	189.50	33	250.80	48
158.90	72	171.80	279	189.90	26	261.30	25
159.15	223	172.05	536	221.30	21	266.80	46
159.95	88	172.95	1083	222.90	21	267.30	17
160.90	280	174.10	150165	225.20	21	268.00	43

Average of 10.380 to 10.387 min.: VL042772.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
280.00	22						