
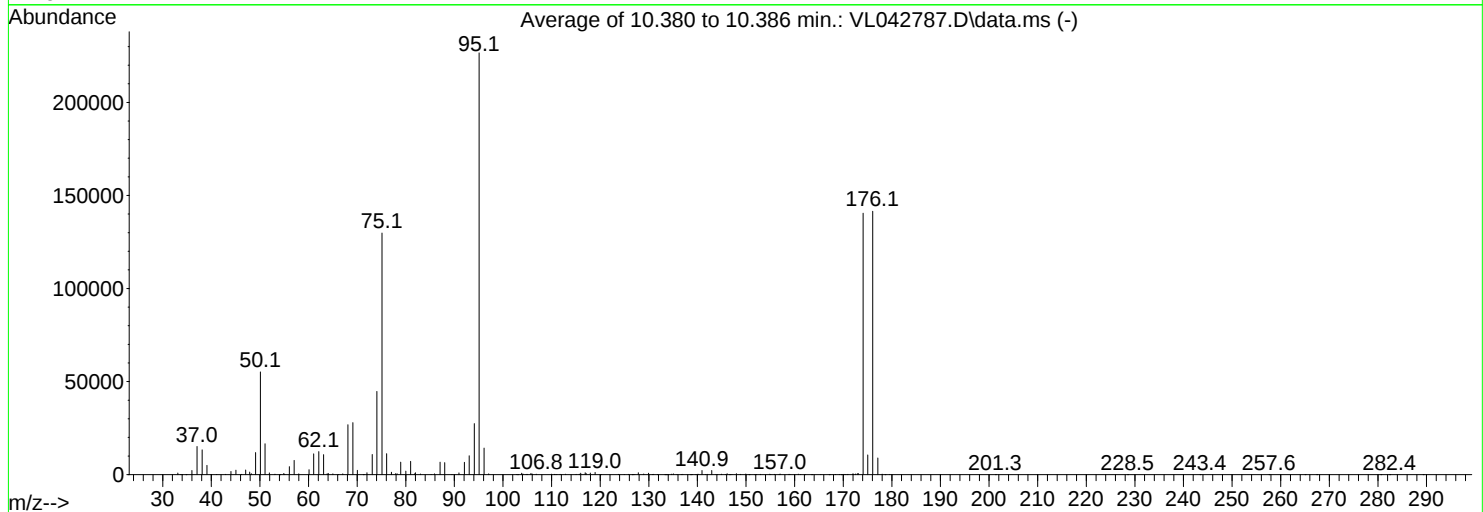


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL073125\
Data File : VL042787.D
Acq On : 31 Jul 2025 07:46
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jul 24 05:24:41 2025

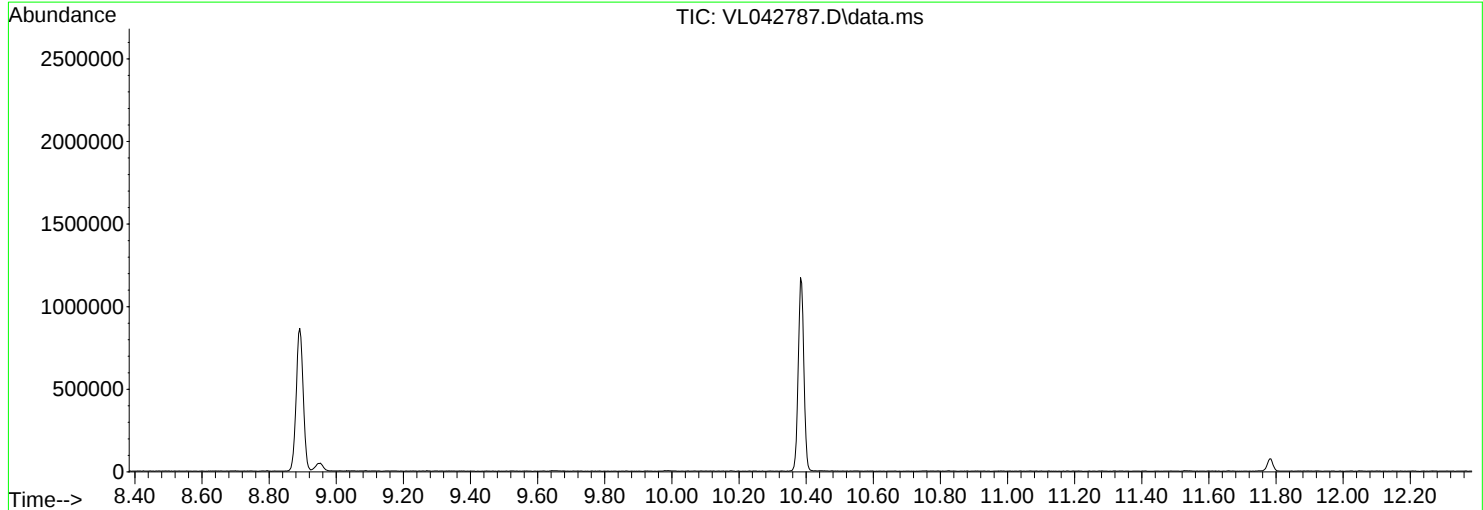

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	55155	PASS
75	95	30	66	57.3	129853	PASS
95	95	100	100	100.0	226624	PASS
96	95	5	9	6.3	14293	PASS
173	174	0.00	2	0.4	628	PASS
174	95	50	120	62.0	140456	PASS
175	174	4	9	7.5	10600	PASS
176	174	93	101	100.7	141471	PASS
177	176	5	9	6.3	8945	PASS

Average of 10.380 to 10.386 min.: VL042787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	840	44.05	1737	54.10	32	64.05	661
33.70	82	45.05	2380	54.90	569	65.00	421
33.90	20	46.20	183	55.10	277	66.20	8
34.80	25	47.05	2469	56.05	4284	67.05	47
36.00	2245	47.90	1340	57.05	7620	68.10	26797
37.05	15155	48.20	519	58.00	474	69.10	27928
38.10	13295	49.10	11853	60.10	2632	70.05	2302
39.10	4999	50.10	55155	61.05	11169	71.25	36
40.00	104	51.05	16620	62.10	12394	72.00	1064
41.10	61	51.95	914	63.10	10755	73.10	10825
42.95	160	53.10	259	63.80	408	74.05	44701

Average of 10.380 to 10.386 min.: VL042787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	129853	85.20	133	97.05	460	110.60	148
76.05	11227	85.90	445	102.75	48	110.90	106
77.05	1320	87.05	6685	103.00	25	111.10	52
77.90	541	88.00	6414	103.85	756	111.75	176
78.20	519	89.50	69	104.10	317	112.90	226
78.95	6707	90.95	974	104.75	201	115.05	162
80.00	1865	92.05	6661	105.00	207	115.70	250
81.00	7111	93.05	10144	105.75	689	116.00	803
81.80	467	94.10	27440	106.00	362	116.90	1068
82.00	1071	95.10	226624	106.85	251	117.10	608
83.05	343	96.10	14293	110.00	269	117.95	825

Average of 10.380 to 10.386 min.: VL042787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	1199	130.75	101	138.60	17	145.80	50
120.00	47	131.00	162	138.95	103	146.10	508
123.75	159	131.80	82	139.70	53	146.60	19
124.95	57	133.30	29	140.10	281	147.10	52
125.85	151	133.60	42	140.95	2233	148.00	500
126.60	23	133.90	22	141.70	80	148.85	152
126.80	61	134.70	276	142.05	220	149.95	349
127.10	59	135.05	418	142.95	2212	150.60	19
127.85	1068	135.80	55	143.80	93	151.80	20
128.95	350	136.70	127	144.10	134	152.15	99
129.95	755	137.00	201	144.95	251	152.95	158

Average of 10.380 to 10.386 min.: VL042787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.90	285	163.50	26	172.10	355	201.30	21
155.10	125	165.40	66	172.50	358	228.50	30
155.85	138	167.10	31	172.90	509	243.40	24
156.80	79	168.40	122	173.10	628	257.60	24
157.00	311	169.25	123	174.10	140456	265.00	17
158.80	175	169.60	33	175.05	10600	267.40	17
159.00	180	170.15	153	176.05	141471	280.60	27
160.00	92	170.40	88	177.10	8945	282.40	33
160.75	230	170.80	92	178.00	233	289.30	28
161.25	77	170.95	178	178.60	17		
162.00	28	171.90	327	179.55	53		