


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL080118\
 Data File : VL032327.D
 Acq On : 1 Aug 2018 15:30
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL072718AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jul 27 07:05:37 2018
 Last Update : Fri Jul 27 07:05:37 2018

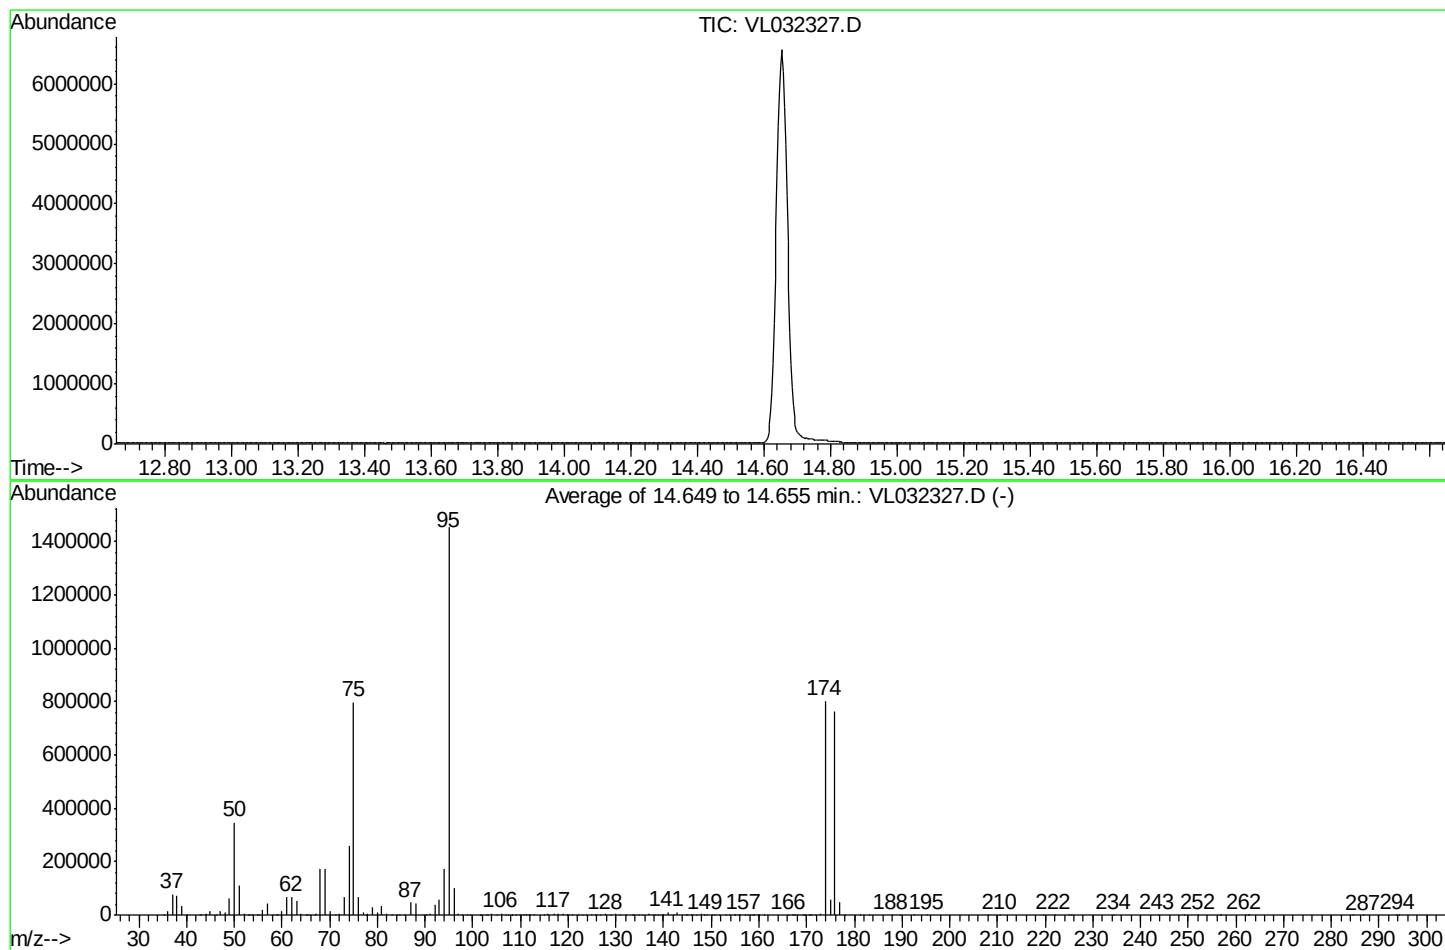

AutoFind: Scans 4218, 4219, 4220; Background Corrected with Scan 4194

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	347946	PASS
75	95	30	66	54.9	798698	PASS
95	95	100	100	100.0	1453568	PASS
96	95	5	9	6.9	99893	PASS
173	174	0.00	2	0.8	6652	PASS
174	95	50	120	55.3	803242	PASS
175	174	4	9	7.2	58061	PASS
176	174	93	101	95.0	763349	PASS
177	176	5	9	6.4	48997	PASS