
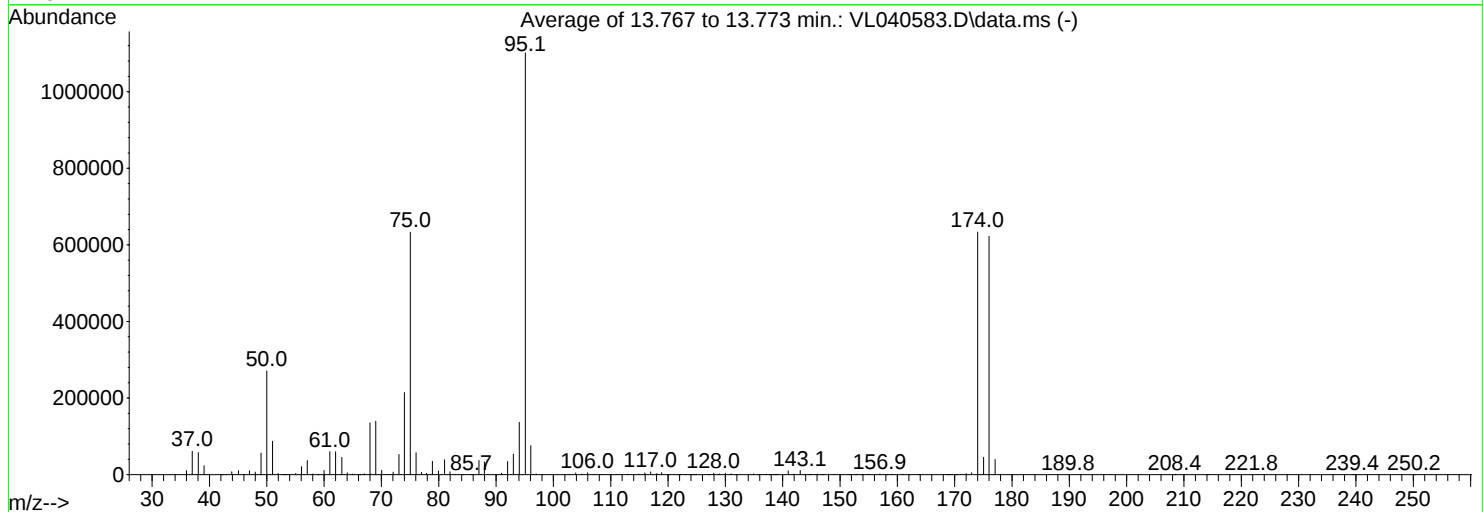


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080423\
 Data File : VL040583.D
 Acq On : 4 Aug 2023 7:52
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL071023AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Jul 10 16:32:00 2023

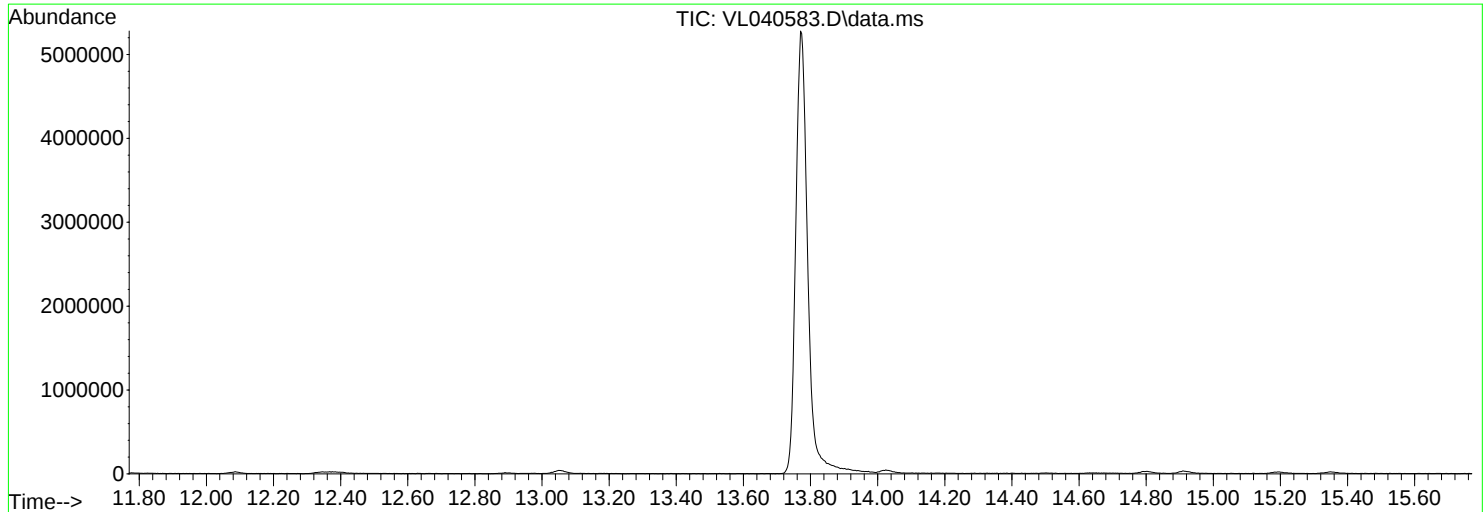

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.6	270933	PASS
75	95	30	66	57.5	633131	PASS
95	95	100	100	100.0	1101504	PASS
96	95	5	9	6.9	75544	PASS
173	174	0.00	2	0.8	4949	PASS
174	95	50	120	57.5	633600	PASS
175	174	4	9	7.1	45248	PASS
176	174	93	101	98.2	622165	PASS
177	176	5	9	6.4	39747	PASS

Average of 13.767 to 13.773 min.: VL040583.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	10542	47.00	10036	57.05	36848	66.20	141
37.00	61213	48.00	6887	58.05	2085	66.90	92
38.05	57672	49.00	56392	58.90	120	67.05	207
39.05	23472	50.00	270933	60.00	11116	68.00	13532
39.95	1118	51.00	87352	61.00	60299	69.00	139712
41.95	136	51.95	3426	62.00	59821	70.05	11138
42.20	101	52.90	253	63.10	45315	71.00	494
42.90	740	53.30	174	64.05	4917	72.05	6604
43.90	7677	54.05	389	65.00	1852	73.05	52880
45.05	10381	55.05	2815	65.20	756	74.00	214549
46.10	1070	56.05	20853	65.90	258	75.05	633131

Average of 13.767 to 13.773 min.: VL040583.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	57261	87.00	37016	104.95	1492	114.90	1141
77.00	6050	87.95	33541	105.95	5209	115.95	4586
77.85	3564	90.95	3746	107.05	933	116.95	7190
78.90	34499	92.00	34491	108.00	176	117.90	1298
79.95	9694	93.00	53357	109.80	482	118.05	2788
81.00	38832	94.05	136811	110.15	374	118.90	5569
81.95	7553	95.10	1.1015e+006	110.90	1001	119.90	161
82.90	1037	96.05	75544	111.20	349	120.10	136
84.15	122	97.00	1891	111.85	841	121.80	212
85.70	160	102.85	449	112.10	391	122.05	236
86.05	638	103.90	4708	112.95	1202	123.00	371

Average of 13.767 to 13.773 min.: VL040583.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.85	701	134.00	443	140.95	9882	148.90	563
124.10	171	134.90	1812	141.95	1650	149.95	1053
124.50	51	135.70	179	143.05	10849	150.20	465
124.80	153	135.95	383	143.85	739	151.60	187
126.00	559	136.90	379	144.60	204	152.70	187
127.00	208	137.10	1286	145.00	928	153.00	1214
127.95	3826	137.70	86	145.70	276	153.70	140
128.95	1796	138.30	72	146.05	1351	154.05	317
130.00	3645	138.70	55	146.80	141	154.90	1251
131.00	2240	139.00	128	147.15	658	155.10	497
131.80	185	139.95	876	147.95	1844	156.05	360

Average of 13.767 to 13.773 min.: VL040583.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.95	1647	170.30	130	214.10	51		
158.20	159	171.05	638	221.80	77		
159.05	1466	172.00	2939	239.40	53		
160.90	813	172.95	4949	250.20	98		
161.10	281	174.00	633600				
162.00	52	175.05	45248				
163.70	129	176.00	622165				
168.70	155	177.05	39747				
169.15	137	178.00	1370				
169.60	326	189.80	104				
170.10	460	208.40	81				