
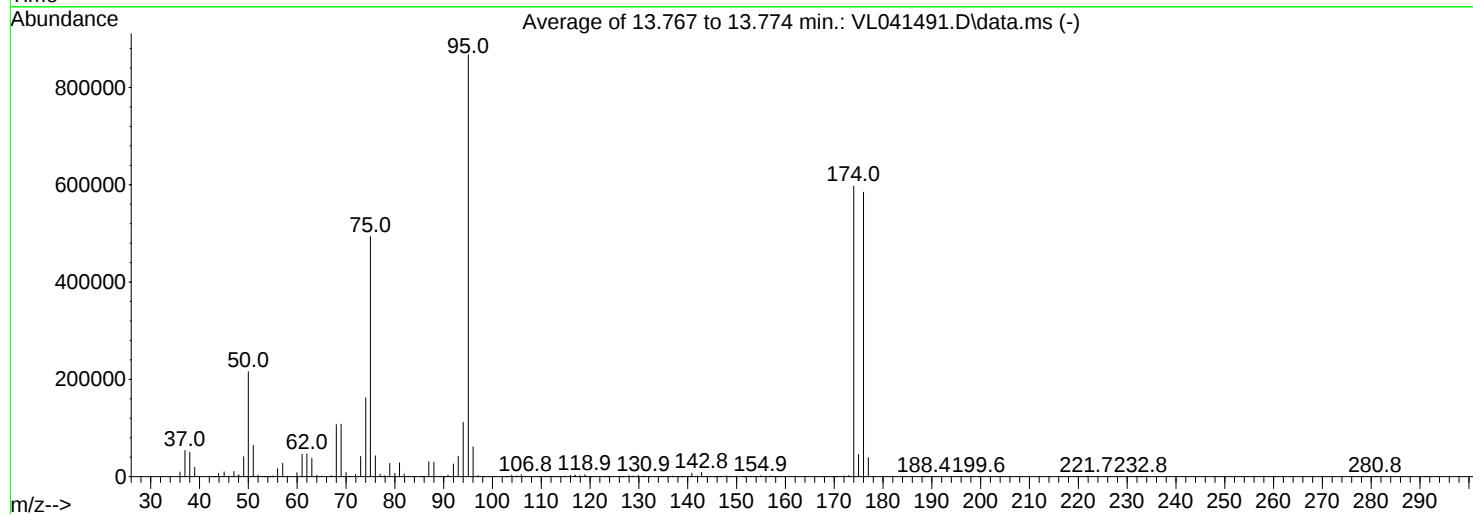


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080524\
Data File : VL041491.D
Acq On : 5 Aug 2024 7:35
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Aug 06 01:32:58 2024

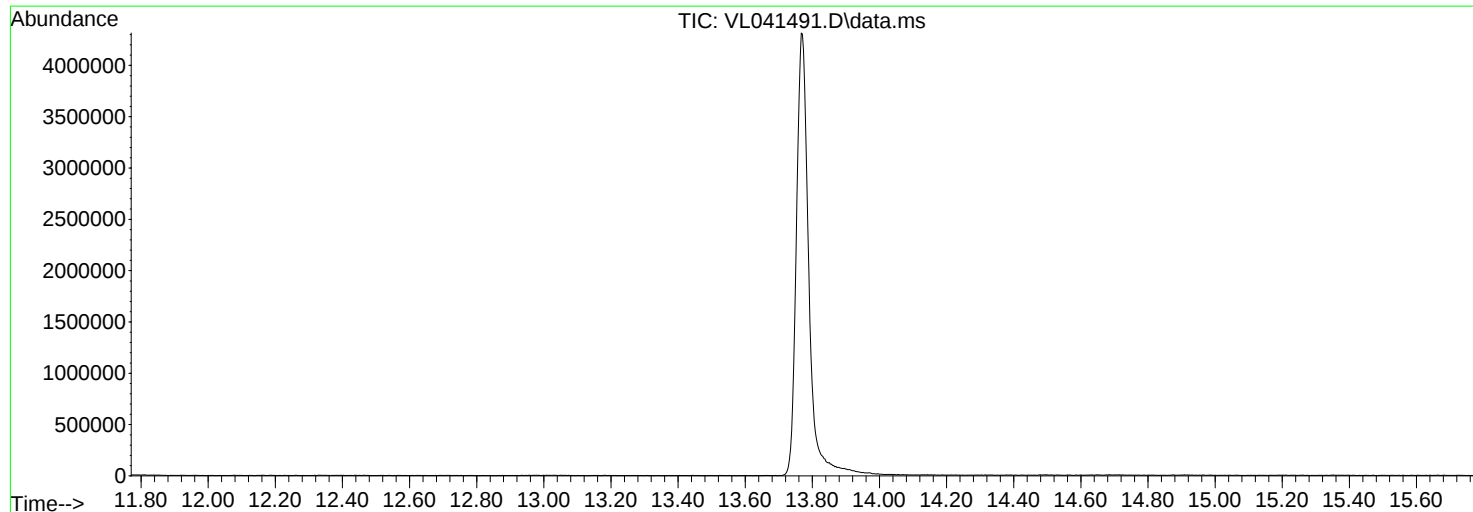

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	215808	PASS
75	95	30	66	56.9	493547	PASS
95	95	100	100	100.0	866987	PASS
96	95	5	9	7.0	61088	PASS
173	174	0.00	2	0.4	2303	PASS
174	95	50	120	68.9	597269	PASS
175	174	4	9	7.6	45509	PASS
176	174	93	101	97.9	584875	PASS
177	176	5	9	6.7	39267	PASS

Average of 13.767 to 13.774 min.: VL041491.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	9479	47.05	10684	54.90	1012	65.05	1061
37.00	53597	47.90	2051	55.10	870	66.95	212
38.00	49912	48.05	3925	56.00	16453	68.00	10686
39.00	19088	49.05	41224	57.05	27720	69.00	10801
39.90	382	50.00	215808	58.00	1152	70.00	8571
42.70	91	51.00	64376	58.80	251	70.95	382
43.00	247	52.00	3412	59.95	8122	71.95	4170
43.20	171	52.80	197	61.00	46528	73.00	41456
43.90	6997	53.20	114	62.00	46365	74.05	162325
45.05	9866	53.80	237	63.00	37787	75.00	493547
45.85	696	54.20	90	64.05	2991	76.00	42635

Average of 13.767 to 13.774 min.: VL041491.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	4945	88.00	29971	102.70	82	112.25	380
77.85	2032	89.55	194	103.00	162	112.95	654
78.95	26829	90.10	54	103.95	2900	114.80	925
80.00	7343	90.90	3201	105.00	1524	115.95	2553
80.95	28304	92.00	26173	105.90	3808	116.80	1597
81.90	5128	93.00	41872	106.80	1047	116.95	3162
82.90	781	94.00	111803	109.70	253	117.85	2043
83.85	145	95.05	866987	109.90	328	118.10	977
85.40	98	96.05	61088	110.60	294	118.90	3678
86.00	486	97.05	1934	110.95	575	119.10	1315
86.95	30525	98.20	121	111.75	814	120.20	136

Average of 13.767 to 13.774 min.: VL041491.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.75	258	128.95	879	139.10	228	146.90	680
123.00	95	129.85	3100	139.95	531	147.90	1737
123.65	168	130.95	1362	140.85	7261	148.60	138
124.05	441	132.00	109	141.95	1256	148.90	448
124.85	274	134.00	175	142.85	8508	149.90	1056
125.80	231	134.70	518	143.85	782	151.50	99
126.00	176	134.90	556	144.70	365	151.80	116
126.70	100	135.10	402	144.90	208	152.00	355
126.95	214	135.80	121	145.70	139	152.85	765
127.95	2694	136.95	1490	146.00	889	153.10	238
128.70	439	138.70	150	146.50	67	153.75	392

Average of 13.767 to 13.774 min.: VL041491.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.00	183	168.40	297	177.00	39267		
154.95	2010	169.05	326	177.80	523		
155.85	300	169.60	257	178.05	627		
156.70	386	170.20	151	188.40	63		
157.05	1413	170.60	361	199.60	73		
157.70	61	171.90	1288	221.70	51		
158.30	73	172.20	722	232.80	78		
158.90	810	173.00	2303	278.30	61		
160.90	860	174.00	597269	280.80	163		
161.90	221	175.00	45509	291.00	72		
167.80	59	176.00	584875				

Instrument :

MSVOA_L

ClientSampleId :

BFB