
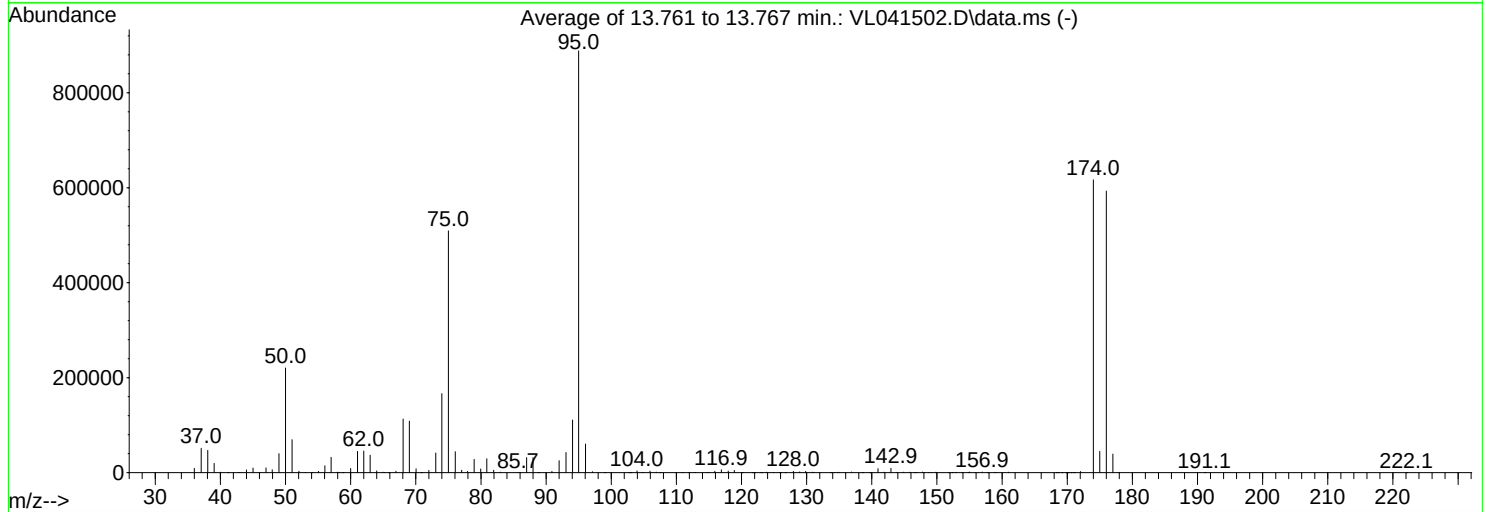


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080824\
Data File : VL041502.D
Acq On : 8 Aug 2024 7:31
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Aug 06 01:32:58 2024

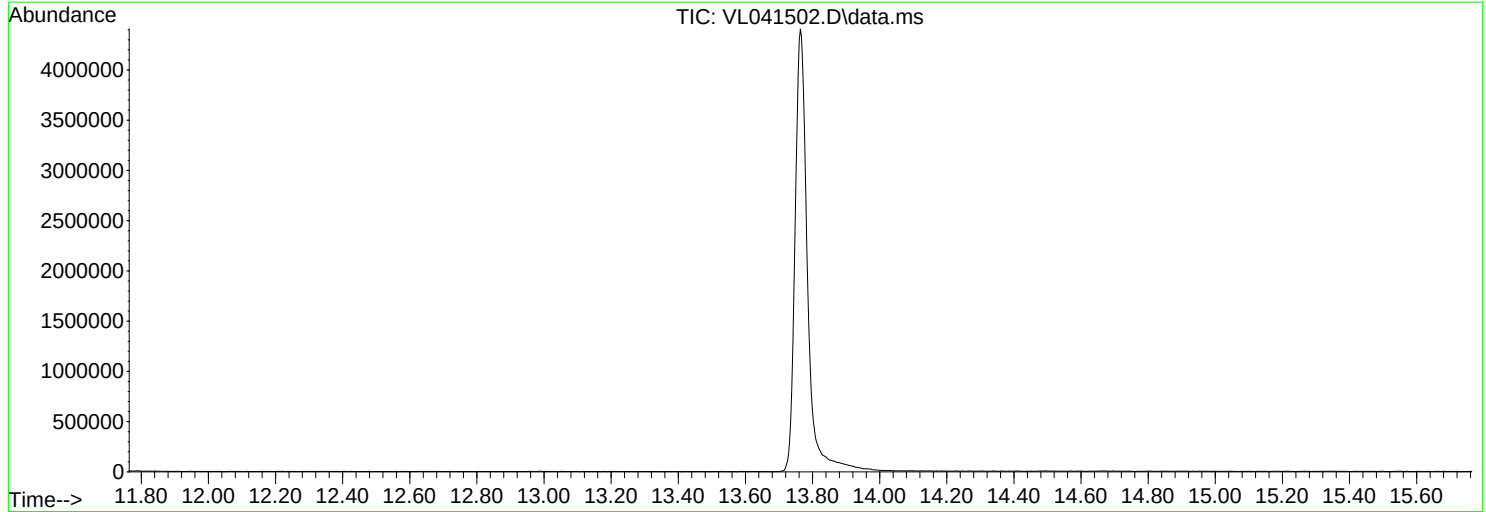

AutoFind: Scans 3470, 3471, 3472; Background Corrected with Scan 3447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.8	220352	PASS
75	95	30	66	57.3	509397	PASS
95	95	100	100	100.0	888405	PASS
96	95	5	9	6.8	60357	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.4	616853	PASS
175	174	4	9	7.3	44741	PASS
176	174	93	101	96.2	593237	PASS
177	176	5	9	6.6	39235	PASS

Average of 13.761 to 13.767 min.: VL041502.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	9187	47.00	10020	58.00	864	66.95	3061
37.05	51341	47.95	5988	58.25	764	68.05	11306
38.05	47011	49.00	40131	58.80	71	69.00	10839
39.05	19617	50.00	220352	60.00	8825	70.05	8041
40.05	867	51.00	69389	61.05	44901	70.80	76
41.15	187	52.05	2902	62.00	45475	71.05	389
42.80	256	53.05	249	63.00	36861	72.00	4729
43.00	218	54.00	100	64.00	3653	73.05	41365
44.00	5878	55.05	2810	64.95	1097	74.00	166464
45.00	9862	56.05	14647	65.20	216	75.00	509397
46.10	353	57.00	32467	65.85	121	76.05	44301

Average of 13.761 to 13.767 min.: VL041502.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	4978	88.80	145	103.95	3874	112.70	200
77.95	2848	90.90	2697	104.70	305	112.95	454
78.95	27891	92.00	25139	104.95	826	114.75	415
79.95	7726	93.05	42613	105.95	3442	115.00	193
80.90	29264	94.05	110955	106.90	1193	115.90	2969
81.95	4960	95.00	888405	107.50	121	116.90	6008
83.00	900	96.05	60357	110.00	485	117.95	3263
85.70	605	97.10	1957	110.80	330	118.90	4836
86.05	511	99.00	53	111.05	754	120.10	69
87.00	31656	102.70	68	111.85	426	121.70	180
88.00	31848	103.00	165	112.10	279	122.00	94

Average of 13.761 to 13.767 min.: VL041502.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.90	248	131.10	608	140.95	8554	149.15	380
123.10	128	132.00	246	141.90	1052	149.85	1016
123.80	898	133.70	60	142.95	9188	151.80	144
124.90	366	134.25	283	143.85	749	152.30	104
125.80	235	134.70	593	144.90	990	152.80	259
126.00	112	135.00	860	145.85	1095	153.00	697
126.70	148	136.00	294	146.60	110	153.85	368
127.95	2863	136.90	1483	146.95	354	154.05	305
128.95	1802	138.55	155	147.80	1482	154.80	593
129.85	2821	139.70	92	148.10	204	155.00	1310
130.85	968	139.95	543	148.75	271	155.90	219

Average of 13.761 to 13.767 min.: VL041502.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.30	208	170.15	185	191.10	57		
156.95	1434	170.60	188	222.10	50		
157.80	146	171.00	121				
158.00	316	171.30	228				
158.90	613	172.05	2416				
159.10	398	174.00	616853				
161.00	901	175.00	44741				
168.30	129	176.00	593237				
168.60	94	177.00	39235				
169.20	158	177.90	264				
169.80	71	178.05	579				