


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL081220\
 Data File : VL035379.D
 Acq On : 12 Aug 2020 10:29
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081220AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Aug 12 20:32:44 2020
 Last Update : Wed Aug 12 20:32:44 2020

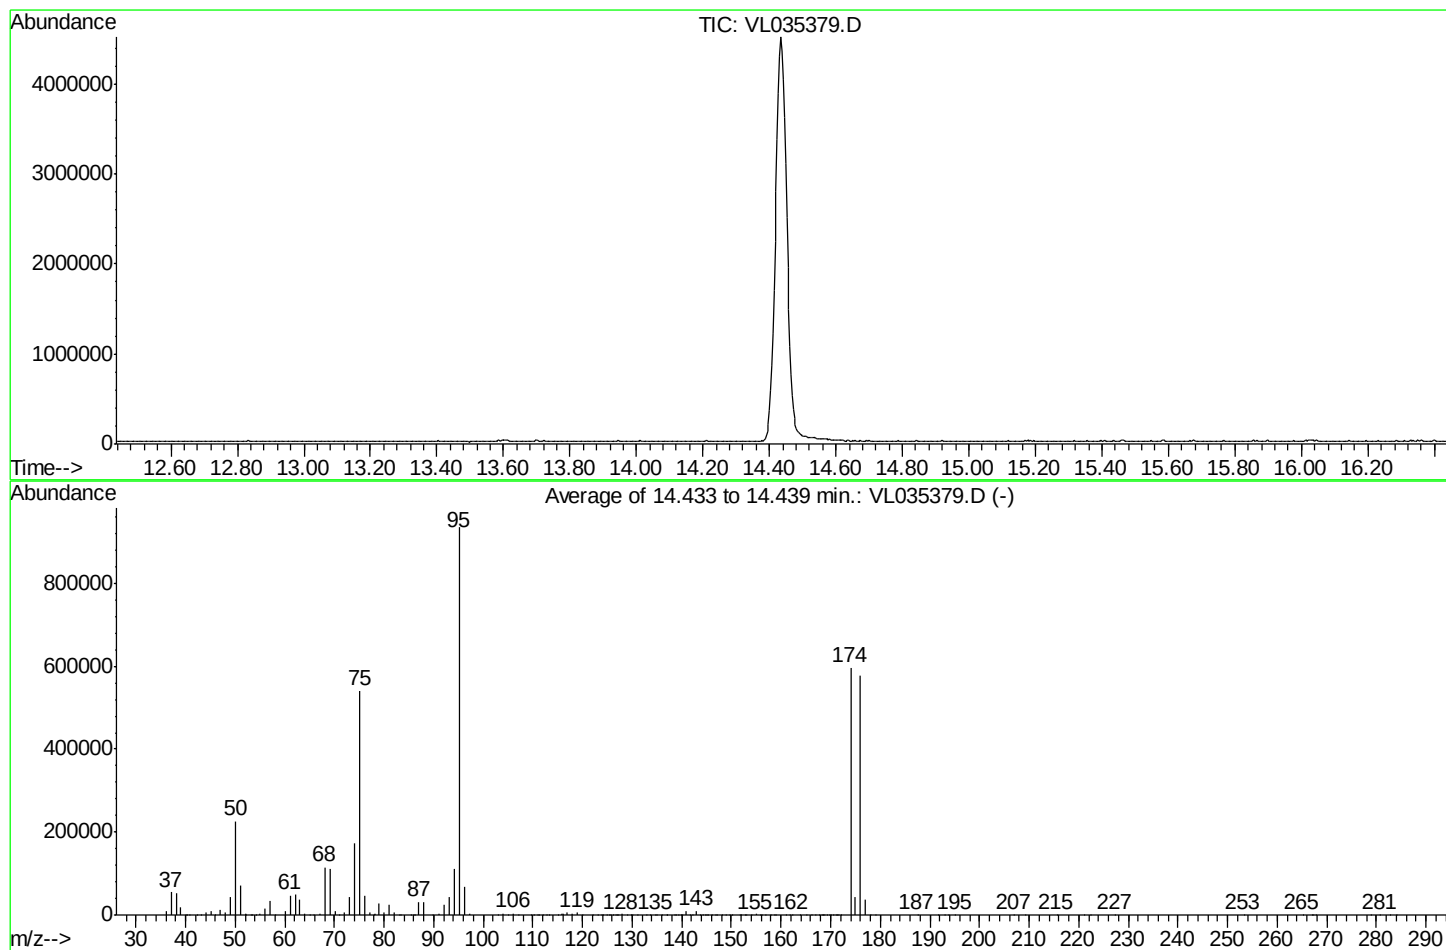

AutoFind: Scans 3622, 3623, 3624; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	226858	PASS
75	95	30	66	57.8	540885	PASS
95	95	100	100	100.0	934990	PASS
96	95	5	9	7.1	66541	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.9	597098	PASS
175	174	4	9	7.5	44650	PASS
176	174	93	101	96.6	576832	PASS
177	176	5	9	6.7	38544	PASS