


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL081321\
 Data File : VL037441.D
 Acq On : 13 Aug 2021 9:54
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081221AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 13 01:37:35 2021
 Last Update : Fri Aug 13 01:37:35 2021

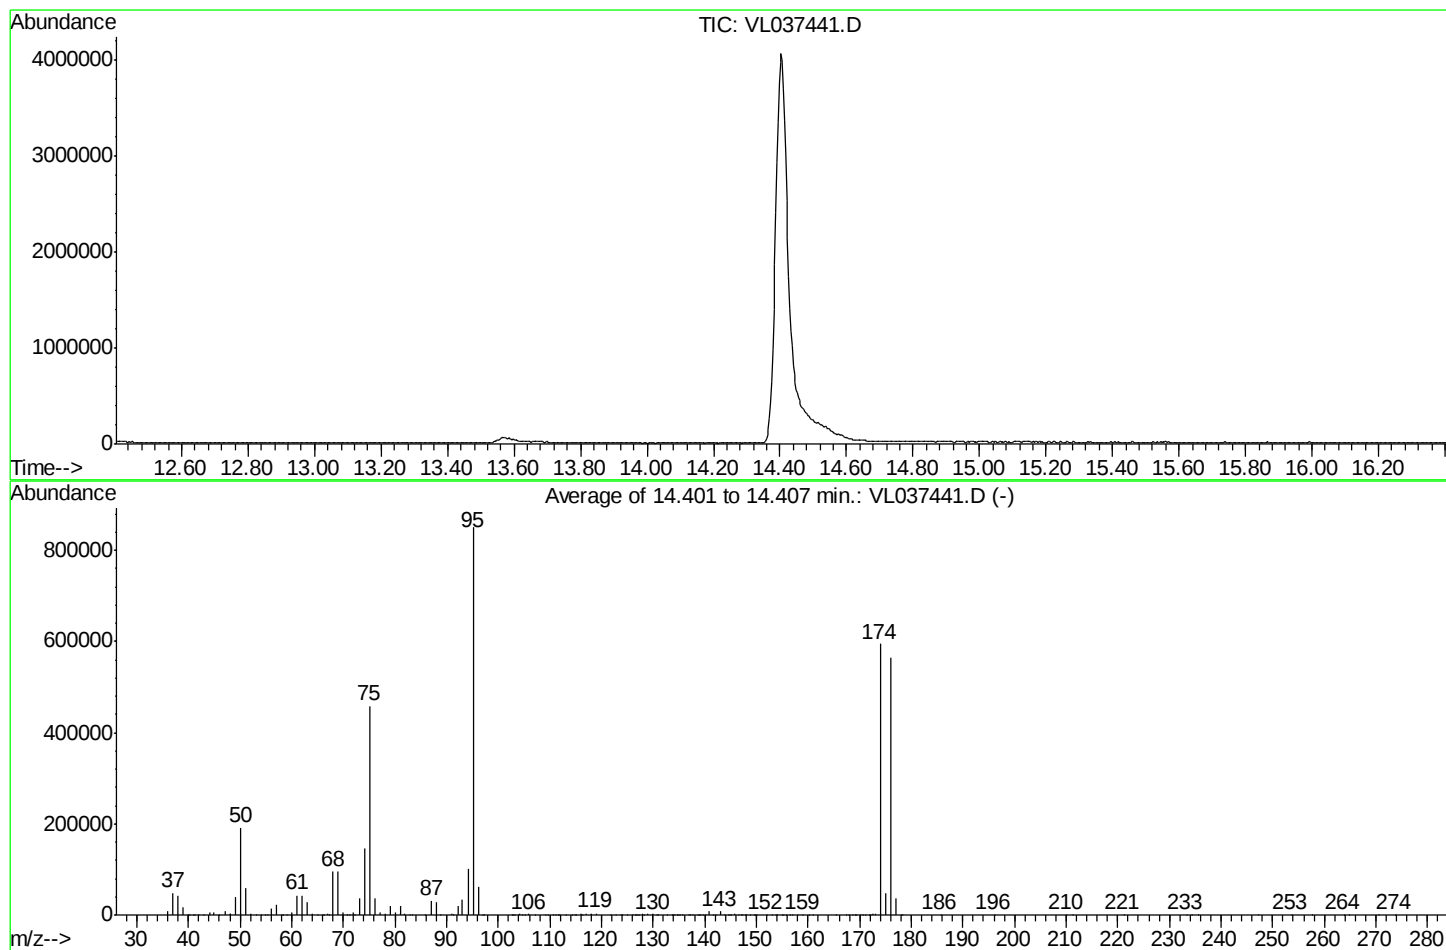

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.6	192384	PASS
75	95	30	66	54.0	458858	PASS
95	95	100	100	100.0	850346	PASS
96	95	5	9	7.1	60746	PASS
173	174	0.00	2	0.6	3322	PASS
174	95	50	120	69.9	594304	PASS
175	174	4	9	7.8	46573	PASS
176	174	93	101	95.0	564608	PASS
177	176	5	9	6.7	37837	PASS