


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL081618\
 Data File : VL032377.D
 Acq On : 16 Aug 2018 13:31
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081518AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Aug 15 14:58:02 2018
 Last Update : Wed Aug 15 14:58:02 2018

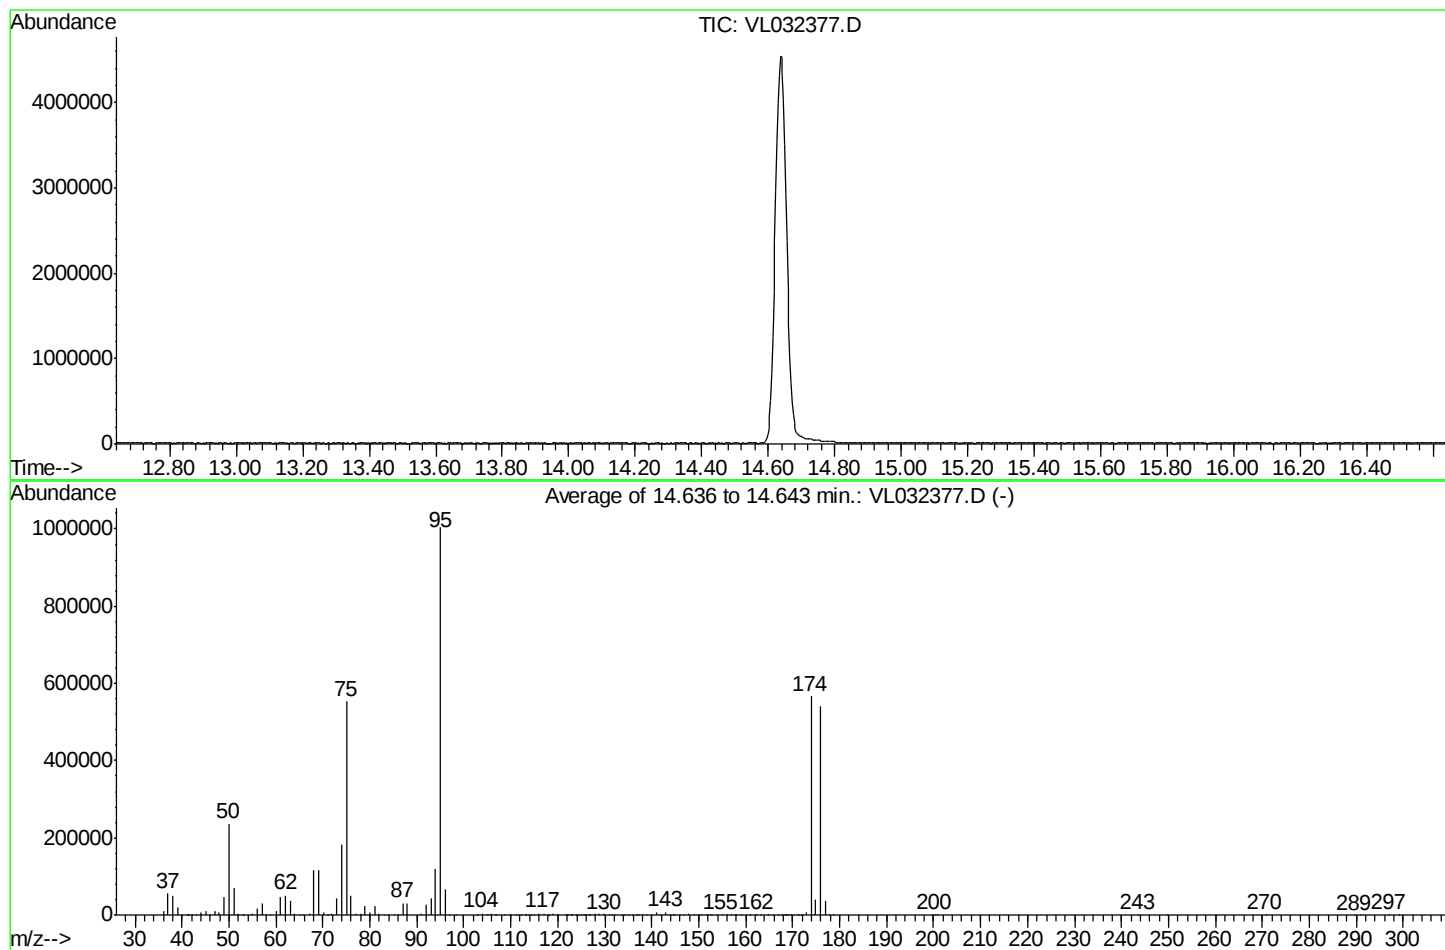

AutoFind: Scans 4214, 4215, 4216; Background Corrected with Scan 4191

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	236695	PASS
75	95	30	66	55.1	553450	PASS
95	95	100	100	100.0	1004373	PASS
96	95	5	9	6.5	65501	PASS
173	174	0.00	2	0.9	5315	PASS
174	95	50	120	56.4	566592	PASS
175	174	4	9	7.0	39653	PASS
176	174	93	101	95.6	541418	PASS
177	176	5	9	6.6	36002	PASS