

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL081921\
 Data File : VL037501.D
 Acq On : 19 Aug 2021 16:37
 Operator : SY/AP
 Sample : M3480-02
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SR-SG-2

Manual Integrations
 APPROVED

MMDadoda
 8/20/2021 6:31:10 PM

Quant Time: Aug 20 00:52:00 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL081621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 2021
 QLast Update : Tue Aug 17 02:13:47 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	1436542	10.00	ppbv	0.03
33) 1,4-Difluorobenzene	7.18	114	4136783	10.00	ppbv	0.03
55) Chlorobenzene-d5	12.09	117	3546399	10.00	ppbv	0.03

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.42	95	2473530	9.82	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.20%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.06	85	29692m	0.129	ppbv	
3) Chlorodifluoromethane	2.99	51	1649489	5.996	ppbv #	85
4) Chloromethane	3.14	50	70836	0.721	ppbv	91
9) Propene	3.02	41	64502	0.655	ppbv	85
10) Heptane	8.13	43	52881	0.233	ppbv	97
11) Trichlorofluoromethane	3.96	101	41659m	0.193	ppbv	
13) Ethanol	3.61	45	6282770	655.999	ppbv	99
15) Acetone	3.85	43	5778926	39.528	ppbv	96
17) tert-Butyl alcohol	4.31	59	420699	3.150	ppbv	100
19) Isopropyl Alcohol	3.98	45	4571578	54.581	ppbv	100
20) Methylene Chloride	4.35	84	351820	4.806	ppbv	96
26) Hexane	5.69	57	385043	2.122	ppbv #	54
27) Carbon Disulfide	4.57	76	28034m	0.173	ppbv	
29) Chloroform	5.76	83	97562m	0.379	ppbv	
34) 2-Butanone	5.25	43	840733	4.977	ppbv #	90
35) Carbon Tetrachloride	7.02	117	13548m	0.055	ppbv	
36) Benzene	6.90	78	2842200	8.173	ppbv	98
38) Trichloroethene	7.84	130	67459	0.473	ppbv #	88
50) 4-Methyl-2-Pentanone	8.75	43	136016m	0.617	ppbv	
51) 2-Hexanone	10.14	43	159158	1.570	ppbv #	87
52) Tetrachloroethene	11.22	164	23127m	0.162	ppbv	
53) Toluene	9.81	91	500177	1.260	ppbv	98
58) Ethyl Benzene	12.71	91	403542	0.820	ppbv	93
59) m/p-Xylene	12.97	91	1725818	4.045	ppbv	92
60) o-Xylene	13.69	91	487474	1.224	ppbv	98
61) Styrene	13.53	104	58080m	0.281	ppbv	
62) Isopropylbenzene	14.67	105	1132021	2.014	ppbv	96
69) p-Isopropyltoluene	17.65	119	93041m	0.160	ppbv	
70) n-Butylbenzene	18.55	91	86103m	0.155	ppbv	
72) 4-Ethyltoluene	15.84	105	56331m	0.119	ppbv	
73) 1,3,5-Trimethylbenzene	16.00	105	73902	0.168	ppbv	100
74) 1,2,4-Trimethylbenzene	16.76	105	249141	0.532	ppbv #	67
79) Naphthalene	22.19	128	233205	0.744	ppbv #	93
80) Naphthalene,2-methyl-	24.97	142	23661	0.271	ppbv #	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL081921\
Data File : VL037501.D
Acq On : 19 Aug 2021 16:37
Operator : SY/AP
Sample : M3480-02
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:10 PM

Quant Time: Aug 20 00:52:00 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL081621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug
QLast Update : Tue Aug 17 02:13:47 2021
Response via : Initial Calibration

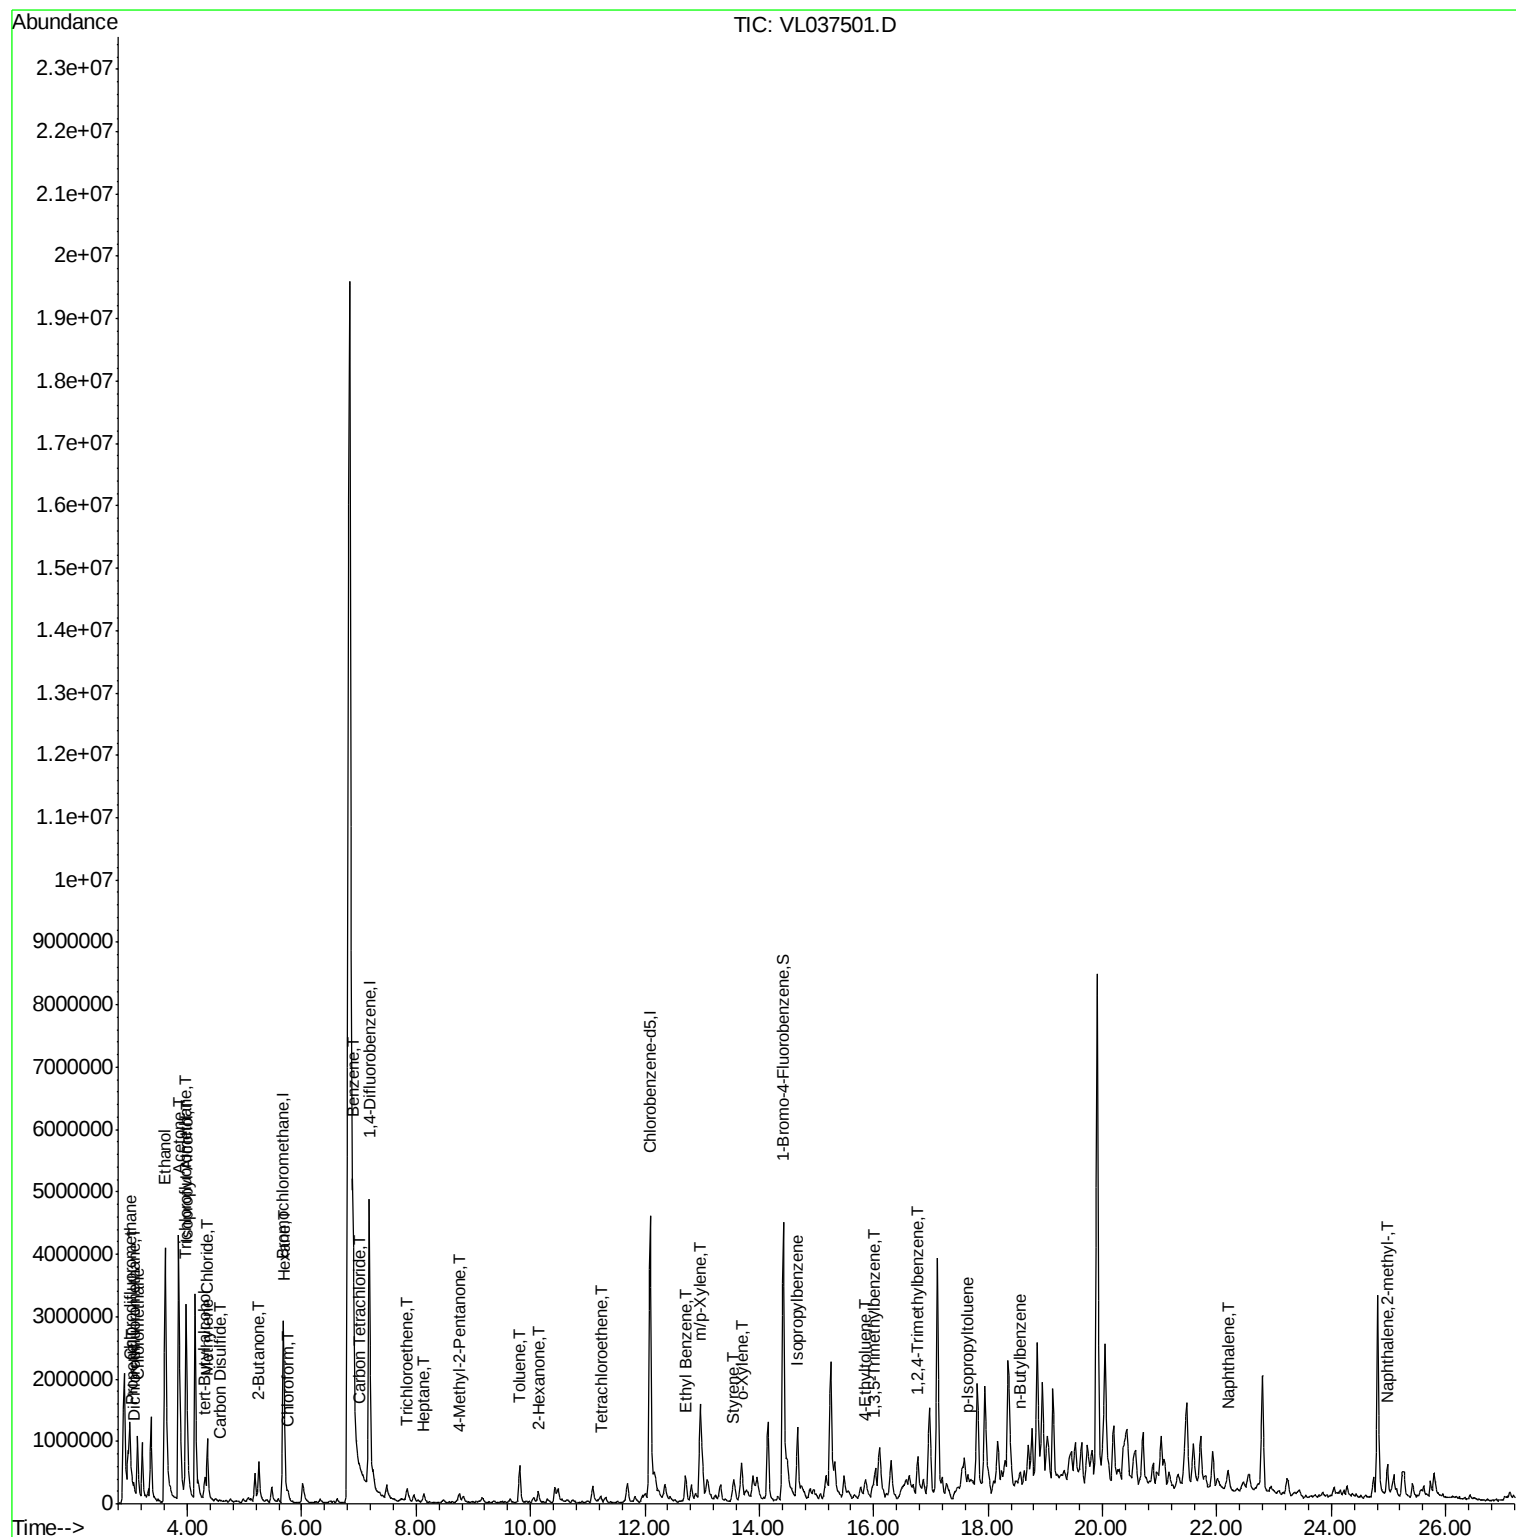

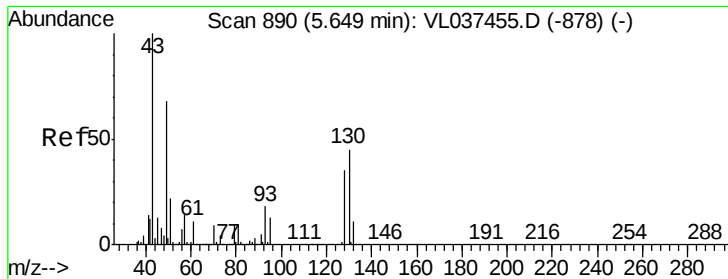

#1





Bromochloromethane
Concen: 10.000 ppbv
RT: 5.67 min Scan# 898
Delta R.T. 0.03 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion: 49 Resp: 1436542
Ion Ratio Lower Upper
49 100
128 52.4 27.5 82.4
130 68.1 34.0 101.8

Manual Integrations
APPROVED




MMDadoda
8/20/2021 6:31:10 PM

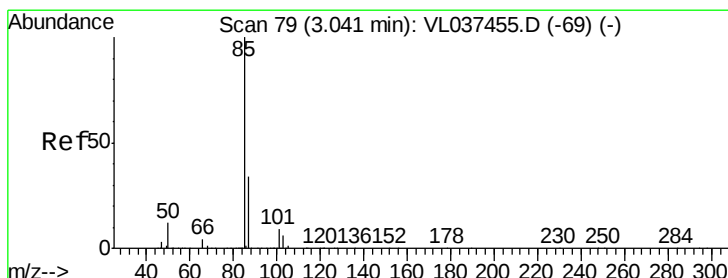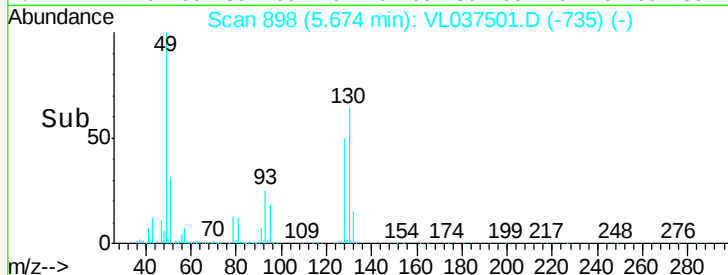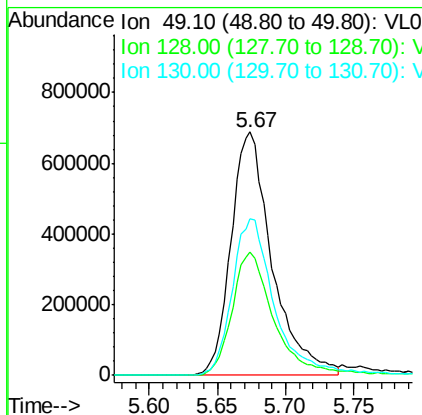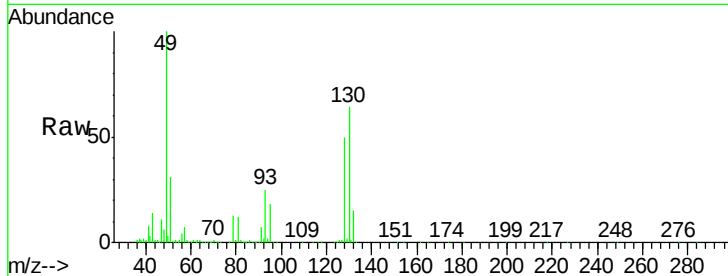


#2

Dichlorodifluoromethane
Concen: 0.129 ppbv m
RT: 3.06 min Scan# 84
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion: 85 Resp: 29692
Ion Ratio Lower Upper
85 100
87 30.7 27.6 41.4

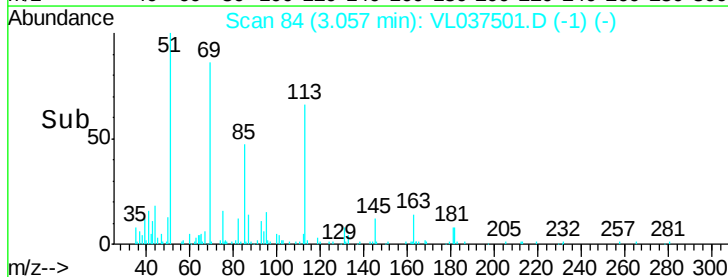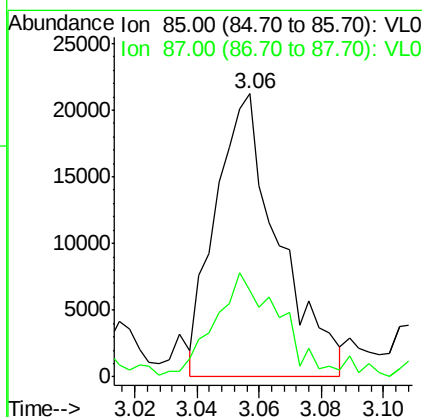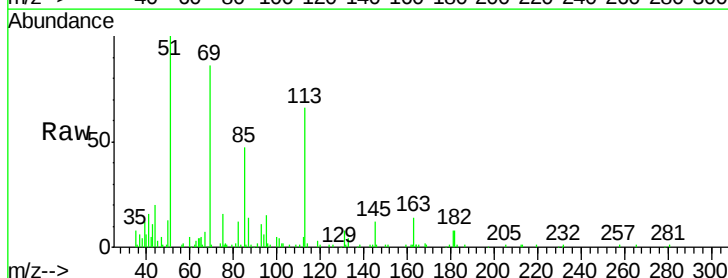







#3
Chlorodifluoromethane
Concen: 5.996 ppbv
RT: 2.99 min Scan# 64
Delta R.T. 0.01 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion: 51 Resp: 1649489
Ion Ratio Lower Upper
51 100
67 11.2 14.2 21.2#




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

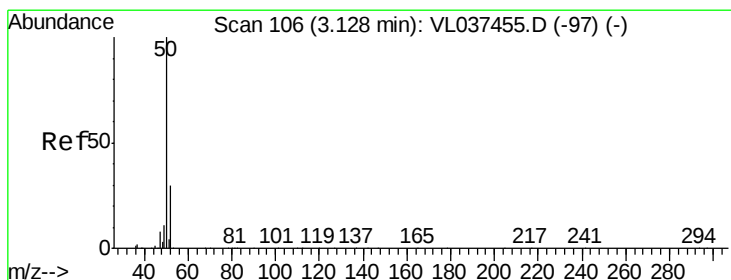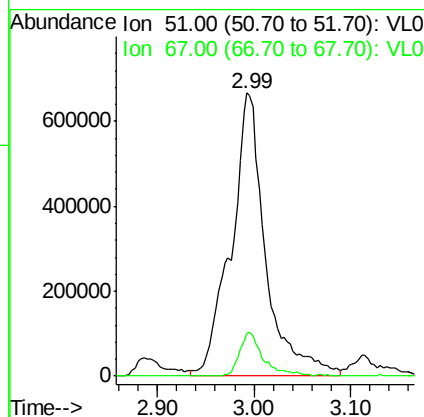

#4
Chloromethane
Concen: 0.721 ppbv
RT: 3.14 min Scan# 111
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion: 50 Resp: 70836
Ion Ratio Lower Upper
50 100
52 25.1 24.0 36.0

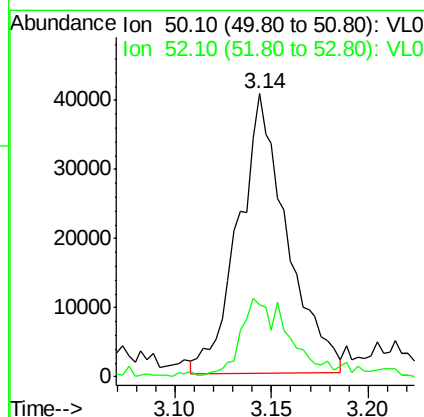



#9

Propene

Concen: 0.655 ppbv

RT: 3.02 min Scan# 74

Delta R.T. 0.03 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Instrument :

MSVOA_L

ClientSampleId :

SR-SG-2

Tot Ion: 41 Resp: 64502





Ion Ratio Lower Upper

41 100

42 55.3 53.7 80.5

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:10 PM

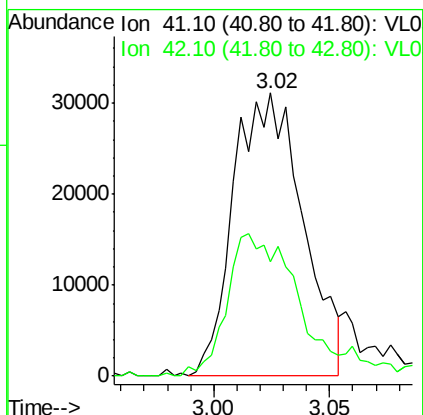

#10

Heptane

Concen: 0.233 ppbv

RT: 8.13 min Scan# 1662

Delta R.T. 0.03 min

Lab File: VL037501.D




Acq: 19 Aug 2021 16:37


Tgt Ion: 43 Resp: 52881

Ion Ratio Lower Upper

43 100

57 53.7 41.0 61.6

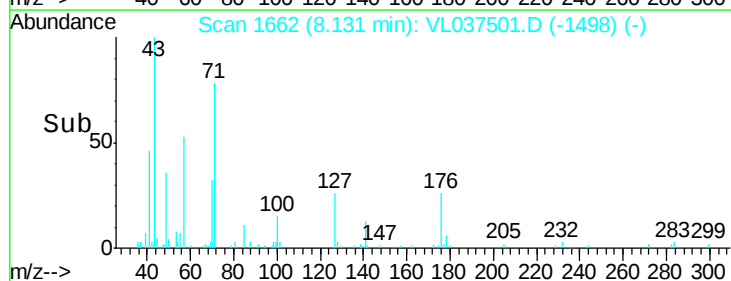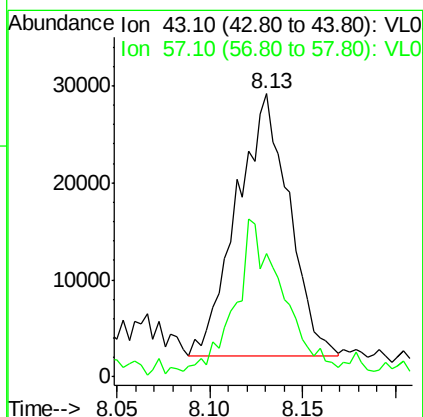

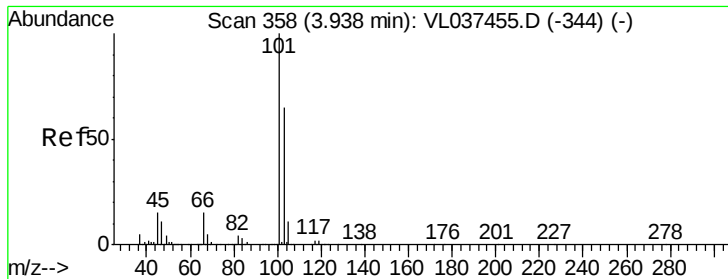





#11
 Trichlorofluoromethane
 Concen: 0.193 ppbv m
 RT: 3.96 min Scan# 365
 Delta R.T. 0.02 min
 Lab File: VL037501.D
 Acq: 19 Aug 2021 16:37

Instrument :
 MSVOA_L
 ClientSampled :
 SR-SG-2

Tot Ion:101 Resp: 41659
 Ion Ratio Lower Upper
 101 100
 103 47.7 51.8 77.6#




Manual Integrations
 APPROVED


MMDadoda
 8/20/2021 6:31:10 PM

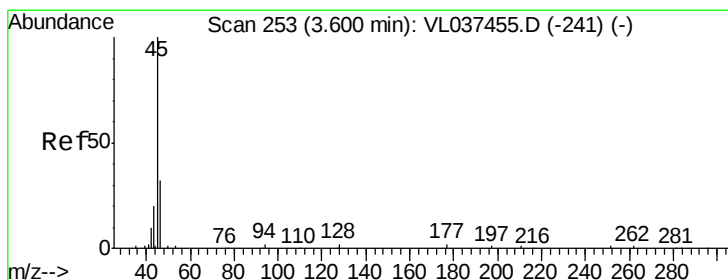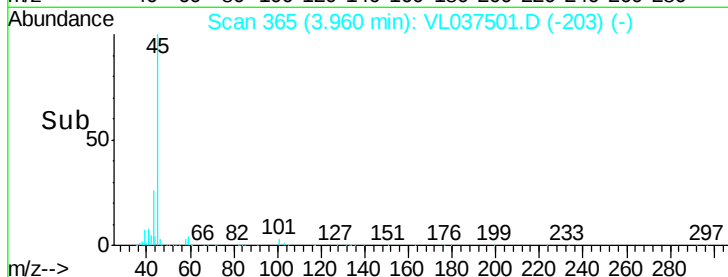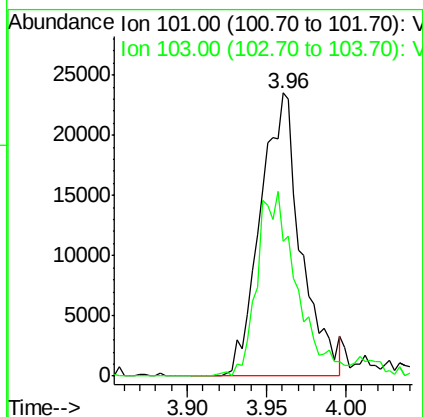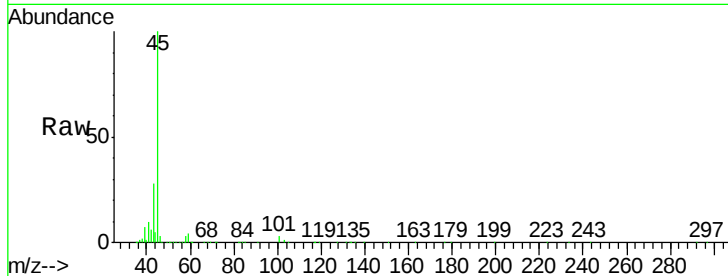

#13
 Ethanol
 Concen: 655.999 ppbv
 RT: 3.61 min Scan# 256
 Delta R.T. 0.01 min
 Lab File: VL037501.D
 Acq: 19 Aug 2021 16:37

Tgt Ion: 45 Resp: 6282770
 Ion Ratio Lower Upper
 45 100
 46 35.9 14.1 56.5

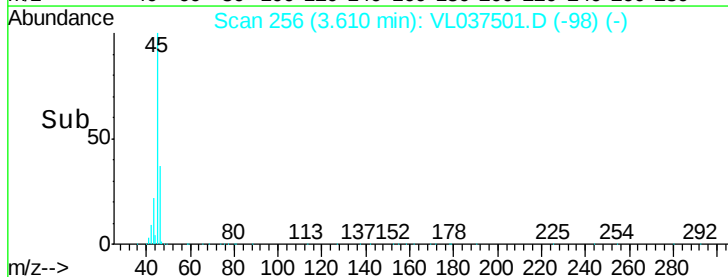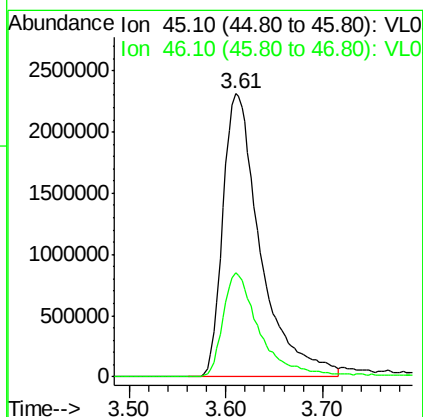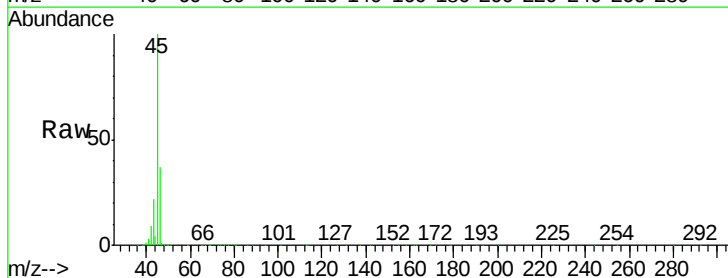

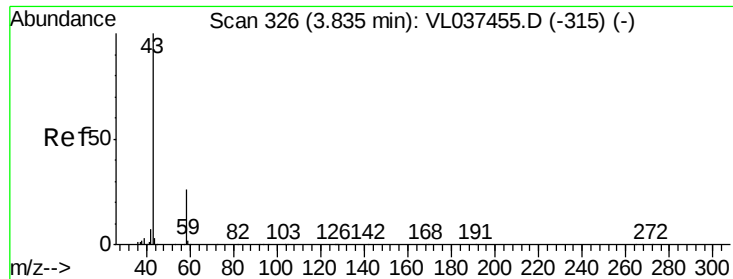





#15
Acetone
Concen: 39.528 ppbv
RT: 3.85 min Scan# 330
Delta R.T. 0.01 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion: 43 Resp: 5778926
Ion Ratio Lower Upper
43 100
58 28.8 24.8 37.2




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

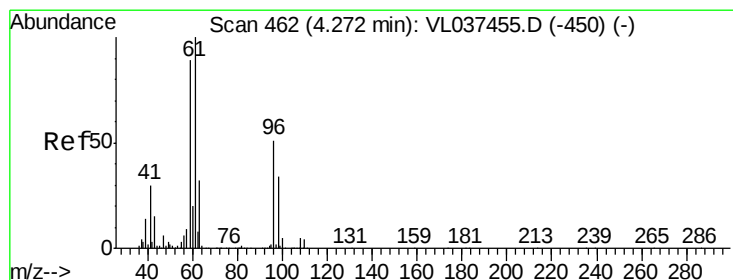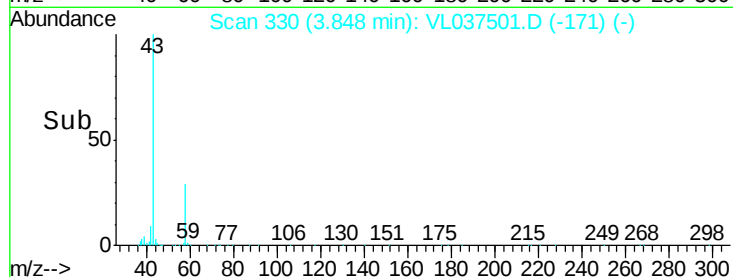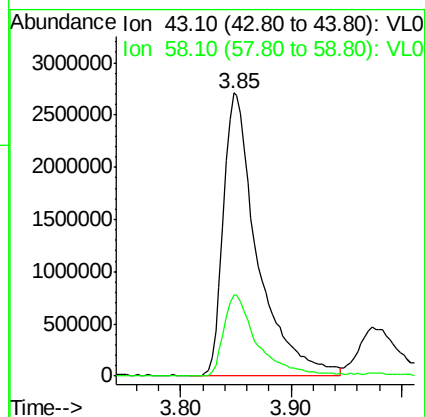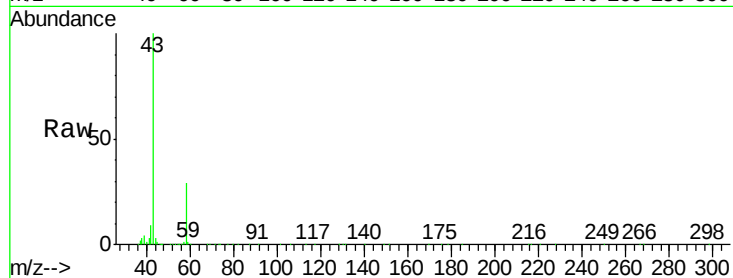

#17
tert-Butyl alcohol
Concen: 3.150 ppbv
RT: 4.31 min Scan# 473
Delta R.T. 0.04 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion: 59 Resp: 420699
Ion Ratio Lower Upper
59 100
57 10.3 8.3 12.5

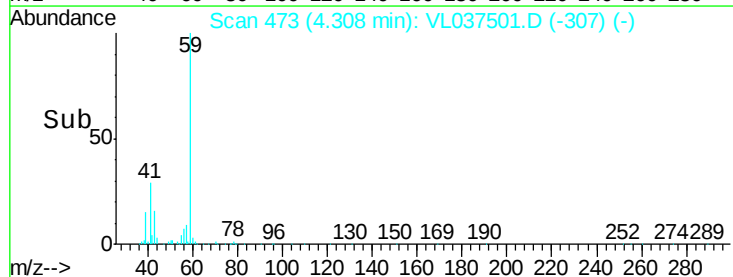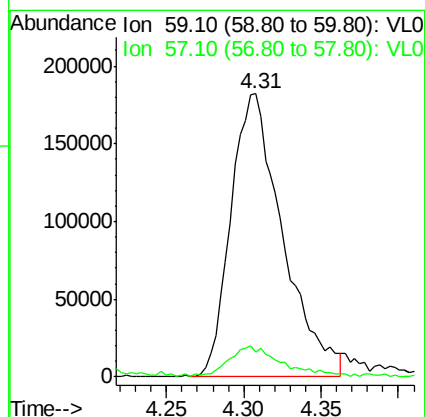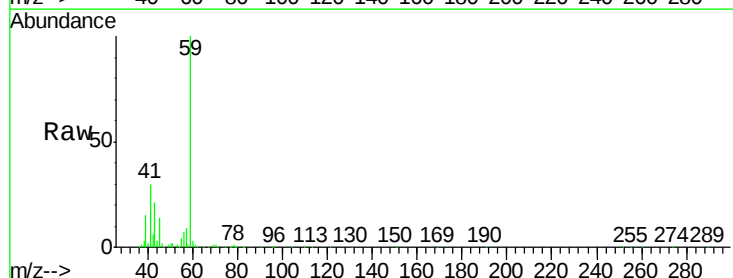

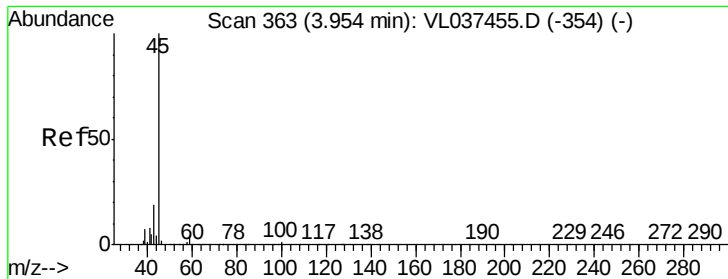

#19

Isopropyl Alcohol

Concen: 54.581 ppbv

RT: 3.98 min Scan# 370

Delta R.T. 0.02 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Instrument :

MSVOA_L

ClientSampleId :

SR-SG-2

Tot Ion: 45 Resp: 4571578





Ion Ratio Lower Upper

45 100

58 1.9 1.4 2.2

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:10 PM

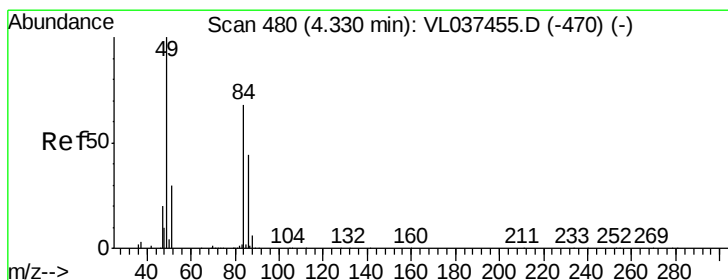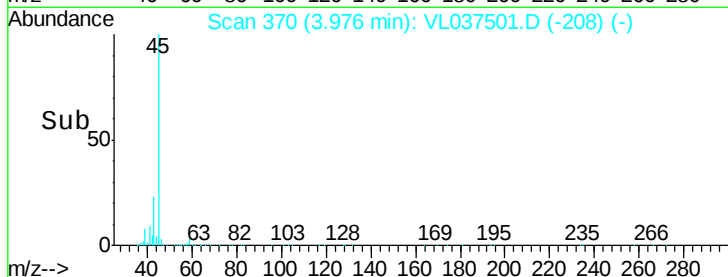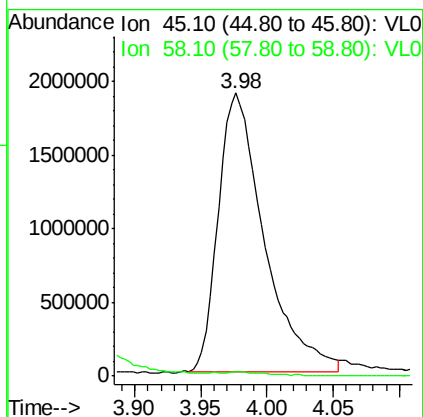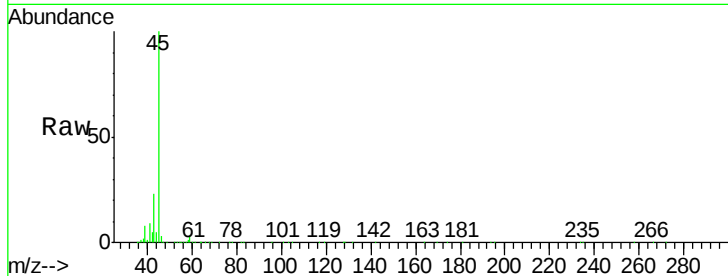

#20

Methylene Chloride

Concen: 4.806 ppbv

RT: 4.35 min Scan# 486

Delta R.T. 0.02 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Tgt Ion: 84 Resp: 351820




Ion Ratio Lower Upper


84 100

49 154.5 118.2 177.2

51 42.2 36.6 55.0

86 63.4 51.8 77.6

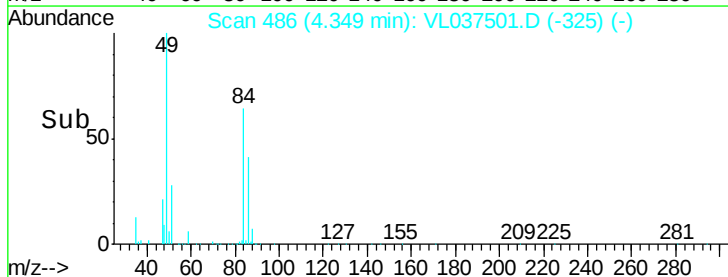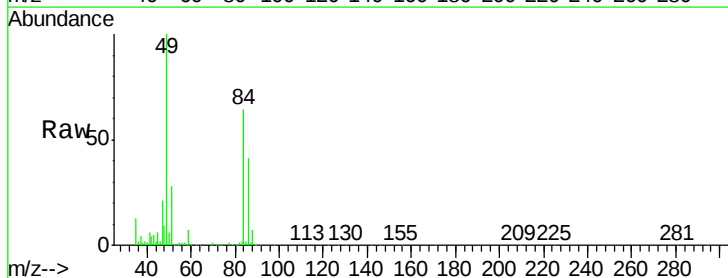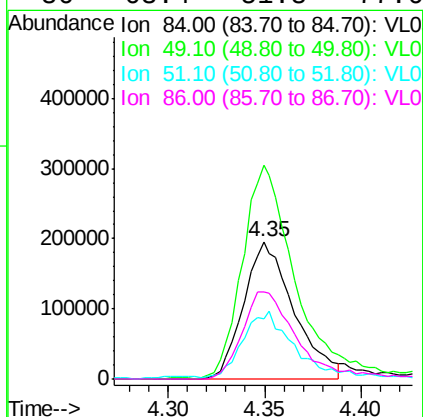



#26

Hexane

Concen: 2.122 ppbv

RT: 5.69 min Scan# 904

Delta R.T. 0.03 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Instrument :

MSVOA_L




ClientSampleId :

SR-SG-2

Tot Ion	57	Resp	385043
Ion	Ratio	Lower	Upper
57	100		
41	93.0	72.3	108.5
43	96.4	172.3	258.5#
56	55.3	42.8	64.2

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:10 PM

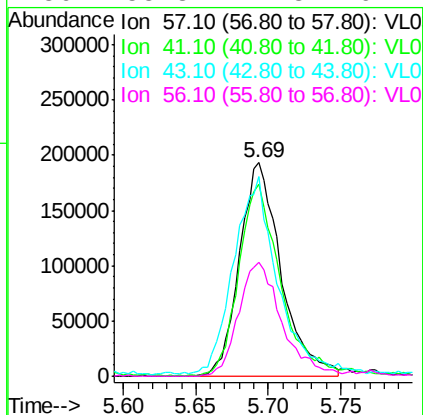

#27

Carbon Disulfide

Concen: 0.173 ppbv m





RT: 4.57 min Scan# 554


Delta R.T. 0.03 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Tgt Ion	76	Resp	28034
Ion	Ratio	Lower	Upper
76	100		
44	45.7	13.9	20.9#
78	10.0	7.9	11.9

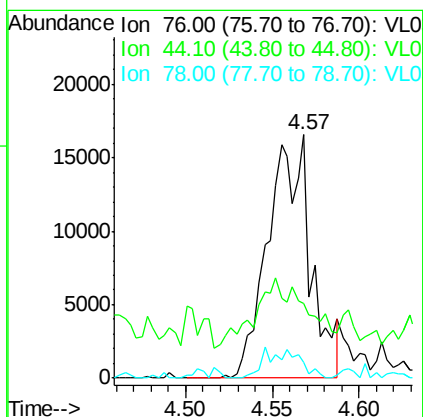







#29
Chloroform
Concen: 0.379 ppbv m
RT: 5.76 min Scan# 925
Delta R.T. 0.03 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampled :
SR-SG-2

Tot Ion: 83 Resp: 97562
Ion Ratio Lower Upper
83 100
85 68.7 52.3 78.5




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

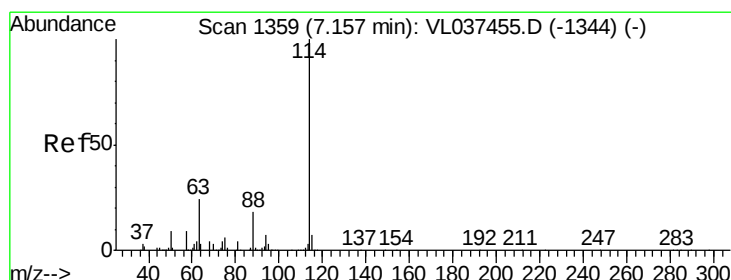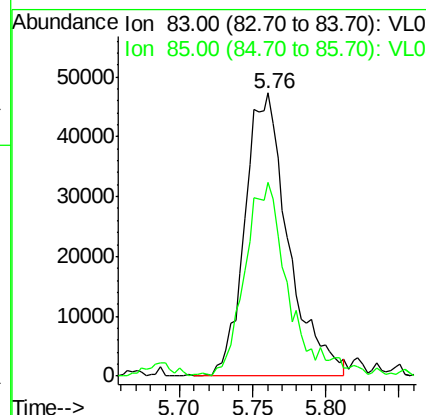

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.18 min Scan# 1367
Delta R.T. 0.03 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion: 114 Resp: 4136783
Ion Ratio Lower Upper
114 100
63 23.9 19.3 28.9
88 17.9 14.2 21.4

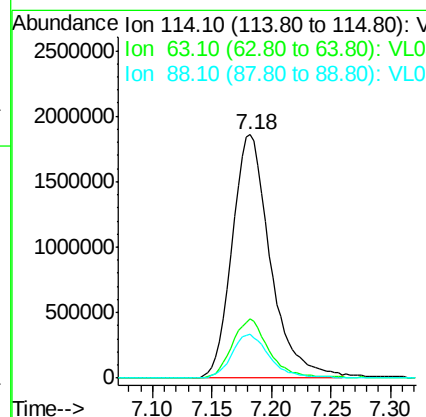







#34
2-Butanone
Concen: 4.977 ppbv
RT: 5.25 min Scan# 766
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion	Ratio	Lower	Upper
43	100		
72	26.6	17.4	26.0#




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

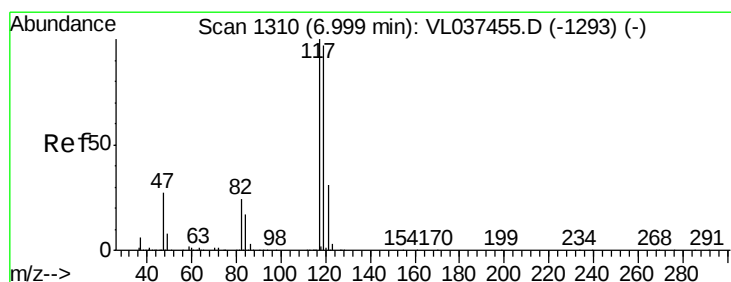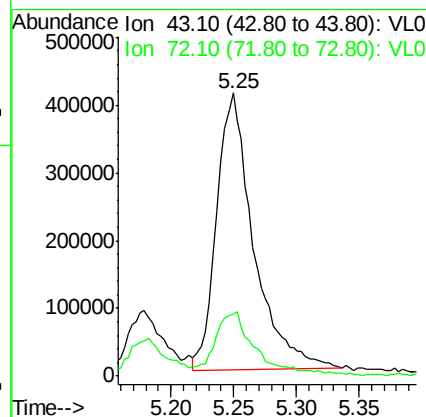

#35
Carbon Tetrachloride
Concen: 0.055 ppbv m
RT: 7.02 min Scan# 1318
Delta R.T. 0.03 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion	Ratio	Lower	Upper
117	100		
119	78.1	77.3	115.9
121	21.5	25.2	37.8#

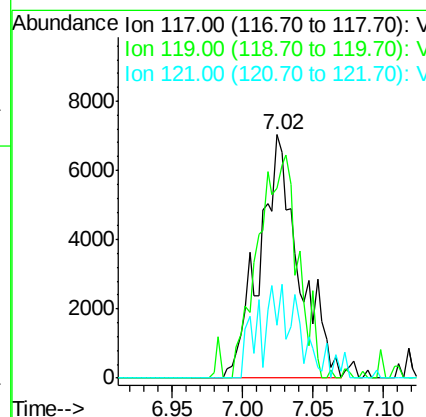

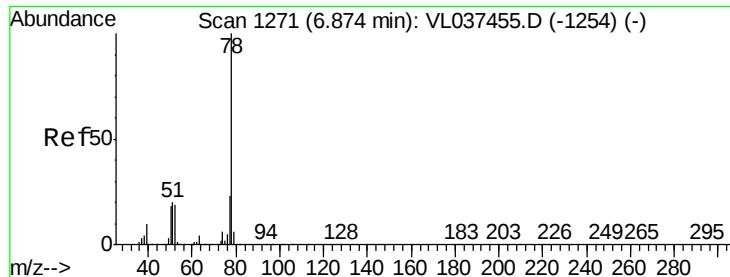

#36

Benzene

Concen: 8.173 ppbv

RT: 6.90 min Scan# 1278

Delta R.T. 0.02 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Instrument :

MSVOA_L

ClientSampleId :

SR-SG-2

Tot Ion: 78 Resp: 2842200

Ion Ratio Lower Upper





78 100

77 23.2 18.2 27.4

50 16.7 14.6 21.8

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:10 PM

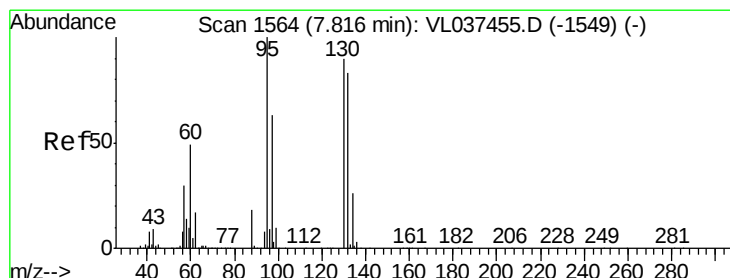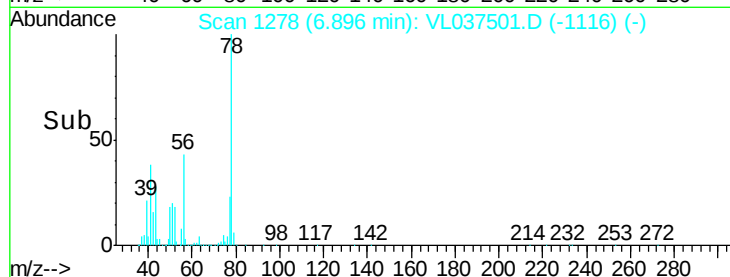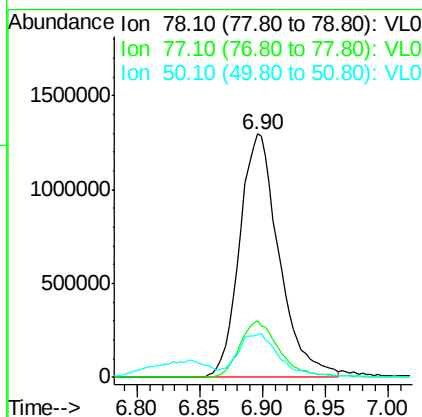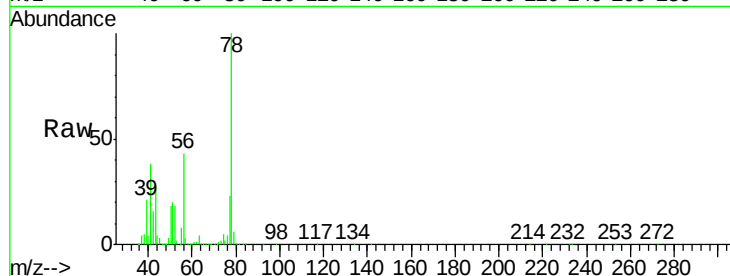

#38

Trichloroethene

Concen: 0.473 ppbv

RT: 7.84 min Scan# 1571

Delta R.T. 0.02 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Tgt Ion: 130 Resp: 67459




Ion Ratio Lower Upper


130 100

95 100.8 89.2 133.8

132 89.6 74.0 111.0

97 48.5 56.6 84.8#

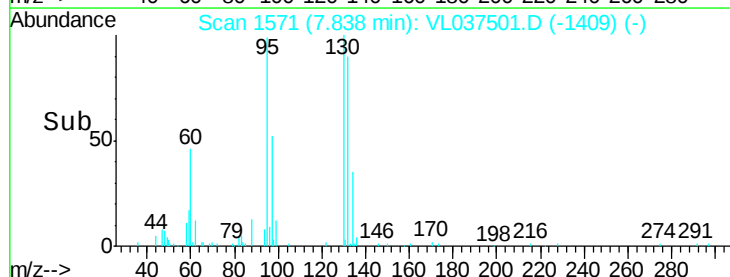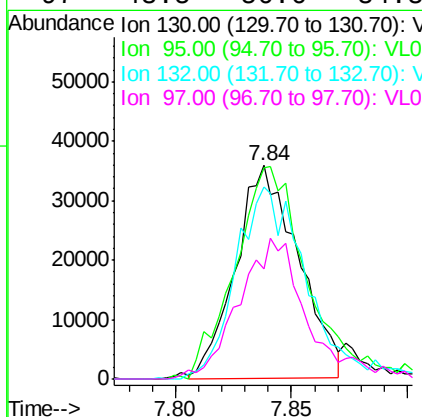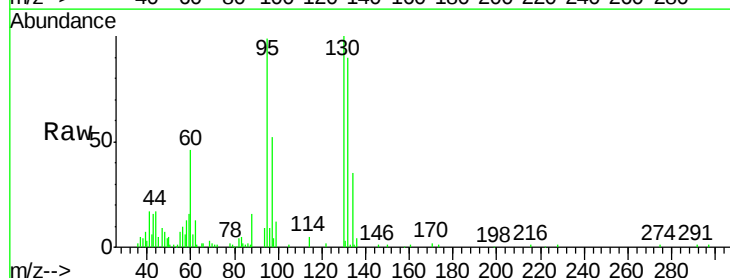







#50
4-Methyl-2-Pentanone
Concen: 0.617 ppbv m
RT: 8.75 min Scan# 1855
Delta R.T. 0.03 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion	Ratio	Lower	Upper
43	100		
58	32.4	29.9	44.9




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

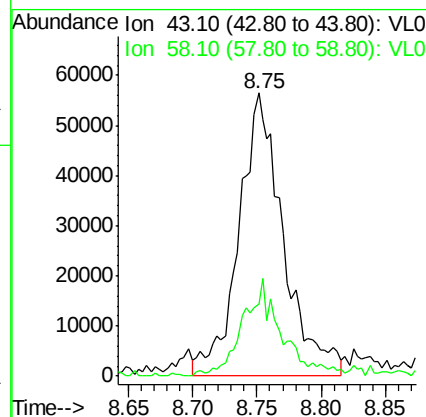

#51
2-Hexanone
Concen: 1.570 ppbv
RT: 10.14 min Scan# 2286
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion	Ratio	Lower	Upper
43	100		
58	42.2	41.0	61.6
98	0.9	0.3	0.5#

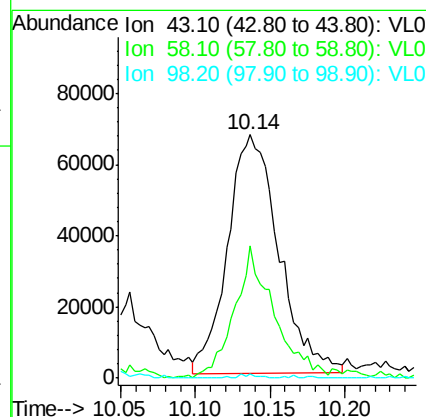







#52
Tetrachloroethene
Concen: 0.162 ppbv m
RT: 11.22 min Scan# 2623
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion	Ratio	Lower	Upper
164	100		
166	93.5	100.7	151.1#
129	66.8	80.9	121.3#
131	78.9	80.2	120.4#




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

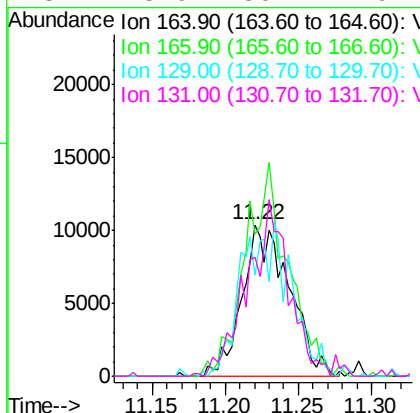

#53
Toluene
Concen: 1.260 ppbv
RT: 9.81 min Scan# 2184
Delta R.T. 0.03 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion	Ratio	Lower	Upper
91	100		
92	59.8	48.8	73.2

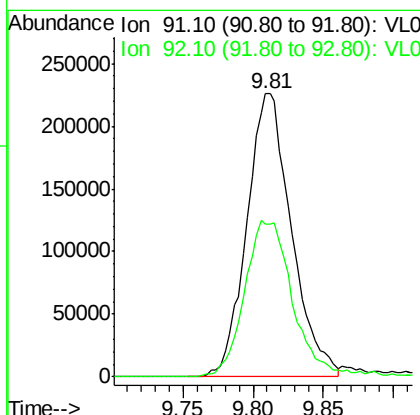



#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.09 min Scan# 2893

Delta R.T. 0.03 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Instrument :

MSVOA_L

ClientSampleId :

SR-SG-2

Tot Ion:117 Resp: 3546399

Ion Ratio Lower Upper


117 100

82 66.5 52.9 79.3

119 33.5 24.8 37.2

Manual Integrations
APPROVED




MMDadoda
8/20/2021 6:31:10 PM



Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

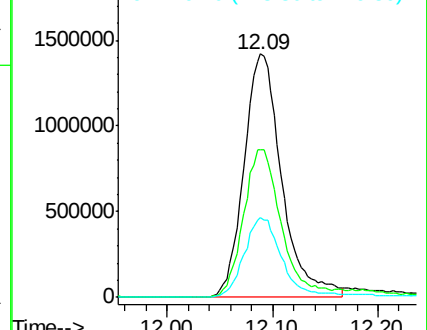

#58

Ethyl Benzene

Concen: 0.820 ppbv

RT: 12.71 min Scan# 3087

Delta R.T. 0.02 min

Lab File: VL037501.D


Acq: 19 Aug 2021 16:37

Tgt Ion: 91 Resp: 403542

Ion Ratio Lower Upper



91 100


106 28.4 25.7 38.5



Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 106.10 (105.80 to 106.80): V

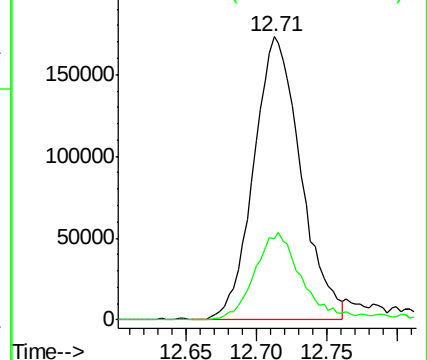







#59
m/p-Xylene
Concen: 4.045 ppbv
RT: 12.97 min Scan# 3167
Delta R.T. -0.00 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion: 91 Resp: 1725818
Ion Ratio Lower Upper
91 100
106 51.5 36.9 55.3




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

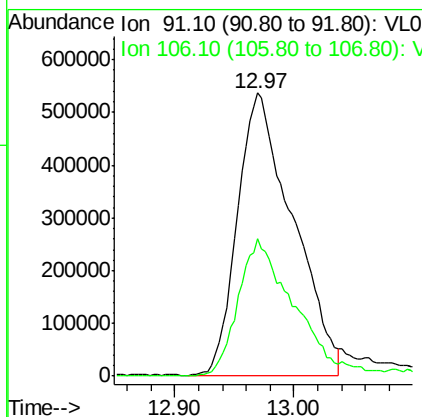

#60
o-Xylene
Concen: 1.224 ppbv
RT: 13.69 min Scan# 3392
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion: 91 Resp: 487474
Ion Ratio Lower Upper
91 100
106 46.2 23.7 71.1

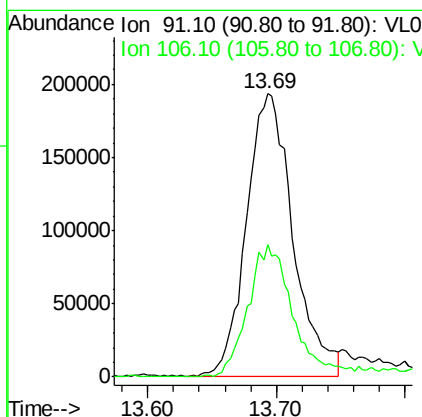







#61
Stvrene
Concen: 0.281 ppbv m
RT: 13.53 min Scan# 3341
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion	Ratio	Lower	Upper
104	100		
78	54.6	41.3	61.9
103	45.8	39.4	59.0




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

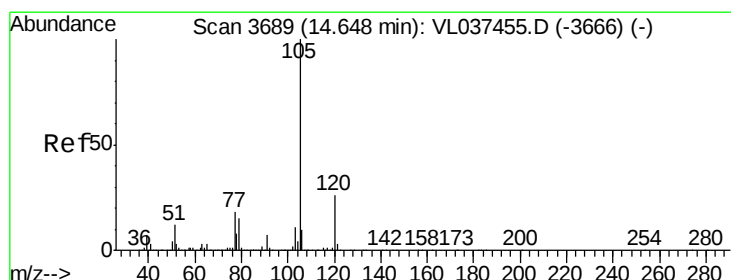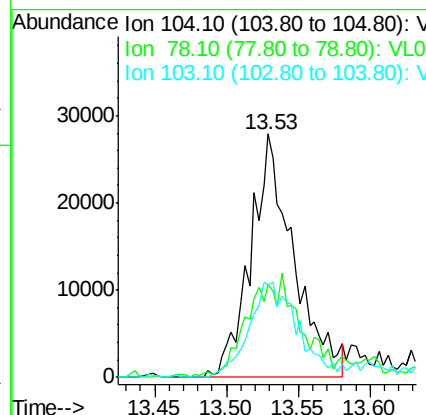

#62
Isopropylbenzene
Concen: 2.014 ppbv
RT: 14.67 min Scan# 3696
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion	Ratio	Lower	Upper
105	100		
120	28.7	21.5	32.3

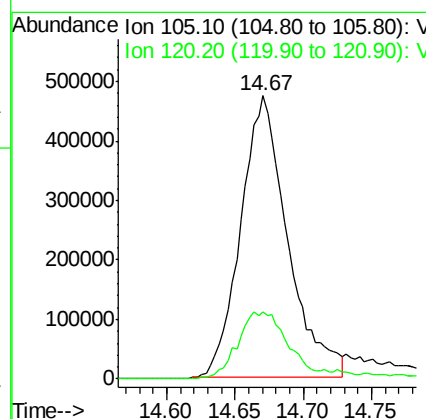







#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.817 ppbv
 RT: 14.42 min Scan# 3617
 Delta R.T. 0.02 min
 Lab File: VL037501.D
 Acq: 19 Aug 2021 16:37

Instrument :
 MSVOA_L
 ClientSampleId :
 SR-SG-2

Tot Ion: 95 Resp: 2473530
 Ion Ratio Lower Upper
 95 100
 174 78.1 59.6 89.4
 175 5.9 4.6 7.0




Manual Integrations
 APPROVED


MMDadoda
 8/20/2021 6:31:10 PM

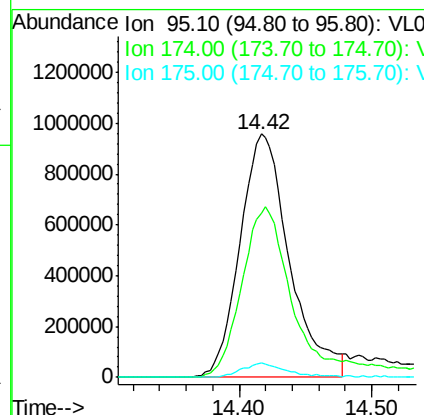

#69
 p-Isopropyltoluene
 Concen: 0.160 ppbv m
 RT: 17.65 min Scan# 4622
 Delta R.T. 0.02 min
 Lab File: VL037501.D
 Acq: 19 Aug 2021 16:37

Tgt Ion: 119 Resp: 93041
 Ion Ratio Lower Upper
 119 100
 134 26.2 21.1 31.7
 91 0.0 22.4 33.6#

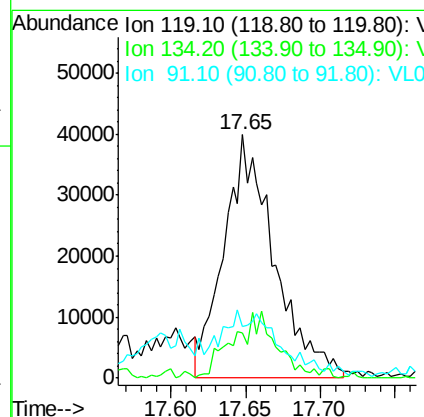

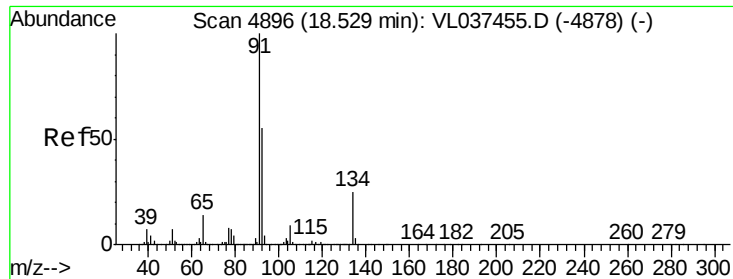





#70
n-Butylbenzene
Concen: 0.155 ppbv m
RT: 18.55 min Scan# 4903
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-2

Tot Ion	Ratio	Lower	Upper
91	100		
92	0.0	44.0	66.0#
134	59.9	19.5	29.3#




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:10 PM

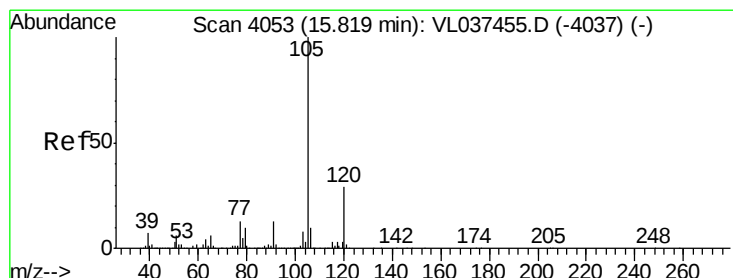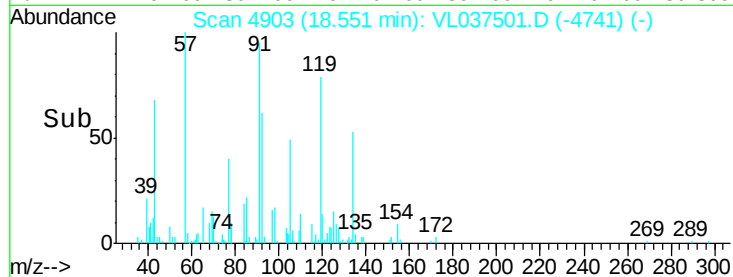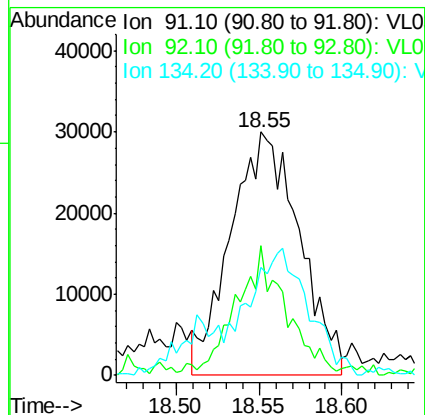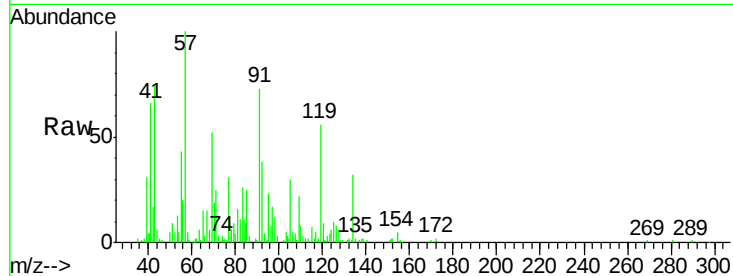

#72
4-Ethyltoluene
Concen: 0.119 ppbv m
RT: 15.84 min Scan# 4060
Delta R.T. 0.02 min
Lab File: VL037501.D
Acq: 19 Aug 2021 16:37

Tgt Ion	Ratio	Lower	Upper
105	100		
120	0.0	24.7	37.1#
91	0.0	9.8	14.8#
77	0.0	10.6	15.8#

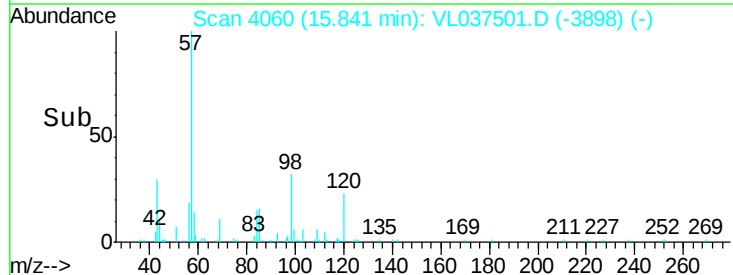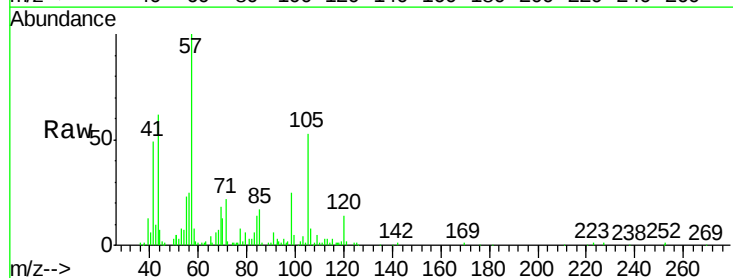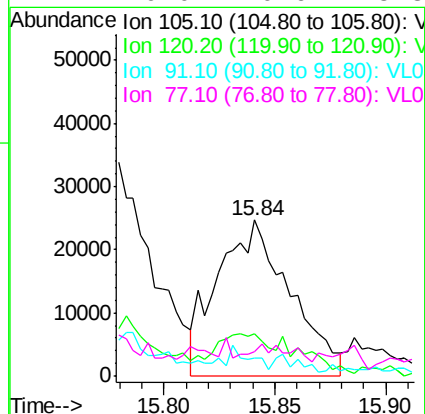

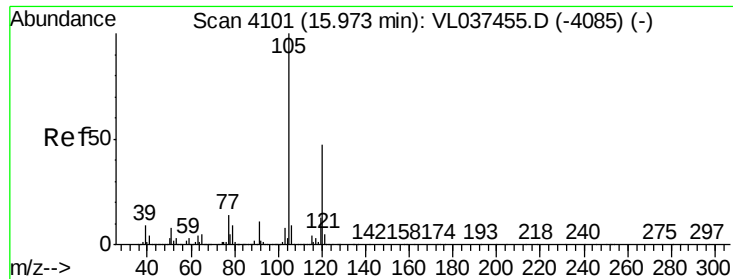





#73
 1,3,5-Trimethylbenzene
 Concen: 0.168 ppbv
 RT: 16.00 min Scan# 4109
 Delta R.T. 0.03 min
 Lab File: VL037501.D
 Acq: 19 Aug 2021 16:37

Instrument :
 MSVOA_L
 ClientSampleId :
 SR-SG-2

Tot Ion	Ratio	Lower	Upper
105	100		
120	46.9	37.6	56.4




Manual Integrations
 APPROVED


MMDadoda
 8/20/2021 6:31:10 PM

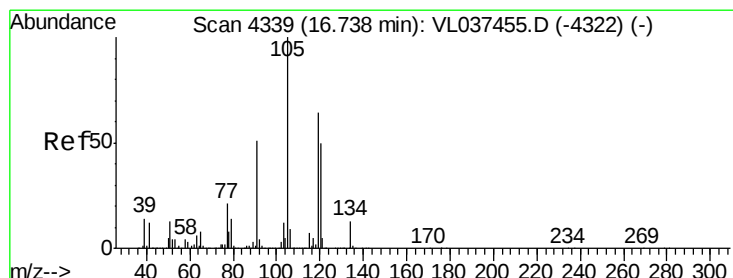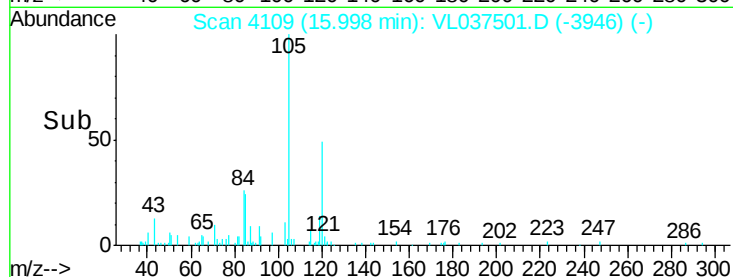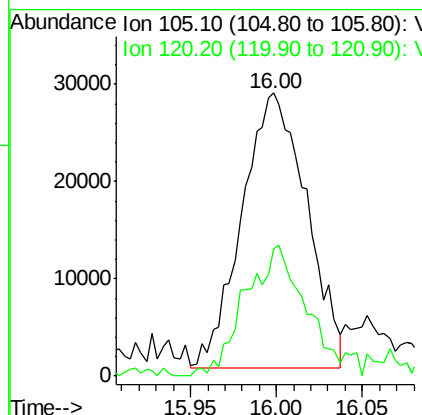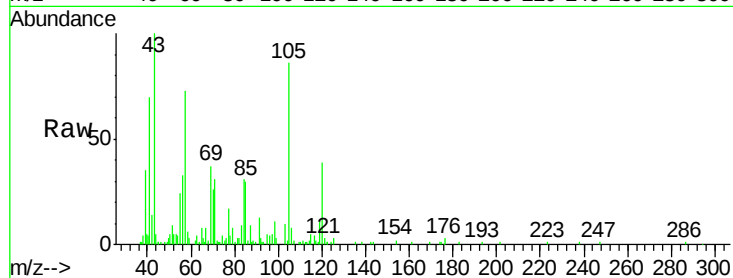

#74
 1,2,4-Trimethylbenzene
 Concen: 0.532 ppbv
 RT: 16.76 min Scan# 4347
 Delta R.T. 0.03 min
 Lab File: VL037501.D
 Acq: 19 Aug 2021 16:37

Tgt Ion	Ratio	Lower	Upper
105	100		
120	42.1	40.4	60.6
91	11.1	44.6	67.0#
77	17.4	17.8	26.6#

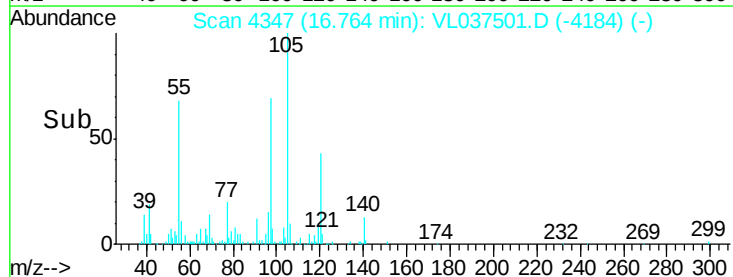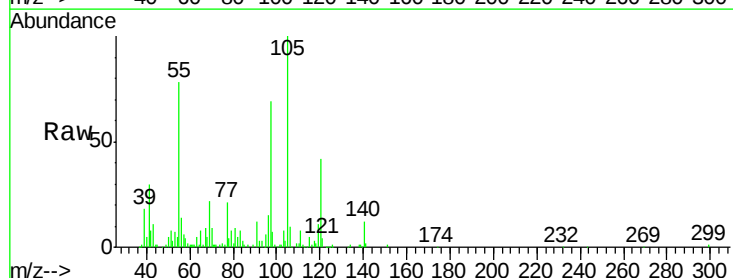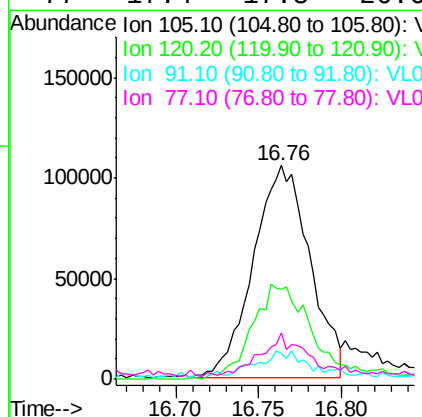



#79

Naphthalene

Concen: 0.744 ppbv

RT: 22.19 min Scan# 6035

Delta R.T. 0.03 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Instrument :

MSVOA_L





ClientSampleId :

SR-SG-2

Tot Ion	Ratio	Resp	Lower	Upper
128	100	233205		
127	14.3	9.4	14.2#	
129	8.3	8.8	13.2#	

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:10 PM

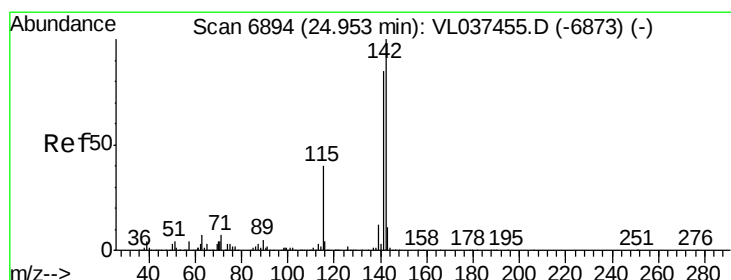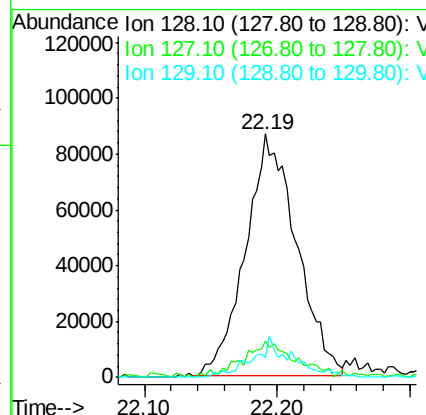

#80

Naphthalene, 2-methyl-

Concen: 0.271 ppbv

RT: 24.97 min Scan# 6900

Delta R.T. 0.02 min

Lab File: VL037501.D

Acq: 19 Aug 2021 16:37

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	23661		
141	95.0	64.7	97.1	
115	56.8	28.4	42.6#	

