

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL081921\
 Data File : VL037507.D
 Acq On : 19 Aug 2021 20:33
 Operator : SY/AP
 Sample : M3480-05
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SR-SG-5

Manual Integrations
 APPROVED

MMDadoda
 8/20/2021 6:31:20 PM

Quant Time: Aug 20 15:06:00 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL081621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 2021
 QLast Update : Tue Aug 17 02:13:47 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	1419813	10.00	ppbv	0.02
33) 1,4-Difluorobenzene	7.18	114	4075670	10.00	ppbv	0.02
55) Chlorobenzene-d5	12.09	117	3486874	10.00	ppbv	0.03

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.42	95	2397675	9.68	ppbv	0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.80%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.06	85	46857	0.206	ppbv	93
3) Chlorodifluoromethane	2.98	51	2374813m	8.735	ppbv	
9) Propene	3.01	41	201479	2.071	ppbv	96
10) Heptane	8.12	43	24644m	0.110	ppbv	
11) Trichlorofluoromethane	3.96	101	58922	0.276	ppbv	97
13) Ethanol	3.61	45	3443099	363.738	ppbv	95
15) Acetone	3.85	43	11090171	76.750	ppbv	99
17) tert-Butyl alcohol	4.30	59	393378	2.980	ppbv	97
19) Isopropyl Alcohol	3.97	45	925463	11.179	ppbv #	1
20) Methylene Chloride	4.35	84	3014822	41.672	ppbv	99
26) Hexane	5.69	57	2308736	12.873	ppbv #	46
27) Carbon Disulfide	4.56	76	93643	0.586	ppbv #	93
29) Chloroform	5.76	83	215404	0.847	ppbv	99
30) Cyclohexane	7.14	84	27478m	0.184	ppbv	
31) cis-1,2-Dichloroethene	5.55	61	234123m	1.442	ppbv	
32) 1,1,1-Trichloroethane	6.51	97	20177m	0.081	ppbv	
34) 2-Butanone	5.25	43	1023815	6.152	ppbv	96
35) Carbon Tetrachloride	7.03	117	19455m	0.081	ppbv	
36) Benzene	6.90	78	50242m	0.147	ppbv	
38) Trichloroethene	7.84	130	1392791	9.908	ppbv	96
40) 1,4-Dioxane	7.84	88	52420m	1.625	ppbv	
41) Tetrahydrofuran	6.06	42	84689m	1.056	ppbv	
44) 2,2,4-Trimethylpentane	7.87	57	58347m	0.101	ppbv	
50) 4-Methyl-2-Pentanone	8.76	43	102064m	0.470	ppbv	
51) 2-Hexanone	10.15	43	67800m	0.679	ppbv	
52) Tetrachloroethene	11.23	164	184837m	1.317	ppbv	
53) Toluene	9.81	91	166838	0.426	ppbv	95
59) m/p-Xylene	12.98	91	56161m	0.134	ppbv	
79) Naphthalene	22.19	128	713931m	2.316	ppbv	
80) Naphthalene, 2-methyl-	24.97	142	9901	0.115	ppbv #	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL081921\
Data File : VL037507.D
Acq On : 19 Aug 2021 20:33
Operator : SY/AP
Sample : M3480-05
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:20 PM

Quant Time: Aug 20 15:06:00 2021
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL081621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug
QLast Update : Tue Aug 17 02:13:47 2021
Response via : Initial Calibration

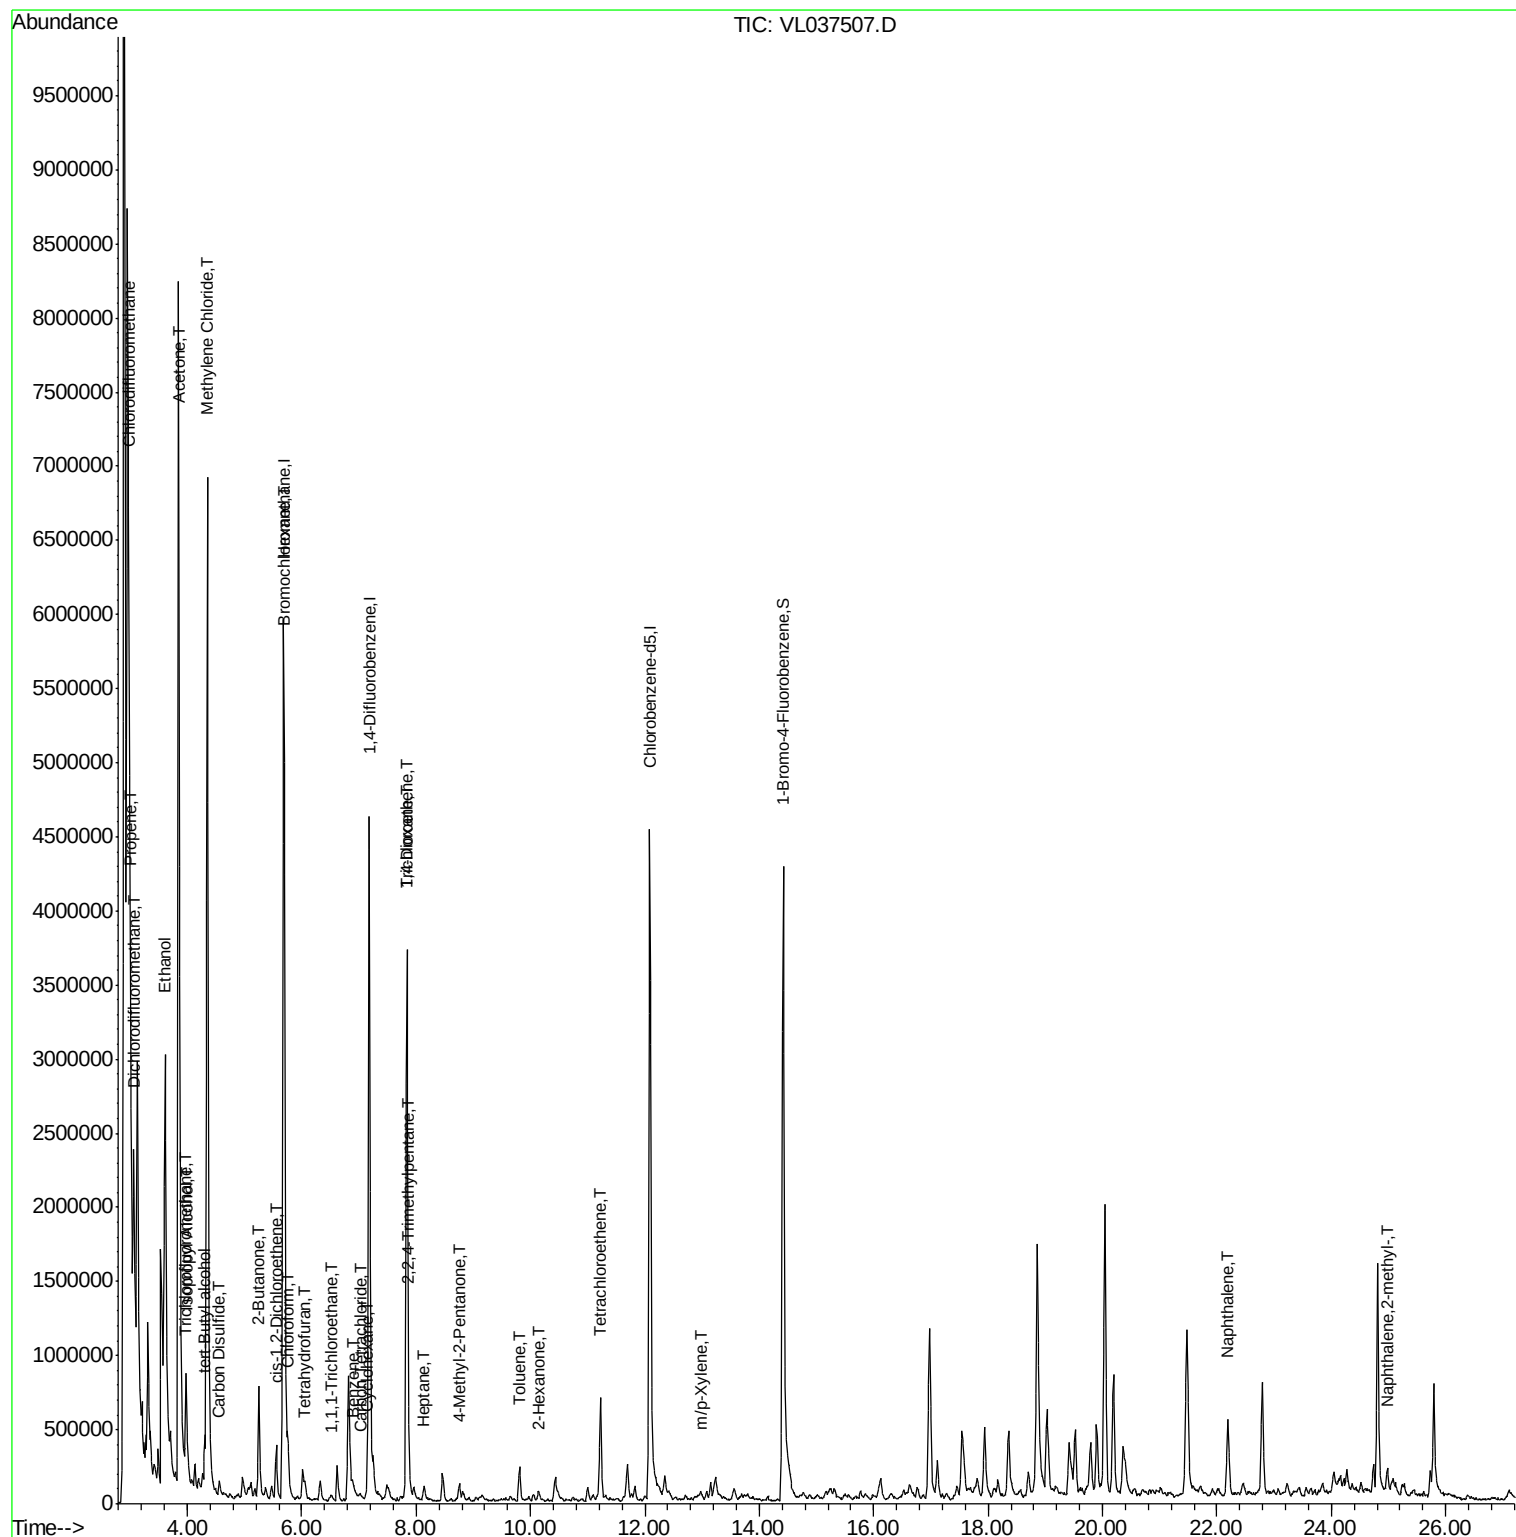

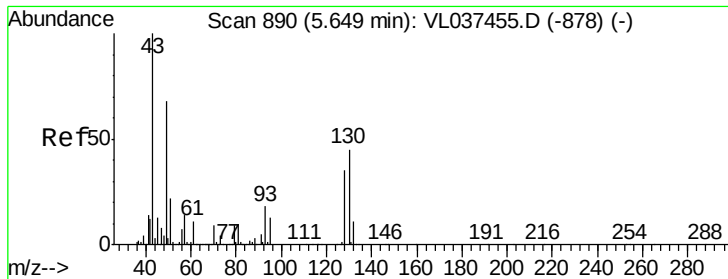

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.67 min Scan# 897

Delta R.T. 0.02 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33

Instrument :

MSVOA_L

ClientSampled :

SR-SG-5

Tot Ion: 49 Resp: 1419813

Ion Ratio Lower Upper





49 100

128 53.2 27.5 82.4

130 67.1 34.0 101.8

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:20 PM

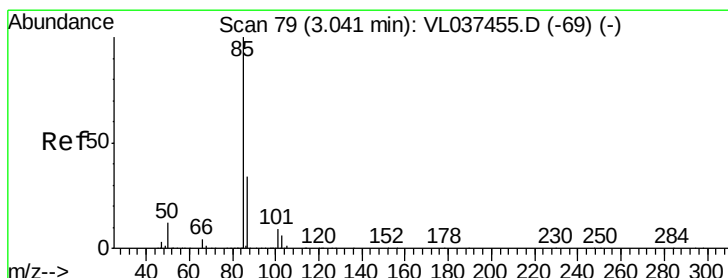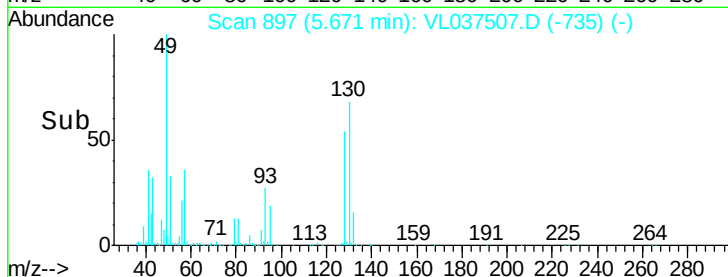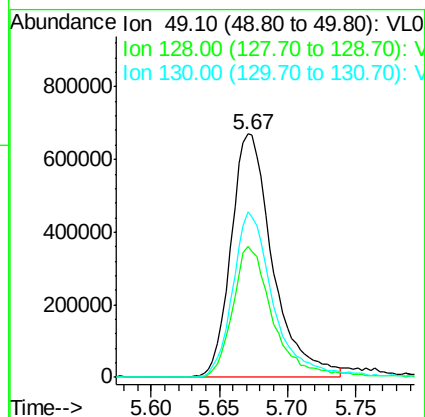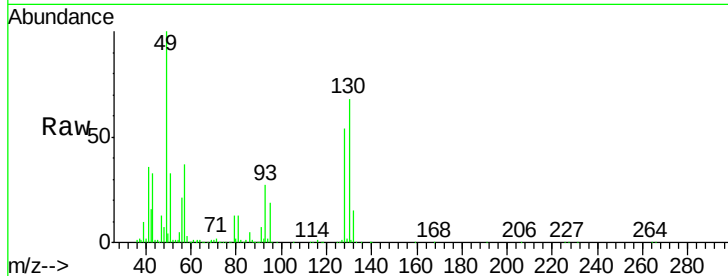

#2

Dichlorodifluoromethane

Concen: 0.206 ppbv

RT: 3.06 min Scan# 84

Delta R.T. 0.02 min

Lab File: VL037507.D




Acq: 19 Aug 2021 20:33


Tgt Ion: 85 Resp: 46857

Ion Ratio Lower Upper

85 100

87 30.7 27.6 41.4

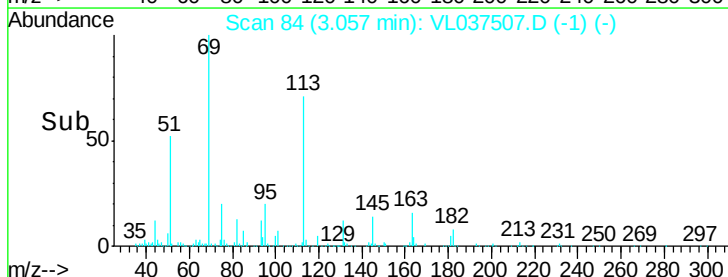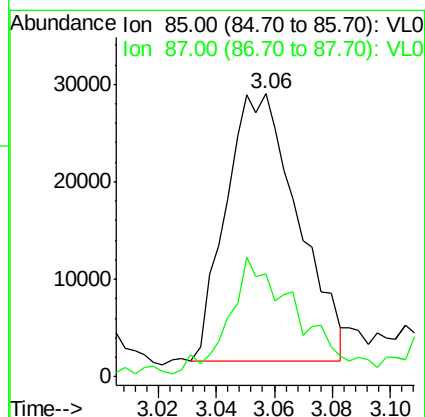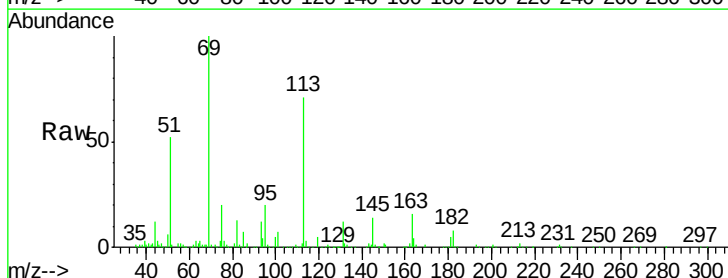



#3

Chlorodifluoromethane

Concen: 8.735 ppbv

RT: 2.98 min Scan# 60

Delta R.T. -0.00 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33

Instrument :

MSVOA_L

ClientSampleId :

SR-SG-5

Tot Ion: 51 Resp: 2374813


Ion Ratio Lower Upper

51 100

67 4.4 14.2 21.2#




Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:20 PM



Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

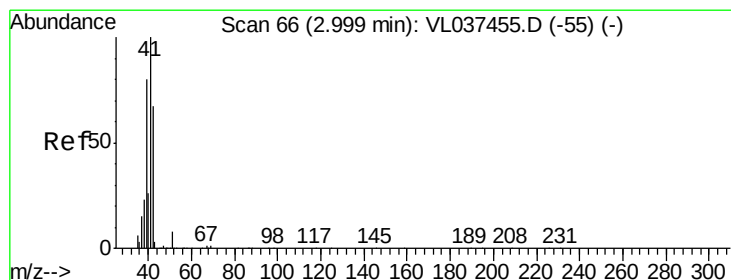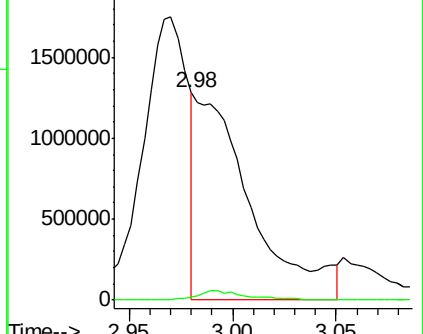

#9

Propene

Concen: 2.071 ppbv

RT: 3.01 min Scan# 70

Delta R.T. 0.01 min

Lab File: VL037507.D


Acq: 19 Aug 2021 20:33

Tgt Ion: 41 Resp: 201479

Ion Ratio Lower Upper



41 100


42 64.3 53.7 80.5



Abundance Ion 41.10 (40.80 to 41.80): VL0

Ion 42.10 (41.80 to 42.80): VL0

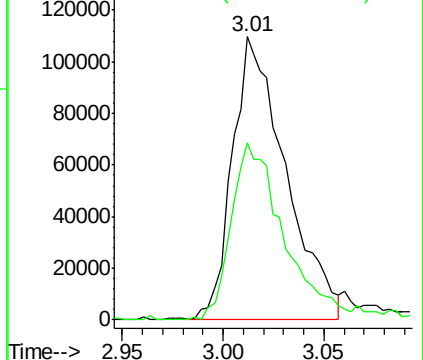







#10
 Heptane
 Concen: 0.110 ppbv m
 RT: 8.12 min Scan# 1659
 Delta R.T. 0.02 min
 Lab File: VL037507.D
 Acq: 19 Aug 2021 20:33

Instrument :
 MSVOA_L
 ClientSampled :
 SR-SG-5

Tot Ion: 43 Resp: 24644
 Ion Ratio Lower Upper
 43 100
 57 0.0 41.0 61.6#




Manual Integrations
 APPROVED


MMDadoda
 8/20/2021 6:31:20 PM

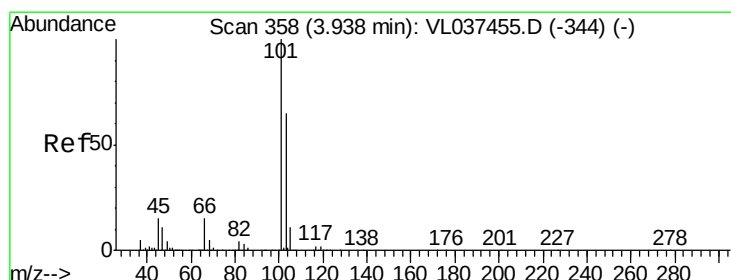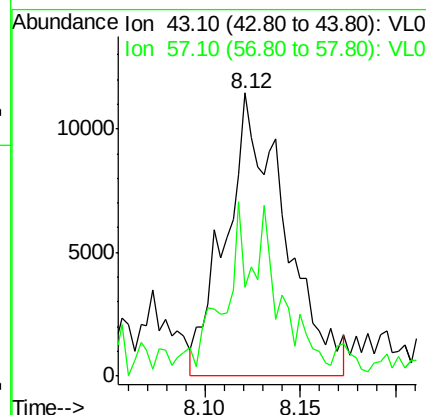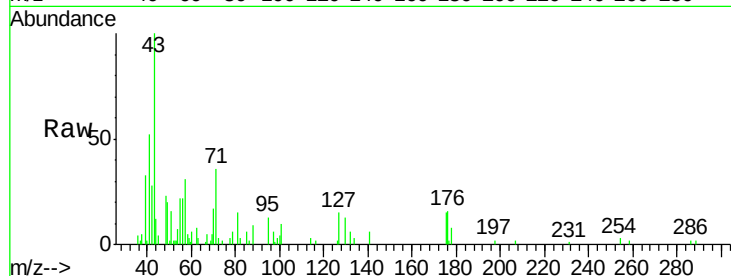

#11
 Trichlorofluoromethane
 Concen: 0.276 ppbv
 RT: 3.96 min Scan# 364
 Delta R.T. 0.02 min
 Lab File: VL037507.D
 Acq: 19 Aug 2021 20:33

Tgt Ion: 101 Resp: 58922
 Ion Ratio Lower Upper
 101 100
 103 67.3 51.8 77.6

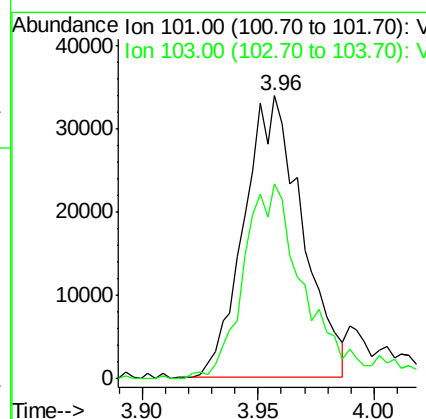







#13
Ethanol
Concen: 363.738 ppbv
RT: 3.61 min Scan# 257
Delta R.T. 0.01 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion: 45 Resp: 3443099
Ion Ratio Lower Upper
45 100
46 38.2 14.1 56.5




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:20 PM

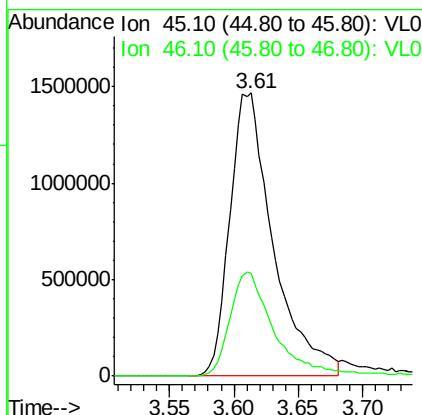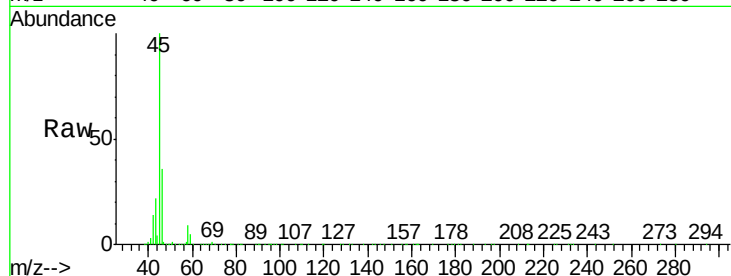

#15
Acetone
Concen: 76.750 ppbv
RT: 3.85 min Scan# 330
Delta R.T. 0.01 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion: 43 Resp: 11090171
Ion Ratio Lower Upper
43 100
58 31.4 24.8 37.2

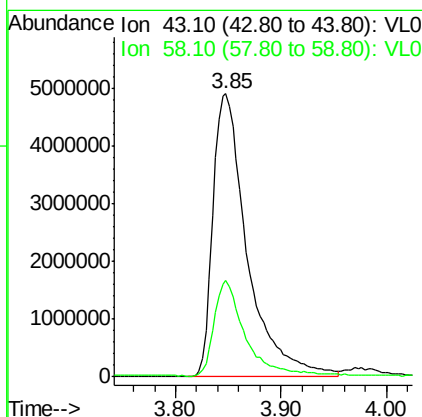

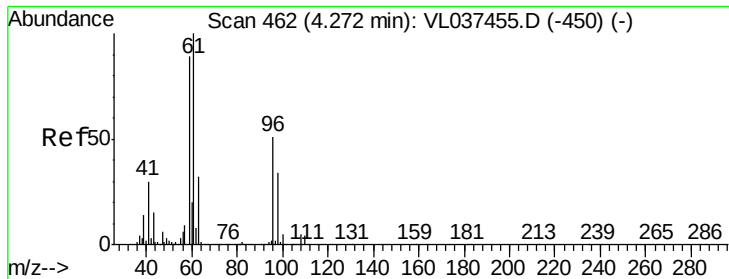

#17





tert-Butyl alcohol
Concen: 2.980 ppbv
RT: 4.30 min Scan# 472
Delta R.T. 0.03 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion	Ratio	Lower	Upper
59	100		
57	11.6	8.3	12.5

Manual Integrations
APPROVED




MMDadoda
8/20/2021 6:31:20 PM

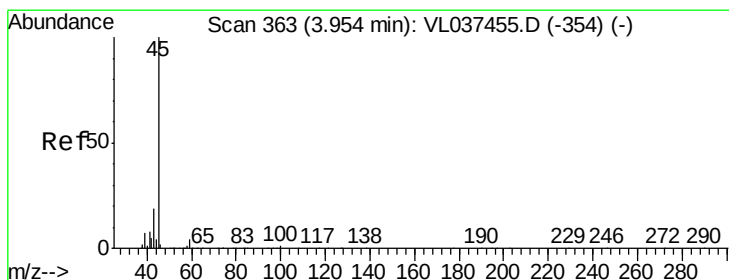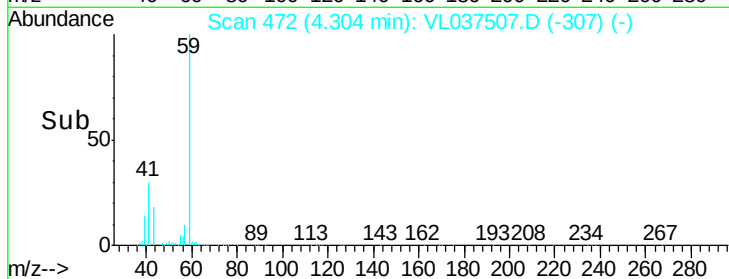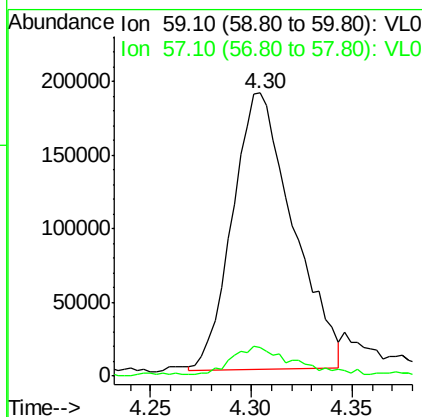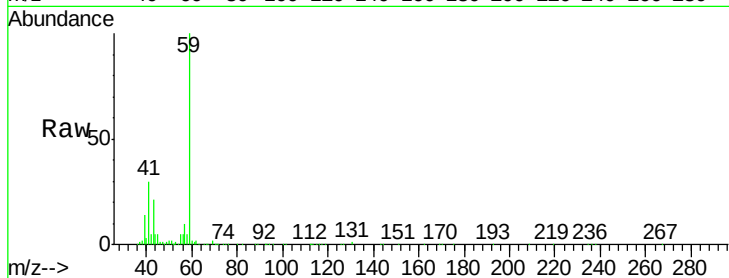


#19

Isopropyl Alcohol
Concen: 11.179 ppbv
RT: 3.97 min Scan# 369
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion	Ratio	Lower	Upper
45	100		
58	376.4	1.4	2.2#

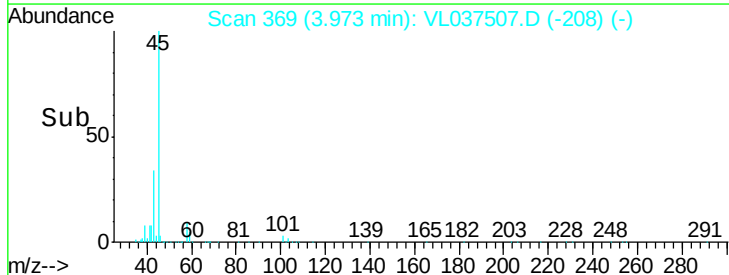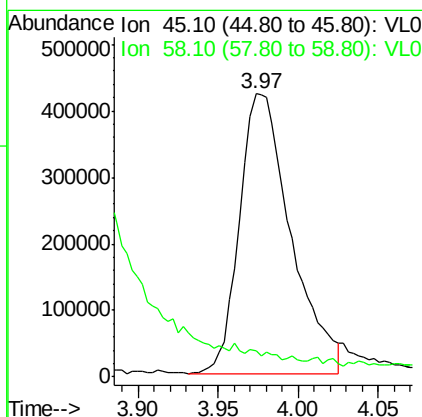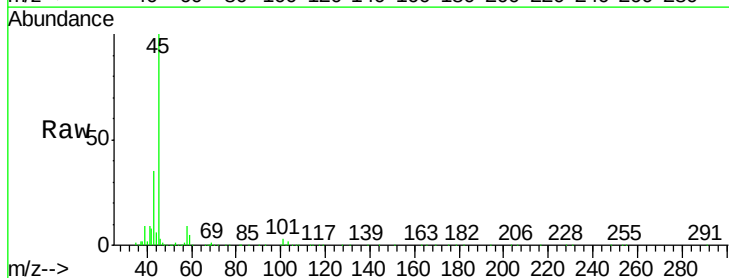

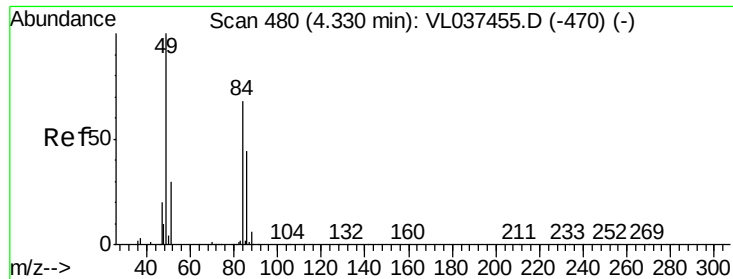





#20
Methvlene Chloride
Concen: 41.672 ppbv
RT: 4.35 min Scan# 486
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion	Ratio	Lower	Upper
84	100		
49	149.6	118.2	177.2
51	47.3	36.6	55.0
86	64.5	51.8	77.6




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:20 PM

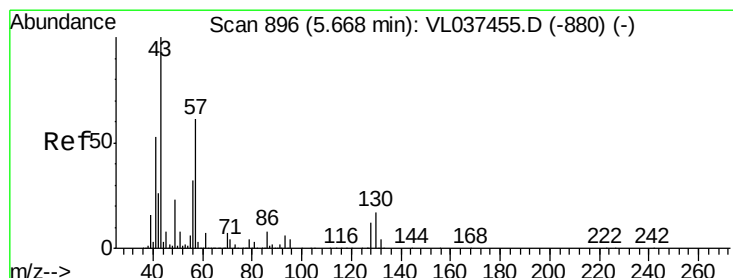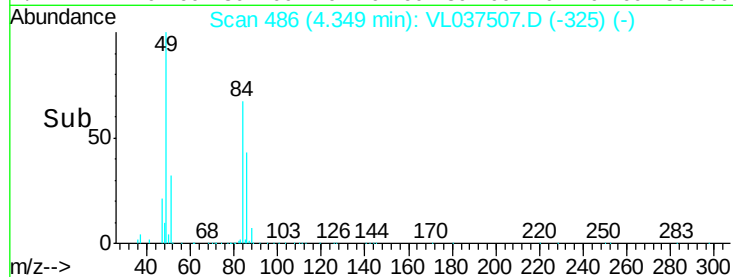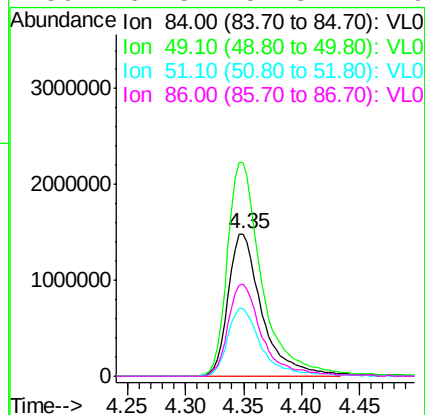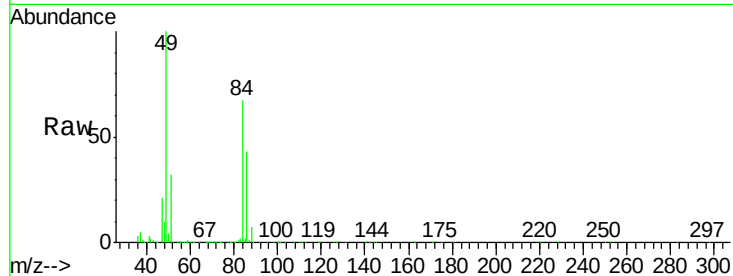

#26
Hexane
Concen: 12.873 ppbv
RT: 5.69 min Scan# 903
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion	Ratio	Lower	Upper
57	100		
41	87.7	72.3	108.5
43	73.8	172.3	258.5#
56	53.2	42.8	64.2

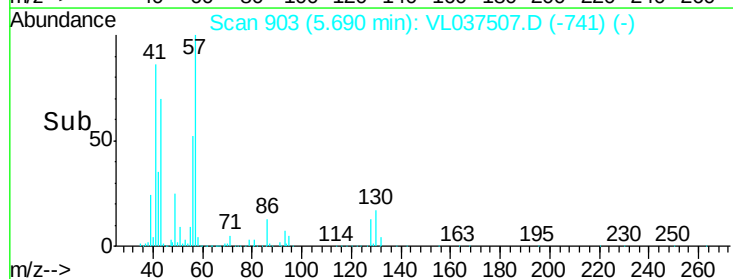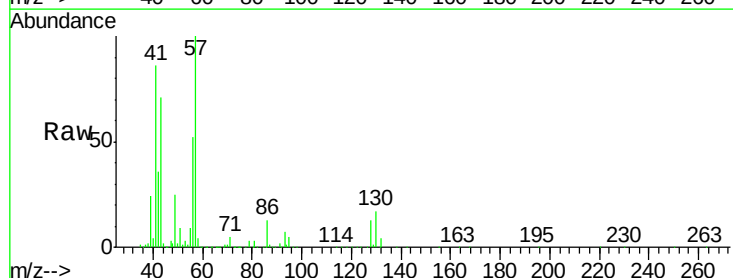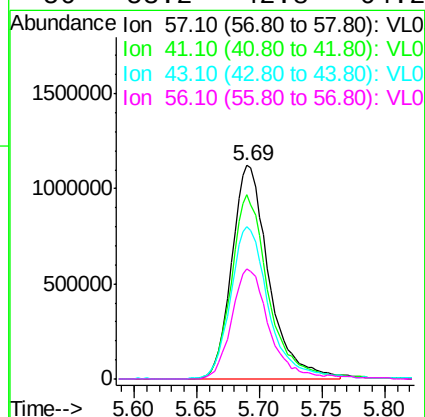







#27
Carbon Disulfide
Concen: 0.586 ppbv
RT: 4.56 min Scan# 550
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion	Ratio	Lower	Upper
76	100		
44	22.1	13.9	20.9#
78	9.6	7.9	11.9




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:20 PM

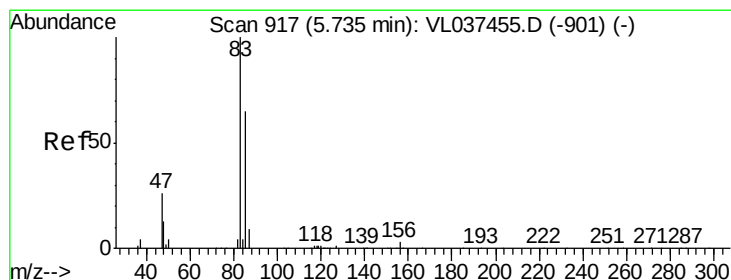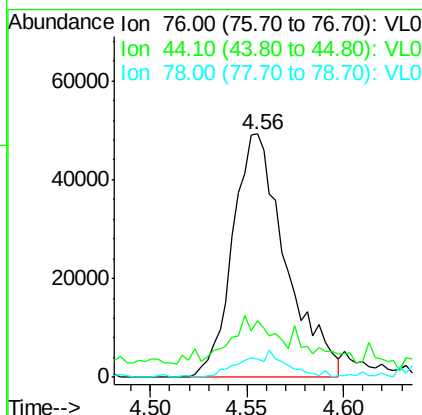

#29
Chloroform
Concen: 0.847 ppbv
RT: 5.76 min Scan# 924
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion	Ratio	Lower	Upper
83	100		
85	65.9	52.3	78.5

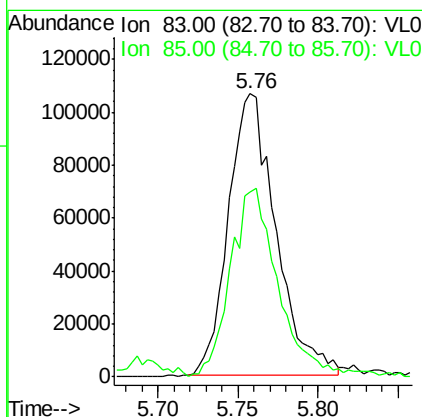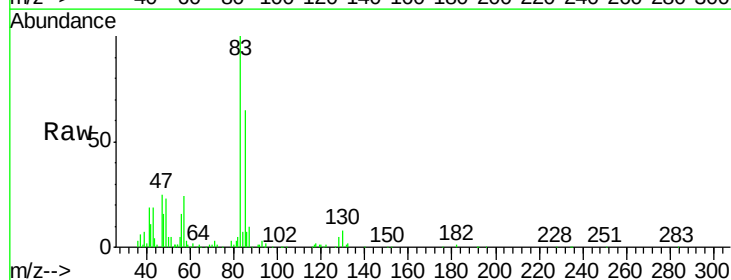

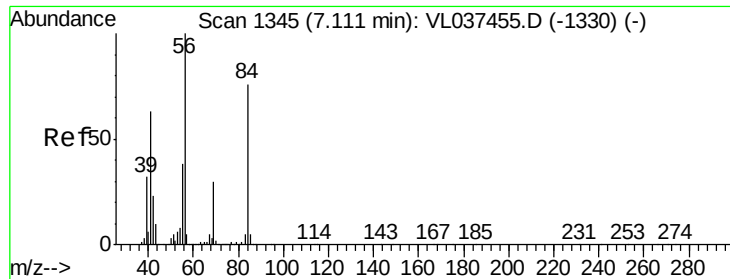





#30
Cyclohexane
Concen: 0.184 ppbv m
RT: 7.14 min Scan# 1353
Delta R.T. 0.03 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion	Ratio	Lower	Upper
84	100		
56	0.0	110.6	165.8#
41	108.0	67.0	100.6#




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:20 PM

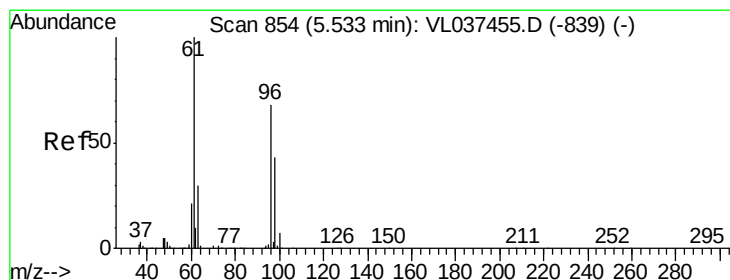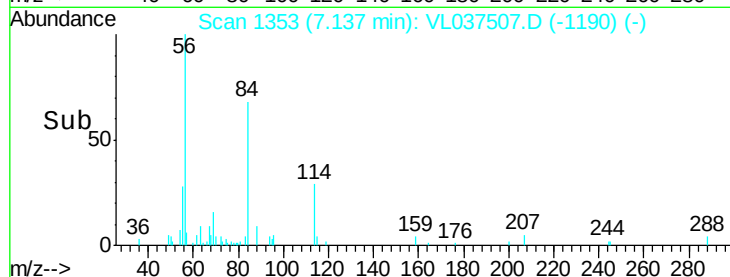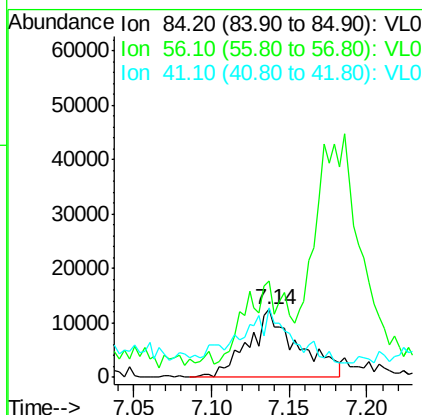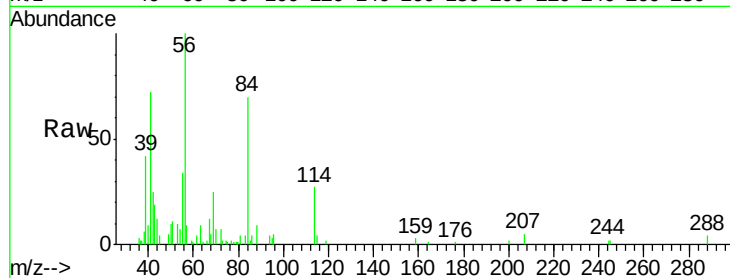

#31
cis-1,2-Dichloroethene
Concen: 1.442 ppbv m
RT: 5.55 min Scan# 860
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion	Ratio	Lower	Upper
61	100		
96	73.5	54.8	82.2
98	46.4	34.2	51.2

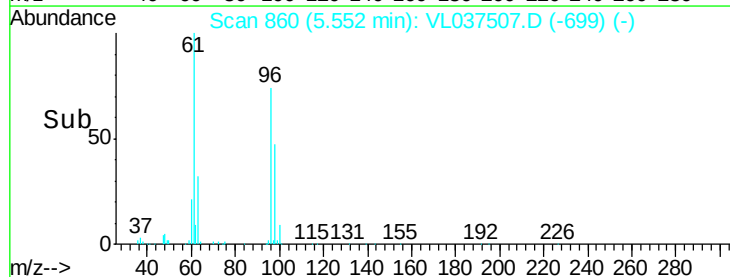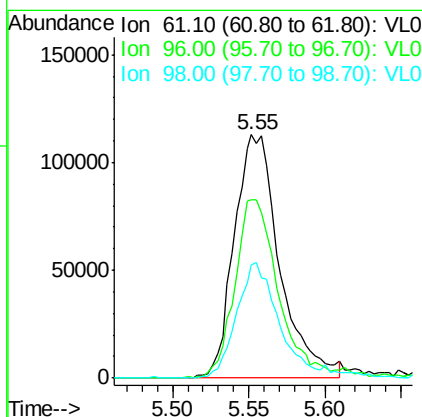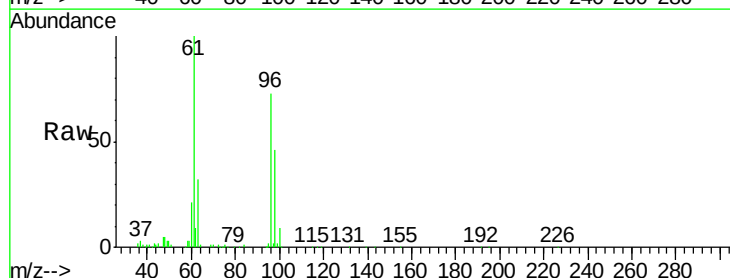



#32

1,1,1-Trichloroethane

Concen: 0.081 ppbv m

RT: 6.51 min Scan# 1159

Delta R.T. 0.02 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33

Instrument :

MSVOA_L

ClientSampleId :

SR-SG-5

Tot Ion: 97 Resp: 20177

Ion Ratio Lower Upper





97 100

99 0.0 51.8 77.6#

61 0.0 39.6 59.4#

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:20 PM

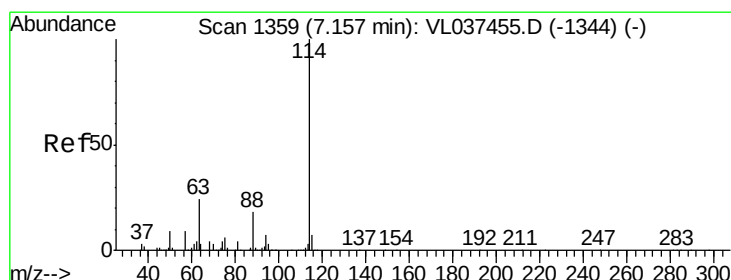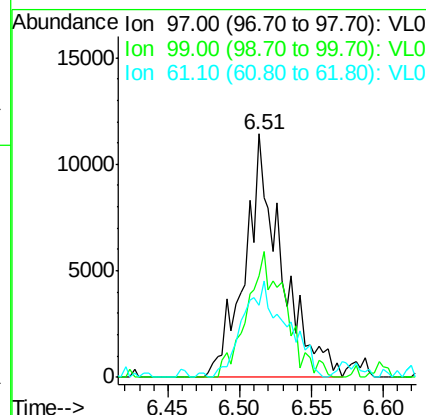

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.18 min Scan# 1366

Delta R.T. 0.02 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33




Tgt Ion: 114 Resp: 4075670


Ion Ratio Lower Upper

114 100

63 23.5 19.3 28.9

88 18.0 14.2 21.4

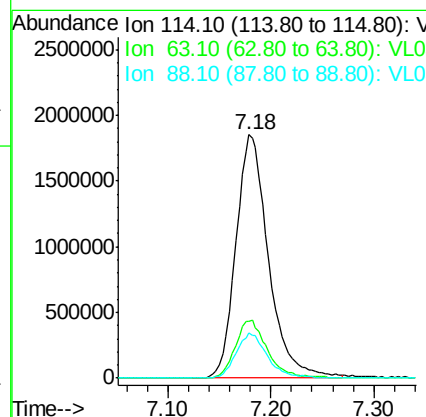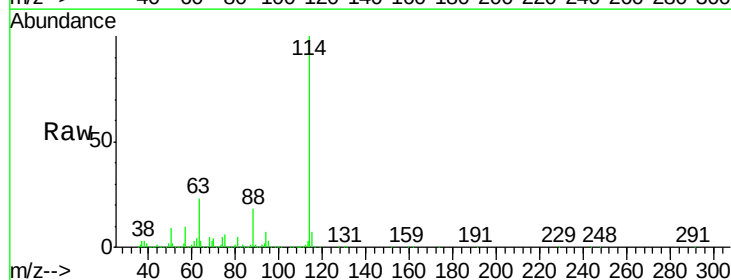

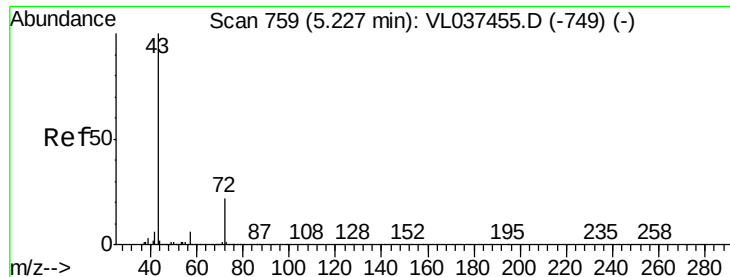

#34

2-Butanone

Concen: 6.152 ppbv

RT: 5.25 min Scan# 766

Delta R.T. 0.02 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33

Instrument :

MSVOA_L

ClientSampled :

SR-SG-5

Tot Ion: 43 Resp: 1023815


Ion Ratio Lower Upper

43 100

72 23.8 17.4 26.0




Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:20 PM

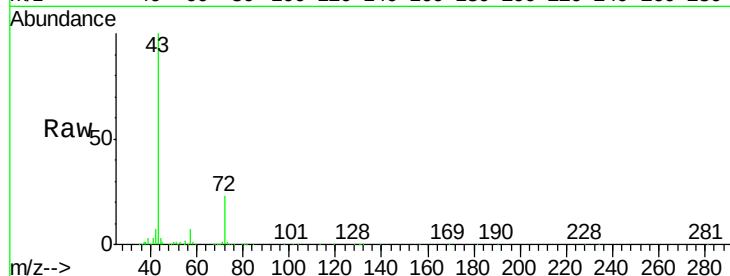

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 72.10 (71.80 to 72.80): VL0

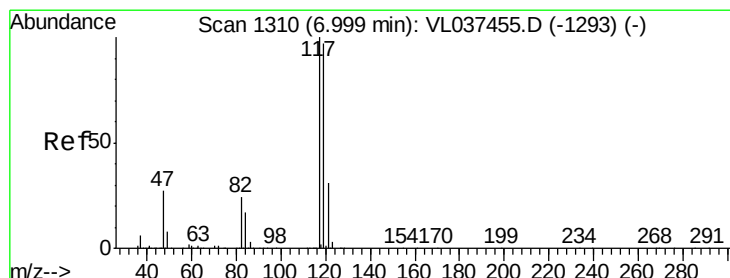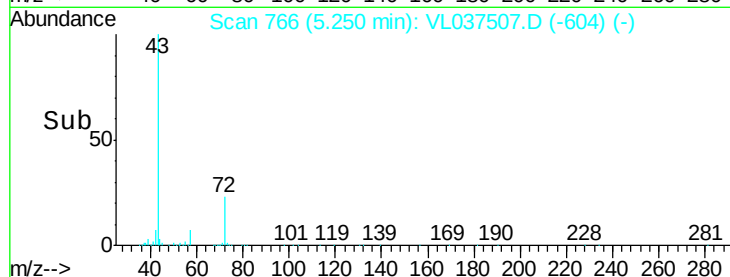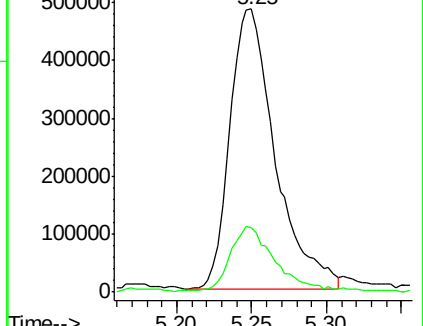

#35

Carbon Tetrachloride

Concen: 0.081 ppbv m

RT: 7.03 min Scan# 1319

Delta R.T. 0.03 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33


Tgt Ion: 117 Resp: 19455

Ion Ratio Lower Upper

117 100

119 58.8 77.3 115.9#



121 22.0 25.2 37.8#

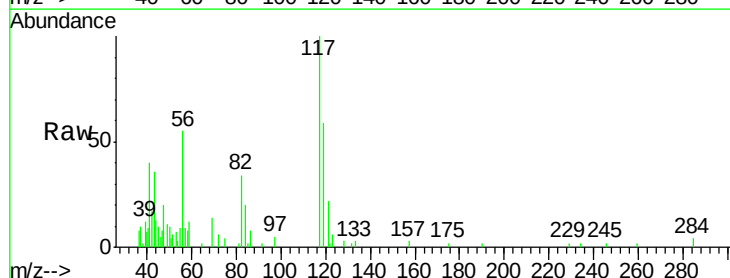


Abundance Ion 117.00 (116.70 to 117.70): V

Ion 119.00 (118.70 to 119.70): V

Ion 121.00 (120.70 to 121.70): V

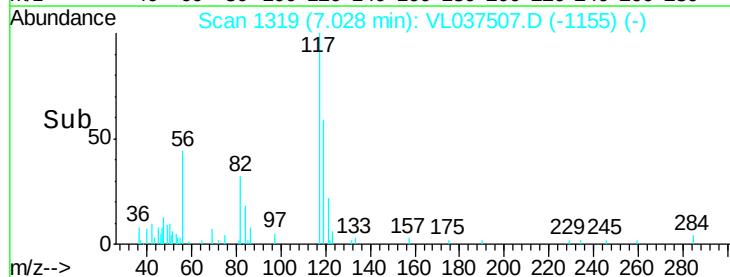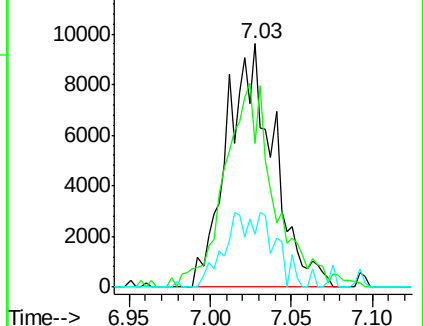







#36
Benzene
Concen: 0.147 ppbv m
RT: 6.90 min Scan# 1280
Delta R.T. 0.03 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion	Ratio	Lower	Upper
78	100		
77	16.9	18.2	27.4#
50	21.3	14.6	21.8




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:20 PM

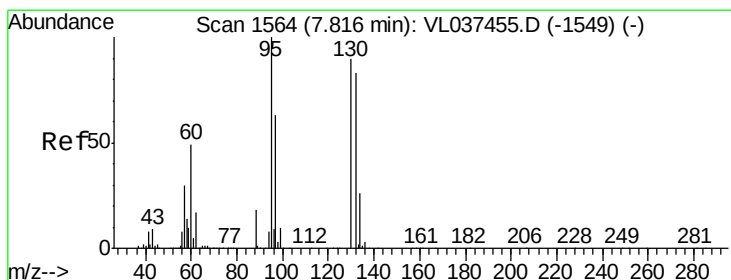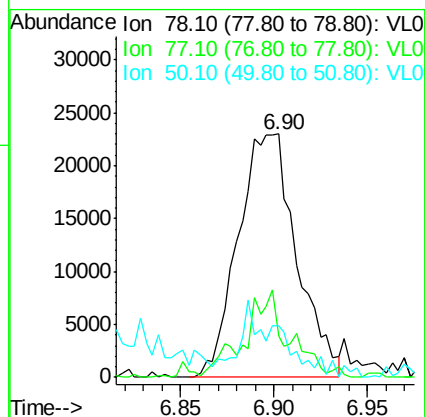

#38
Trichloroethene
Concen: 9.908 ppbv
RT: 7.84 min Scan# 1571
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion	Ratio	Lower	Upper
130	100		
95	108.1	89.2	133.8
132	99.0	74.0	111.0
97	69.8	56.6	84.8

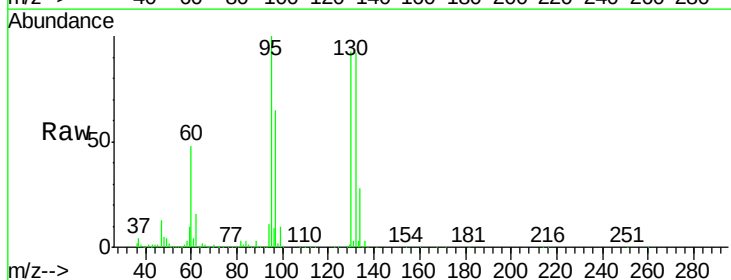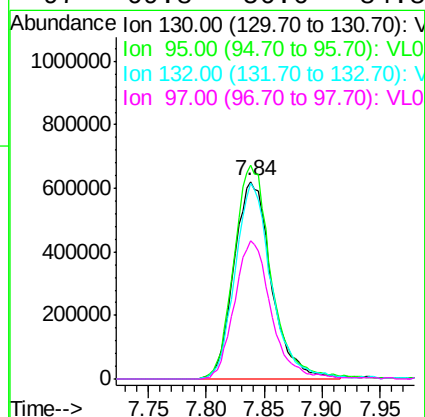







#40
1,4-Dioxane
Concen: 1.625 ppbv m
RT: 7.84 min Scan# 1573
Delta R.T. 0.03 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion	88	Resp	52420
Ion	Ratio	Lower	Upper
88	100		
58	92.6	0.0	0.0#
43	0.0	0.0	0.0
57	0.0	0.0	0.0




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:20 PM

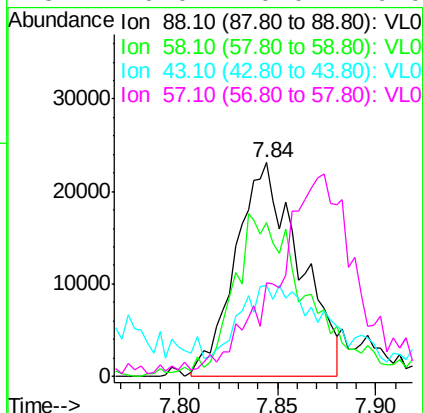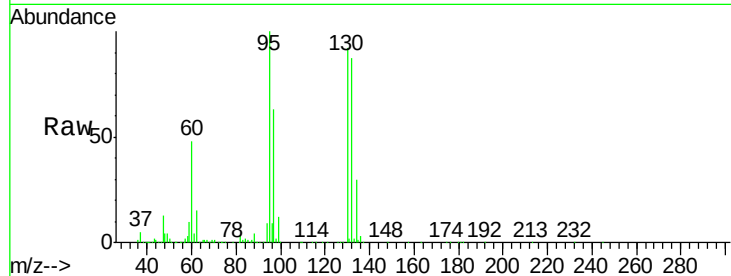

#41
Tetrahydrofuran
Concen: 1.056 ppbv m
RT: 6.06 min Scan# 1017
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion	42	Resp	84689
Ion	Ratio	Lower	Upper
42	100		
72	0.0	32.2	48.4#
71	0.0	30.5	45.7#

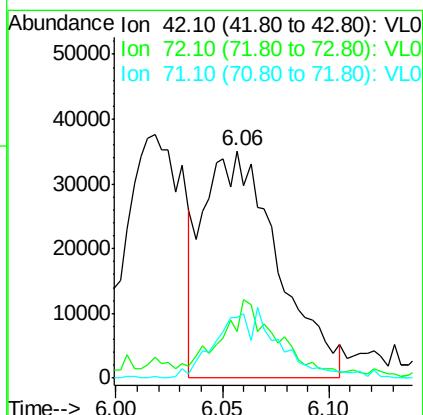

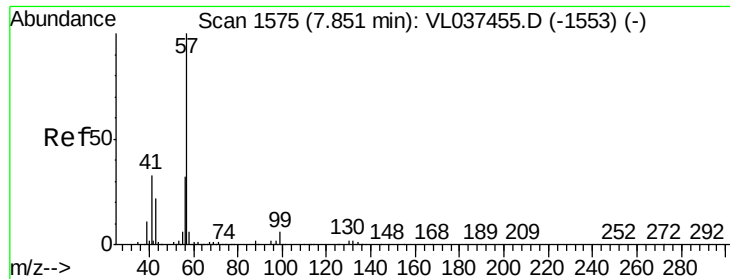





#44
 2,2,4-Trimethylpentane
 Concen: 0.101 ppbv m
 RT: 7.87 min Scan# 1582
 Delta R.T. 0.02 min
 Lab File: VL037507.D
 Acq: 19 Aug 2021 20:33

Instrument :
 MSVOA_L
 ClientSampleId :
 SR-SG-5

Tot Ion	Ratio	Lower	Upper
57	100		
41	33.6	26.2	39.4
56	36.2	25.4	38.2




Manual Integrations
 APPROVED


MMDadoda
 8/20/2021 6:31:20 PM

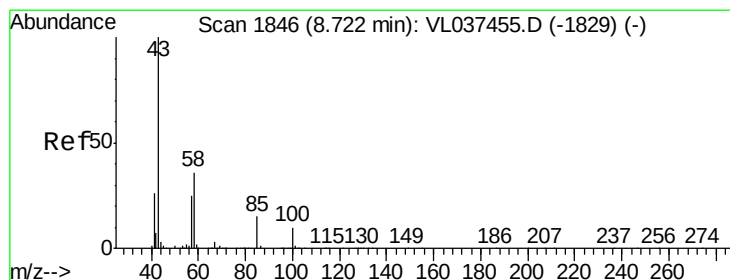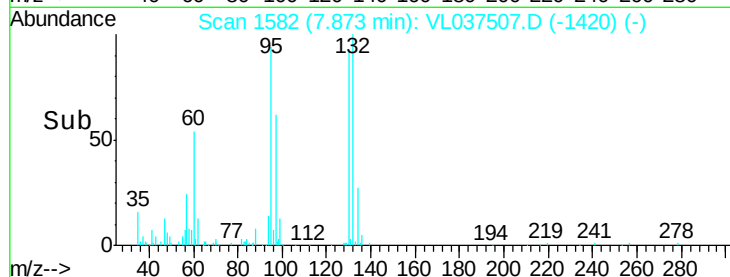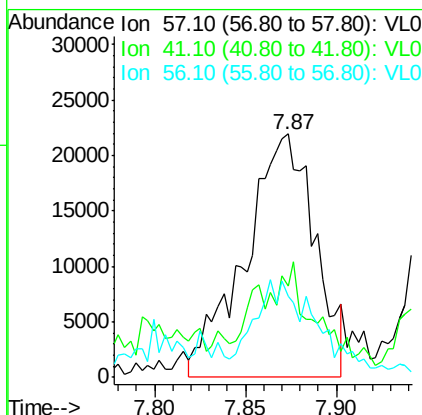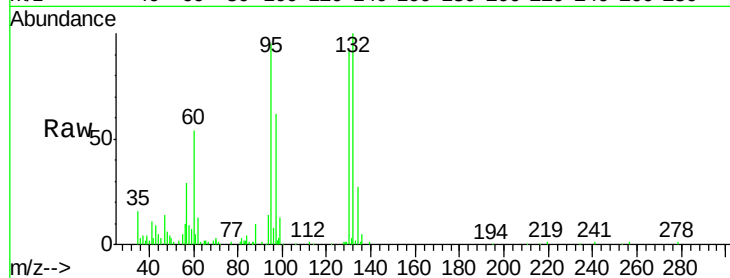

#50
 4-Methyl-2-Pentanone
 Concen: 0.470 ppbv m
 RT: 8.76 min Scan# 1858
 Delta R.T. 0.04 min
 Lab File: VL037507.D
 Acq: 19 Aug 2021 20:33

Tgt Ion	Ratio	Lower	Upper
43	100		
58	38.4	29.9	44.9

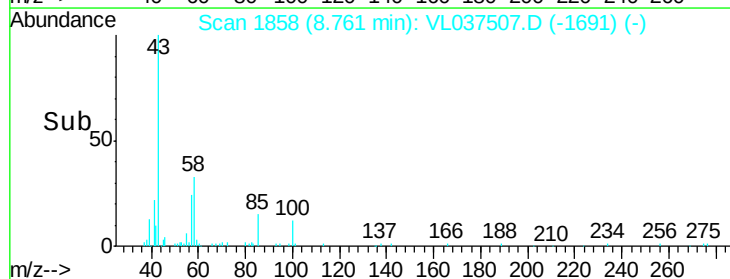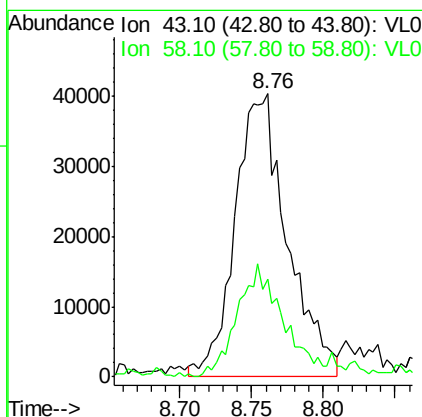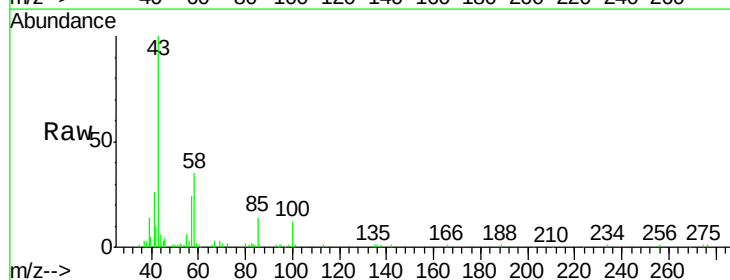

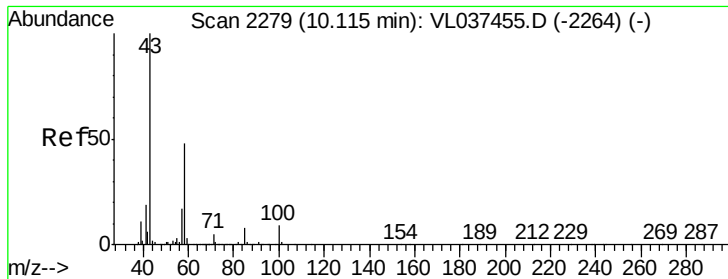

#51

2-Hexanone

Concen: 0.679 ppbv m

RT: 10.15 min Scan# 2289

Delta R.T. 0.03 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33

Instrument :

MSVOA_L





ClientSampleId :

SR-SG-5

Tot Ion:	43	Resp:	67800
Ion Ratio	Lower	Upper	
43	100		
58	0.0	41.0	61.6#
98	0.0	0.3	0.5#

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:20 PM

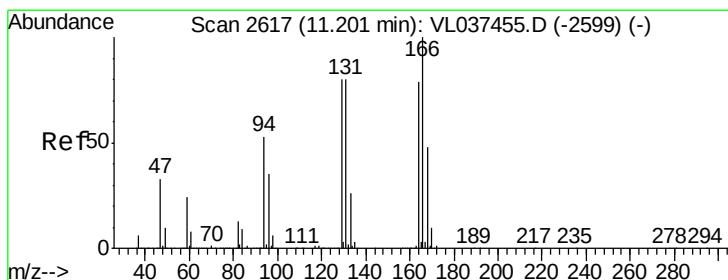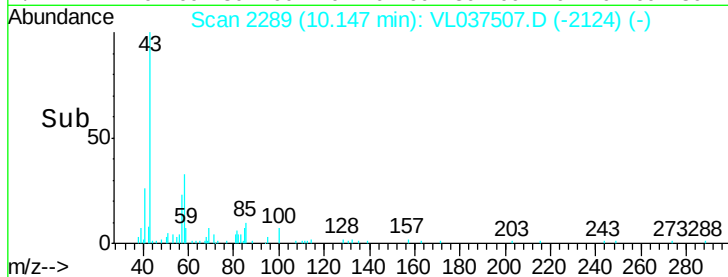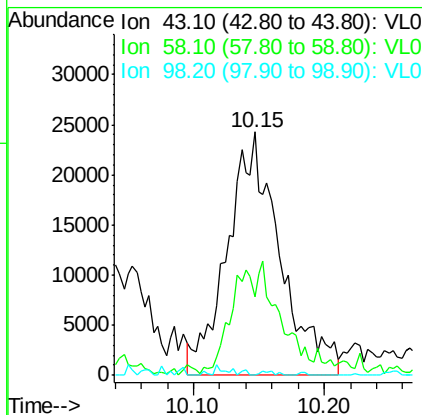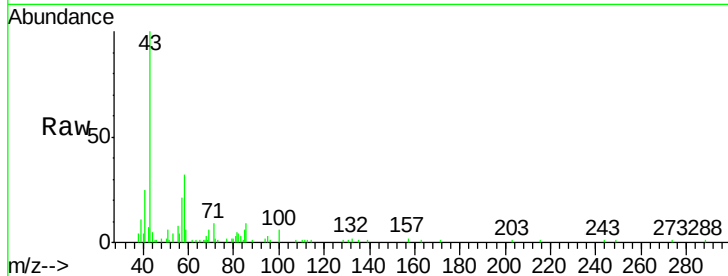

#52

Tetrachloroethene

Concen: 1.317 ppbv m




RT: 11.23 min Scan# 2626


Delta R.T. 0.03 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33

Tgt Ion:	164	Resp:	184837
Ion Ratio	Lower	Upper	
164	100		
166	108.6	100.7	151.1
129	87.9	80.9	121.3
131	80.7	80.2	120.4

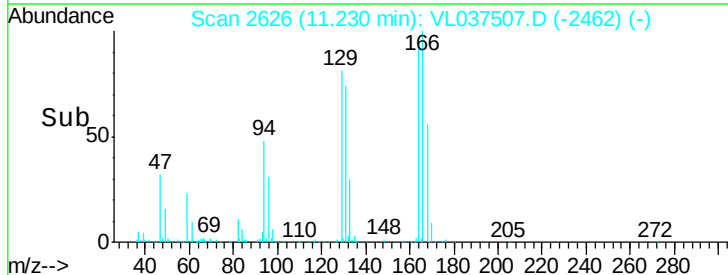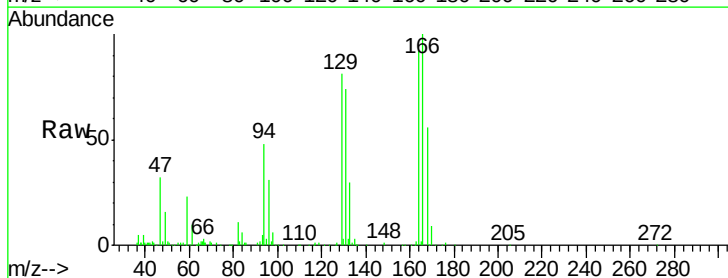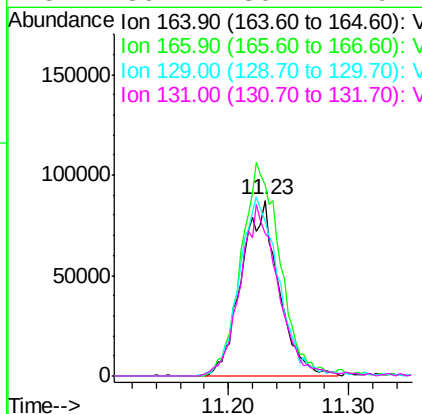



#53

Toluene

Concen: 0.426 ppbv

RT: 9.81 min Scan# 2184

Delta R.T. 0.03 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33

Instrument :

MSVOA_L

ClientSampleId :

SR-SG-5

Tot Ion: 91 Resp: 166838





Ion Ratio Lower Upper

91 100

92 64.7 48.8 73.2

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:20 PM

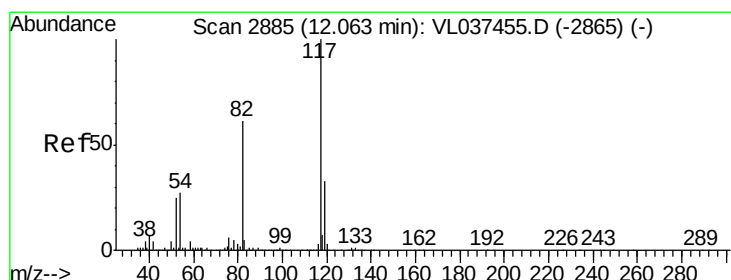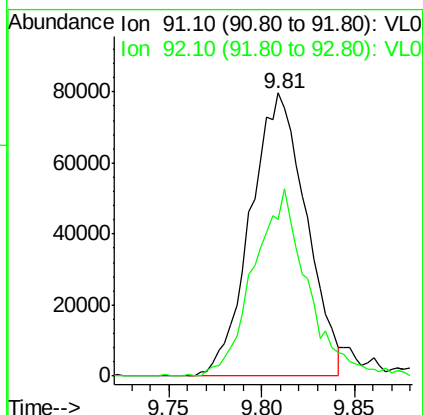

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.09 min Scan# 2893

Delta R.T. 0.03 min

Lab File: VL037507.D

Acq: 19 Aug 2021 20:33




Tgt Ion: 117 Resp: 3486874


Ion Ratio Lower Upper

117 100

82 65.2 52.9 79.3

119 34.3 24.8 37.2

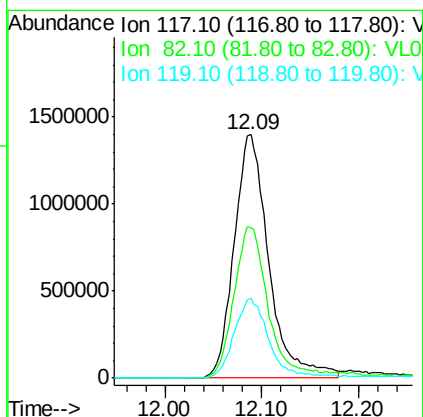

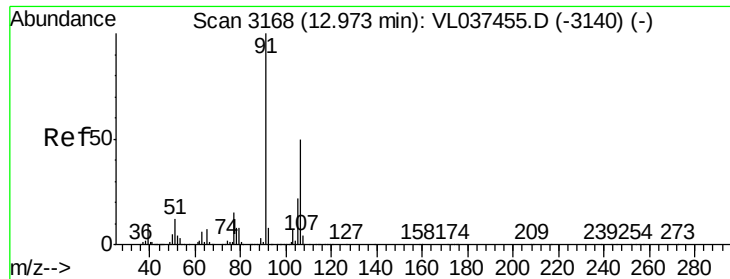





#59
m/p-Xylene
Concen: 0.134 ppbv m
RT: 12.98 min Scan# 3169
Delta R.T. 0.00 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion: 91 Resp: 56161
Ion Ratio Lower Upper
91 100
106 0.0 36.9 55.3#




Manual Integrations
APPROVED


MMDadoda
8/20/2021 6:31:20 PM

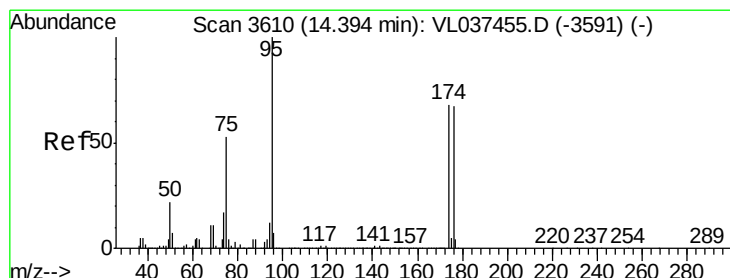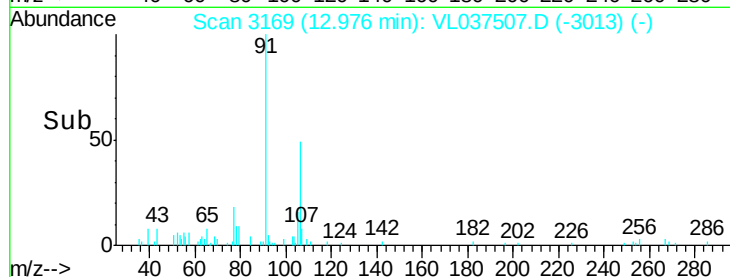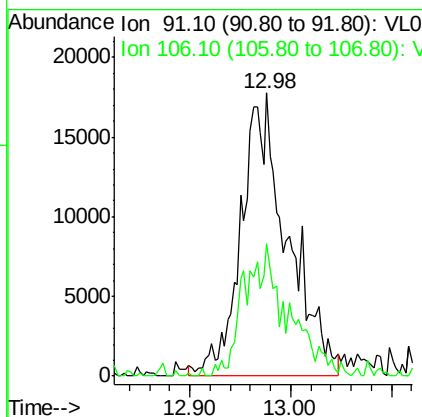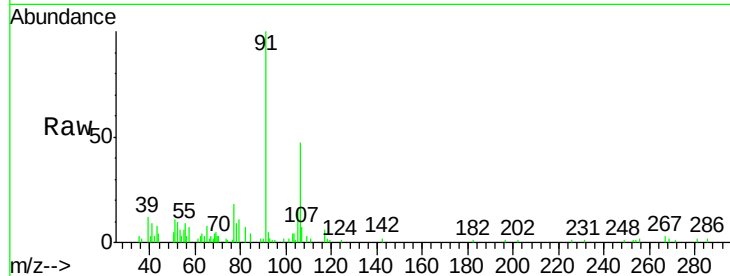

#68
1-Bromo-4-Fluorobenzene
Concen: 9.679 ppbv
RT: 14.42 min Scan# 3618
Delta R.T. 0.03 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion: 95 Resp: 2397675
Ion Ratio Lower Upper
95 100
174 77.3 59.6 89.4
175 5.7 4.6 7.0

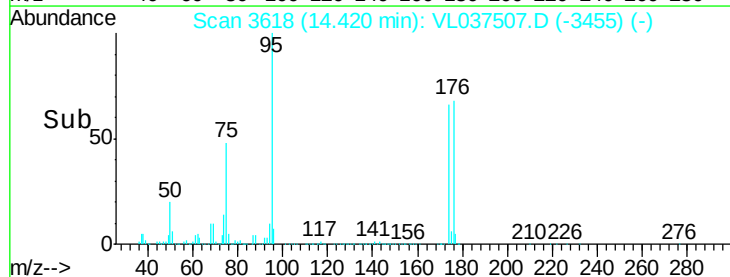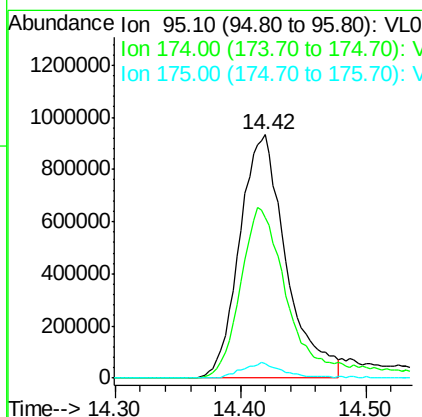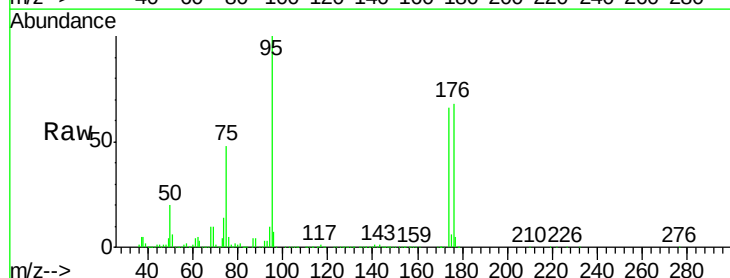







#79
Naphthalene
Concen: 2.316 ppbv m
RT: 22.19 min Scan# 6035
Delta R.T. 0.03 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Instrument :
MSVOA_L
ClientSampleId :
SR-SG-5

Tot Ion	Ratio	Resp	Lower	Upper
128	100	713931		
127	10.8		9.4	14.2
129	9.7		8.8	13.2

Manual Integrations
APPROVED

MMDadoda
8/20/2021 6:31:20 PM

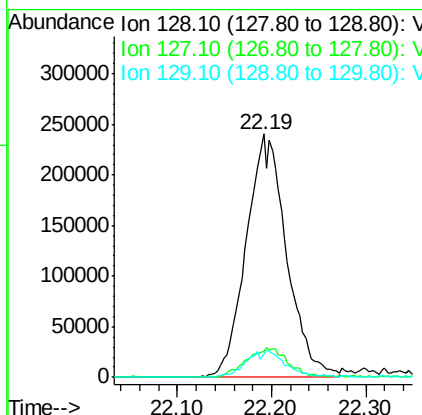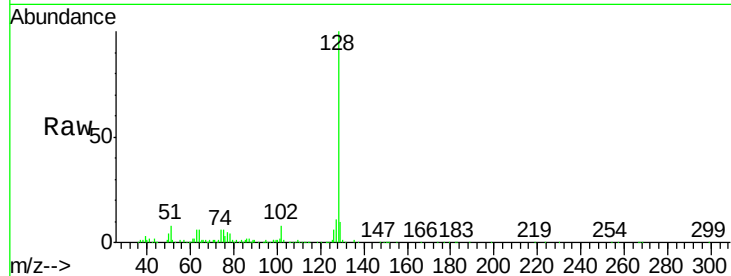

#80
Naphthalene, 2-methyl-
Concen: 0.115 ppbv
RT: 24.97 min Scan# 6900
Delta R.T. 0.02 min
Lab File: VL037507.D
Acq: 19 Aug 2021 20:33

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	9901		
141	111.0		64.7	97.1#
115	40.4		28.4	42.6

