


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL081921\
 Data File : VL037494.D
 Acq On : 19 Aug 2021 10:25
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
 Last Update : Tue Aug 17 02:13:47 2021

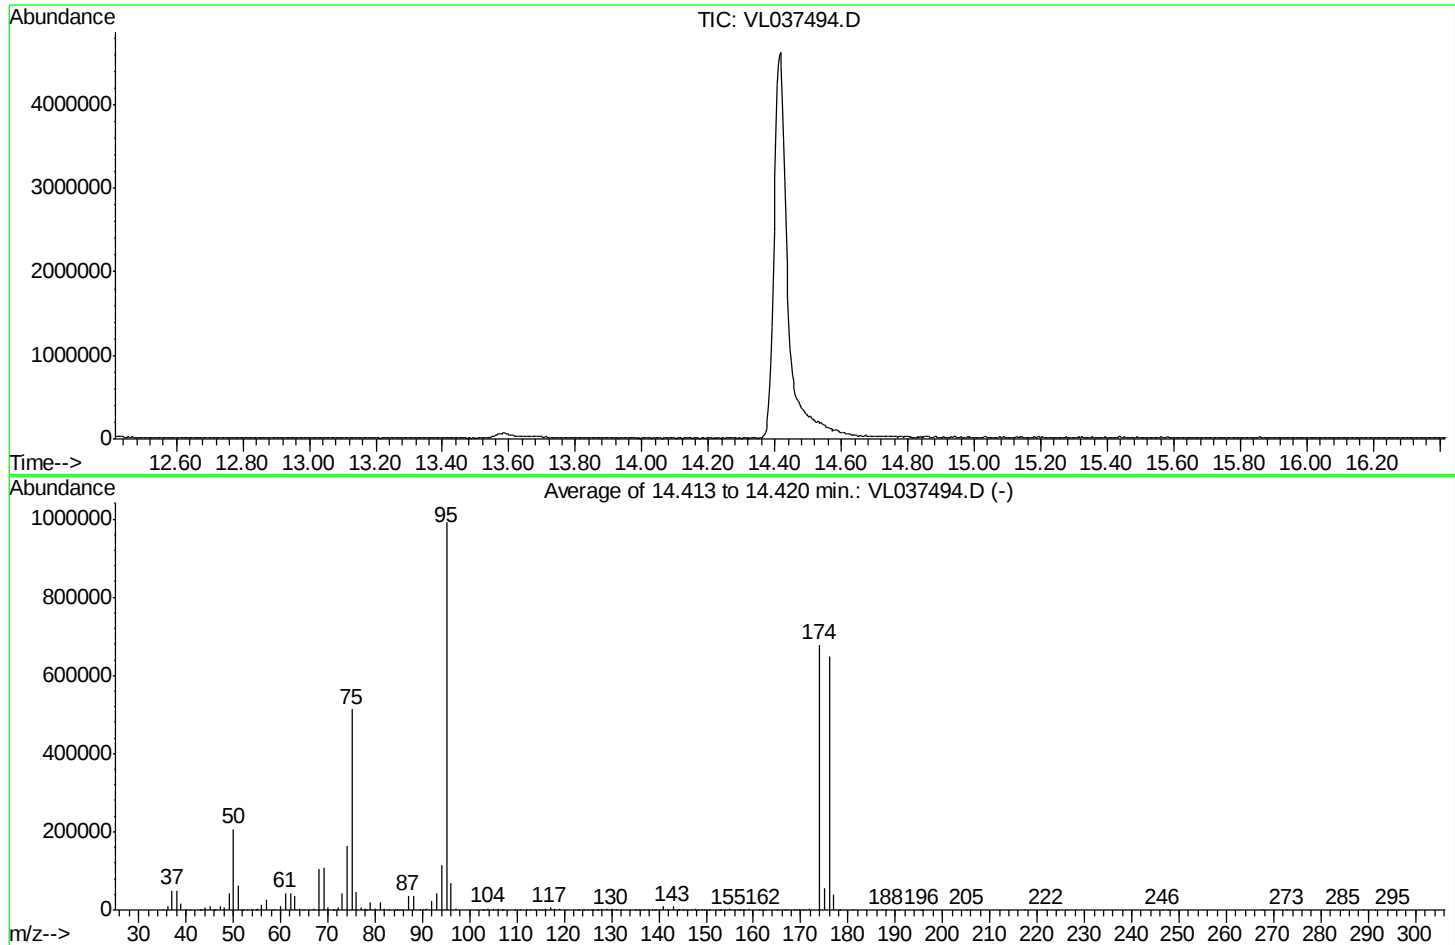

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.9	207253	PASS
75	95	30	66	51.8	513177	PASS
95	95	100	100	100.0	991317	PASS
96	95	5	9	6.9	68266	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.5	678613	PASS
175	174	4	9	8.0	54368	PASS
176	174	93	101	95.7	649386	PASS
177	176	5	9	6.1	39898	PASS