
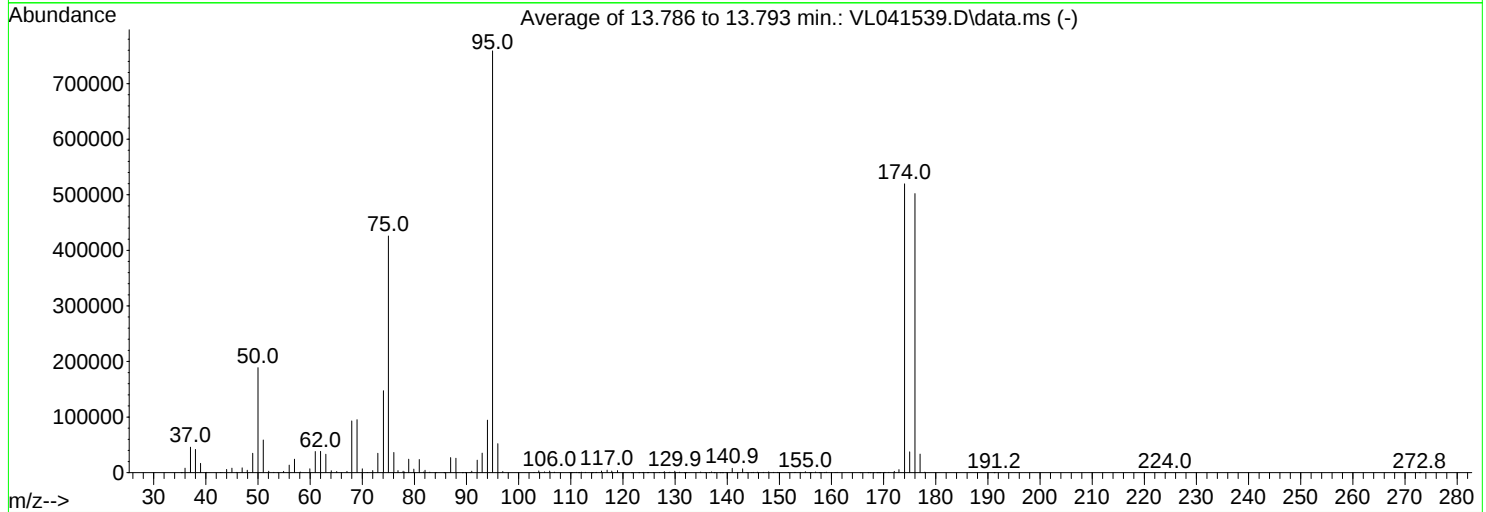


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081924\
Data File : VL041539.D
Acq On : 19 Aug 2024 8:10
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Aug 20 02:10:04 2024

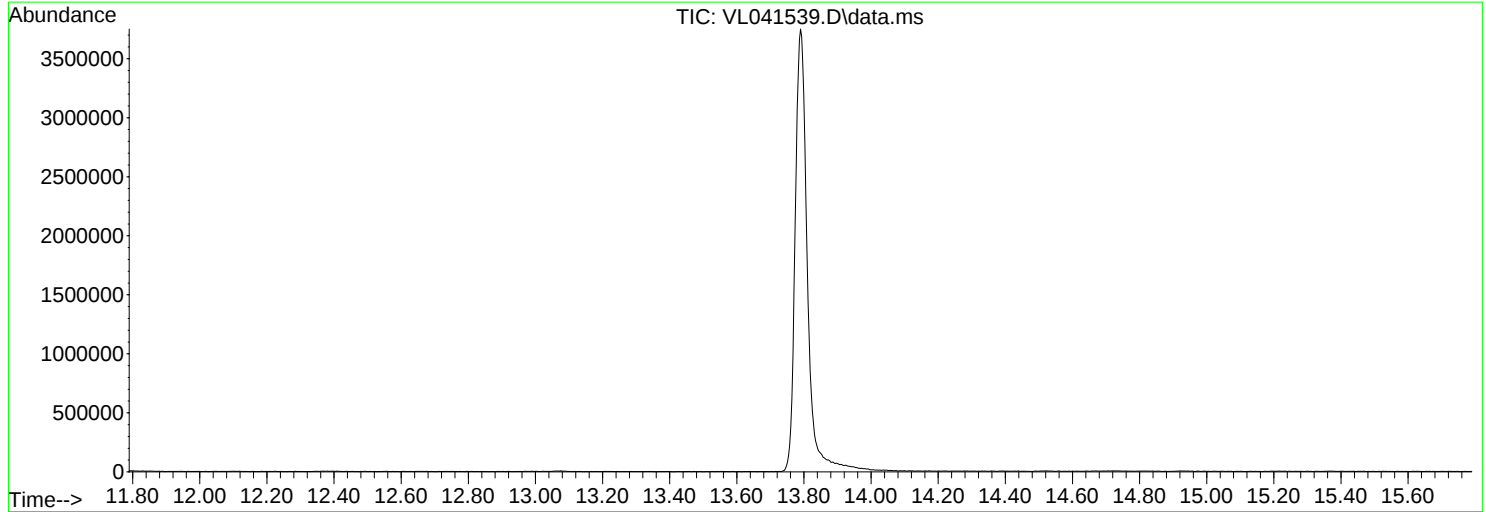

AutoFind: Scans 3478, 3479, 3480; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	188907	PASS
75	95	30	66	56.1	425728	PASS
95	95	100	100	100.0	758997	PASS
96	95	5	9	6.9	52083	PASS
173	174	0.00	2	1.0	5439	PASS
174	95	50	120	68.5	519701	PASS
175	174	4	9	7.2	37573	PASS
176	174	93	101	96.6	502080	PASS
177	176	5	9	6.6	33307	PASS

Average of 13.786 to 13.793 min.: VL041539.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.30	56	46.95	8701	58.10	1100	70.00	6801
36.00	8012	47.95	4457	59.95	7039	70.95	3711
37.05	45675	49.00	34977	61.00	37928	72.00	3691
38.00	41853	50.00	188907	62.00	38269	73.00	3480
39.00	16707	51.00	58685	63.00	33200	74.05	147349
40.05	707	52.05	2558	64.05	3446	75.00	425728
42.80	212	53.05	619	65.10	2112	76.05	36421
43.10	192	53.85	341	65.95	242	76.85	3722
44.00	5819	54.90	2401	67.05	2363	77.85	2682
45.00	8065	56.00	13525	68.00	93024	78.10	1085
45.95	709	57.00	24189	69.00	95173	78.90	24189

Average of 13.786 to 13.793 min.: VL041539.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.90	6429	90.70	698	105.95	2837	114.95	602
80.95	23549	91.00	2624	106.85	923	115.90	2835
81.80	1165	92.05	22363	109.85	356	116.95	4655
82.05	4255	93.00	35147	110.10	142	117.85	2801
82.95	935	94.00	94568	110.60	181	118.95	3704
84.00	91	95.00	758997	111.05	559	119.90	68
85.70	158	96.00	52083	111.50	126	121.65	138
86.95	27144	96.95	2017	112.05	806	123.05	158
87.95	26051	102.95	292	112.85	492	123.70	161
89.20	55	103.85	3263	114.10	64	123.95	457
89.80	120	104.95	1368	114.80	220	124.70	88

Average of 13.786 to 13.793 min.: VL041539.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.95	166	134.90	1240	142.95	7015	151.75	187
125.90	273	135.80	217	143.75	219	153.00	670
127.00	167	136.60	203	143.95	253	154.00	541
127.80	705	137.00	1368	144.70	204	155.00	1804
127.95	1714	137.50	96	145.00	718	155.80	56
128.80	404	138.65	143	145.85	967	156.20	187
129.00	763	139.10	144	146.90	692	156.95	1051
129.95	2716	139.80	240	147.95	1460	157.70	74
130.85	913	140.00	265	148.90	567	158.00	196
131.80	65	140.95	7789	149.70	588	158.70	197
132.00	67	142.05	680	149.95	355	159.00	800

Average of 13.786 to 13.793 min.: VL041539.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.70	221	172.05	2186				
161.05	728	172.95	5439				
165.50	142	174.00	519701				
167.00	113	175.00	37573				
167.40	100	176.00	502080				
168.00	79	177.00	33307				
168.70	122	177.90	988				
169.00	112	191.20	65				
169.30	140	224.00	59				
170.25	465	272.80	75				
171.00	721						