
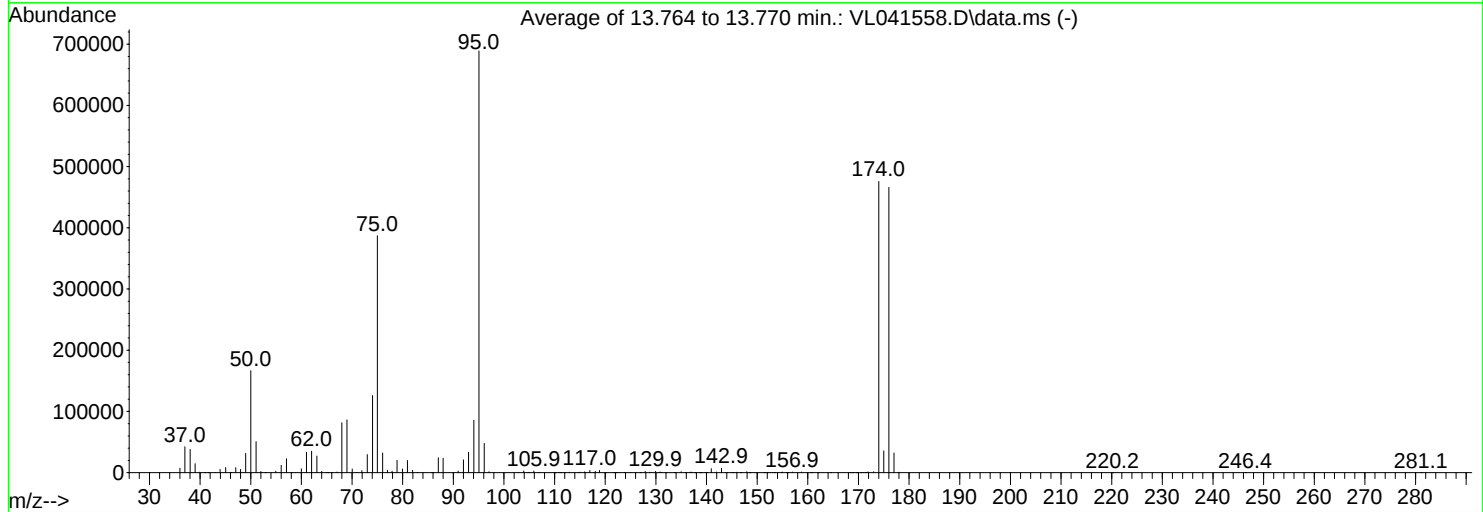


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL082124\
Data File : VL041558.D
Acq On : 21 Aug 2024 7:51
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Aug 22 01:05:17 2024

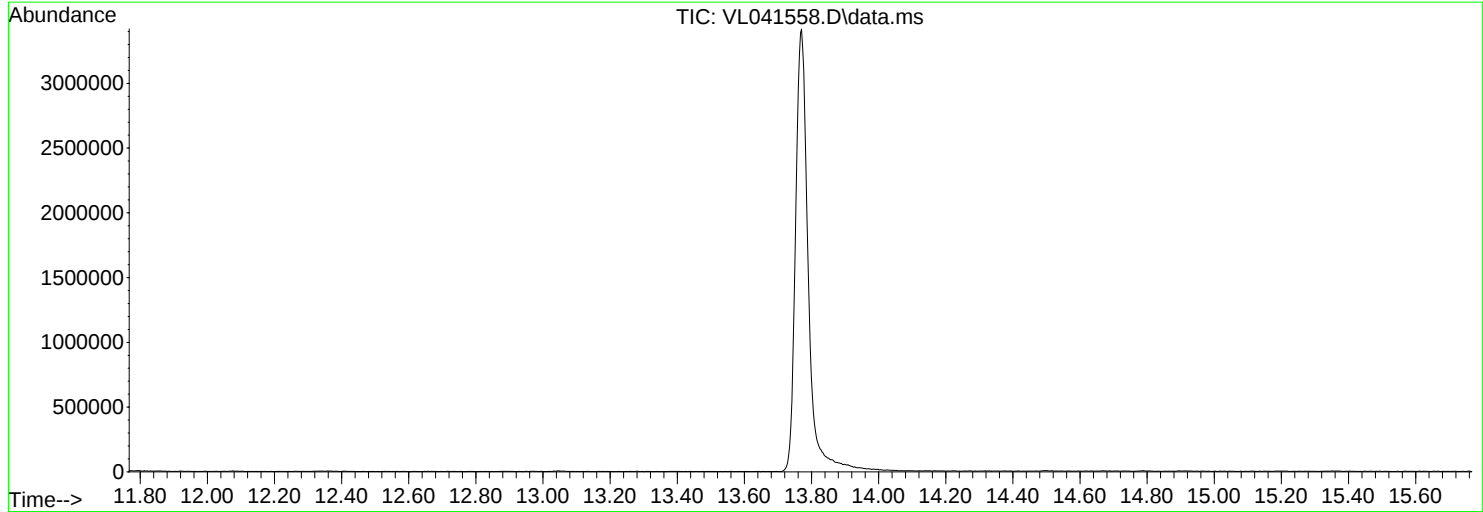

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	166507	PASS
75	95	30	66	56.2	387285	PASS
95	95	100	100	100.0	689131	PASS
96	95	5	9	7.0	47901	PASS
173	174	0.00	2	0.3	1633	PASS
174	95	50	120	69.0	475840	PASS
175	174	4	9	7.5	35480	PASS
176	174	93	101	97.9	466005	PASS
177	176	5	9	6.9	32283	PASS

Average of 13.764 to 13.770 min.: VL041558.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7282	46.20	194	58.00	493	67.05	116
37.00	42365	47.05	8249	58.20	346	68.00	8151
38.05	38021	48.00	5181	58.90	164	69.00	8639
39.00	14713	49.00	31323	60.00	6366	70.05	611
39.90	878	50.00	166507	61.00	33208	70.95	241
40.90	89	51.05	50725	62.00	34928	71.95	3375
41.60	77	52.00	1954	63.05	27304	73.00	29533
43.10	253	52.90	54	64.00	2216	74.05	125997
43.95	5178	54.95	2475	64.95	372	75.00	387285
45.05	8289	56.00	12144	65.20	116	76.05	32093
45.90	301	57.05	22749	65.90	55	77.00	3989

Average of 13.764 to 13.770 min.: VL041558.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.90	2370	92.00	20821	105.90	2717	115.90	1334
78.90	20131	93.00	33125	106.95	560	116.10	580
79.95	6026	94.05	85493	109.90	497	116.95	3756
80.95	19976	95.05	689131	110.10	121	117.80	714
81.95	3796	96.10	47901	110.85	604	118.05	1910
82.95	566	97.05	1596	111.20	135	118.85	3626
85.70	149	102.90	336	111.90	452	120.00	62
86.10	430	103.90	2994	112.10	273	121.70	110
87.05	24424	104.60	216	112.90	737	122.10	70
88.00	23568	104.90	472	114.70	226	122.70	189
90.95	2623	105.10	446	115.00	792	123.80	524

Average of 13.764 to 13.770 min.: VL041558.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.00	198	133.70	99	141.95	931	148.50	94
126.00	314	135.00	1528	142.95	7115	148.80	385
126.90	136	135.85	135	143.80	190	149.55	195
127.90	2069	136.75	921	144.10	361	150.05	647
128.75	829	137.05	696	144.85	449	151.40	82
129.05	507	137.70	67	145.20	81	151.75	195
129.95	2140	138.70	101	145.80	293	152.00	156
130.60	260	138.90	93	145.95	856	152.70	176
130.85	929	139.75	328	146.70	147	153.10	256
131.10	170	140.10	420	146.95	199	153.40	70
131.90	50	140.95	6610	147.95	1616	154.00	377

Average of 13.764 to 13.770 min.: VL041558.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.80	569	168.90	78	177.00	32283		
155.00	1010	169.60	73	178.00	906		
155.80	60	169.95	247	220.20	72		
156.05	129	170.50	157	246.40	53		
156.95	1179	171.05	354	281.10	50		
158.75	995	171.40	138				
160.60	144	171.90	1354				
160.95	659	173.00	1633				
162.00	59	174.00	475840				
164.50	55	175.00	35480				
168.40	73	176.00	466005				