


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL082522\
 Data File : VL039578.D
 Acq On : 25 Aug 2022 13:17
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081722AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Fri Aug 26 06:05:16 2022

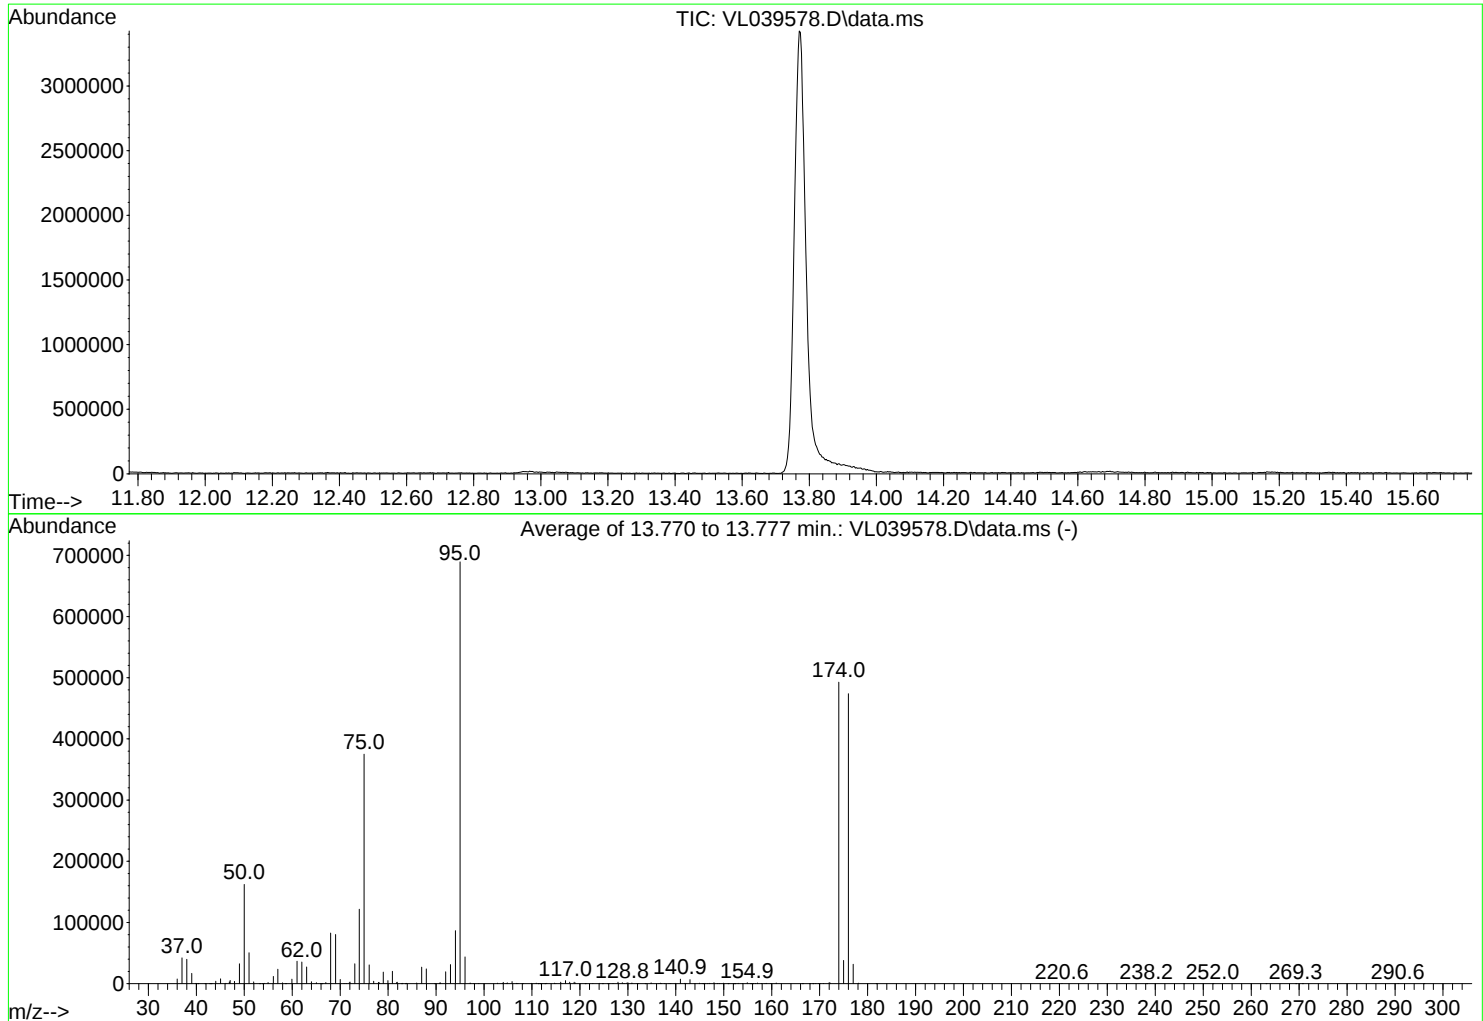

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.5	162219	PASS
75	95	30	66	54.4	375104	PASS
95	95	100	100	100.0	689344	PASS
96	95	5	9	6.3	43768	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.5	492736	PASS
175	174	4	9	7.7	37909	PASS
176	174	93	101	96.2	473856	PASS
177	176	5	9	6.7	31781	PASS

Average of 13.770 to 13.777 min.: VL039578.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7725	46.15	577	54.95	1851	65.90	121
37.00	42051	46.90	2865	56.05	11892	66.20	8
38.00	39760	47.05	5252	57.00	23547	67.00	176
39.05	16716	47.95	3763	57.95	1216	68.00	8269
39.90	473	49.00	32389	58.60	60	69.05	80405
40.30	151	50.00	162219	59.95	7392	70.00	6704
41.80	106	51.00	50480	61.00	36624	70.80	282
42.80	132	51.95	2871	62.00	35245	71.25	311
43.10	134	53.20	115	63.00	27280	71.90	1651
44.05	3997	53.80	77	64.00	3105	72.05	2647
45.05	7778	54.15	599	65.05	1664	73.05	32520

Average of 13.770 to 13.777 min.: VL039578.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.00	121709	82.80	117	93.00	31219	104.85	1272
75.00	375104	83.05	584	94.05	86560	105.85	3332
76.05	30659	83.60	70	95.00	689344	106.75	475
77.00	4014	83.85	422	96.05	43768	106.90	262
78.00	1995	85.95	1047	97.10	984	107.10	167
78.20	1225	87.00	26832	97.90	215	108.00	84
79.00	18936	87.95	24211	98.90	200	109.90	632
79.95	5033	89.70	71	102.80	705	110.90	691
80.90	20093	90.70	977	103.80	638	111.30	87
81.80	1873	90.95	1381	104.00	2234	111.70	149
81.90	2370	92.00	19416	104.60	211	111.95	240

Average of 13.770 to 13.777 min.: VL039578.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
112.30	160	122.70	184	130.85	957	140.95	7316
112.70	105	124.05	645	131.95	157	141.85	627
113.10	443	124.70	71	133.60	79	142.10	626
114.70	685	125.80	53	134.85	1447	142.95	6561
115.00	371	126.10	303	136.50	179	144.00	362
116.00	2262	126.90	163	136.80	821	144.95	877
117.00	5011	127.95	2458	137.00	333	145.50	192
117.85	2264	128.85	1519	137.70	203	145.70	142
118.80	2346	129.20	312	138.60	188	146.05	590
119.00	1403	129.80	930	138.95	208	146.65	174
121.10	53	130.00	1704	139.90	626	147.05	430

Average of 13.770 to 13.777 min.: VL039578.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.95	1541	156.00	61	169.20	314	181.80	82
148.70	375	156.60	290	169.80	163	220.55	284
149.05	415	157.05	1095	170.10	367	238.20	136
149.95	738	157.90	210	170.80	169	245.90	62
150.90	55	158.60	302	172.00	1793	252.00	62
152.00	119	158.95	497	172.20	1137	263.10	63
152.30	57	159.85	337	174.00	492736	269.30	118
153.00	562	160.95	1118	175.00	37909	270.70	57
153.95	234	166.40	89	176.00	473856	290.65	193
154.90	1548	167.90	82	177.00	31781	296.00	55
155.60	65	168.60	136	178.10	746		