

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL090320\
 Data File : VL035533.D
 Acq On : 3 Sep 2020 16:34
 Operator : SY/AP
 Sample : L3898-01DUP
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IA-1DUP

Manual Integrations
 APPROVED

MMDadoda
 9/8/2020 4:06:18 PM

Quant Time: Sep 04 07:16:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug 27 2020
 QLast Update : Thu Aug 27 06:46:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.69	49	1003983	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.20	114	4294605	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.12	117	4231143	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.46	95	3115290	10.37	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	103.70%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.06	85	45879	0.264	ppbv	89
3) Chlorodifluoromethane	2.99	51	50047m	0.451	ppbv	
4) Chloromethane	3.15	50	32959	0.554	ppbv	99
9) Propene	3.02	41	29763	0.695	ppbv	84
10) Heptane	8.15	43	60090	0.523	ppbv	100
11) Trichlorofluoromethane	3.97	101	68268	0.269	ppbv	96
13) Ethanol	3.63	45	4104832	386.748	ppbv	99
15) Acetone	3.86	43	1118157	10.098	ppbv	96
17) tert-Butyl alcohol	4.33	59	43916	0.326	ppbv	98
19) Isopropyl Alcohol	4.00	45	1817133	27.508	ppbv	99
20) Methylene Chloride	4.36	84	1323649	16.050	ppbv	96
26) Hexane	5.71	57	616473	5.562	ppbv #	51
30) Cyclohexane	7.16	84	31328	0.264	ppbv #	89
34) 2-Butanone	5.26	43	740369	5.809	ppbv	98
35) Carbon Tetrachloride	7.05	117	14765	0.068	ppbv #	90
36) Benzene	6.92	78	121435	0.437	ppbv	97
43) Methyl Methacrylate	8.04	69	21753m	0.202	ppbv	
44) 2,2,4-Trimethylpentane	7.90	57	234306	0.641	ppbv #	87
50) 4-Methyl-2-Pentanone	8.78	43	41901	0.227	ppbv	97
52) Tetrachloroethene	11.26	164	9162m	0.056	ppbv	
53) Toluene	9.84	91	1250337	3.577	ppbv	98
58) Ethyl Benzene	12.75	91	172874	0.396	ppbv	92
59) m/p-Xylene	13.00	91	522991	1.434	ppbv	97
60) o-Xylene	13.73	91	181643	0.495	ppbv	98
72) 4-Ethyltoluene	15.88	105	90337	0.194	ppbv #	96
73) 1,3,5-Trimethylbenzene	16.04	105	89755m	0.208	ppbv	
74) 1,2,4-Trimethylbenzene	16.81	105	328225	0.692	ppbv #	72
79) Naphthalene	22.26	128	1574829	2.993	ppbv	96
80) Naphthalene,2-methyl-	25.02	142	69437	0.387	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL090320\
Data File : VL035533.D
Acq On : 3 Sep 2020 16:34
Operator : SY/AP
Sample : L3898-01DUP
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
IA-1DUP

Manual Integrations
APPROVED

MMDadoda
9/8/2020 4:06:18 PM

Quant Time: Sep 04 07:16:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug
QLast Update : Thu Aug 27 06:46:28 2020
Response via : Initial Calibration

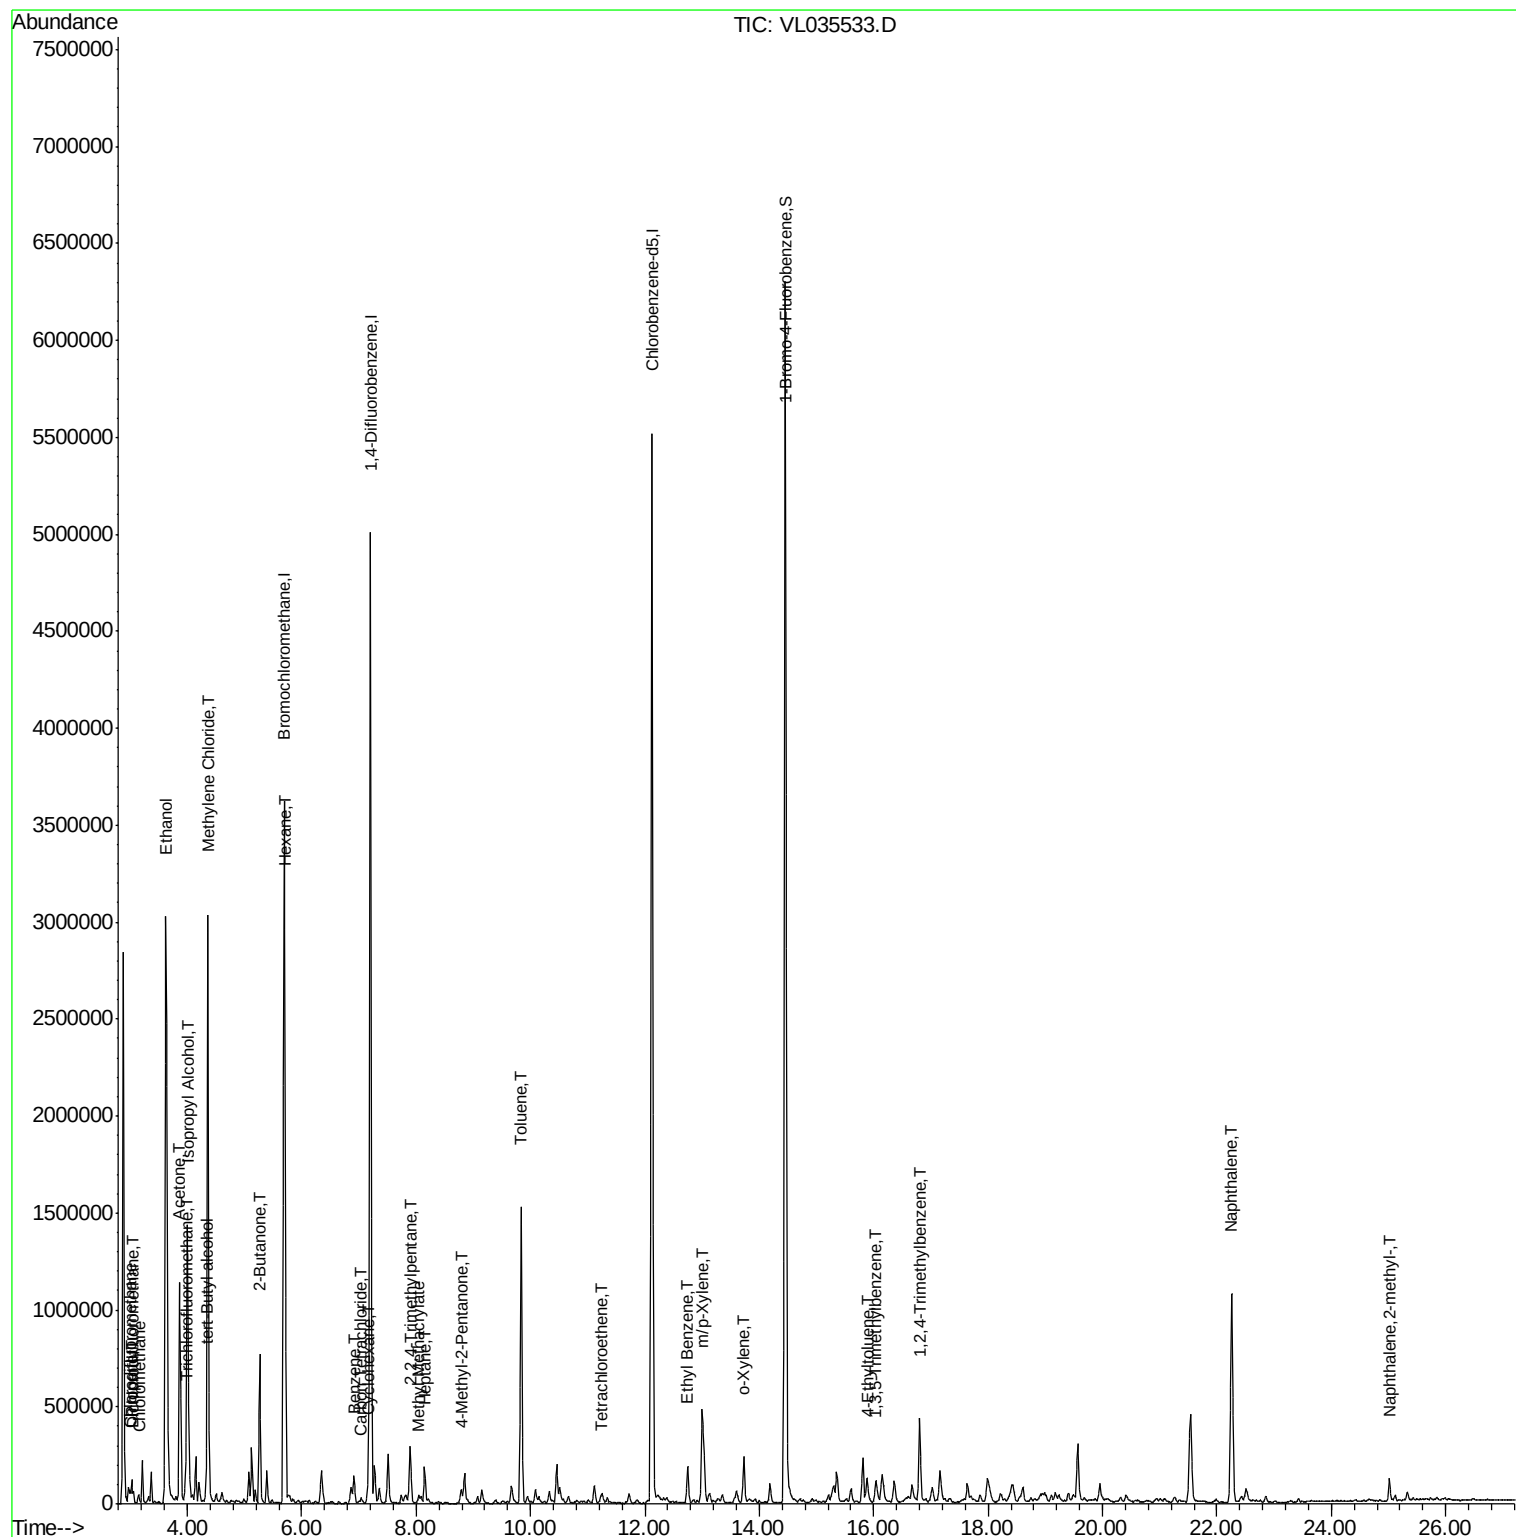

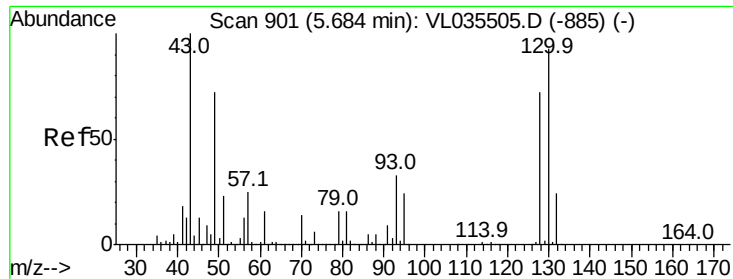

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.69 min Scan# 902

Delta R.T. 0.00 min

Lab File: VL035533.D

Acq: 3 Sep 2020 16:34

Instrument :

MSVOA_L

ClientSampleId :

IA-1DUP

Tot Ion: 49 Resp: 1003983

Ion Ratio Lower Upper

49 100

128 95.3 50.0 150.1





130 123.2 64.4 193.2

Manual Integrations

APPROVED

MMDadoda

9/8/2020 4:06:18 PM

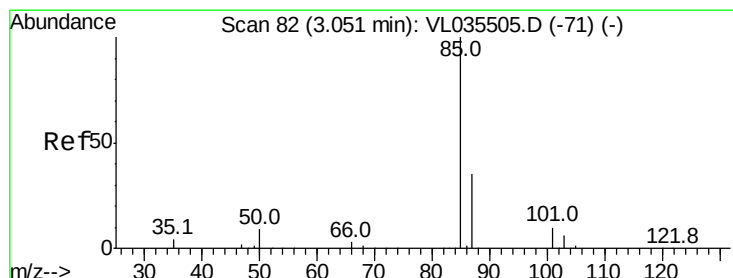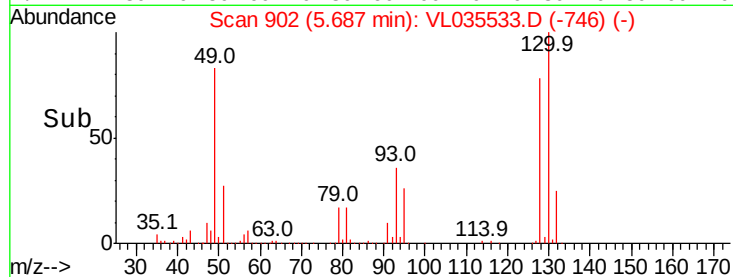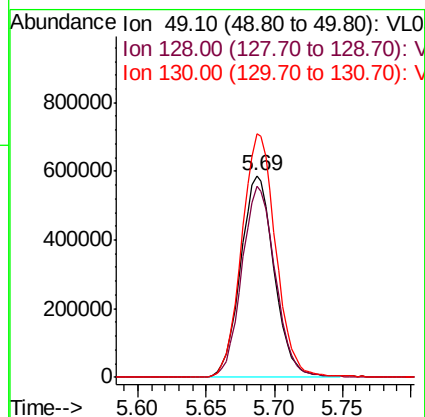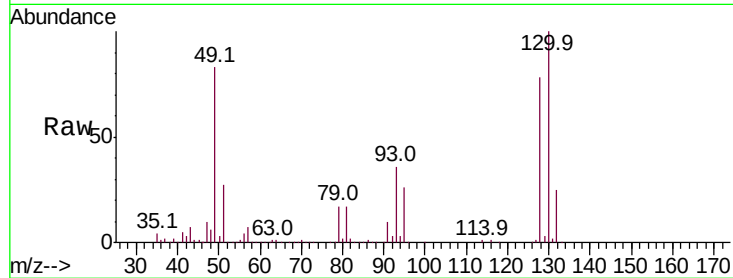

#2

Dichlorodifluoromethane

Concen: 0.264 ppbv

RT: 3.06 min Scan# 84

Delta R.T. 0.01 min

Lab File: VL035533.D




Acq: 3 Sep 2020 16:34


Tgt Ion: 85 Resp: 45879

Ion Ratio Lower Upper

85 100

87 28.3 28.0 42.0

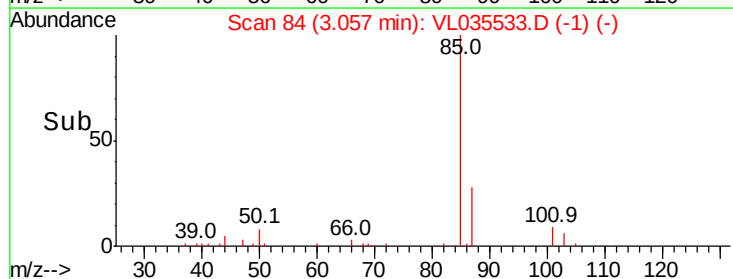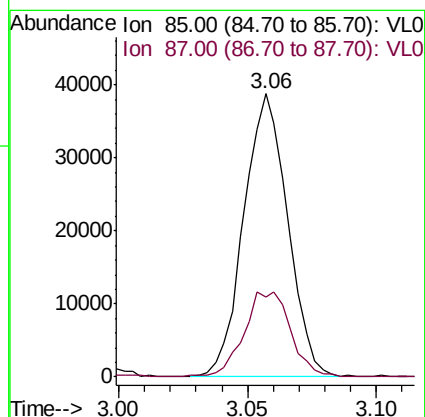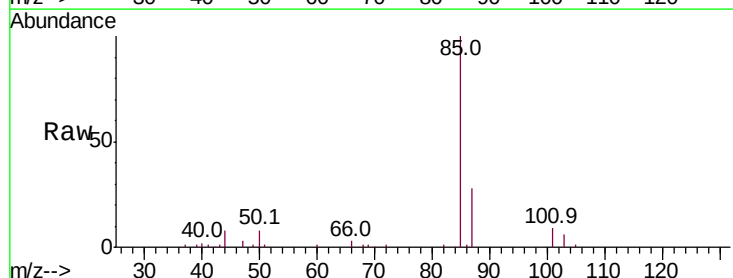







#3
Chlorodifluoromethane
Concen: 0.451 ppbv
RT: 2.99 min Scan# 64
Delta R.T. 0.00 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Instrument :
MSVOA_L
ClientSampleId :
IA-1DUP

Tot Ion	51	Resp	50047
Ion Ratio	100	Lower	Upper
67	22.2	17.8	26.8




Manual Integrations
APPROVED


MMDadoda
9/8/2020 4:06:18 PM

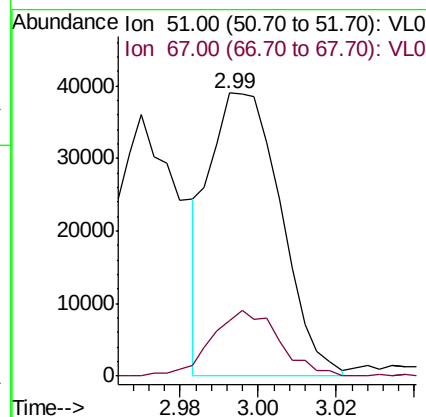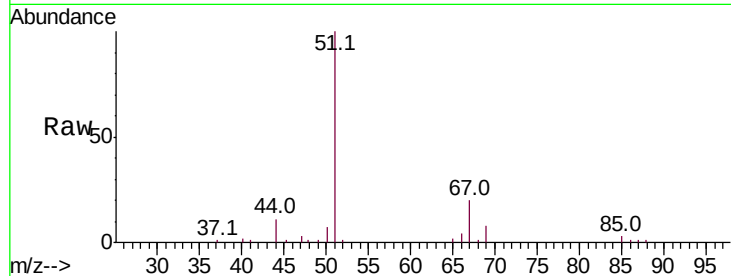

#4
Chloromethane
Concen: 0.554 ppbv
RT: 3.15 min Scan# 113
Delta R.T. 0.01 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Tgt Ion	50	Resp	32959
Ion Ratio	100	Lower	Upper
52	34.0	27.7	41.5

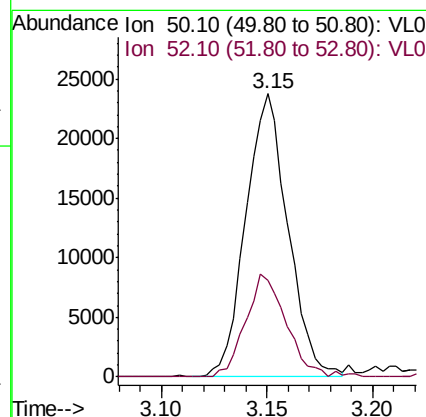

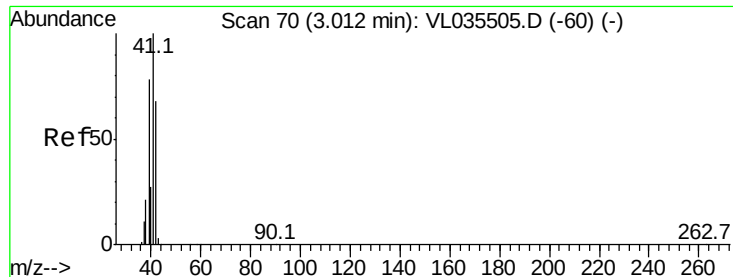

#9

Propene

Concen: 0.695 ppbv

RT: 3.02 min Scan# 74

Delta R.T. 0.01 min

Lab File: VL035533.D

Acq: 3 Sep 2020 16:34

Instrument :

MSVOA_L

ClientSampleId :

IA-1DUP

Tot Ion: 41 Resp: 29763

Ion Ratio Lower Upper





41 100

42 57.0 56.3 84.5

Manual Integrations
APPROVED

MMDadoda

9/8/2020 4:06:18 PM

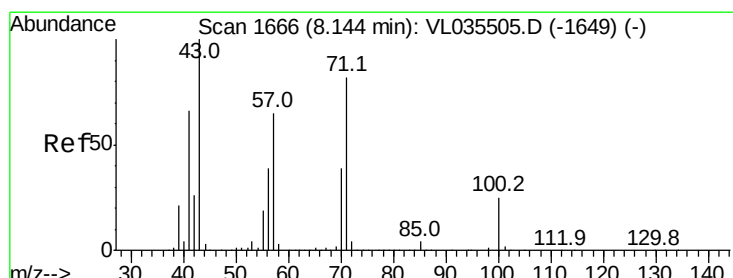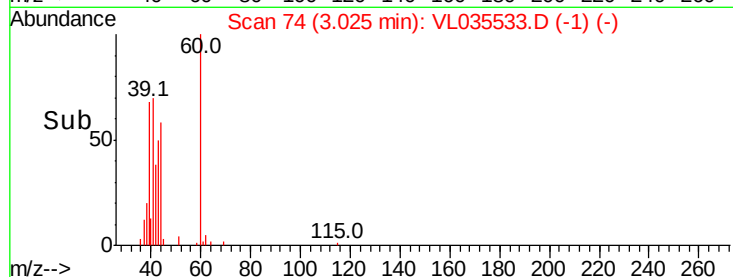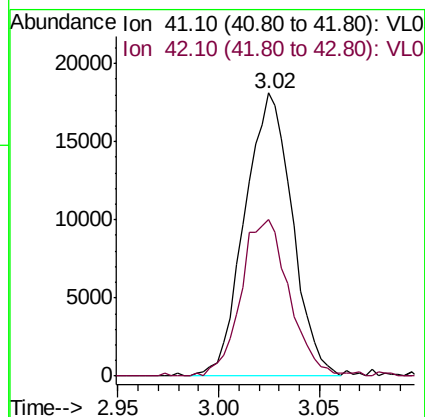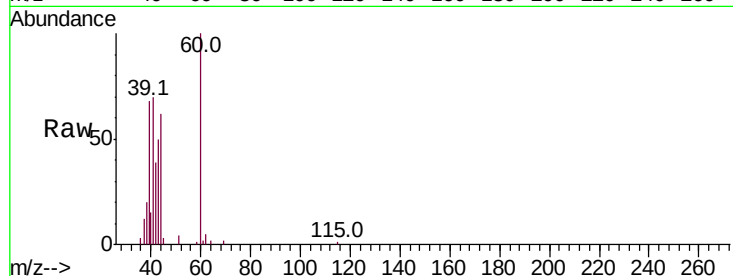

#10

Heptane

Concen: 0.523 ppbv

RT: 8.15 min Scan# 1668

Delta R.T. 0.01 min

Lab File: VL035533.D




Acq: 3 Sep 2020 16:34


Tgt Ion: 43 Resp: 60090

Ion Ratio Lower Upper

43 100

57 64.1 51.4 77.0

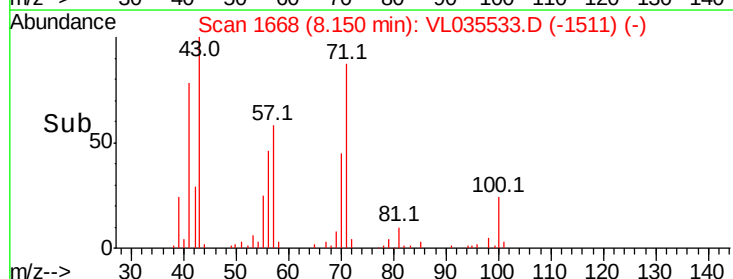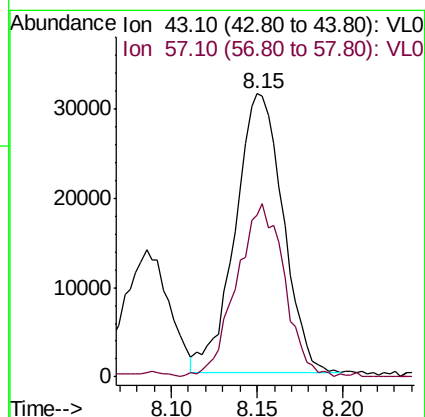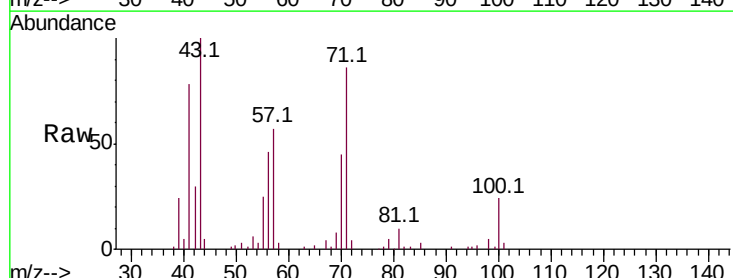







#11
 Trichlorofluoromethane
 Concen: 0.269 ppbv
 RT: 3.97 min Scan# 367
 Delta R.T. 0.01 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Instrument :
 MSVOA_L
 ClientSampleId :
 IA-1DUP

Tot Ion:101 Resp: 68268
 Ion Ratio Lower Upper
 101 100
 103 65.3 54.5 81.7




Manual Integrations
 APPROVED


MMDadoda
 9/8/2020 4:06:18 PM

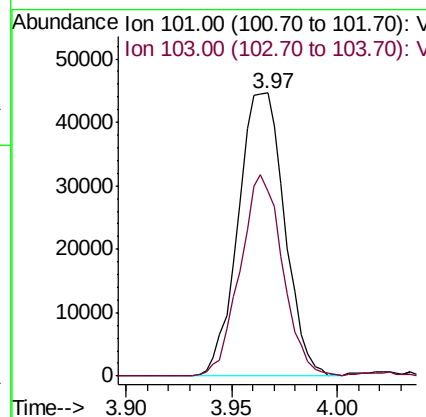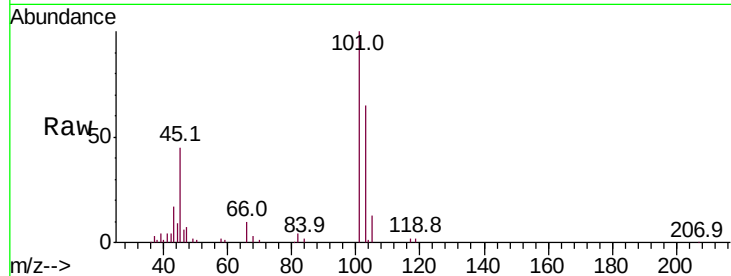

#13
 Ethanol
 Concen: 386.748 ppbv
 RT: 3.63 min Scan# 262
 Delta R.T. 0.02 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Tgt Ion: 45 Resp: 4104832
 Ion Ratio Lower Upper
 45 100
 46 37.5 15.2 60.6

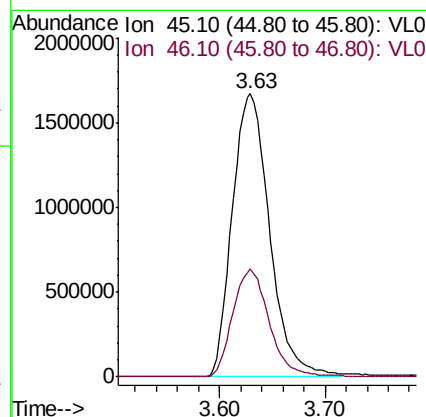

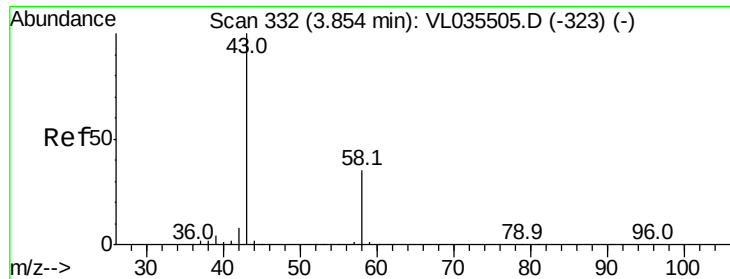





#15
Acetone
Concen: 10.098 ppbv
RT: 3.86 min Scan# 334
Delta R.T. 0.01 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Instrument :
MSVOA_L
ClientSampleId :
IA-1DUP

Tot Ion: 43 Resp: 1118157
Ion Ratio Lower Upper
43 100
58 33.1 28.4 42.6




Manual Integrations
APPROVED


MMDadoda
9/8/2020 4:06:18 PM

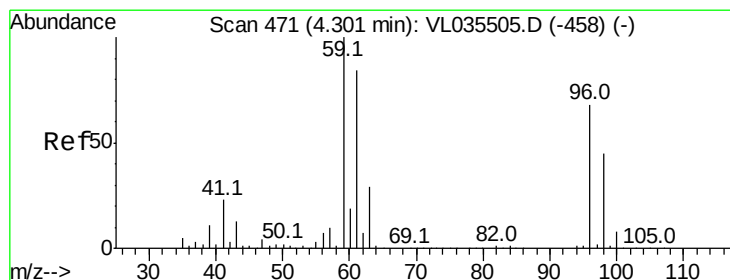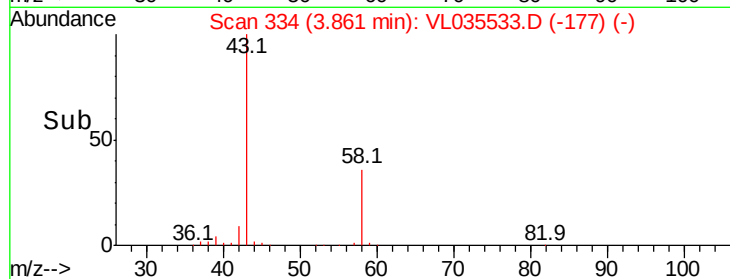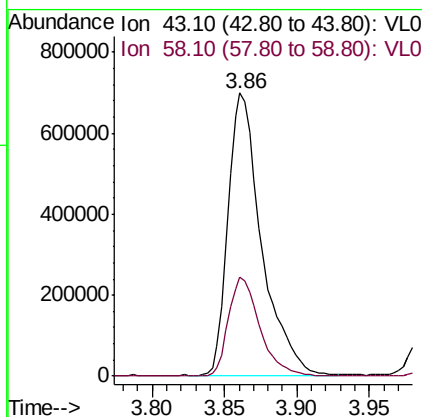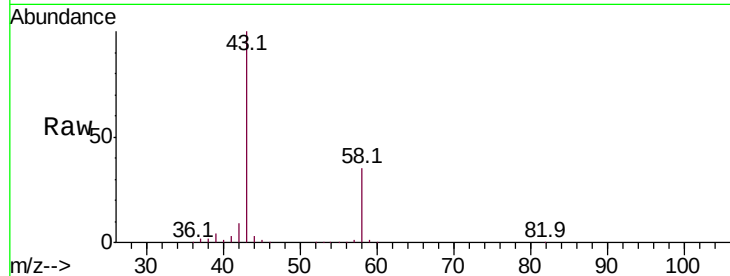

#17
tert-Butyl alcohol
Concen: 0.326 ppbv
RT: 4.33 min Scan# 480
Delta R.T. 0.03 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Tgt Ion: 59 Resp: 43916
Ion Ratio Lower Upper
59 100
57 11.4 8.4 12.6

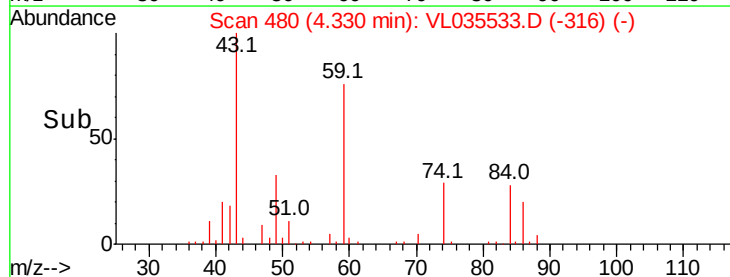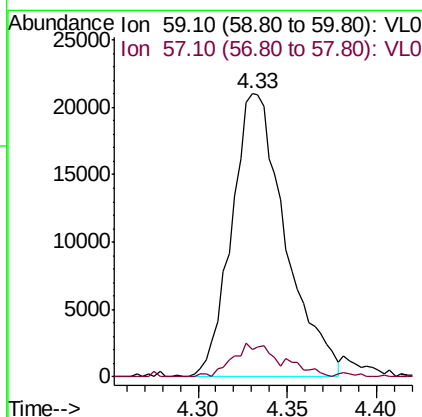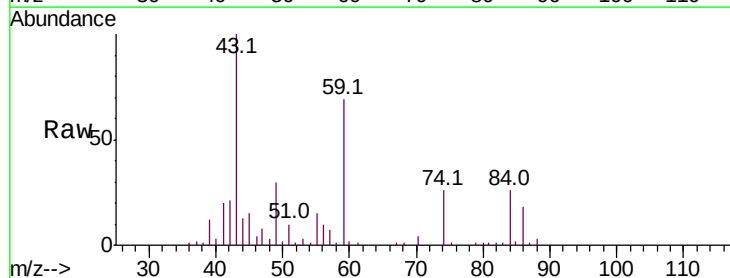



#19





Isopropyl Alcohol
 Concen: 27.508 ppbv
 RT: 4.00 min Scan# 377
 Delta R.T. 0.02 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Instrument :
 MSVOA_L
 ClientSampleId :
 IA-1DUP

Tot Ion: 45 Resp: 1817133
 Ion Ratio Lower Upper
 45 100
 58 2.2 2.0 3.0

Manual Integrations
 APPROVED




MMDadoda
 9/8/2020 4:06:18 PM

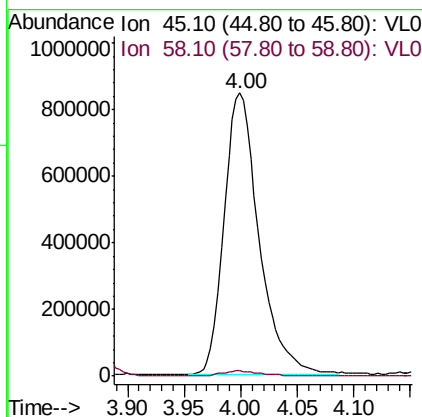


#20

Methylene Chloride
 Concen: 16.050 ppbv
 RT: 4.36 min Scan# 489
 Delta R.T. 0.01 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Tgt Ion: 84 Resp: 1323649
 Ion Ratio Lower Upper
 84 100
 49 86.3 65.4 98.0
 51 27.6 21.5 32.3
 86 68.1 52.9 79.3

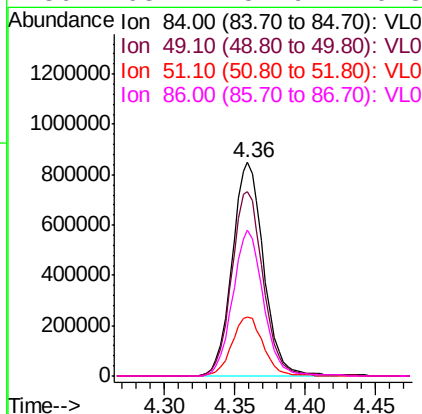







#26
Hexane
Concen: 5.562 ppbv
RT: 5.71 min Scan# 909
Delta R.T. 0.01 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Instrument :
MSVOA_L
ClientSampled :
IA-1DUP

Tot Ion	Ratio	Lower	Upper
57	100		
41	68.4	55.9	83.9
43	63.9	141.8	212.8#
56	53.7	41.8	62.8




Manual Integrations
APPROVED


MMDadoda
9/8/2020 4:06:18 PM

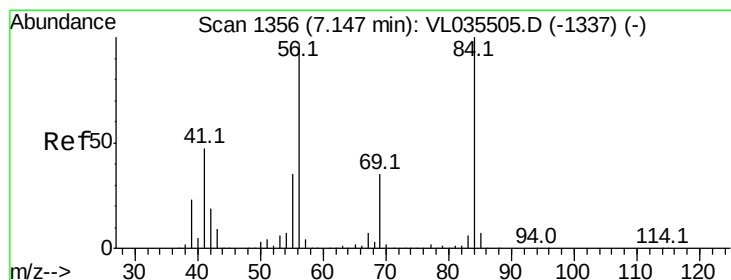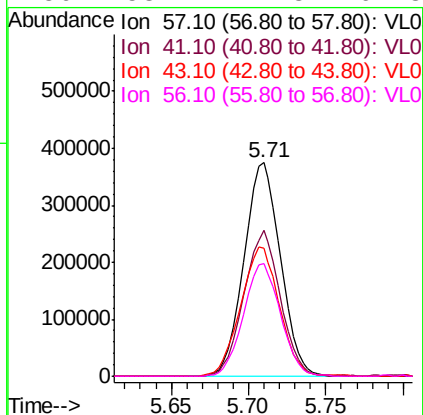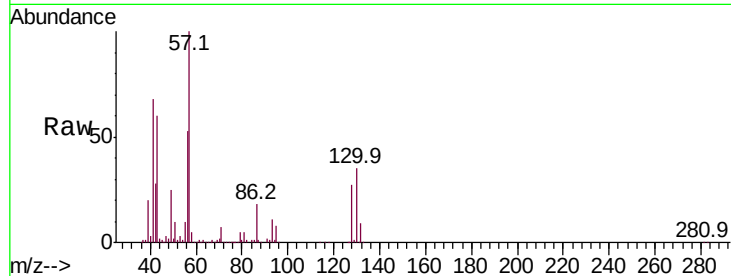

#30
Cyclohexane
Concen: 0.264 ppbv
RT: 7.16 min Scan# 1359
Delta R.T. 0.01 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Tgt Ion	Ratio	Lower	Upper
84	100		
56	92.7	80.1	120.1
41	60.4	38.1	57.1#

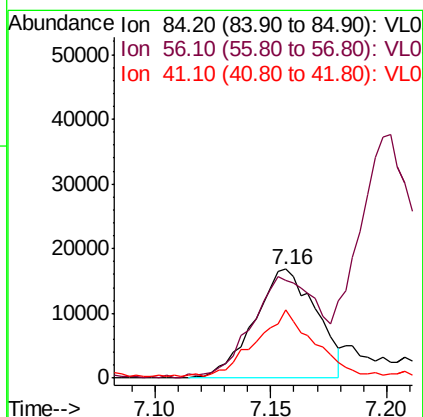







#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.20 min Scan# 1373
 Delta R.T. 0.01 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Instrument :
 MSVOA_L
 ClientSampleId :
 IA-1DUP

Tot Ion	Ratio	Lower	Upper
114	100		
63	18.4	14.7	22.1
88	16.7	13.4	20.2




Manual Integrations
 APPROVED


MMDadoda
 9/8/2020 4:06:18 PM

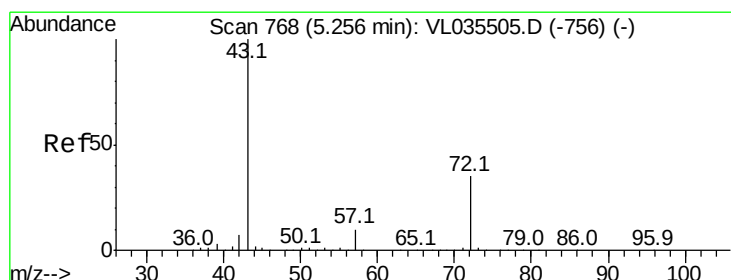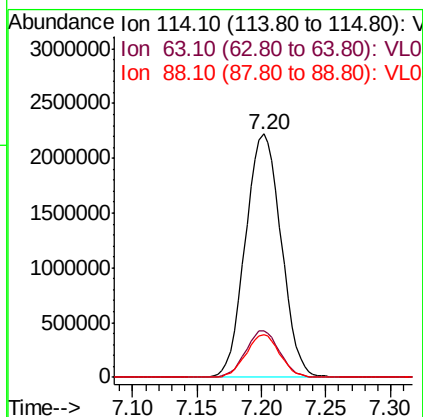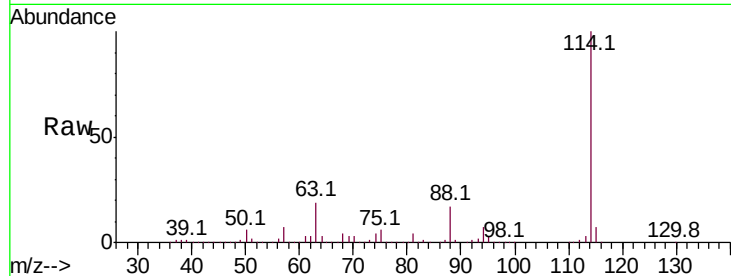

#34
 2-Butanone
 Concen: 5.809 ppbv
 RT: 5.26 min Scan# 770
 Delta R.T. 0.01 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Tgt Ion	Ratio	Lower	Upper
43	100		
72	33.7	27.7	41.5

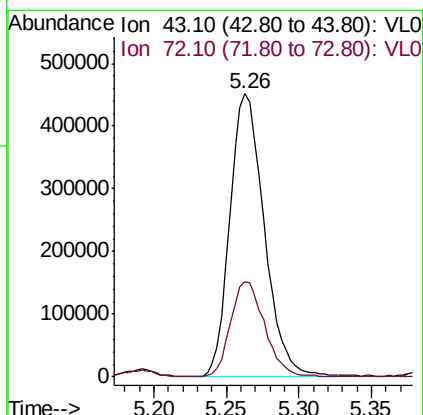

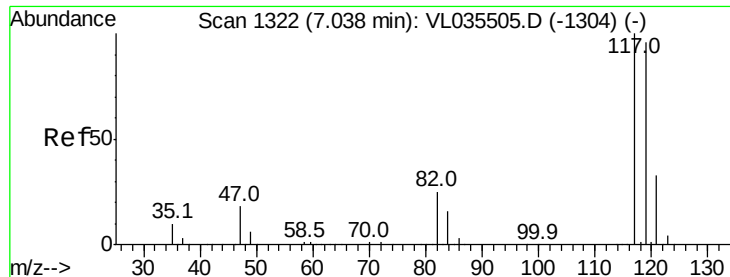

#35





Carbon Tetrachloride
 Concen: 0.068 ppbv
 RT: 7.05 min Scan# 1325
 Delta R.T. 0.01 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Instrument :
 MSVOA_L
 ClientSampled :
 IA-1DUP

Tot Ion	Ratio	Lower	Upper
117	100		
119	88.0	77.2	115.8
121	24.7	26.1	39.1#

Manual Integrations
 APPROVED




MMDadoda
 9/8/2020 4:06:18 PM

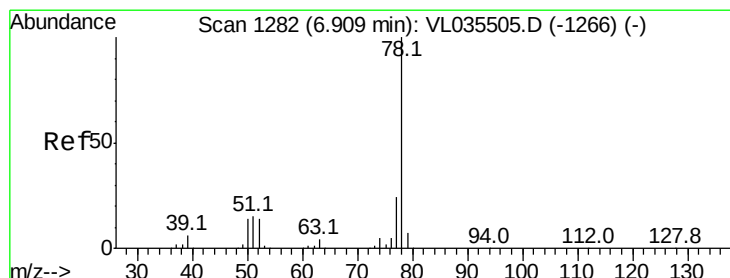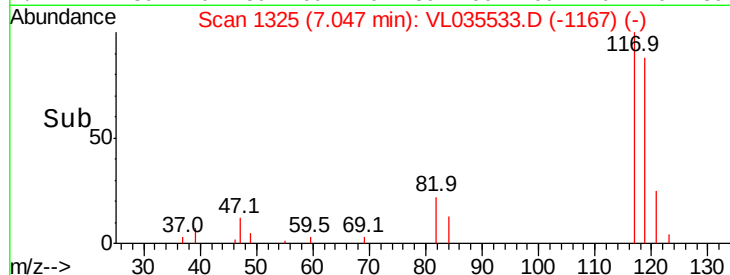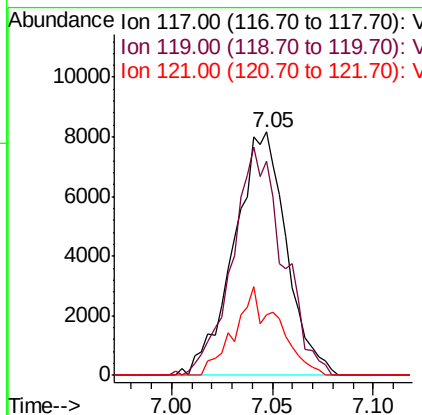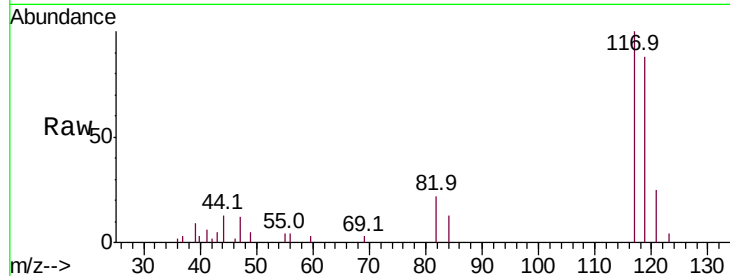


#36

Benzene
 Concen: 0.437 ppbv
 RT: 6.92 min Scan# 1284
 Delta R.T. 0.01 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Tgt Ion	Ratio	Lower	Upper
78	100		
77	21.7	19.3	28.9
50	13.7	11.0	16.6

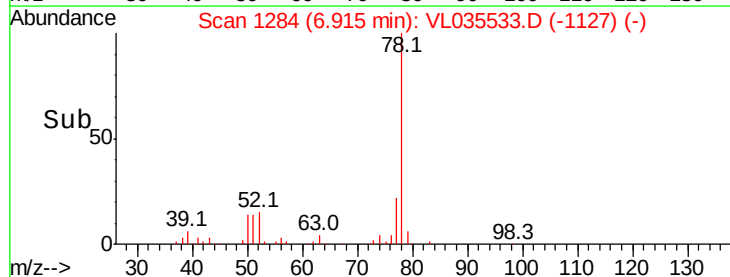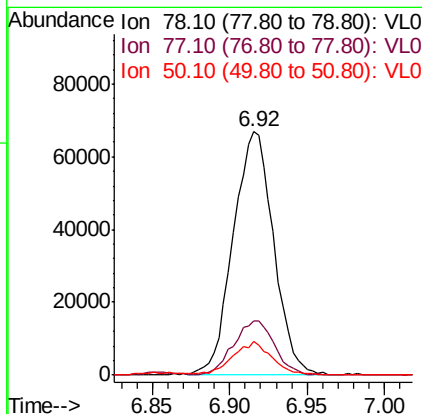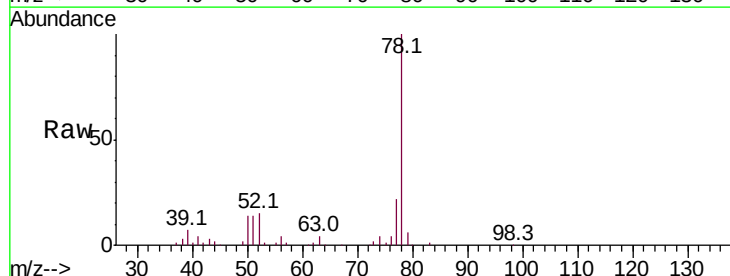



#43

Methyl Methacrylate

Concen: 0.202 ppbv m

RT: 8.04 min Scan# 1635

Delta R.T. 0.01 min

Lab File: VL035533.D

Acq: 3 Sep 2020 16:34

Instrument :

MSVOA_L

ClientSampleId :

IA-1DUP

Tot Ion: 69 Resp: 21753

Ion Ratio Lower Upper

69 100





41 95.2 76.6 114.8

100 34.7 33.8 50.6

Manual Integrations
APPROVED

MMDadoda

9/8/2020 4:06:18 PM

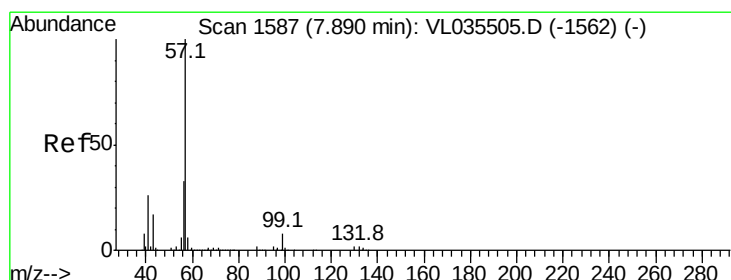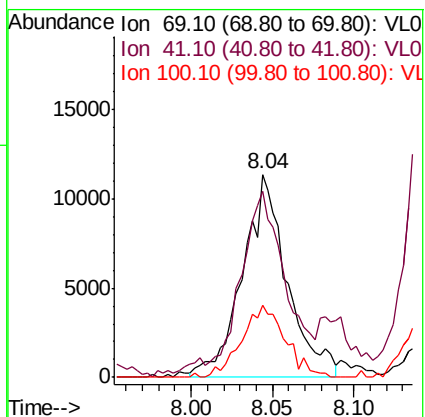

#44

2,2,4-Trimethylpentane

Concen: 0.641 ppbv

RT: 7.90 min Scan# 1589

Delta R.T. 0.01 min

Lab File: VL035533.D

Acq: 3 Sep 2020 16:34




Tgt Ion: 57 Resp: 234306


Ion Ratio Lower Upper

57 100

41 31.7 20.5 30.7#

56 39.2 25.3 37.9#

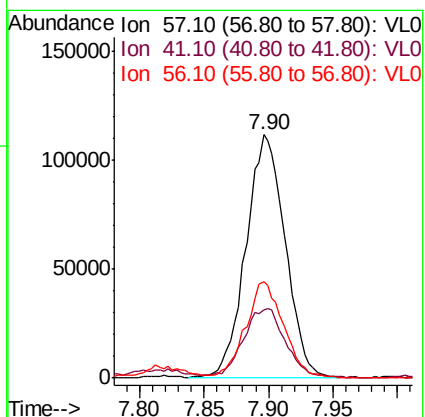

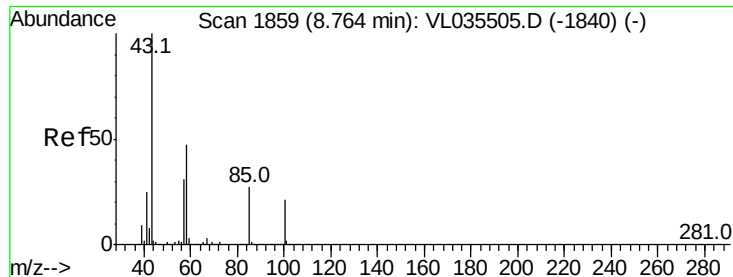

#50

4-Methyl-2-Pentanone

Concen: 0.227 ppbv

RT: 8.78 min Scan# 1864

Delta R.T. 0.02 min

Lab File: VL035533.D

Acq: 3 Sep 2020 16:34

Instrument :

MSVOA_L

ClientSampleId :

IA-1DUP

Tot Ion: 43 Resp: 41901

Ion Ratio Lower Upper





43 100

58 44.8 37.4 56.0

Manual Integrations
APPROVED

MMDadoda

9/8/2020 4:06:18 PM

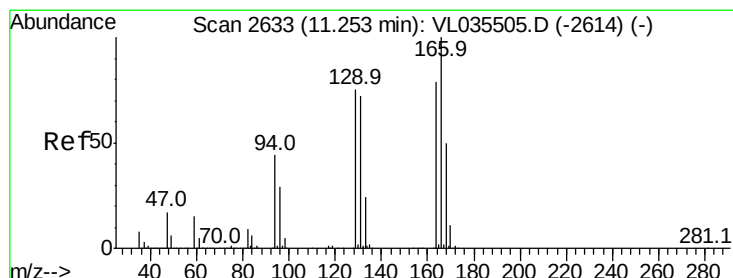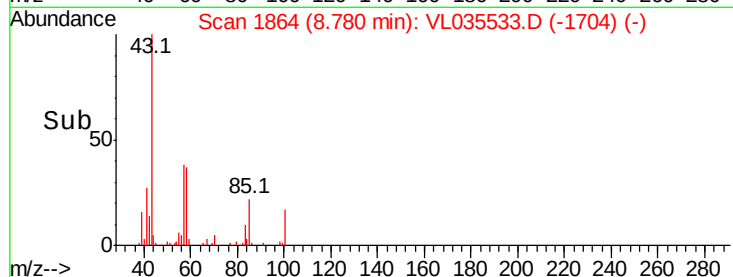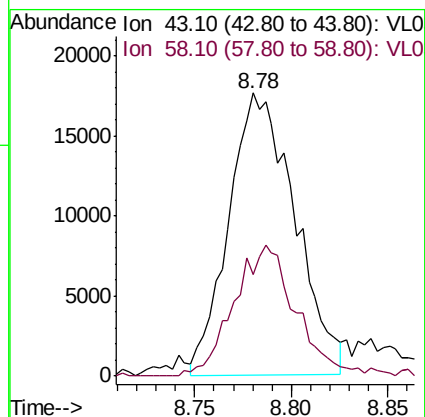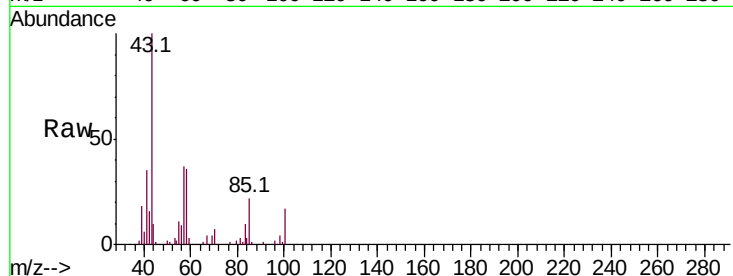

#52

Tetrachloroethene

Concen: 0.056 ppbv m

RT: 11.26 min Scan# 2634

Delta R.T. 0.00 min

Lab File: VL035533.D

Acq: 3 Sep 2020 16:34

Tgt Ion: 164 Resp: 9162




Ion Ratio Lower Upper


164 100

166 110.7 100.9 151.3

129 93.9 75.3 112.9

131 68.1 73.0 109.4#

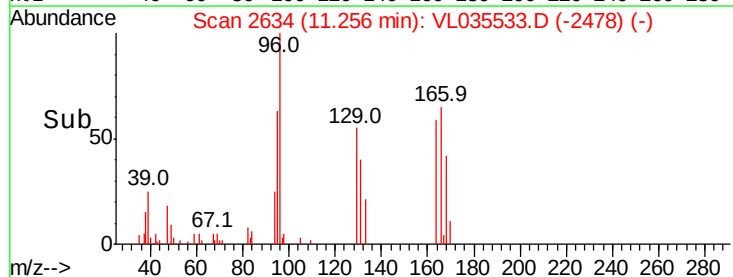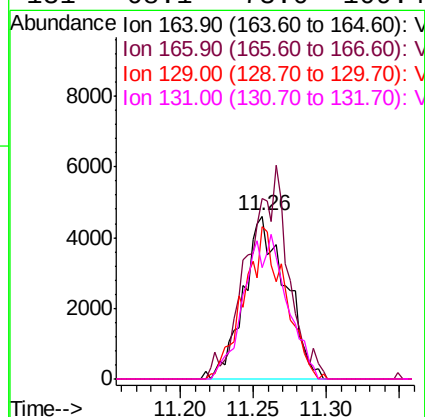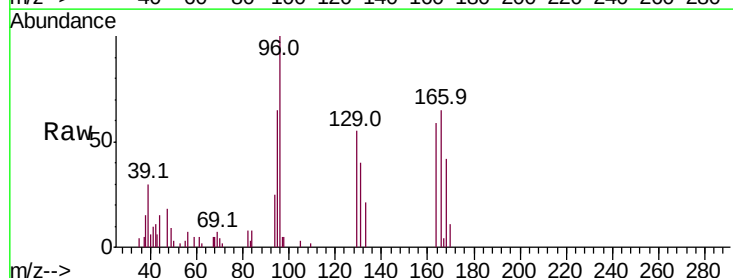







#53
Toluene
Concen: 3.577 ppbv
RT: 9.84 min Scan# 2193
Delta R.T. 0.01 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Instrument :
MSVOA_L
ClientSampleId :
IA-1DUP

Tot Ion: 91 Resp: 1250337
Ion Ratio Lower Upper
91 100
92 60.7 49.8 74.8




Manual Integrations
APPROVED


MMDadoda
9/8/2020 4:06:18 PM

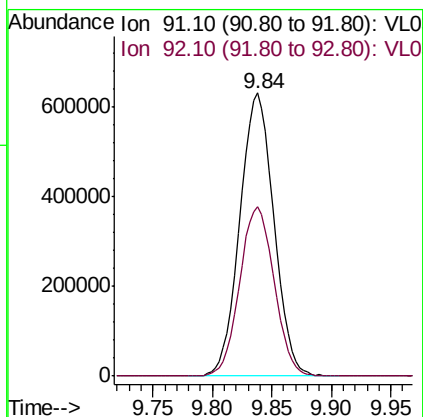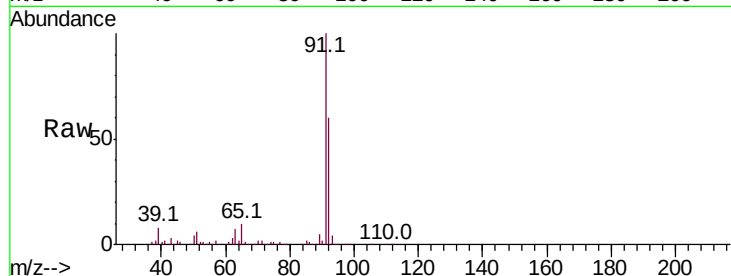

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.12 min Scan# 2904
Delta R.T. 0.01 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Tgt Ion: 117 Resp: 4231143
Ion Ratio Lower Upper
117 100
82 55.0 41.6 62.4
119 34.7 29.3 43.9

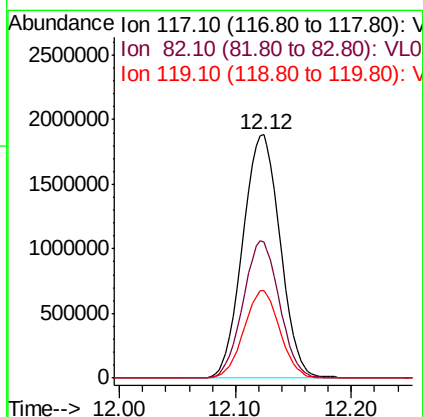



#58

Ethyl Benzene

Concen: 0.396 ppbv

RT: 12.75 min Scan# 3098

Delta R.T. 0.01 min

Lab File: VL035533.D

Acq: 3 Sep 2020 16:34

Instrument :

MSVOA_L

ClientSampleId :

IA-1DUP

Tot Ion: 91 Resp: 172874


Ion Ratio Lower Upper

91 100

106 32.8 30.3 45.5




Manual Integrations
APPROVED

MMDadoda
9/8/2020 4:06:18 PM



Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 106.10 (105.80 to 106.80): V

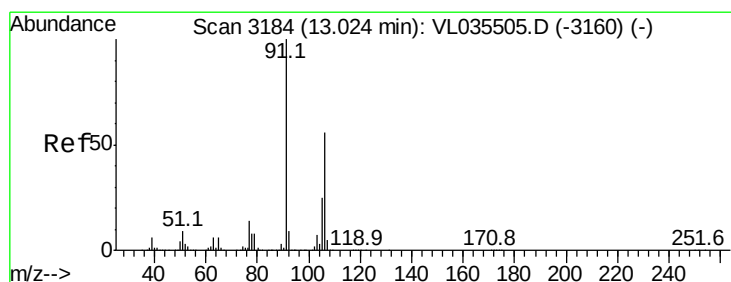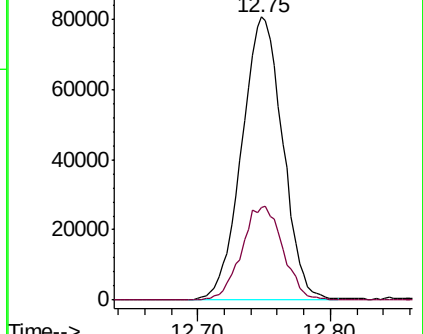

#59

m/p-Xylene

Concen: 1.434 ppbv

RT: 13.00 min Scan# 3177

Delta R.T. -0.02 min

Lab File: VL035533.D


Acq: 3 Sep 2020 16:34

Tgt Ion: 91 Resp: 522991

Ion Ratio Lower Upper



91 100


106 52.1 43.4 65.2

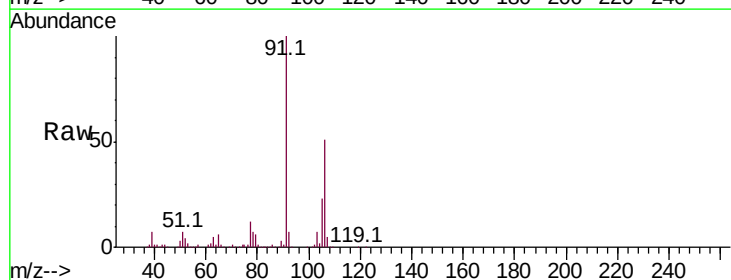

Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 106.10 (105.80 to 106.80): V

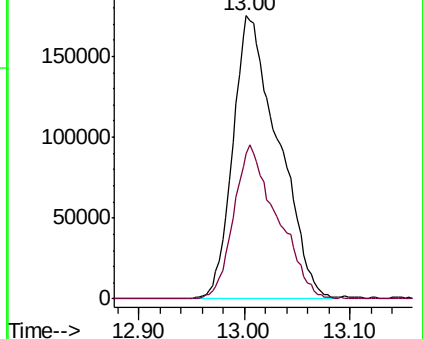







#60
o-Xylene
Concen: 0.495 ppbv
RT: 13.73 min Scan# 3404
Delta R.T. 0.01 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Instrument :
MSVOA_L
ClientSampled :
IA-1DUP

Tot Ion: 91 Resp: 181643
Ion Ratio Lower Upper
91 100
106 50.4 25.8 77.4




Manual Integrations
APPROVED


MMDadoda
9/8/2020 4:06:18 PM

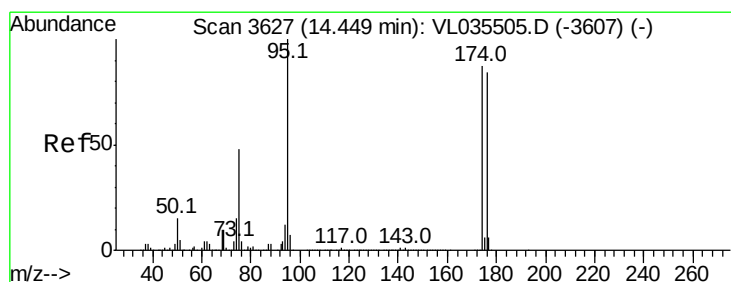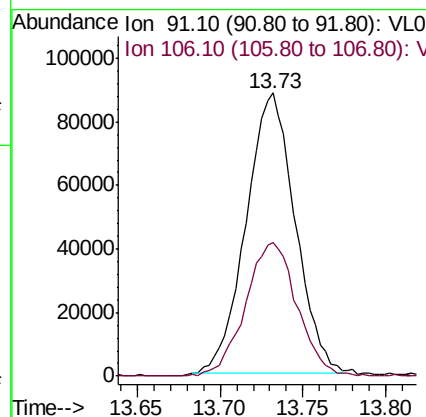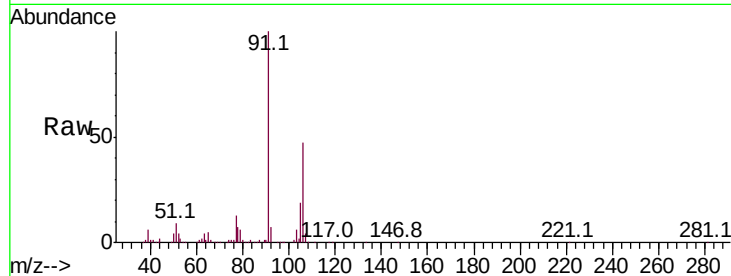

#68
1-Bromo-4-Fluorobenzene
Concen: 10.368 ppbv
RT: 14.46 min Scan# 3629
Delta R.T. 0.01 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Tgt Ion: 95 Resp: 3115290
Ion Ratio Lower Upper
95 100
174 85.3 69.6 104.4
175 6.1 5.1 7.7

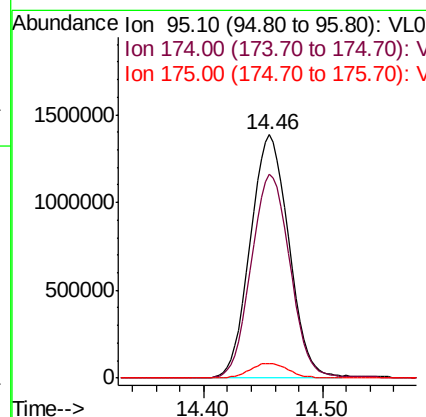

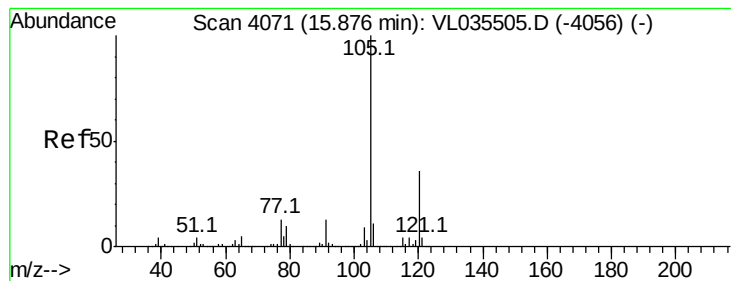


#72
4-Ethyltoluene
Concen: 0.194 ppbv
RT: 15.88 min Scan# 4072
Delta R.T. 0.00 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Instrument :
MSVOA_L
ClientSampleId :
IA-1DUP




Tot Ion:	105	Resp:	90337
Ion Ratio	Lower	Upper	
105	100		
120	33.2	27.4	41.2
91	16.4	9.7	14.5#
77	13.6	9.6	14.4

Manual Integrations
APPROVED

MMDadoda
9/8/2020 4:06:18 PM

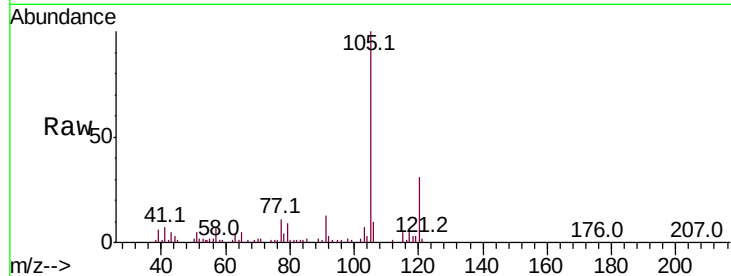


Abundance Ion 105.10 (104.80 to 105.80): V
Ion 120.20 (119.90 to 120.90): V
Ion 91.10 (90.80 to 91.80): VL0
Ion 77.10 (76.80 to 77.80): VL0

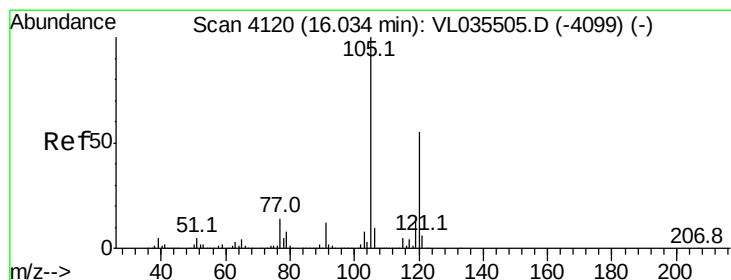
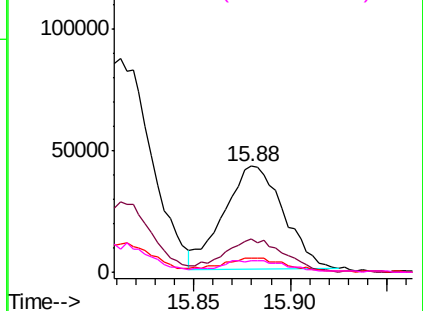



#73
1,3,5-Trimethylbenzene
Concen: 0.208 ppbv m
RT: 16.04 min Scan# 4121
Delta R.T. 0.00 min
Lab File: VL035533.D
Acq: 3 Sep 2020 16:34

Tgt Ion:	105	Resp:	89755
Ion Ratio	Lower	Upper	
105	100		
120	45.5	44.2	66.2



Abundance Ion 105.10 (104.80 to 105.80): V
Ion 120.20 (119.90 to 120.90): V

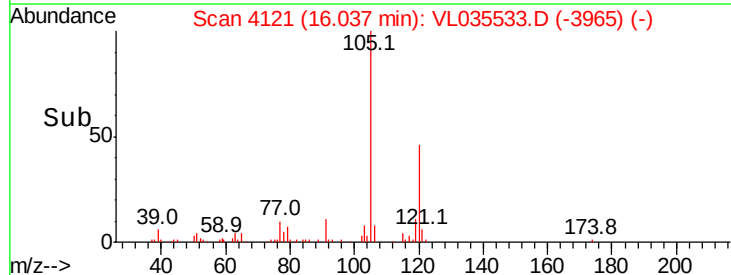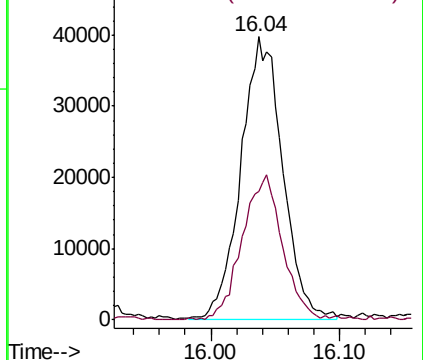







#74
 1,2,4-Trimethylbenzene
 Concen: 0.692 ppbv
 RT: 16.81 min Scan# 4360
 Delta R.T. 0.00 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Instrument :
 MSVOA_L
 ClientSampleId :
 IA-1DUP

Tot Ion	Ratio	Lower	Upper
105	100		
120	47.4	44.4	66.6
91	11.0	37.1	55.7#
77	12.5	16.0	24.0#




Manual Integrations
 APPROVED


MMDadoda
 9/8/2020 4:06:18 PM

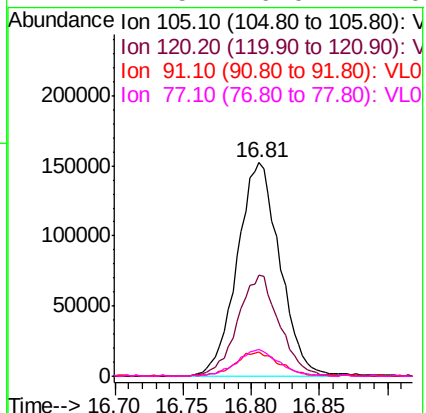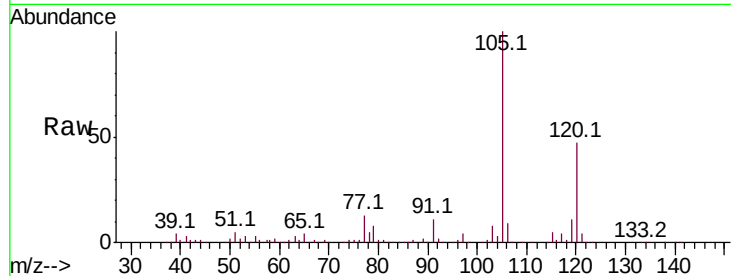

#79
 Naphthalene
 Concen: 2.993 ppbv
 RT: 22.26 min Scan# 6056
 Delta R.T. 0.01 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Tgt Ion	Ratio	Lower	Upper
128	100		
127	12.5	11.4	17.2
129	11.4	10.5	15.7

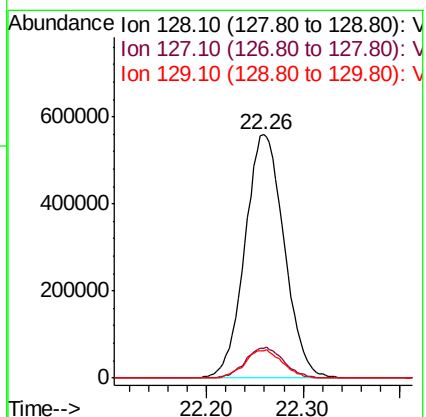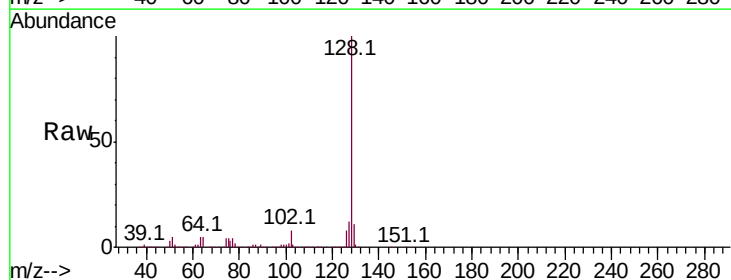




#80
 Naphthalene, 2-methyl-
 Concen: 0.387 ppbv
 RT: 25.02 min Scan# 6914
 Delta R.T. 0.01 min
 Lab File: VL035533.D
 Acq: 3 Sep 2020 16:34

Instrument :
 MSVOA_L
 ClientSampleId :
 IA-1DUP

Tot Ion:	142	Resp:	69437
Ion Ratio	Lower	Upper	
142	100		
141	85.4	67.6	101.4
115	33.6	25.8	38.8

Manual Integrations
 APPROVED

MMDadoda
 9/8/2020 4:06:18 PM



Abundance Ion 142.00 (141.70 to 142.70): V
 Ion 141.00 (140.70 to 141.70): V
 Ion 115.00 (114.70 to 115.70): V

