


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL090320\
 Data File : VL035526.D
 Acq On : 3 Sep 2020 10:05
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL082720AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
 Last Update : Thu Aug 27 06:46:28 2020

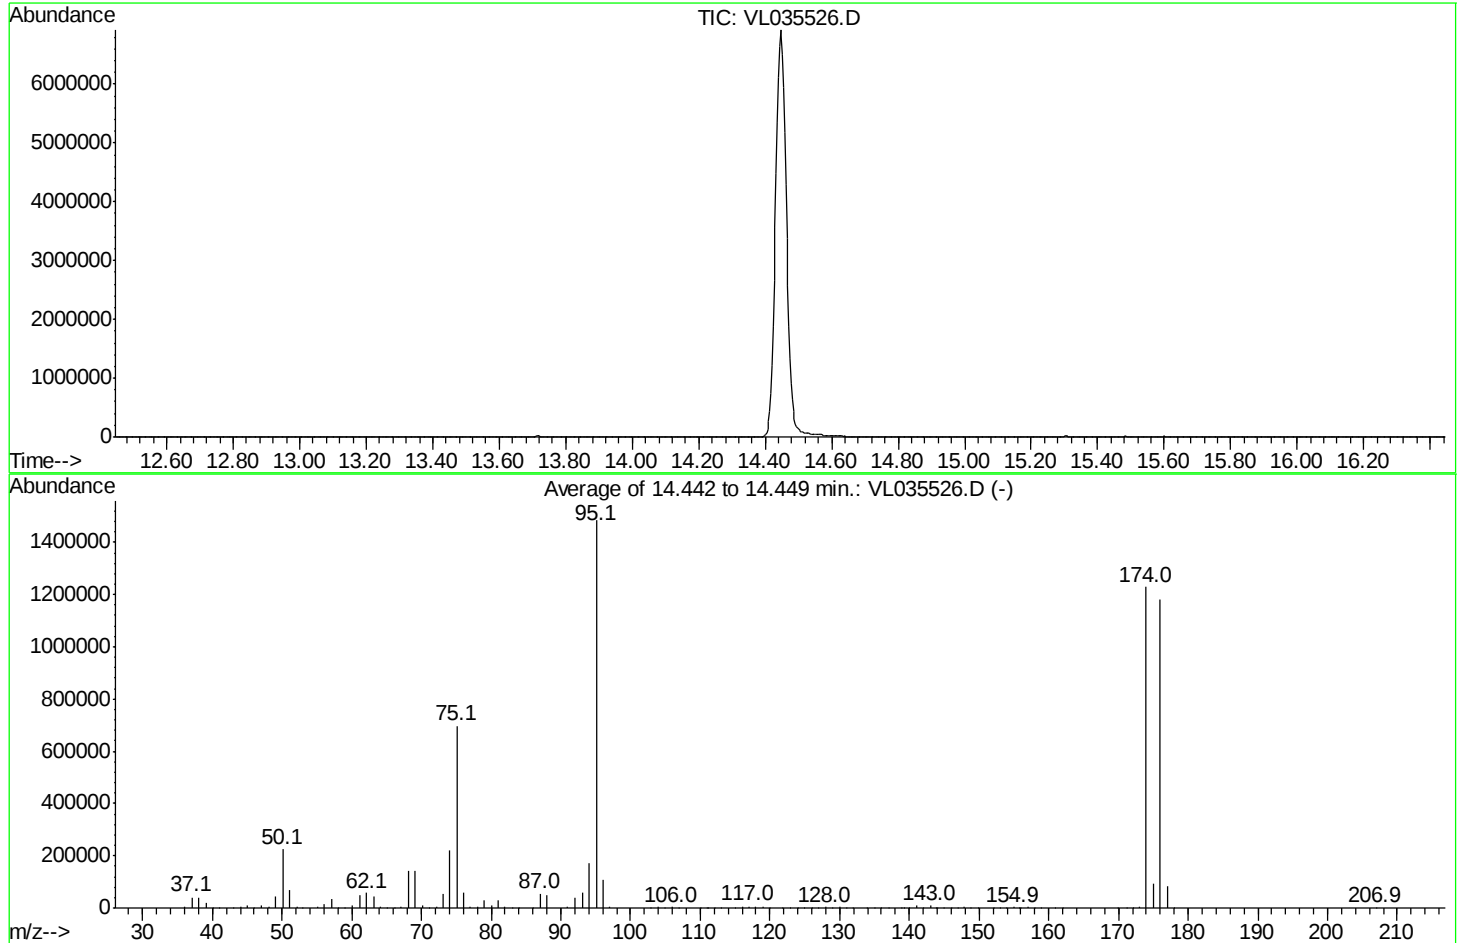

AutoFind: Scans 3625, 3626, 3627; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	15.2	224938	PASS
75	95	30	66	47.0	697642	PASS
95	95	100	100	100.0	1484288	PASS
96	95	5	9	7.4	110058	PASS
173	174	0.00	2	0.5	6206	PASS
174	95	50	120	82.8	1228800	PASS
175	174	4	9	7.5	91552	PASS
176	174	93	101	96.1	1180501	PASS
177	176	5	9	7.1	83850	PASS