

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090321\
 Data File : VL037519.D
 Acq On : 3 Sep 2021 13:50
 Operator : SY/AP
 Sample : CAN 10053
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 CAN 10053

Quant Time: Sep 04 04:21:59 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
 QLast Update : Tue Aug 17 02:13:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.661	49	1454110	10.000	ppbv	0.01
33) 1,4-Difluorobenzene	7.169	114	4209887	10.000	ppbv	0.01
55) Chlorobenzene-d5	12.076	117	3494434	10.000	ppbv	0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.407	95	2495306	10.051	ppbv	0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090321\
Data File : VL037519.D
Acq On : 3 Sep 2021 13:50
Operator : SY/AP
Sample : CAN 10053
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10053

Quant Time: Sep 04 04:21:59 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
QLast Update : Tue Aug 17 02:13:47 2021
Response via : Initial Calibration




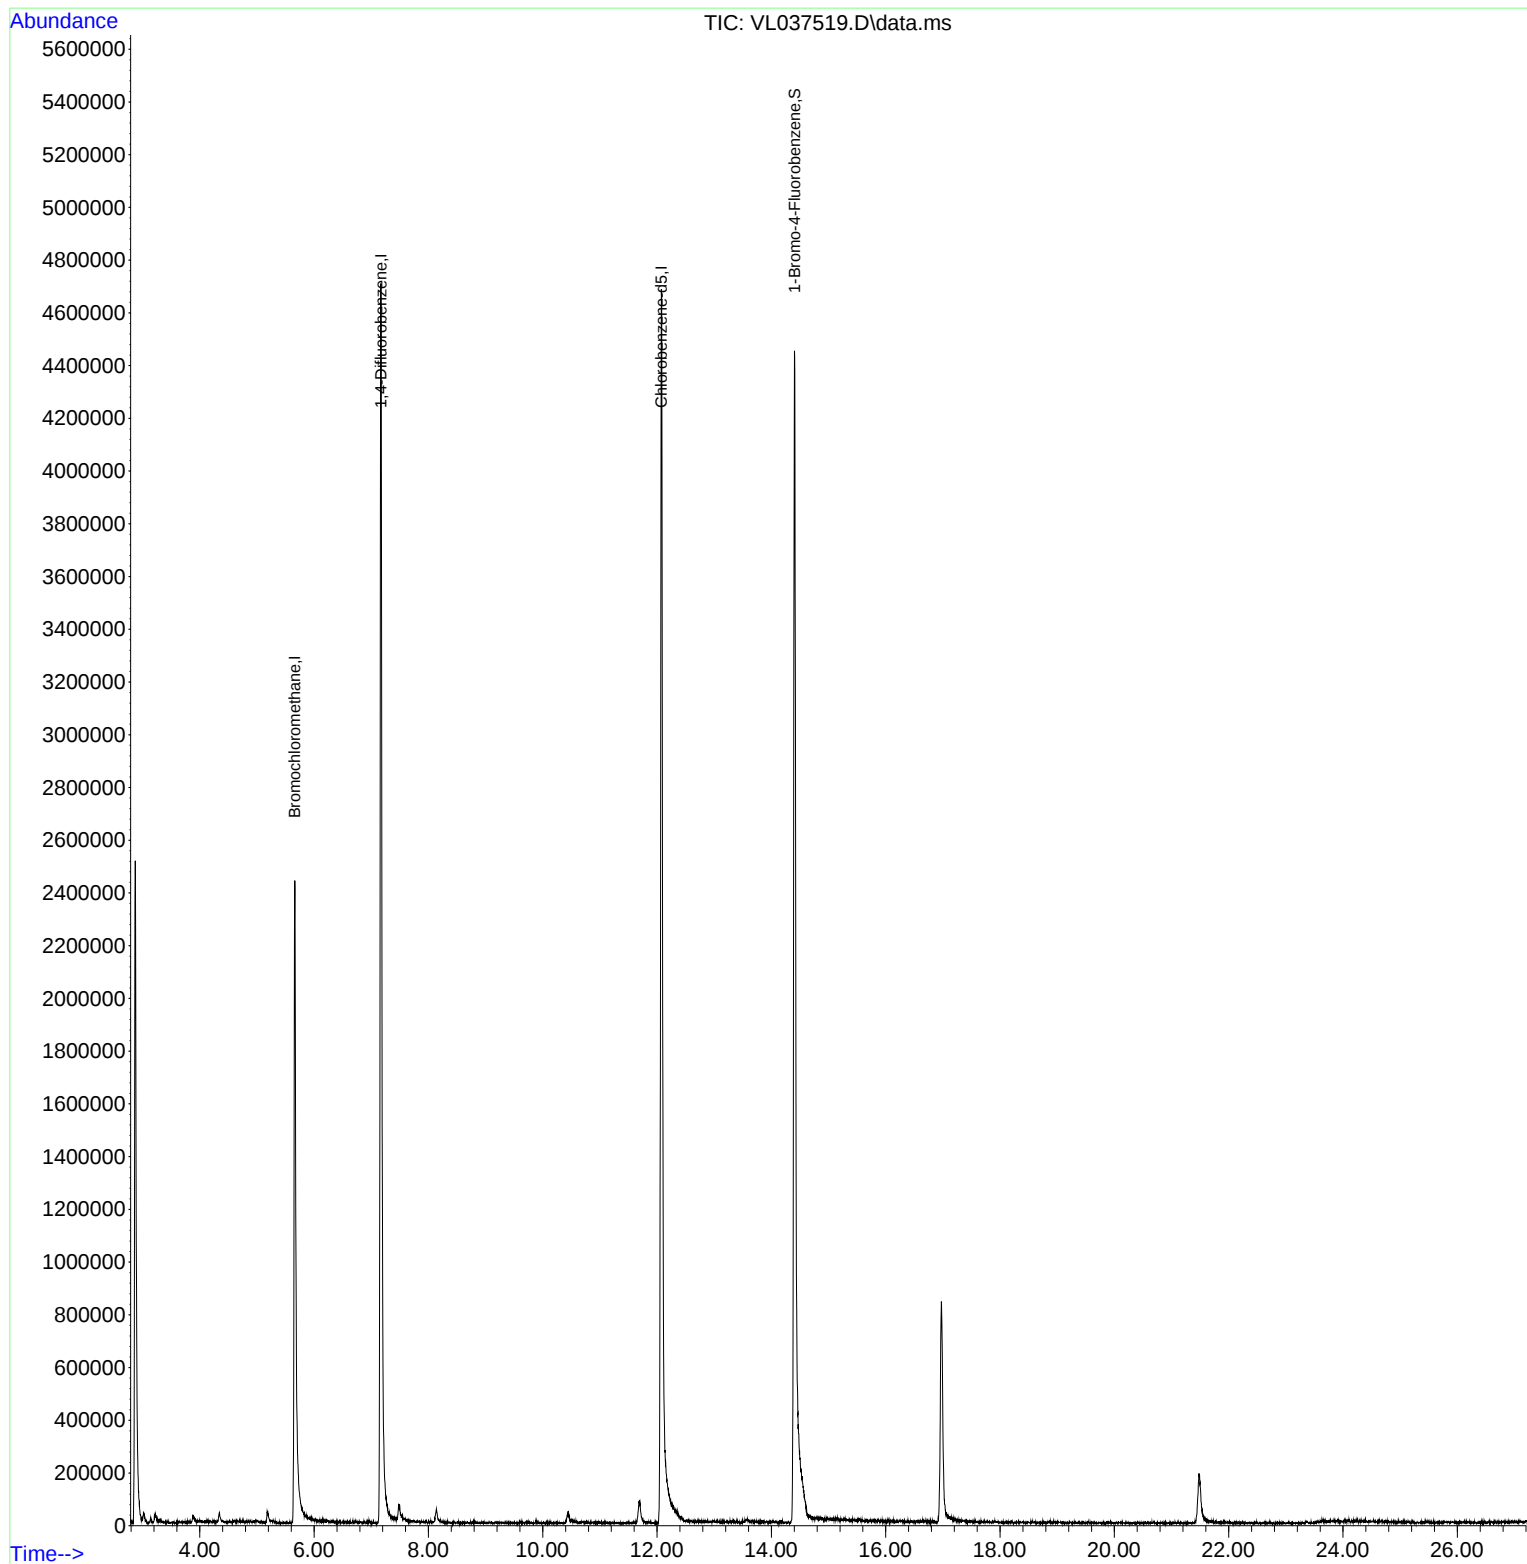


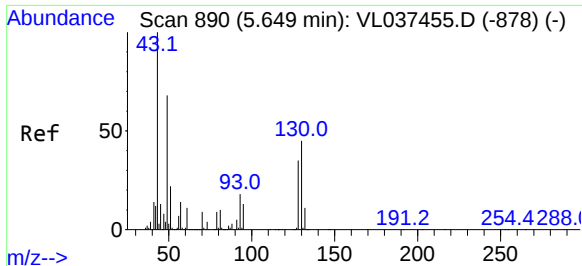

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.661 min Scan# 894
Delta R.T. 0.013 min
Lab File: VL037519.D
Acq: 3 Sep 2021 13:50




Instrument :
MSVOA_L
ClientSampleId :
CAN 10053


Tgt Ion: 49 Resp: 1454110
Ion Ratio Lower Upper
49 100
128 54.3 27.5 82.4
130 69.3 34.0 101.8

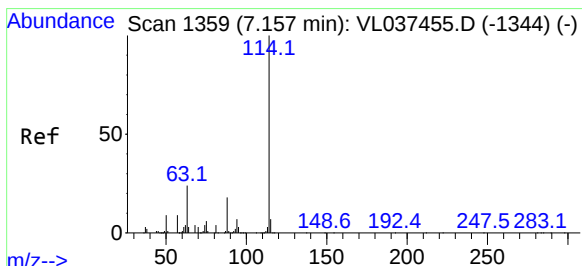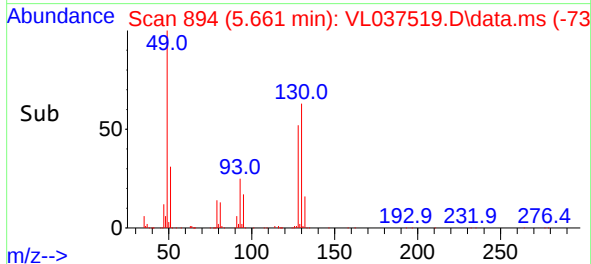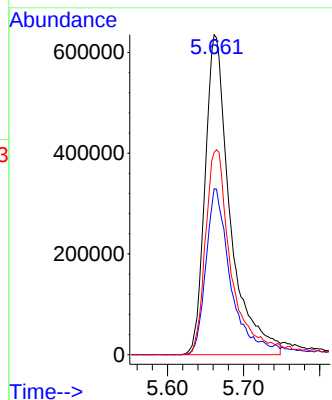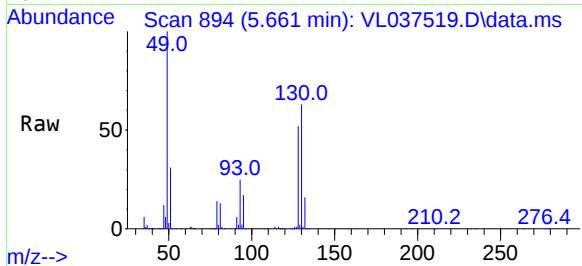

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.169 min Scan# 1363
Delta R.T. 0.013 min
Lab File: VL037519.D
Acq: 3 Sep 2021 13:50

Tgt Ion: 114 Resp: 4209887
Ion Ratio Lower Upper
114 100
63 23.6 19.3 28.9
88 18.1 14.2 21.4


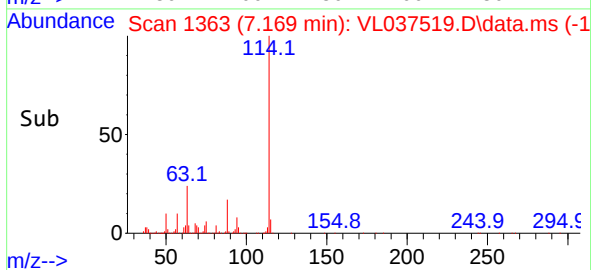
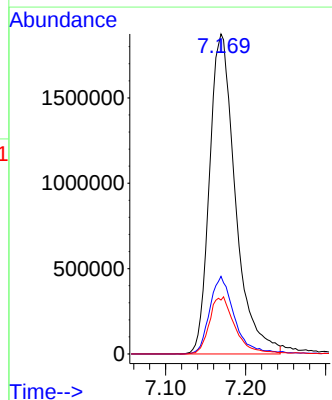
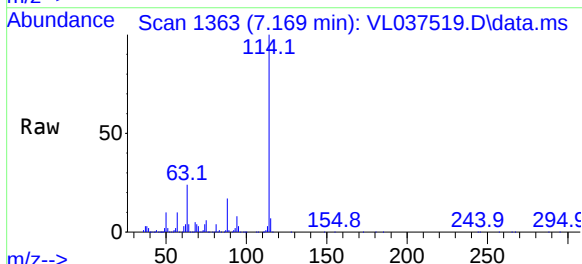


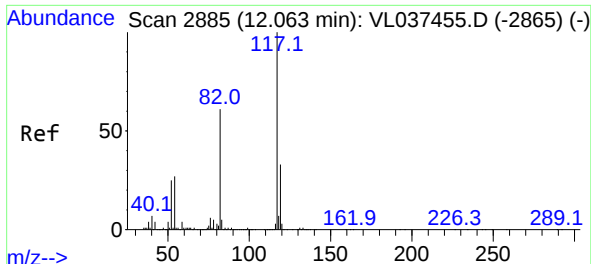

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.076 min Scan# 2889
Delta R.T. 0.013 min
Lab File: VL037519.D
Acq: 3 Sep 2021 13:50

Instrument :
MSVOA_L
ClientSampleId :
CAN 10053

Tgt Ion:117 Resp: 3494434
Ion Ratio Lower Upper
117 100
82 67.3 52.9 79.3
119 35.7 24.8 37.2

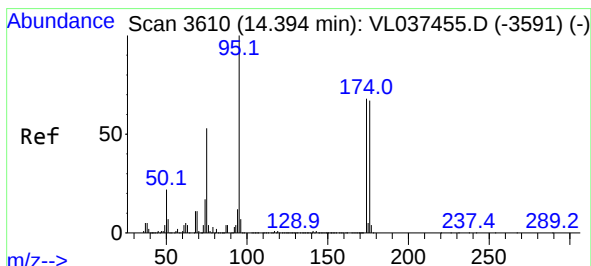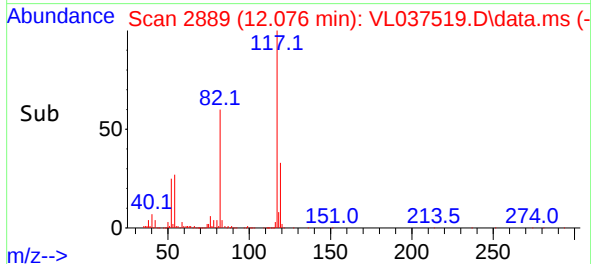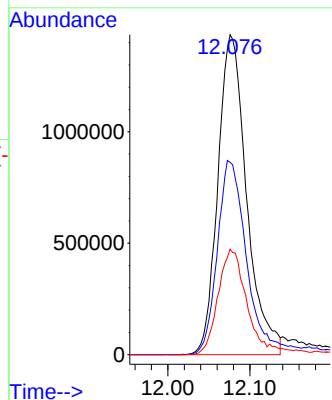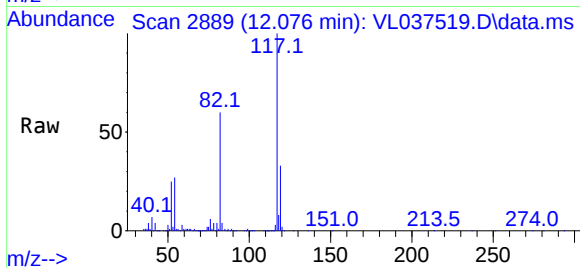

#68
1-Bromo-4-Fluorobenzene
Concen: 10.051 ppbv
RT: 14.407 min Scan# 3614
Delta R.T. 0.013 min
Lab File: VL037519.D
Acq: 3 Sep 2021 13:50

Tgt Ion: 95 Resp: 2495306
Ion Ratio Lower Upper
95 100
174 75.6 59.6 89.4
175 5.6 4.6 7.0

