

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090321\
 Data File : VL037536.D
 Acq On : 4 Sep 2021 00:34
 Operator : SY/AP
 Sample : CAN 10607
 Misc : 400mL/MSVOA_L
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 CAN 10607

Quant Time: Sep 04 04:24:05 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LTue Aug 17 02:13:47 2021
 QLast Update : Tue Aug 17 02:13:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.664	49	1613910	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	7.169	114	4786150	10.000	ppbv	0.01
55) Chlorobenzene-d5	12.079	117	4088543	10.000	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.407	95	3031245	10.436	ppbv	0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	104.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090321\
Data File : VL037536.D
Acq On : 4 Sep 2021 00:34
Operator : SY/AP
Sample : CAN 10607
Misc : 400mL/MSVOA_L
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10607

Quant Time: Sep 04 04:24:05 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
QLast Update : Tue Aug 17 02:13:47 2021
Response via : Initial Calibration




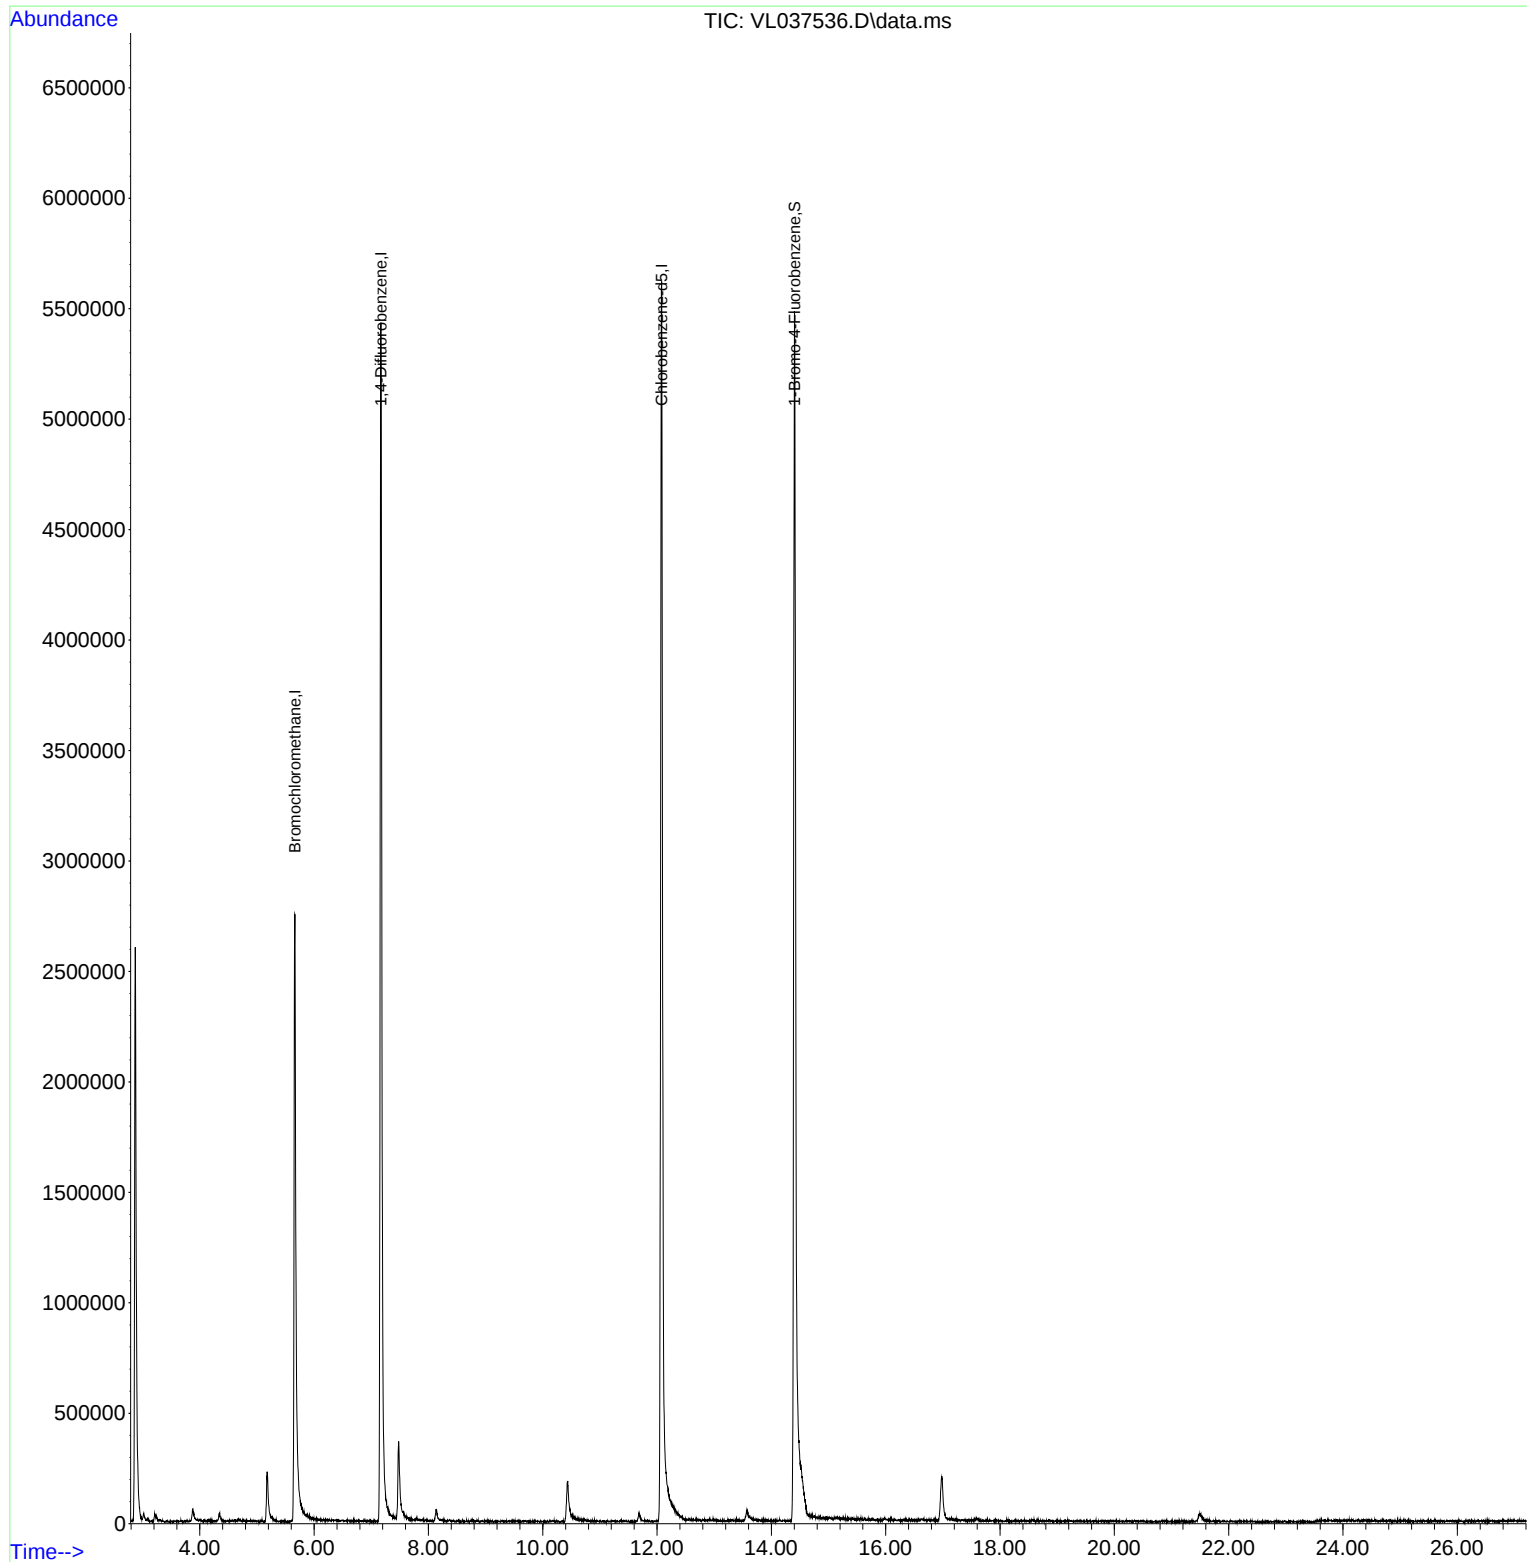


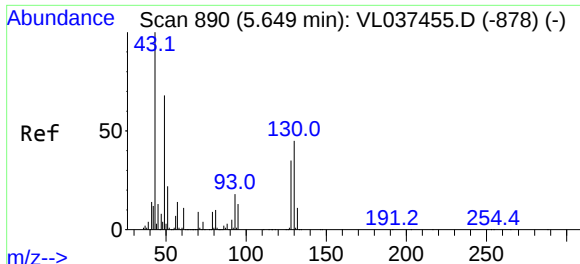

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.664 min Scan# 895
Delta R.T. 0.016 min
Lab File: VL037536.D
Acq: 4 Sep 2021 00:34




Instrument :
MSVOA_L
ClientSampleId :
CAN 10607


Tgt Ion: 49 Resp: 1613910
Ion Ratio Lower Upper
49 100
128 56.0 27.5 82.4
130 70.2 34.0 101.8

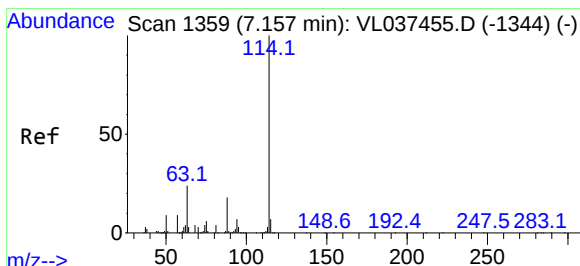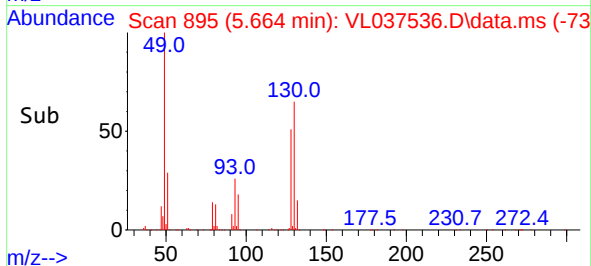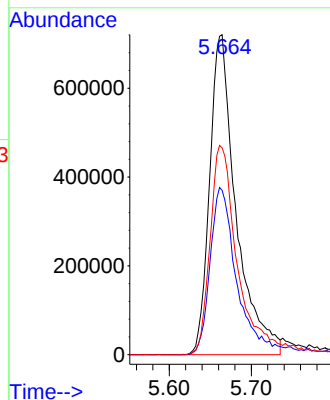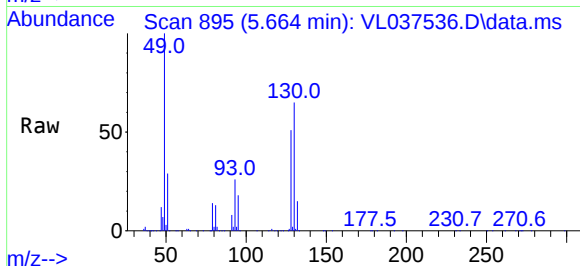

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.169 min Scan# 1363
Delta R.T. 0.013 min
Lab File: VL037536.D
Acq: 4 Sep 2021 00:34

Tgt Ion: 114 Resp: 4786150
Ion Ratio Lower Upper
114 100
63 23.9 19.3 28.9
88 18.1 14.2 21.4

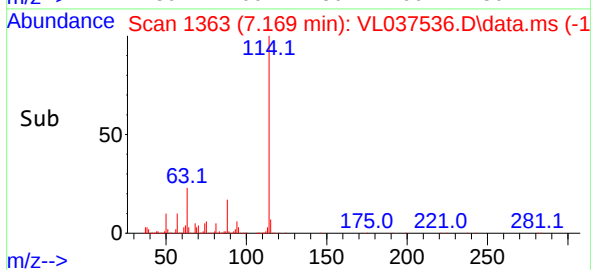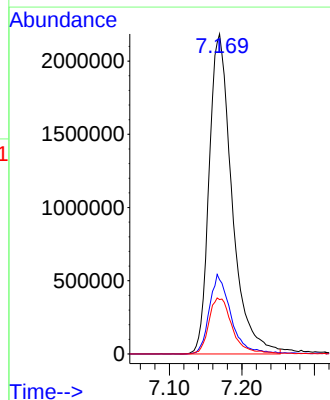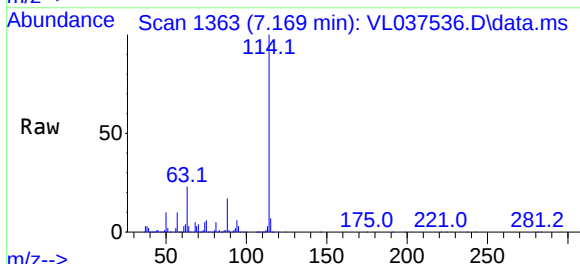




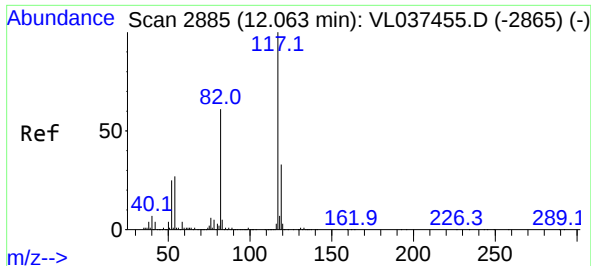


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.079 min Scan# 2890
Delta R.T. 0.016 min
Lab File: VL037536.D
Acq: 4 Sep 2021 00:34

Instrument :
MSVOA_L
ClientSampleId :
CAN 10607

Tgt Ion:117 Resp: 4088543

Ion	Ratio	Lower	Upper
117	100		
82	66.3	52.9	79.3
119	35.2	24.8	37.2

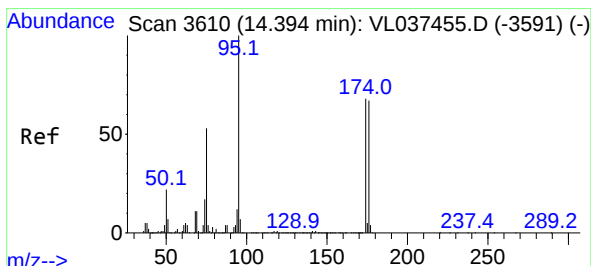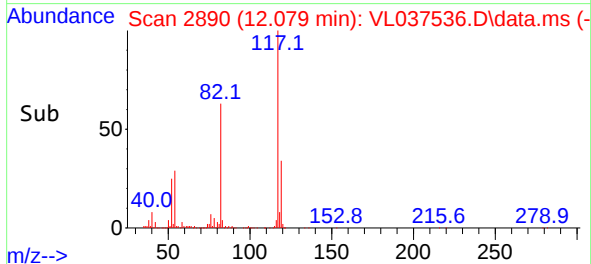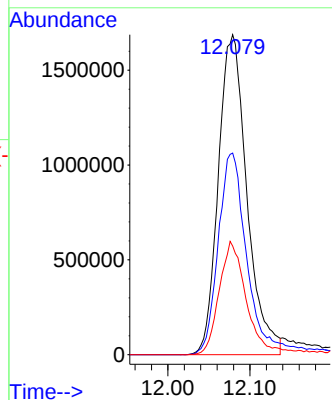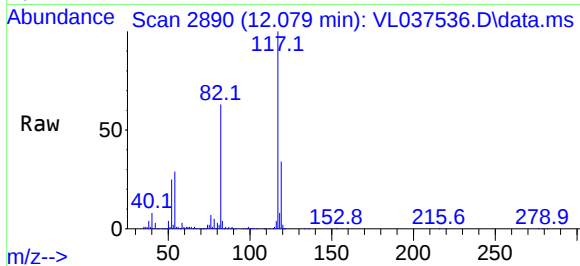

#68
1-Bromo-4-Fluorobenzene
Concen: 10.436 ppbv
RT: 14.407 min Scan# 3614
Delta R.T. 0.013 min
Lab File: VL037536.D
Acq: 4 Sep 2021 00:34

Tgt Ion: 95 Resp: 3031245

Ion	Ratio	Lower	Upper
95	100		
174	75.8	59.6	89.4
175	5.8	4.6	7.0

