


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090321\
 Data File : VL037514.D
 Acq On : 3 Sep 2021 7:40
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
 Last Update : Tue Aug 17 02:13:47 2021

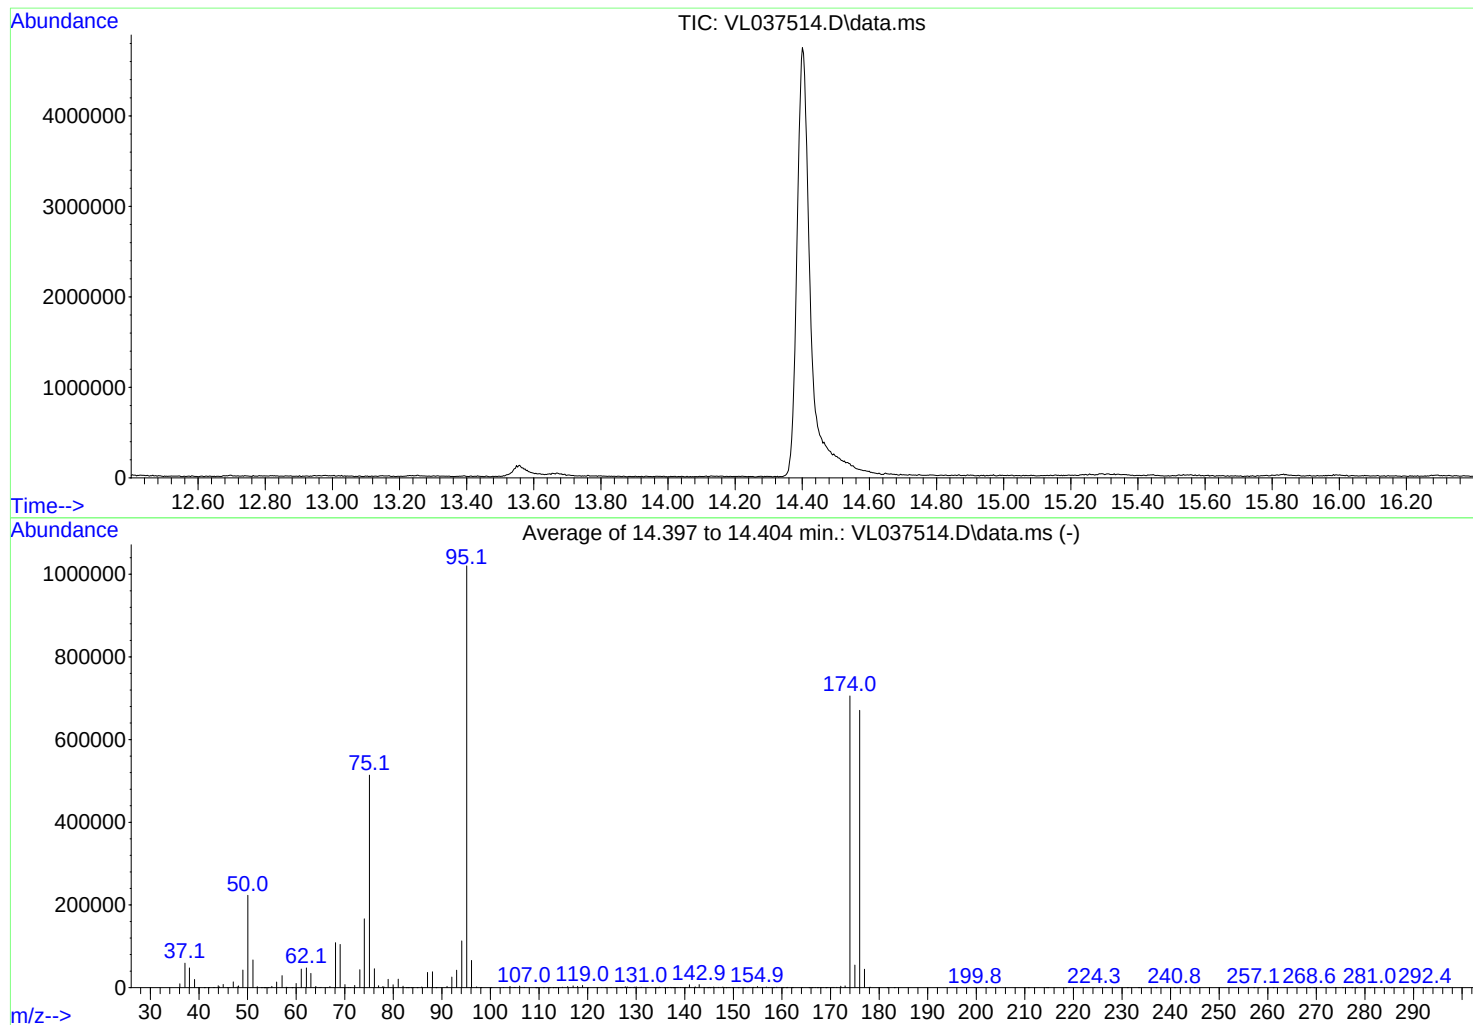

AutoFind: Scans 3611, 3612, 3613; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.9	223339	PASS
75	95	30	66	50.4	513941	PASS
95	95	100	100	100.0	1020288	PASS
96	95	5	9	6.5	65955	PASS
173	174	0.00	2	0.6	4127	PASS
174	95	50	120	69.2	705579	PASS
175	174	4	9	7.7	54558	PASS
176	174	93	101	95.1	670763	PASS
177	176	5	9	6.6	44493	PASS

Average of 14.397 to 14.404 min.: VL037514.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9321	45.00	7740	53.40	120	62.10	47672
37.10	59088	45.90	452	53.60	244	63.05	34317
38.05	47600	46.20	306	54.20	152	64.05	3020
39.10	19731	47.05	13882	55.00	3087	64.90	459
40.00	328	47.90	2046	56.00	13393	65.10	930
41.10	81	48.15	4383	57.10	29037	66.40	293
41.95	91	49.05	42493	57.95	1141	66.95	2676
42.95	479	50.05	223339	58.20	542	68.10	108939
43.20	292	51.10	66896	59.15	169	69.05	104520
43.95	4682	52.00	2556	60.00	10184	70.05	7250
44.20	1868	52.85	196	61.05	44859	70.85	324

Instrument :
MSVOA_L
ClientSampleId :
BFB

Average of 14.397 to 14.404 min.: VL037514.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
71.20	262	81.00	20723	91.05	2998	104.05	2573
72.05	5378	82.00	3605	92.05	25528	104.85	752
73.10	43581	82.70	167	93.05	42280	105.10	424
74.05	166357	83.10	174	94.10	113048	106.00	3831
75.10	513941	83.70	94	95.10	1.02029e+006	106.95	918
76.10	45515	84.20	295	96.10	65955	109.30	80
76.95	4665	84.90	115	97.15	2050	109.50	89
77.85	2868	85.85	1542	98.00	70	109.80	302
78.10	1726	87.05	36720	100.10	58	110.90	100
78.95	20185	88.05	38272	102.70	297	111.05	381
79.95	6901	88.80	191	103.90	1167	111.80	313

Average of 14.397 to 14.404 min.: VL037514.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
112.15	186	121.95	254	128.15	1826	134.75	1358
112.90	132	122.90	350	128.70	440	135.00	501
113.05	495	123.65	241	128.90	385	135.80	170
113.40	51	123.95	347	129.40	577	136.30	112
113.90	53	124.65	385	129.70	1276	136.65	565
114.80	1080	124.90	397	130.00	1876	137.00	814
115.90	2889	125.80	224	131.00	1094	137.20	121
117.00	4320	126.00	315	132.40	270	137.60	77
117.95	2998	126.75	316	133.80	353	137.90	306
118.95	5249	127.00	151	134.10	180	138.20	296
120.00	84	127.75	2252	134.50	115	138.60	369

Average of 14.397 to 14.404 min.: VL037514.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
139.10	657	146.95	823	152.30	68	160.90	166
139.65	472	147.85	1672	153.00	708	161.10	737
140.20	817	148.10	518	154.10	855	162.10	82
140.95	7117	148.50	60	154.95	2845	164.20	277
142.15	1987	149.05	289	156.00	375	165.60	81
142.95	7430	149.30	259	156.80	1782	166.20	154
144.00	510	149.80	210	157.30	403	166.85	326
144.70	222	150.10	662	157.80	342	167.30	229
145.00	676	151.00	157	158.20	82	167.90	208
145.20	197	151.80	562	158.95	1199	168.45	311
145.95	1610	152.00	56	160.20	95	169.00	108

Average of 14.397 to 14.404 min.: VL037514.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
169.20	526	177.90	538	233.40	78	277.30	75
169.45	596	178.15	1042	237.00	55	278.20	115
170.30	809	181.70	180	240.80	117	281.00	159
170.70	680	183.10	62	244.90	95	285.40	107
171.30	755	199.75	270	257.10	176	292.40	202
172.10	3488	210.70	126	258.20	172		
173.00	4127	214.50	270	261.10	66		

174.00	705579	214.70	94	268.60	188
175.00	54558	218.40	165	269.50	73
176.00	670763	224.30	407	273.90	157
177.00	44493	231.10	53	275.40	58

Instrument :
MSVOA_L
ClientSampleId :
BFB