

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090721\
 Data File : VL037544.D
 Acq On : 7 Sep 2021 10:56
 Operator : SY/AP
 Sample : CAN 10595
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 CAN 10595

Quant Time: Sep 08 11:10:16 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
 QLast Update : Tue Aug 17 02:13:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.664	49	1828277	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	7.169	114	5330936	10.000	ppbv	0.01
55) Chlorobenzene-d5	12.079	117	4694779	10.000	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.410	95	3479046	10.431	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	104.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090721\
Data File : VL037544.D
Acq On : 7 Sep 2021 10:56
Operator : SY/AP
Sample : CAN 10595
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10595

Quant Time: Sep 08 11:10:16 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
QLast Update : Tue Aug 17 02:13:47 2021
Response via : Initial Calibration

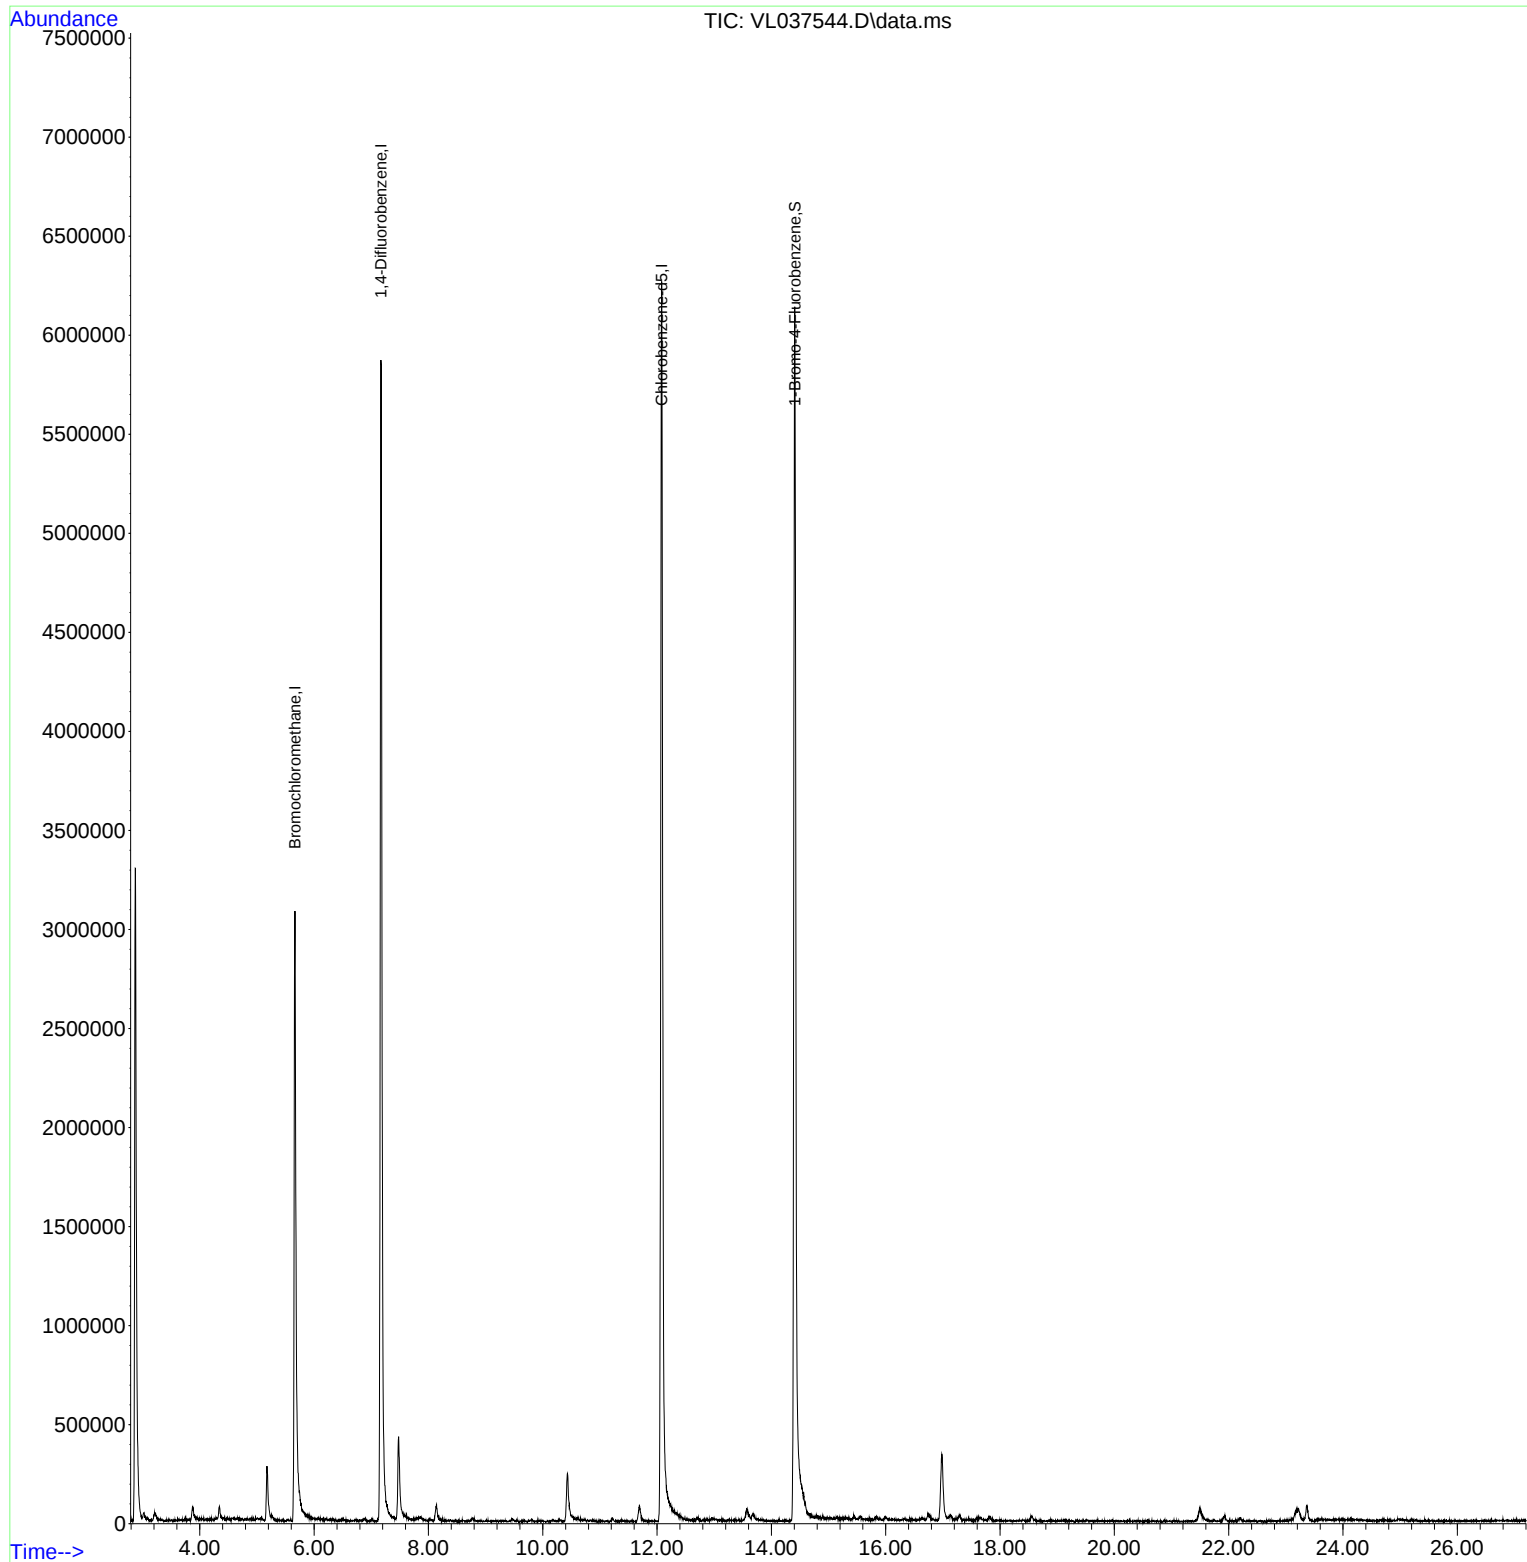




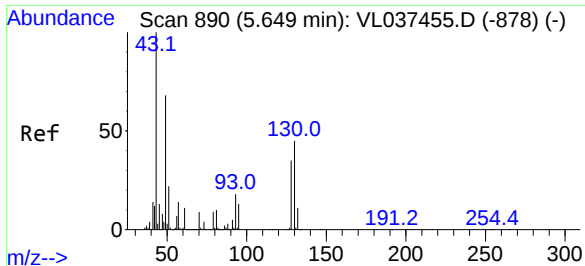


#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.664 min Scan# 895
Delta R.T. 0.016 min
Lab File: VL037544.D
Acq: 7 Sep 2021 10:56

Instrument :
MSVOA_L
ClientSampleId :
CAN 10595

Tgt Ion: 49 Resp: 1828277




Ion	Ratio	Lower	Upper
49	100		
128	52.7	27.5	82.4
130	68.9	34.0	101.8

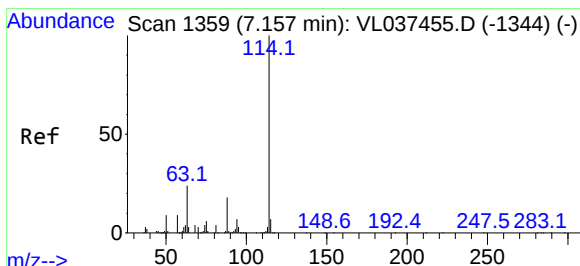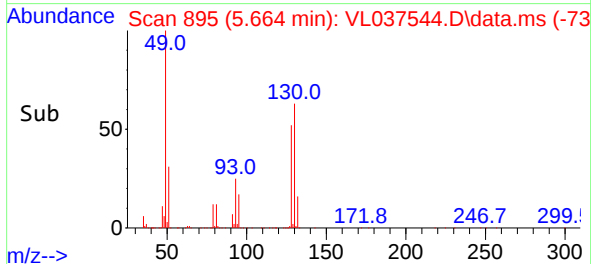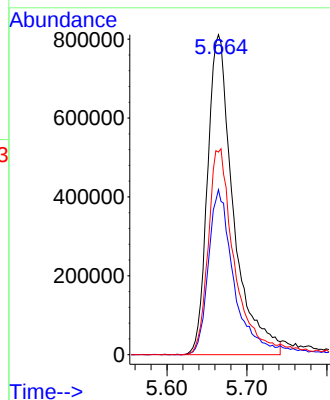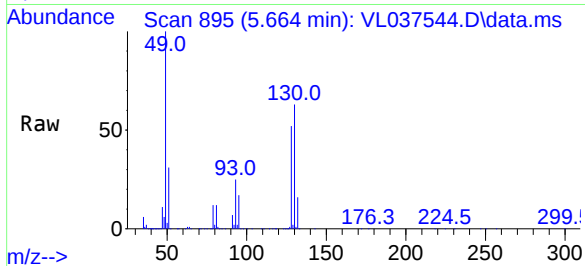


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.169 min Scan# 1363
Delta R.T. 0.013 min
Lab File: VL037544.D
Acq: 7 Sep 2021 10:56

Tgt Ion: 114 Resp: 5330936

Ion	Ratio	Lower	Upper
114	100		
63	24.0	19.3	28.9
88	17.8	14.2	21.4

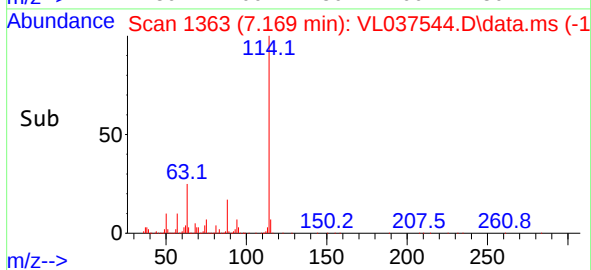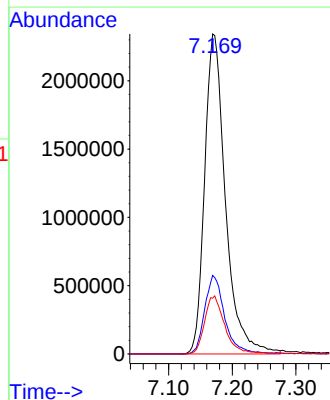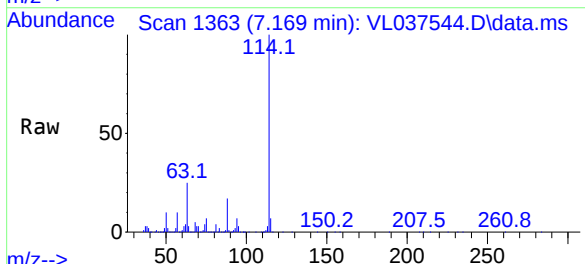




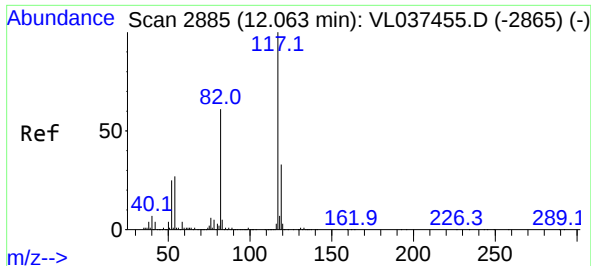


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.079 min Scan# 2890
Delta R.T. 0.016 min
Lab File: VL037544.D
Acq: 7 Sep 2021 10:56

Instrument :
MSVOA_L
ClientSampleId :
CAN 10595

Tgt Ion:117 Resp: 4694779

Ion	Ratio	Lower	Upper
117	100		
82	63.3	52.9	79.3
119	34.0	24.8	37.2

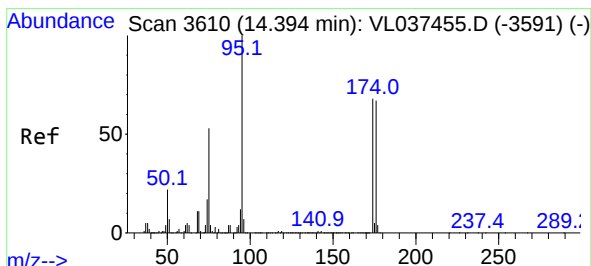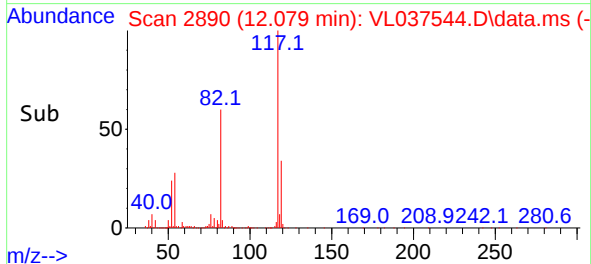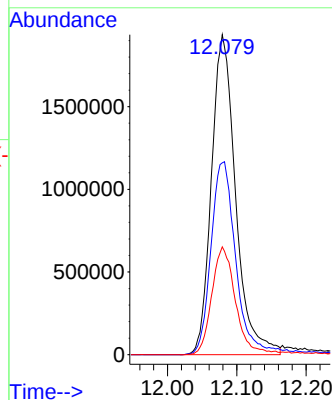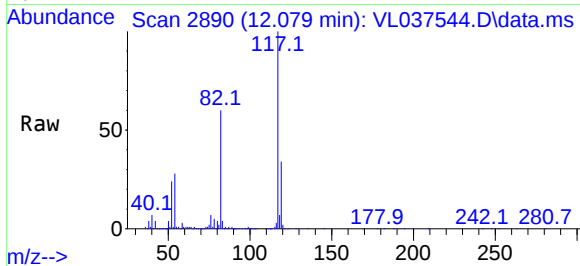

#68
1-Bromo-4-Fluorobenzene
Concen: 10.431 ppbv
RT: 14.410 min Scan# 3615
Delta R.T. 0.016 min
Lab File: VL037544.D
Acq: 7 Sep 2021 10:56

Tgt Ion: 95 Resp: 3479046

Ion	Ratio	Lower	Upper
95	100		
174	72.2	59.6	89.4
175	5.4	4.6	7.0

