

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090721\
 Data File : VL037545.D
 Acq On : 7 Sep 2021 11:33
 Operator : SY/AP
 Sample : CAN 10604
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 CAN 10604

Quant Time: Sep 08 11:10:24 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
 QLast Update : Tue Aug 17 02:13:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.664	49	1689762	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	7.172	114	5079746	10.000	ppbv	0.02
55) Chlorobenzene-d5	12.079	117	4391820	10.000	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.410	95	3307213	10.600	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	106.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090721\
Data File : VL037545.D
Acq On : 7 Sep 2021 11:33
Operator : SY/AP
Sample : CAN 10604
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10604

Quant Time: Sep 08 11:10:24 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
QLast Update : Tue Aug 17 02:13:47 2021
Response via : Initial Calibration

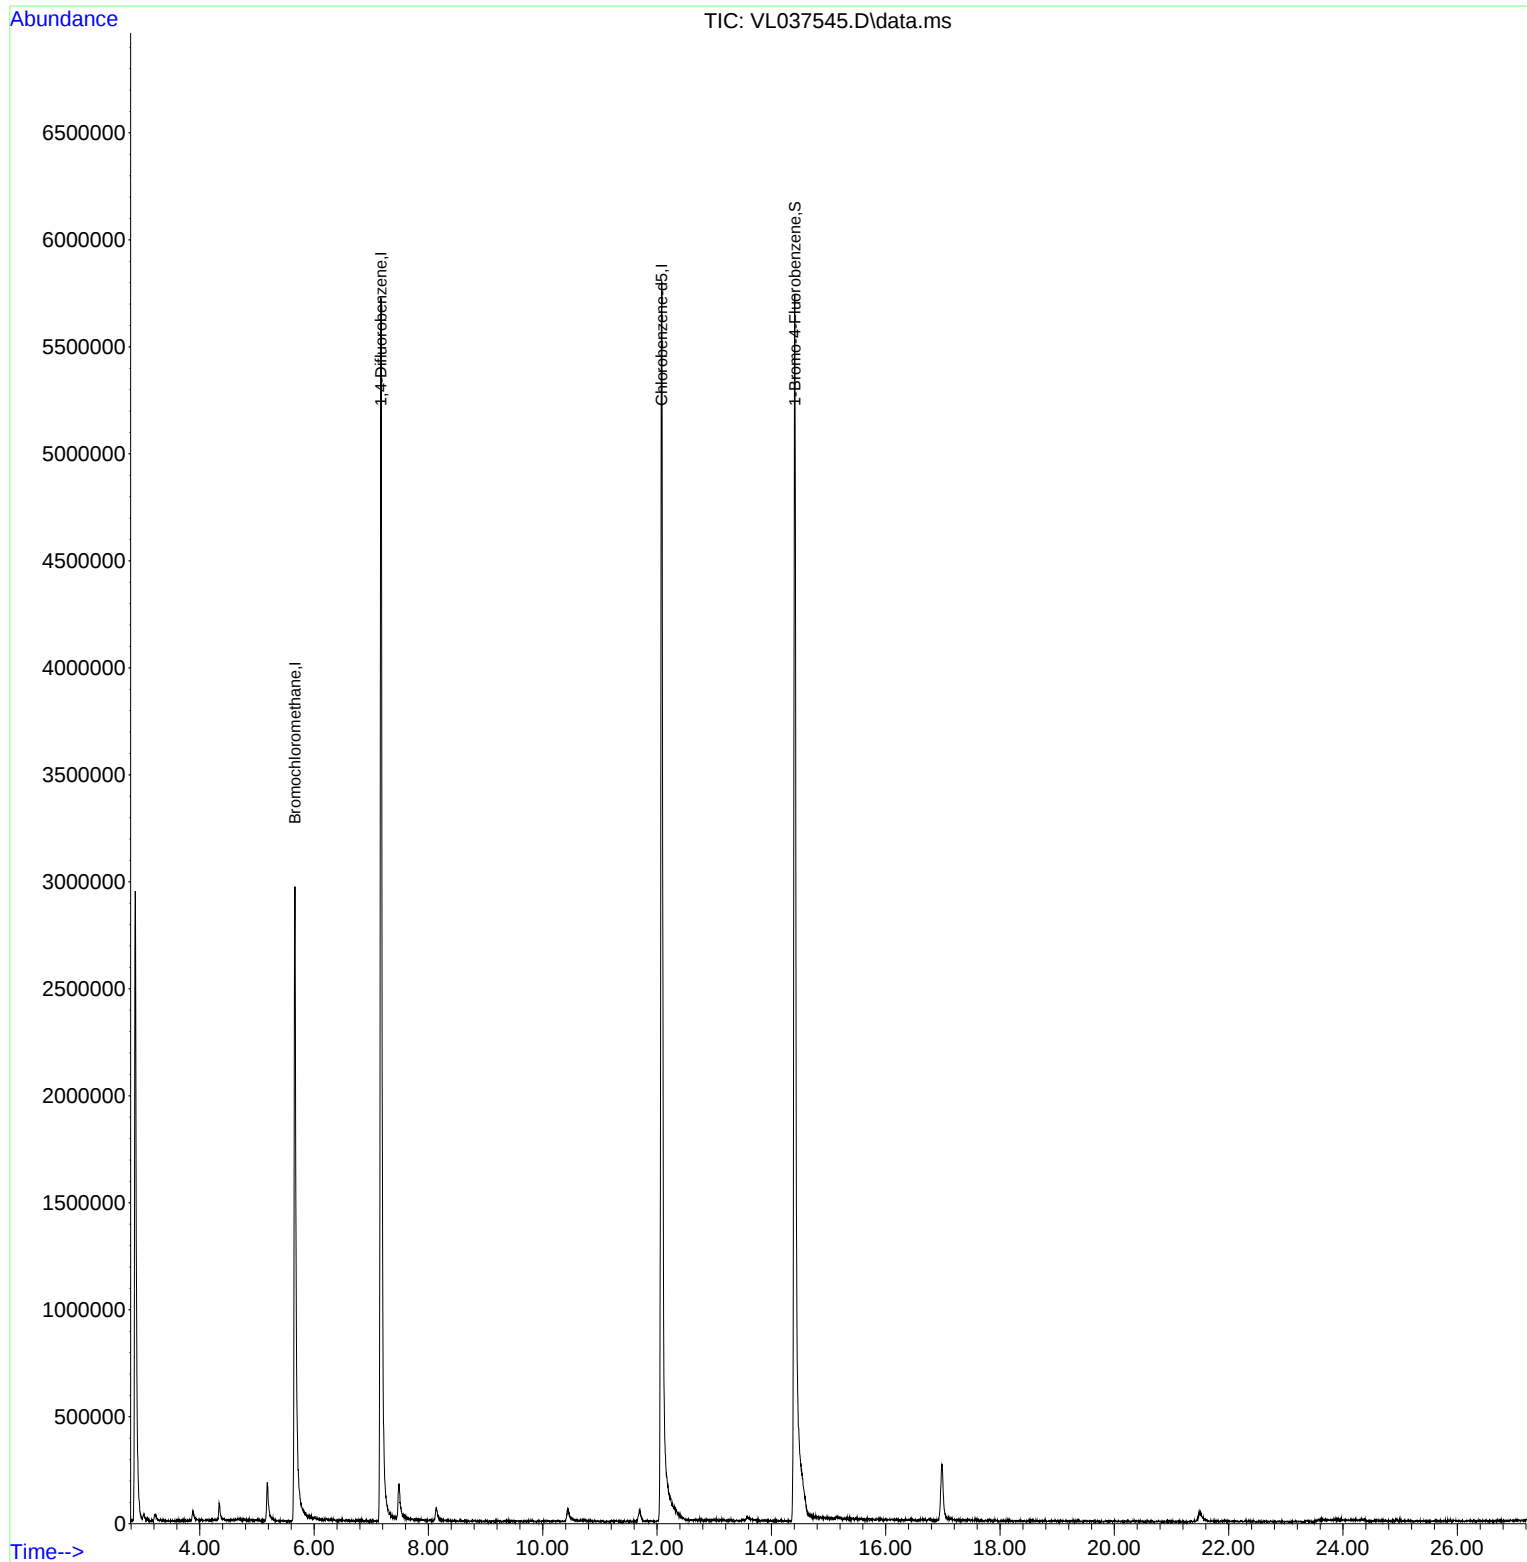




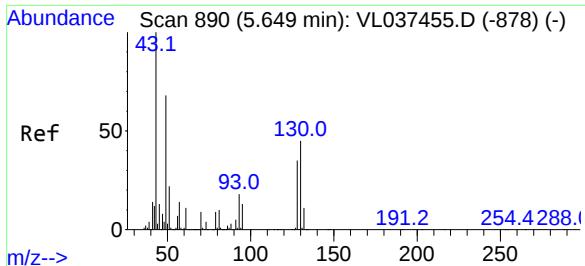


#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.664 min Scan# 895
Delta R.T. 0.016 min
Lab File: VL037545.D
Acq: 7 Sep 2021 11:33

Instrument :
MSVOA_L
ClientSampleId :
CAN 10604

Tgt Ion: 49 Resp: 1689762




Ion	Ratio	Lower	Upper
49	100		
128	54.8	27.5	82.4
130	73.1	34.0	101.8

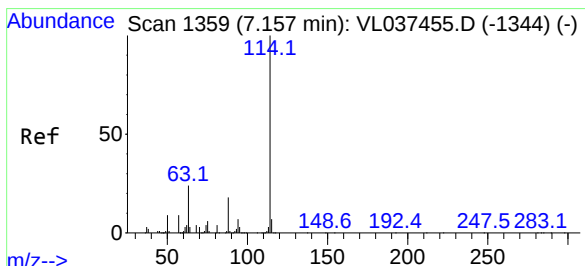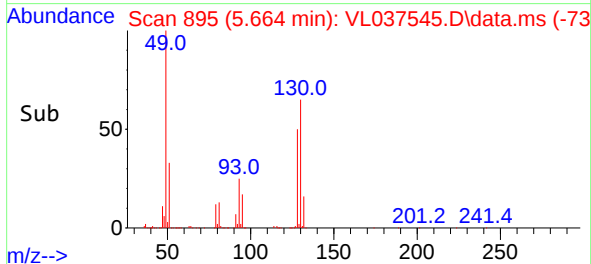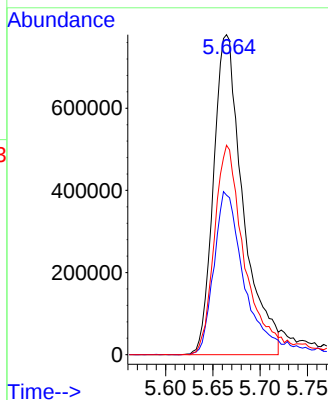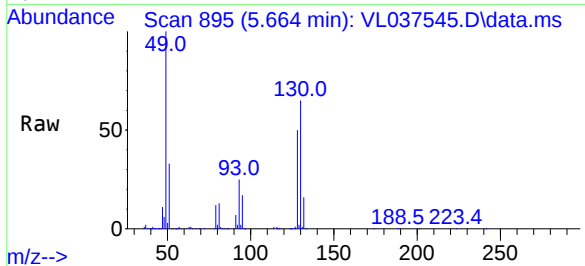


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.172 min Scan# 1364
Delta R.T. 0.016 min
Lab File: VL037545.D
Acq: 7 Sep 2021 11:33

Tgt Ion: 114 Resp: 5079746

Ion	Ratio	Lower	Upper
114	100		
63	24.4	19.3	28.9
88	18.2	14.2	21.4


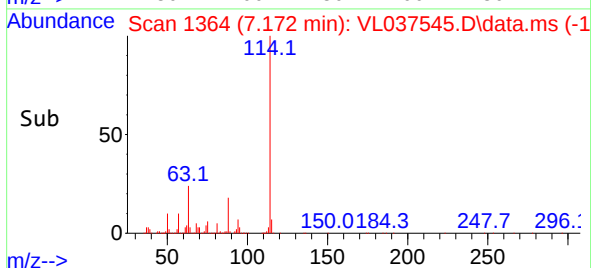
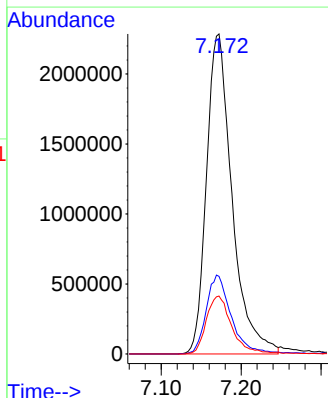
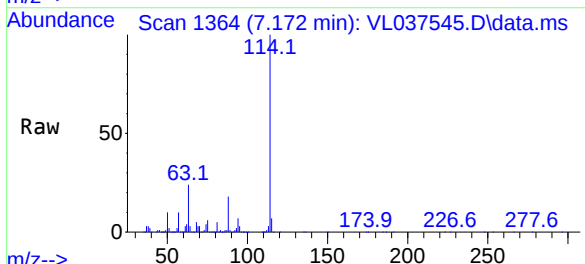


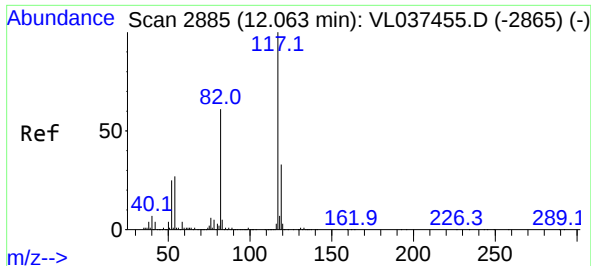

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.079 min Scan# 2890
Delta R.T. 0.016 min
Lab File: VL037545.D
Acq: 7 Sep 2021 11:33

Instrument :
MSVOA_L
ClientSampleId :
CAN 10604

Tgt Ion:117 Resp: 4391820
Ion Ratio Lower Upper
117 100
82 66.4 52.9 79.3
119 34.3 24.8 37.2

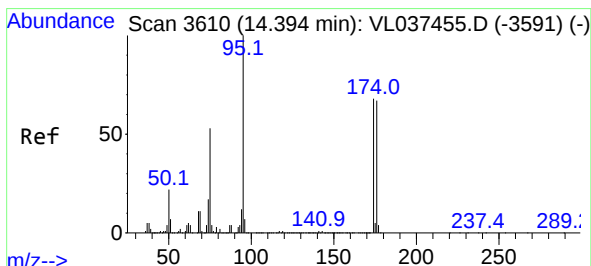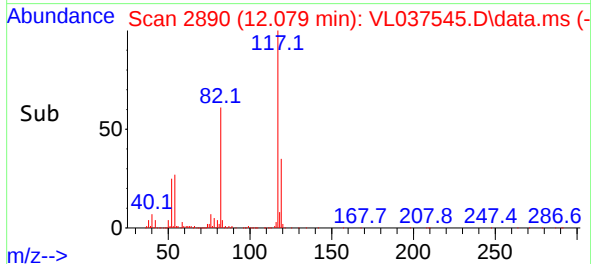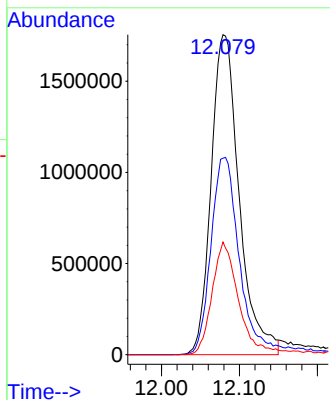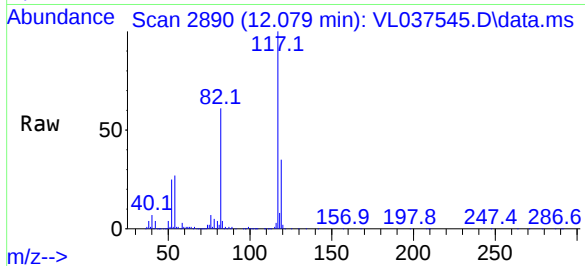

#68
1-Bromo-4-Fluorobenzene
Concen: 10.600 ppbv
RT: 14.410 min Scan# 3615
Delta R.T. 0.016 min
Lab File: VL037545.D
Acq: 7 Sep 2021 11:33

Tgt Ion: 95 Resp: 3307213
Ion Ratio Lower Upper
95 100
174 73.1 59.6 89.4
175 5.3 4.6 7.0

