


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL091018\
 Data File : VL032480.D
 Acq On : 10 Sep 2018 13:04
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL083118AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 31 21:33:46 2018
 Last Update : Fri Aug 31 21:33:46 2018

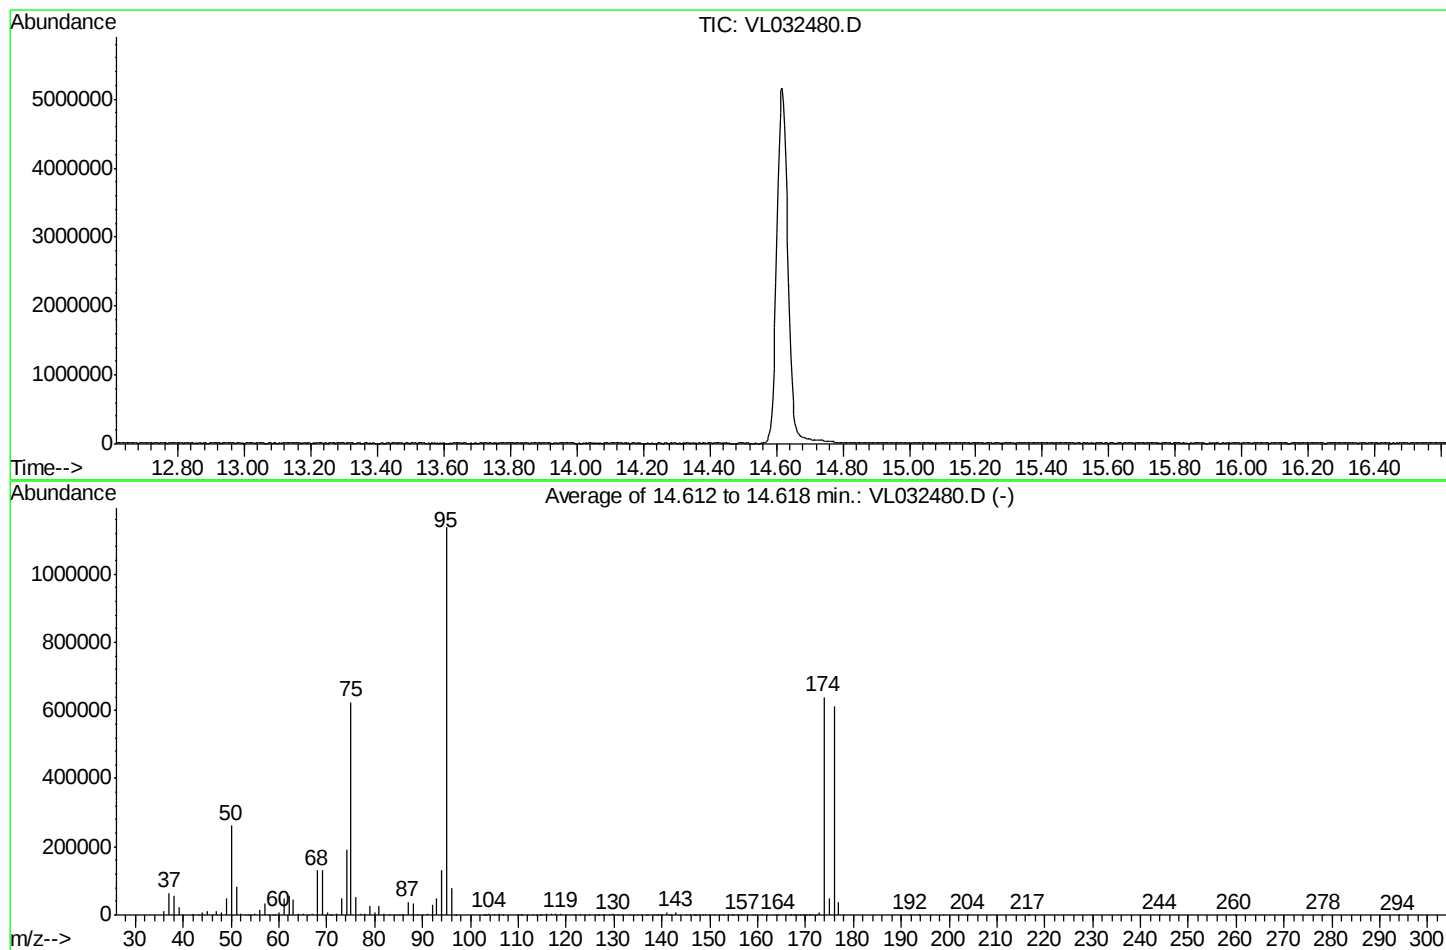

AutoFind: Scans 3631, 3632, 3633; Background Corrected with Scan 3609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.1	262549	PASS
75	95	30	66	54.9	623893	PASS
95	95	100	100	100.0	1136981	PASS
96	95	5	9	6.8	77725	PASS
173	174	0.00	2	1.1	7240	PASS
174	95	50	120	56.3	640064	PASS
175	174	4	9	7.7	49485	PASS
176	174	93	101	95.6	611690	PASS
177	176	5	9	6.4	39186	PASS