
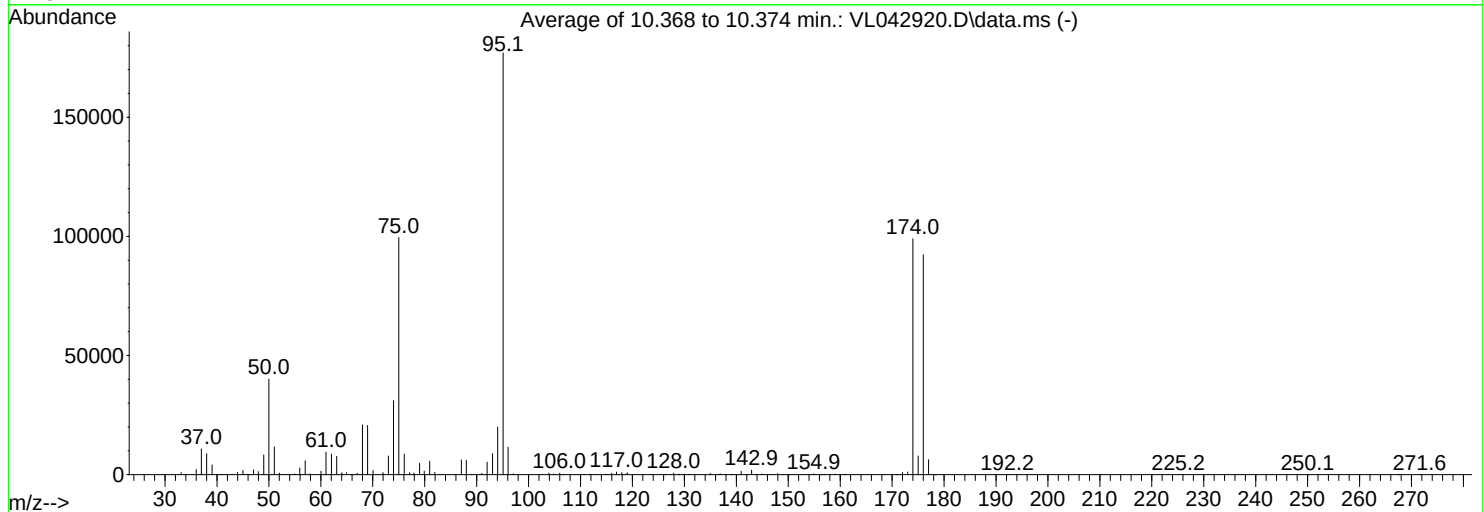


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL091025\
Data File : VL042920.D
Acq On : 10 Sep 2025 08:00
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 09 00:52:26 2025

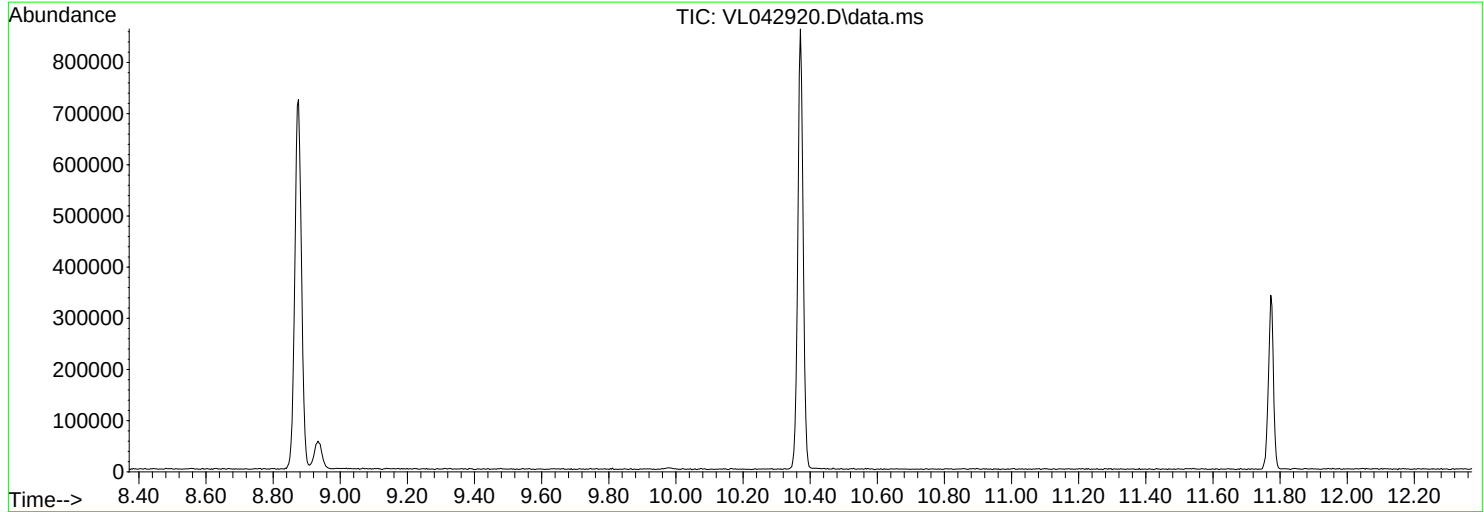

AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.6	40072	PASS
75	95	30	66	56.2	99493	PASS
95	95	100	100	100.0	177003	PASS
96	95	5	9	6.5	11579	PASS
173	174	0.00	2	1.1	1122	PASS
174	95	50	120	55.9	98960	PASS
175	174	4	9	8.0	7895	PASS
176	174	93	101	93.2	92245	PASS
177	176	5	9	6.8	6227	PASS

Average of 10.368 to 10.374 min.: VL042920.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	876	45.00	1774	53.85	119	64.95	78
33.80	16	45.90	104	54.80	163	65.80	2
34.10	149	46.20	69	55.00	306	67.00	57
36.00	2143	47.05	1988	55.95	2803	68.00	2086
37.00	10828	47.95	1311	57.00	5846	69.00	20629
38.00	8801	49.00	8294	57.95	341	70.05	1745
39.05	4125	50.00	40072	60.05	1509	71.95	902
40.80	37	51.05	11612	61.00	9493	73.00	7869
41.70	43	52.05	660	62.05	8604	74.00	31011
42.90	171	52.75	127	63.05	7688	75.00	99493
43.95	930	53.10	42	64.05	797	76.05	8630

Average of 10.368 to 10.374 min.: VL042920.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.10	850	91.00	535	109.60	51	118.80	290
77.95	675	92.00	5254	110.00	98	119.00	753
79.00	4773	93.05	8813	110.80	152	121.95	77
79.90	1505	94.05	19989	111.70	118	126.20	20
80.95	5631	95.10	177003	111.90	61	127.30	73
81.95	934	96.05	11579	112.85	172	127.95	598
82.90	103	97.05	357	114.80	54	128.90	69
85.65	136	103.90	701	115.05	124	129.05	232
87.05	6182	104.85	264	115.95	551	129.80	141
88.00	6018	106.00	622	116.95	1110	130.00	320
89.05	98	106.80	137	117.95	861	130.70	50

Average of 10.368 to 10.374 min.: VL042920.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
131.00	166	143.70	94	156.30	36	172.00	927
134.95	444	144.95	265	156.95	173	173.00	1122
135.90	39	145.95	180	159.05	183	174.00	98960
136.60	55	147.10	52	160.70	71	175.00	7895
136.90	322	147.95	404	161.05	168	176.00	92245
139.00	29	149.10	110	165.05	66	177.00	6227
140.00	103	149.80	31	168.45	142	177.90	133
140.95	1394	150.10	37	170.05	82	178.30	33
141.70	53	151.95	56	170.80	28	192.20	18
142.00	102	152.90	97	171.00	66	225.15	65
142.95	1868	154.95	336	171.60	97	250.05	38

Average of 10.368 to 10.374 min.: VL042920.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
267.50	25						
271.60	32						