


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL091620\
 Data File : VL035626.D
 Acq On : 16 Sep 2020 11:39
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL082720AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Sep 14 15:19:50 2020
 Last Update : Mon Sep 14 15:19:50 2020

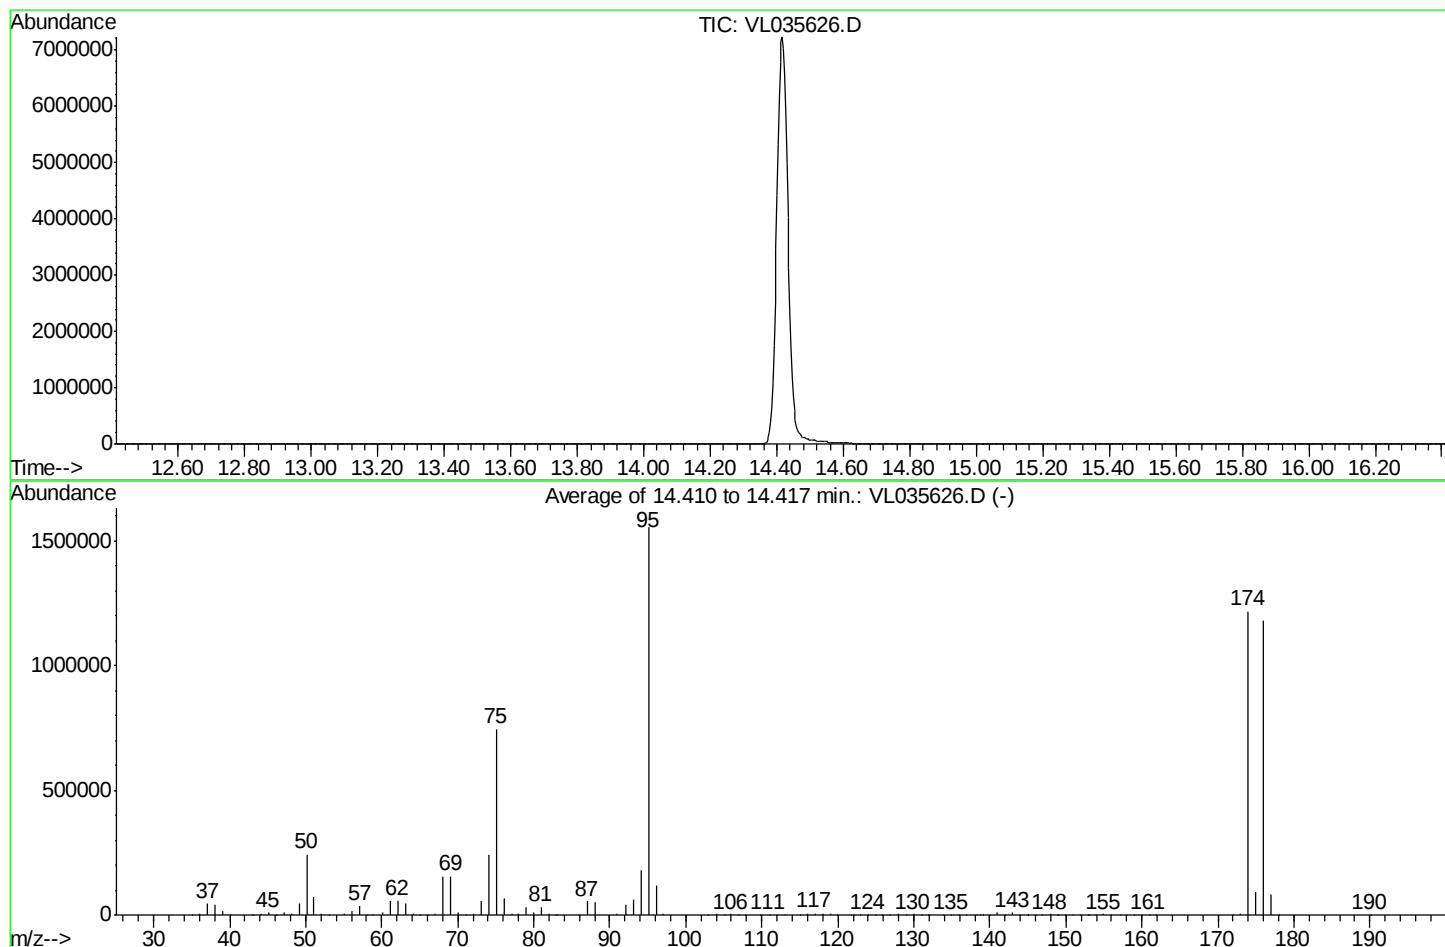

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	15.6	242304	PASS
75	95	30	66	47.9	744938	PASS
95	95	100	100	100.0	1555285	PASS
96	95	5	9	7.5	116762	PASS
173	174	0.00	2	0.5	5941	PASS
174	95	50	120	78.4	1219072	PASS
175	174	4	9	7.6	92946	PASS
176	174	93	101	97.0	1182549	PASS
177	176	5	9	6.9	82058	PASS