
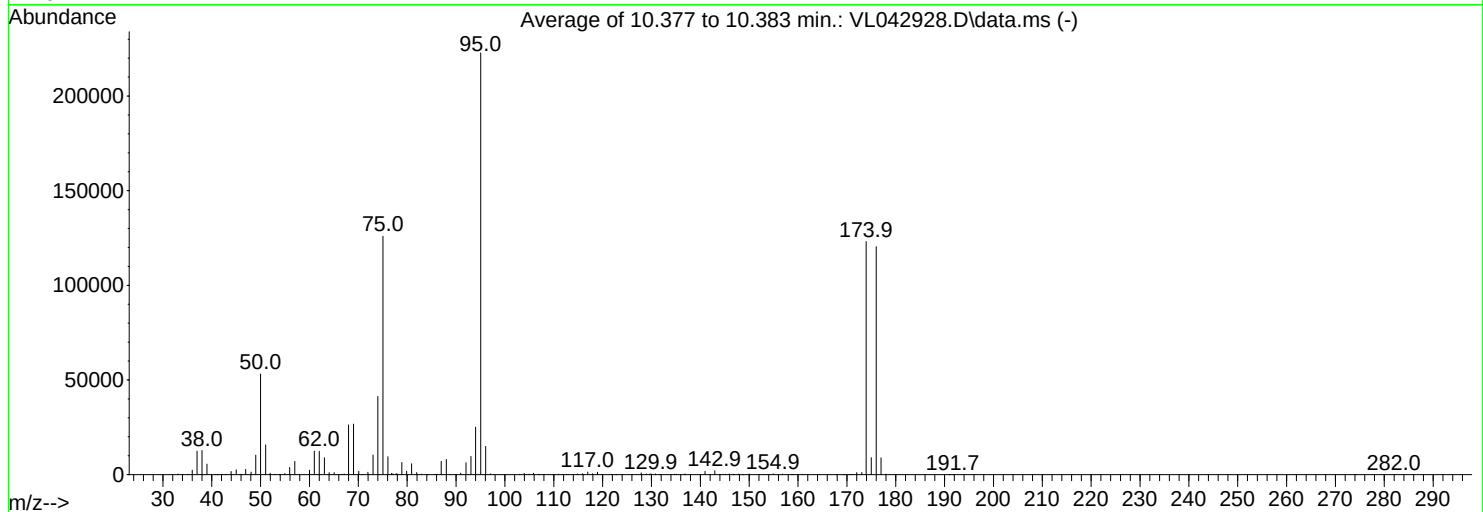


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL091725\
Data File : VL042928.D
Acq On : 17 Sep 2025 07:51
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Sep 18 02:57:46 2025

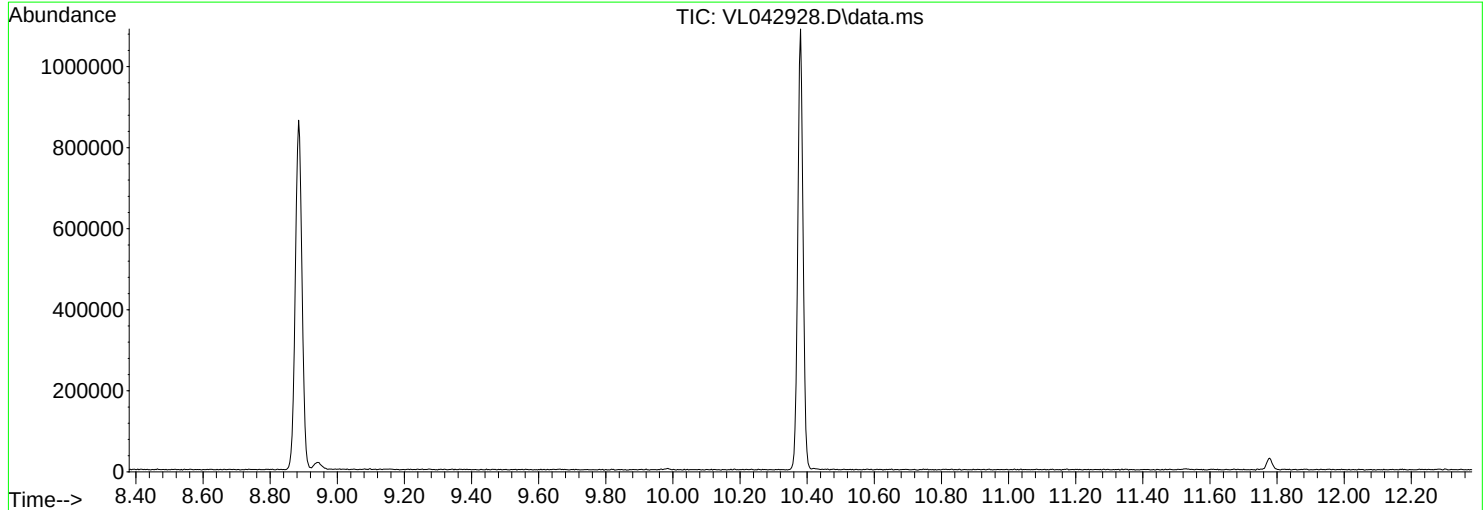

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	53203	PASS
75	95	30	66	56.5	125915	PASS
95	95	100	100	100.0	222805	PASS
96	95	5	9	6.7	14943	PASS
173	174	0.00	2	1.0	1195	PASS
174	95	50	120	55.3	123173	PASS
175	174	4	9	7.3	8935	PASS
176	174	93	101	97.8	120472	PASS
177	176	5	9	7.4	8875	PASS

Average of 10.377 to 10.383 min.: VL042928.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	326	42.90	188	52.95	173	65.05	1064
33.95	137	43.95	1727	53.80	31	65.80	21
34.15	88	45.00	2549	54.95	589	66.80	12
35.10	59	45.80	90	55.95	3828	67.10	37
36.00	2346	46.10	168	57.00	7043	68.00	26323
37.00	12410	46.95	2763	57.95	238	69.00	26749
38.00	12760	48.05	1394	60.00	2402	70.10	1737
39.00	5584	49.00	10330	61.00	12431	70.85	123
39.90	165	50.00	53203	62.00	12338	71.95	1266
40.80	98	51.05	15701	63.05	8980	73.00	10431
41.10	20	51.95	762	64.05	1139	74.00	41301

Average of 10.377 to 10.383 min.: VL042928.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.05	125915	84.10	22	95.05	222805	111.00	217
76.05	9509	85.65	99	96.05	14943	111.75	132
76.80	719	85.90	73	97.05	389	112.00	71
77.10	426	86.10	164	102.95	155	112.70	78
77.75	572	86.95	7006	103.95	649	113.00	78
78.00	236	88.00	8035	104.95	237	114.90	346
78.90	6414	88.80	51	105.85	789	115.85	555
79.90	1780	90.95	755	106.85	143	116.10	202
80.90	5789	92.05	6365	107.05	106	116.95	1338
81.95	1141	93.05	9636	107.80	98	117.90	540
82.95	222	94.00	25107	109.90	186	118.95	1268

Average of 10.377 to 10.383 min.: VL042928.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.70	61	135.10	136	145.15	167	153.75	130
121.85	152	136.80	239	145.70	106	154.90	447
122.70	20	136.95	255	145.95	347	156.80	341
124.00	44	139.90	52	146.70	25	158.05	49
127.90	905	140.95	1812	147.00	118	158.75	193
128.95	381	141.80	48	147.70	75	159.05	84
129.60	137	142.10	188	147.90	344	160.85	194
129.90	558	142.95	2132	148.70	41	161.10	94
130.85	387	143.90	68	150.00	317	167.80	27
131.70	23	144.10	58	152.15	186	169.30	22
134.70	233	144.60	85	153.00	76	169.95	102

Average of 10.377 to 10.383 min.: VL042928.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.45	87	191.70	42				
170.85	125	274.10	31				
171.20	56	282.00	46				
172.00	1099	287.90	20				
173.05	1195						
173.95	123173						
175.00	8935						
176.00	120472						
177.00	8875						
178.00	218						
190.90	17						