

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092225\
 Data File : VL042970.D
 Acq On : 22 Sep 2025 22:48
 Operator : SY/MD
 Sample : Q3130-02DUP
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 131-1A-2DUP


Quant Time: Sep 23 02:57:33 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL092225AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Sep 23 02:39:16 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	146991	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.959	114	437140	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.882	117	389571	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.377	95	296189	10.185	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.900%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.499	85	8516	0.431	ppbv	92
3) Chlorodifluoromethane	1.467	51	561845	22.801	ppbv #	61
4) Chloromethane	1.535	50	3652	0.408	ppbv	97
6) Bromomethane	1.671	94	148	0.052	ppbv #	73
7) Chloroethane	1.467	64	27415	8.727	ppbv	96
9) Propene	1.561	41	25773	2.404	ppbv	91
11) Trichlorofluoromethane	1.881	101	4422	0.232	ppbv	98
12) 1,1,2-Trichlorotrifluo...	2.140	101	952	0.062	ppbv	96
13) Ethanol	1.722	45	384814	370.048	ppbv	95
15) Acetone	1.836	43	118525	6.191	ppbv	96
16) 1,3-Butadiene	1.599	39	1408	0.156	ppbv #	61
17) tert-Butyl alcohol	2.043	59	4197	0.200	ppbv #	82
19) Isopropyl Alcohol	1.887	45	9512	0.826	ppbv #	1
20) Methylene Chloride	2.062	84	14366	1.980	ppbv	97
23) Vinyl Acetate	2.454	43	9099	0.333	ppbv #	91
25) Ethyl Acetate	2.829	43	65319	1.350	ppbv #	92
26) Hexane	2.829	57	53388	2.421	ppbv #	61
30) Cyclohexane	3.852	84	763	0.041	ppbv #	1
31) cis-1,2-Dichloroethene	2.839	61	3462	0.168	ppbv #	24
34) 2-Butanone	2.561	43	11487	0.375	ppbv #	86
35) Carbon Tetrachloride	3.758	117	1168	0.041	ppbv	84
36) Benzene	3.661	78	7565	0.184	ppbv #	90
37) 1,2-Dichloroethane	3.218	62	3337	0.155	ppbv #	93
39) 1,2-Dichloropropane	3.959	63	108795	7.260	ppbv #	23
44) 2,2,4-Trimethylpentane	4.645	57	6315	0.089	ppbv #	44
53) Toluene	6.937	91	18244	0.375	ppbv	100
58) Ethyl Benzene	9.358	91	3940	0.062	ppbv	89
59) m/p-Xylene	9.532	91	6145	0.122	ppbv #	100
60) o-Xylene	9.963	91	3183	0.063	ppbv	95
61) Styrene	9.879	104	1637	0.069	ppbv	90
73) 1,3,5-Trimethylbenzene	11.202	105	1741	0.034	ppbv #	81
74) 1,2,4-Trimethylbenzene	11.536	105	5151	0.091	ppbv #	68
79) Naphthalene	13.513	128	7088	0.142	ppbv	97
80) Naphthalene,2-methyl-	14.459	142	3693	0.239	ppbv	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 23 02:57:33 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL092225AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022
QLast Update : Tue Sep 23 02:39:16 2025
Response via : Initial Calibration









#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.787 min Scan# 81
Delta R.T. 0.003 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion: 49 Resp: 146991
Ion Ratio Lower Upper
49 100
128 46.9 22.9 68.8
130 59.9 29.1 87.3

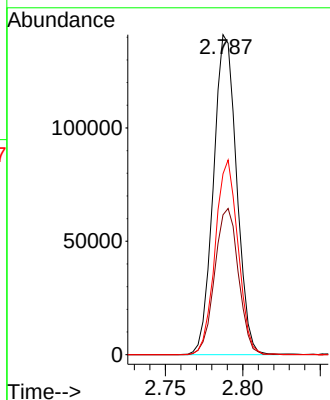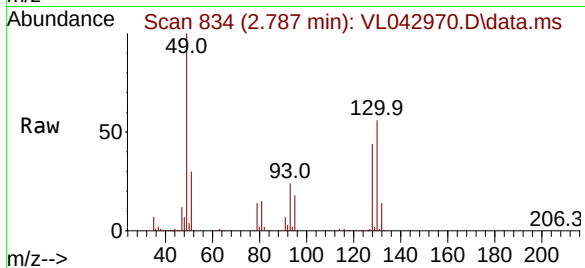

#2
Dichlorodifluoromethane
Concen: 0.431 ppbv
RT: 1.499 min Scan# 436
Delta R.T. 0.003 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 85 Resp: 8516
Ion Ratio Lower Upper
85 100
87 34.7 24.3 36.5


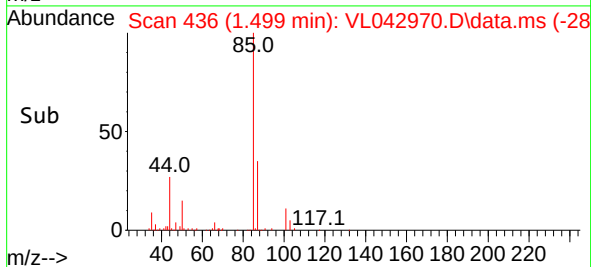
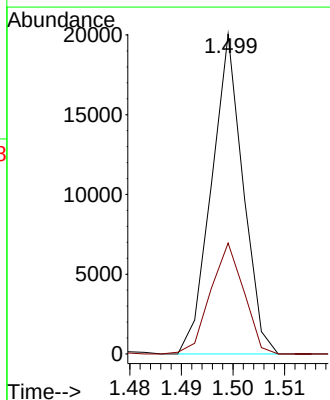
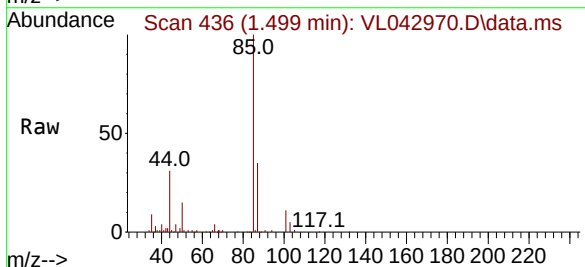




#3
Chlorodifluoromethane
Concen: 22.801 ppbv
RT: 1.467 min Scan# 41
Delta R.T. -0.006 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion: 51 Resp: 561845
Ion Ratio Lower Upper
51 100
67 0.2 13.8 20.8#



#4
Chloromethane
Concen: 0.408 ppbv
RT: 1.535 min Scan# 447
Delta R.T. 0.003 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 50 Resp: 3652
Ion Ratio Lower Upper
50 100
52 34.3 25.9 38.9


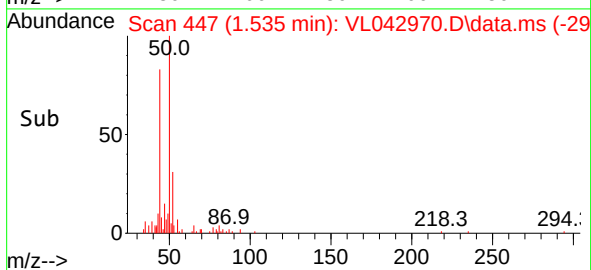






#6
Bromomethane
Concen: 0.052 ppbv
RT: 1.671 min Scan# 41
Delta R.T. 0.003 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion: 94 Resp: 148
Ion Ratio Lower Upper
94 100
96 116.0 72.6 108.8#

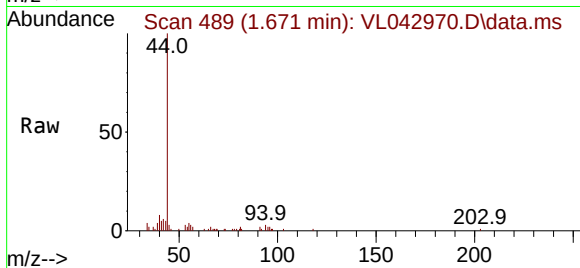

#7
Chloroethane
Concen: 8.727 ppbv
RT: 1.467 min Scan# 426
Delta R.T. -0.236 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 64 Resp: 27415
Ion Ratio Lower Upper
64 100
66 28.5 24.6 36.8

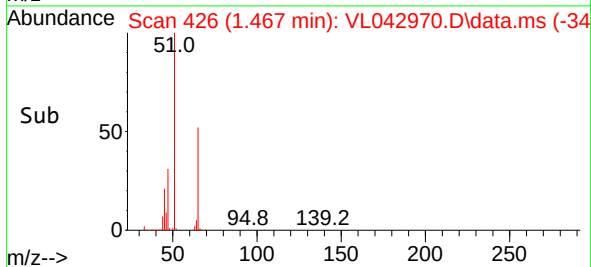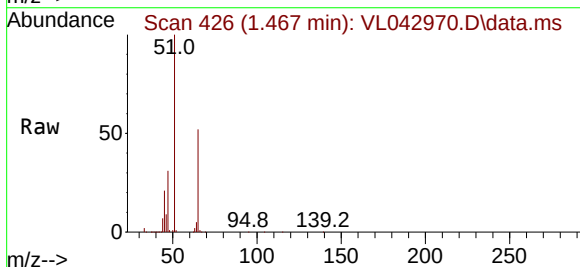



#9

Propene

Concen: 2.404 ppbv

RT: 1.561 min Scan# 41

Delta R.T. 0.078 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Instrument :

MSVOA_L

ClientSampleId :





131-1A-2DUP

Tgt Ion: 41 Resp: 25773

Ion Ratio Lower Upper

41 100

42 79.2 57.4 86.2

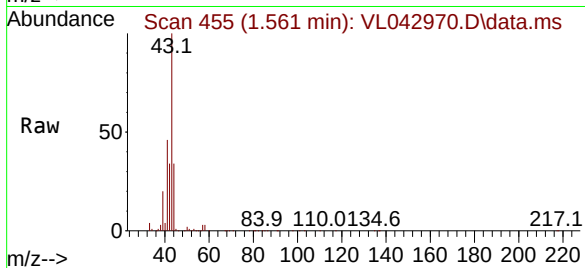

#11

Trichlorofluoromethane

Concen: 0.232 ppbv

RT: 1.881 min Scan# 554

Delta R.T. 0.007 min

Lab File: VL042970.D




Acq: 22 Sep 2025 22:48


Tgt Ion: 101 Resp: 4422

Ion Ratio Lower Upper

101 100

103 64.5 50.1 75.1

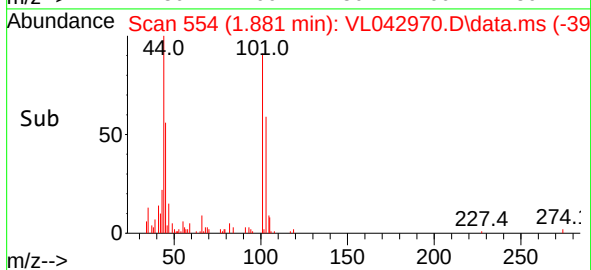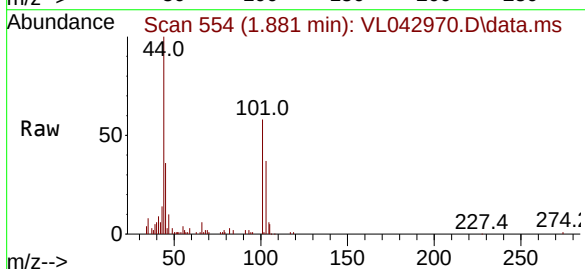



#12

1,1,2-Trichlorotrifluoroethane

Concen: 0.062 ppbv

RT: 2.140 min Scan# 61

Delta R.T. 0.003 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Instrument :

MSVOA_L

ClientSampleId :





131-1A-2DUP

Tgt Ion:101 Resp: 952

Ion Ratio Lower Upper

101 100

151 72.8 55.7 83.5

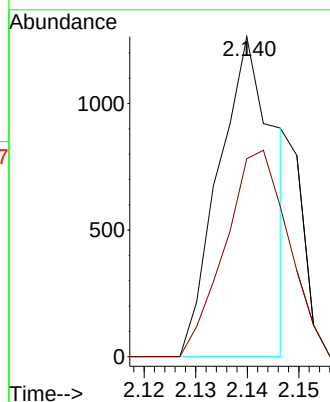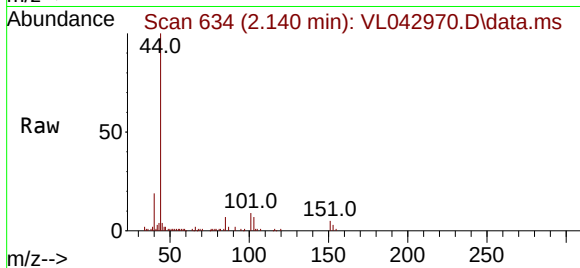

#13

Ethanol

Concen: 370.048 ppbv

RT: 1.722 min Scan# 505

Delta R.T. 0.003 min

Lab File: VL042970.D




Acq: 22 Sep 2025 22:48


Tgt Ion: 45 Resp: 384814

Ion Ratio Lower Upper

45 100

46 37.3 16.2 64.6


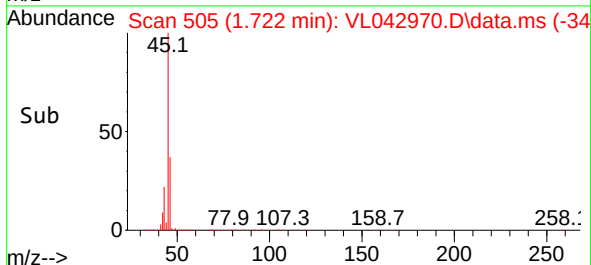
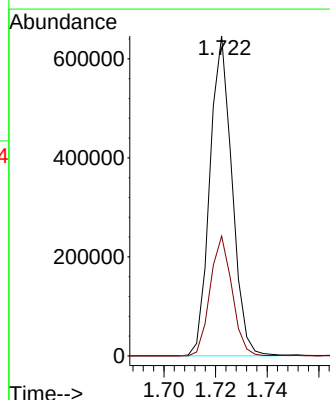
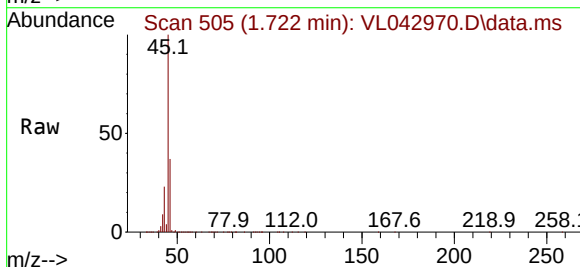




#15
Acetone
Concen: 6.191 ppbv
RT: 1.836 min Scan# 541
Delta R.T. 0.003 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion: 43 Resp: 118525
Ion Ratio Lower Upper
43 100
58 25.8 22.3 33.5

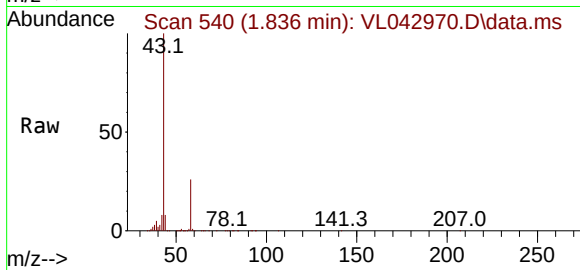

#16
1,3-Butadiene
Concen: 0.156 ppbv
RT: 1.599 min Scan# 467
Delta R.T. -0.006 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 39 Resp: 1408
Ion Ratio Lower Upper
39 100
54 42.8 60.8 91.2#

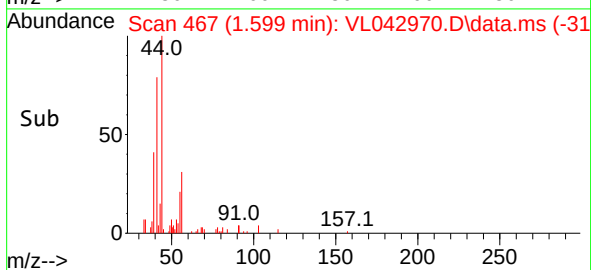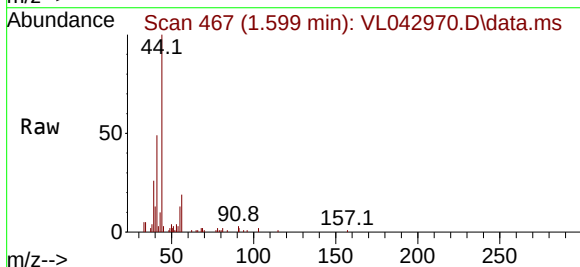



#17

tert-Butyl alcohol

Concen: 0.200 ppbv

RT: 2.043 min Scan# 602

Delta R.T. 0.007 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Instrument :

MSVOA_L

ClientSampleId :





131-1A-2DUP

Tgt Ion: 59 Resp: 4197

Ion Ratio Lower Upper

59 100

57 17.4 8.6 12.8#

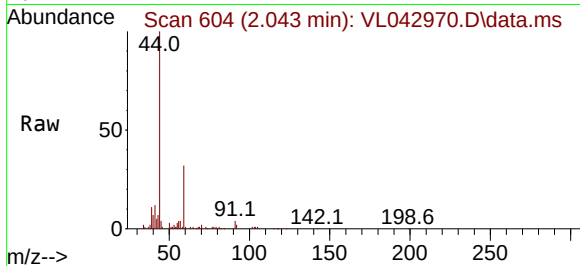

#19

Isopropyl Alcohol

Concen: 0.826 ppbv

RT: 1.887 min Scan# 556

Delta R.T. 0.003 min

Lab File: VL042970.D




Acq: 22 Sep 2025 22:48


Tgt Ion: 45 Resp: 9512

Ion Ratio Lower Upper

45 100

58 326.6 31.0 46.6#

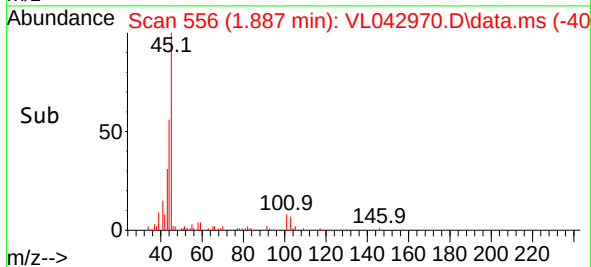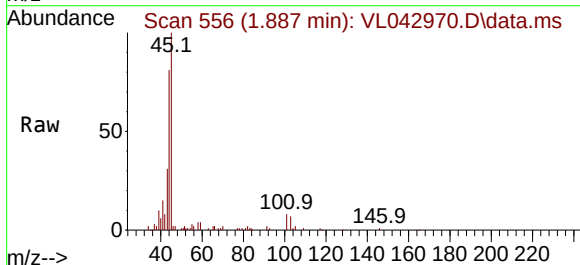







#20
Methylene Chloride
Concen: 1.980 ppbv
RT: 2.062 min Scan# 610
Delta R.T. 0.003 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP

Tgt Ion: 84 Resp: 14366




Ion	Ratio	Lower	Upper
84	100		
49	160.1	124.1	186.1
51	50.7	39.8	59.8
86	61.3	50.9	76.3

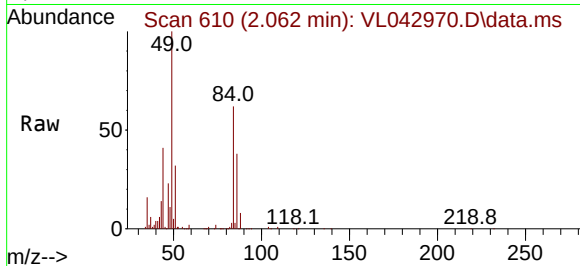


#23
Vinyl Acetate
Concen: 0.333 ppbv
RT: 2.454 min Scan# 731
Delta R.T. -0.006 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 43 Resp: 9099

Ion	Ratio	Lower	Upper
43	100		
86	9.4	6.2	9.2#
42	5.6	7.4	11.0#
44	9.4	4.2	6.2#


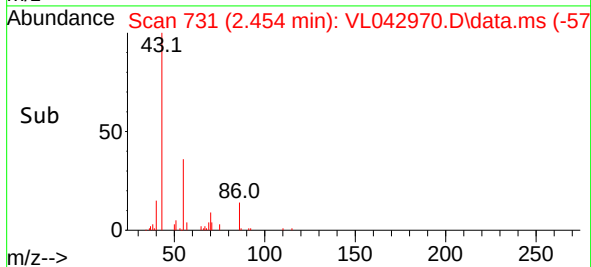

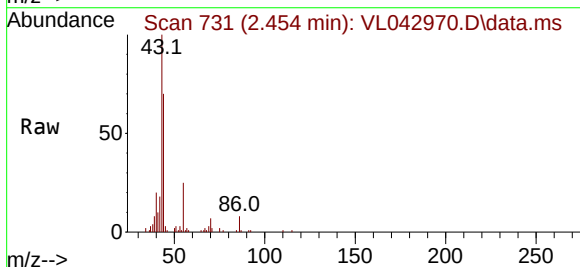




#25
Ethyl Acetate
Concen: 1.350 ppbv
RT: 2.829 min Scan# 847
Delta R.T. 0.000 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion:	43	Resp:	65319
Ion	Ratio	Lower	Upper
43	100		
45	7.1	7.7	11.5#
61	5.4	7.1	10.7#
70	5.8	6.7	10.1#

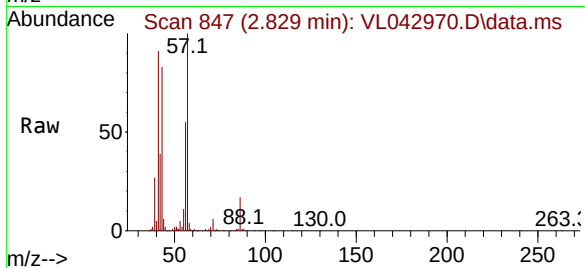

#26
Hexane
Concen: 2.421 ppbv
RT: 2.829 min Scan# 847
Delta R.T. 0.007 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion:	57	Resp:	53388
Ion	Ratio	Lower	Upper
57	100		
41	89.4	71.7	107.5
43	124.3	180.8	271.2#
56	56.3	41.4	62.0

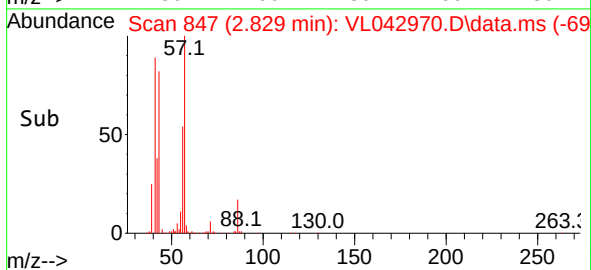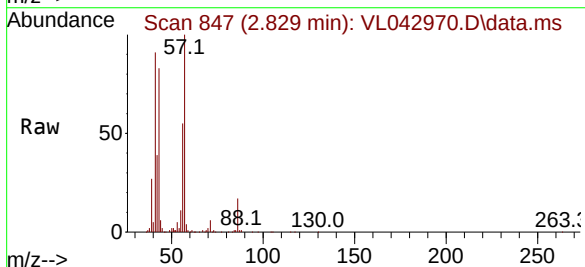



#30

Cyclohexane

Concen: 0.041 ppbv

RT: 3.852 min Scan# 1163

Delta R.T. 0.000 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Instrument :

MSVOA_L

ClientSampleId :

131-1A-2DUP





Tgt Ion: 84 Resp: 763

Ion Ratio Lower Upper

84 100

56 0.0 102.2 153.4#

41 0.0 65.6 98.4#

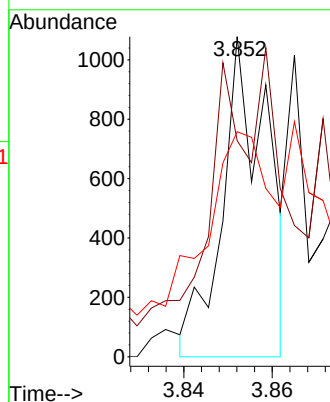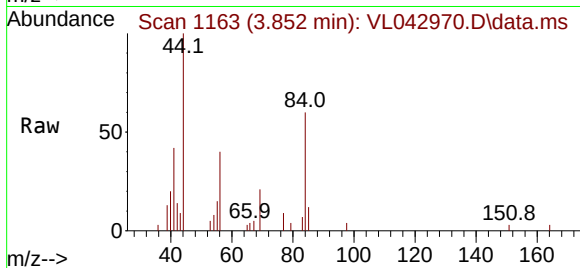

#31

cis-1,2-Dichloroethene

Concen: 0.168 ppbv

RT: 2.839 min Scan# 850

Delta R.T. 0.123 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48




Tgt Ion: 61 Resp: 3462


Ion Ratio Lower Upper

61 100

96 0.0 53.0 79.6#

98 0.0 32.9 49.3#

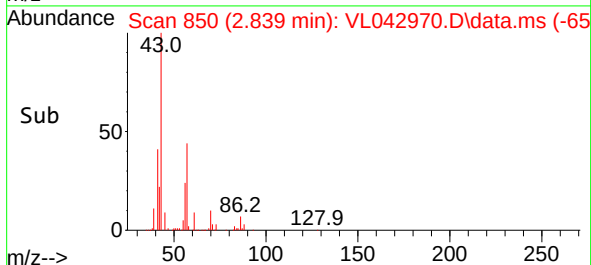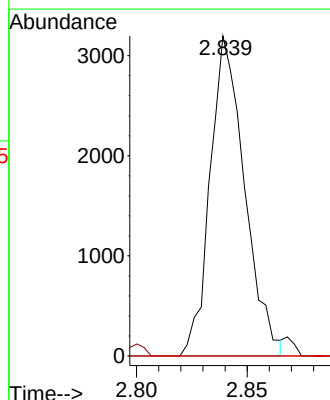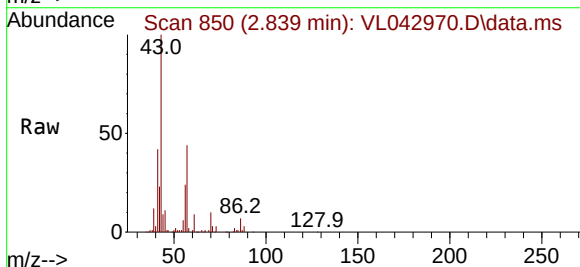



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 3.959 min Scan# 1196

Delta R.T. 0.007 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Instrument :

MSVOA_L

ClientSampleId :

131-1A-2DUP





Tgt Ion:114 Resp: 437140

Ion Ratio Lower Upper

114 100

63 24.9 19.4 29.2

88 17.7 14.2 21.2



#34

2-Butanone

Concen: 0.375 ppbv

RT: 2.561 min Scan# 764

Delta R.T. 0.010 min

Lab File: VL042970.D




Acq: 22 Sep 2025 22:48


Tgt Ion: 43 Resp: 11487

Ion Ratio Lower Upper

43 100

72 28.9 17.7 26.5#


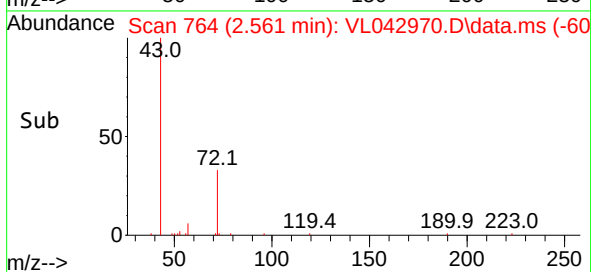




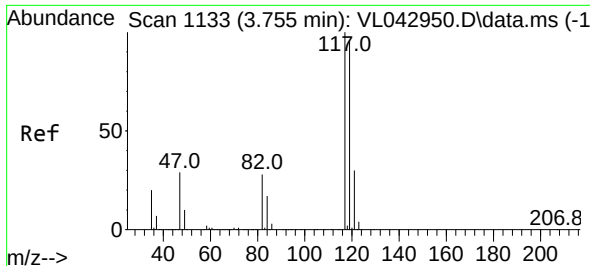

#35
Carbon Tetrachloride
Concen: 0.041 ppbv
RT: 3.758 min Scan# 1133
Delta R.T. 0.003 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion:117 Resp: 1168
Ion Ratio Lower Upper
117 100
119 76.9 76.9 115.3
121 31.5 23.7 35.5

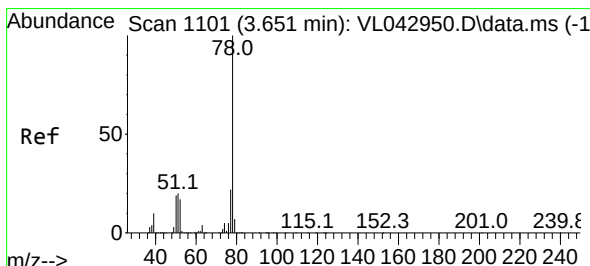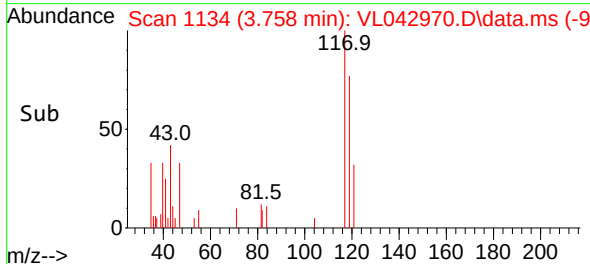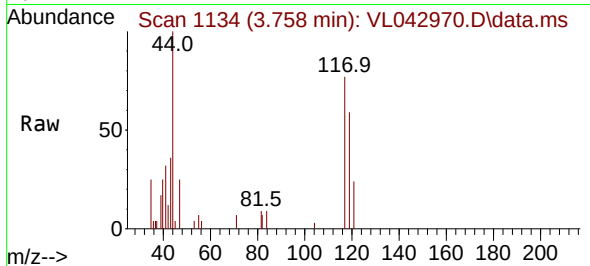

#36
Benzene
Concen: 0.184 ppbv
RT: 3.661 min Scan# 1104
Delta R.T. 0.010 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 78 Resp: 7565
Ion Ratio Lower Upper
78 100
77 14.2 17.8 26.6#
50 17.8 15.0 22.4

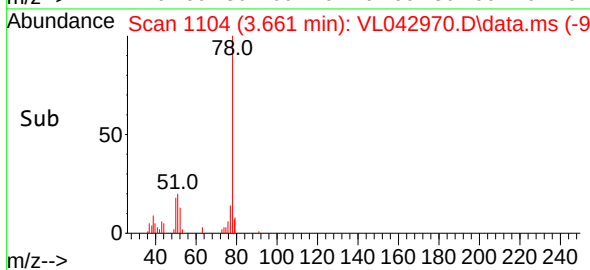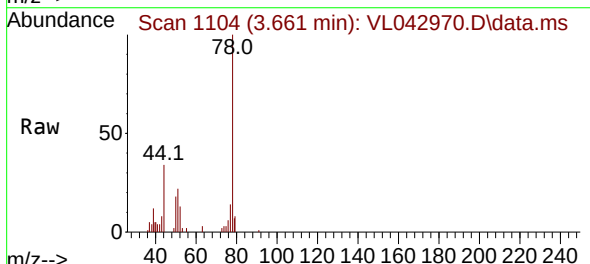



#37

1,2-Dichloroethane

Concen: 0.155 ppbv

RT: 3.218 min Scan# 9

Delta R.T. 0.003 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Instrument :

MSVOA_L

ClientSampleId :





131-1A-2DUP

Tgt Ion: 62 Resp: 3337

Ion Ratio Lower Upper

62 100

98 5.0 5.9 8.9#

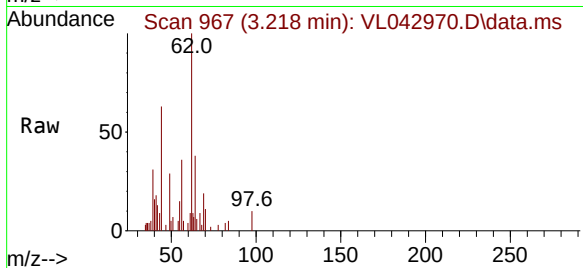

#39

1,2-Dichloropropane

Concen: 7.260 ppbv

RT: 3.959 min Scan# 1196

Delta R.T. -0.346 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48




Tgt Ion: 63 Resp: 108795


Ion Ratio Lower Upper

63 100

41 0.0 57.5 86.3#

62 16.6 58.5 87.7#


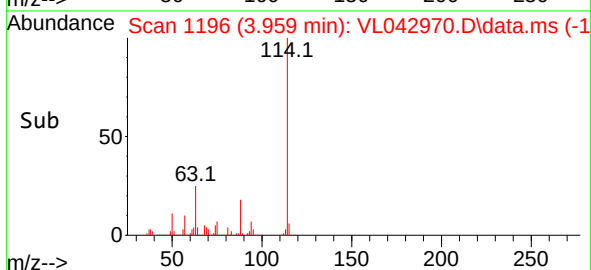

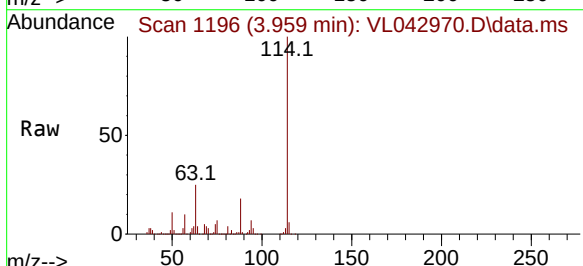




#44
2,2,4-Trimethylpentane
Concen: 0.089 ppbv
RT: 4.645 min Scan# 1408
Delta R.T. 0.013 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion: 57 Resp: 6315
Ion Ratio Lower Upper
57 100
41 68.4 25.5 38.3#
56 58.5 25.8 38.8#

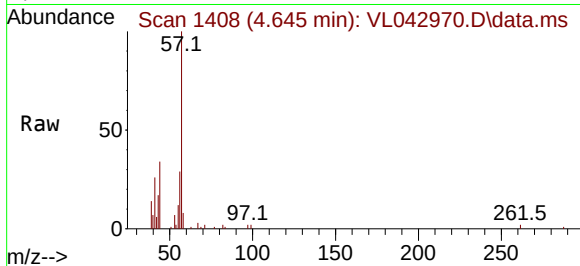

#53
Toluene
Concen: 0.375 ppbv
RT: 6.937 min Scan# 2116
Delta R.T. 0.013 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 91 Resp: 18244
Ion Ratio Lower Upper
91 100
92 60.2 48.2 72.2


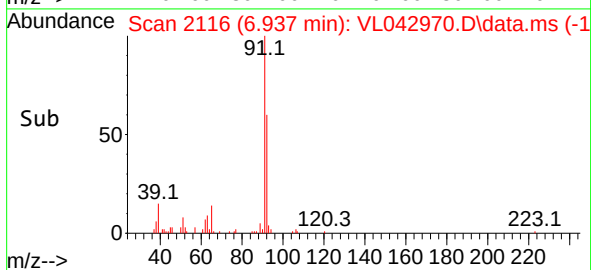

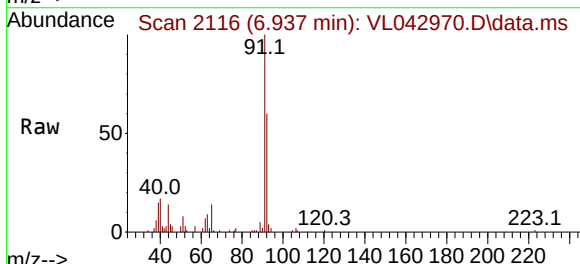




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.882 min Scan# 211
Delta R.T. 0.007 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion:117 Resp: 389571
Ion Ratio Lower Upper
117 100
82 63.8 52.8 79.2
119 32.1 26.5 39.7

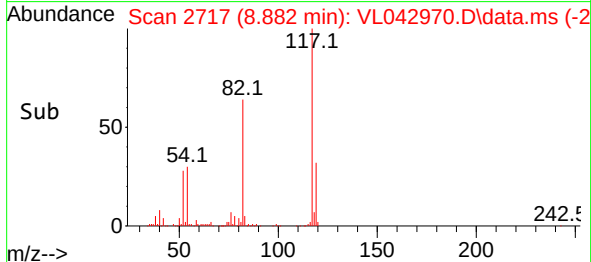

#58
Ethyl Benzene
Concen: 0.062 ppbv
RT: 9.358 min Scan# 2864
Delta R.T. 0.010 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 91 Resp: 3940
Ion Ratio Lower Upper
91 100
106 25.0 24.6 37.0

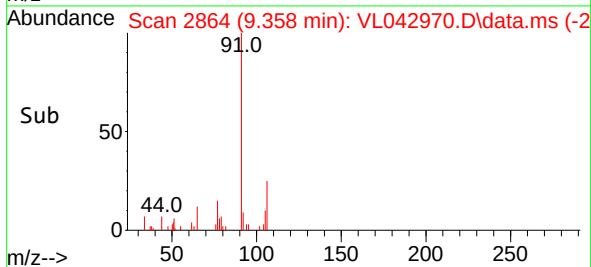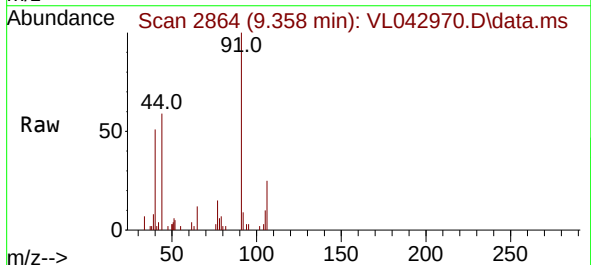



#59

m/p-Xylene

Concen: 0.122 ppbv

RT: 9.532 min Scan# 2916

Delta R.T. 0.007 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Instrument :

MSVOA_L

ClientSampleId :





131-1A-2DUP

Tgt Ion: 91 Resp: 6145

Ion Ratio Lower Upper

91 100

106 63.8 0.0 0.0#

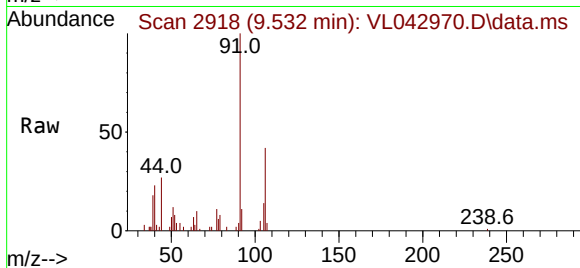

#60

o-Xylene

Concen: 0.063 ppbv

RT: 9.963 min Scan# 3051

Delta R.T. 0.003 min

Lab File: VL042970.D




Acq: 22 Sep 2025 22:48


Tgt Ion: 91 Resp: 3183

Ion Ratio Lower Upper

91 100

106 48.2 22.4 67.0




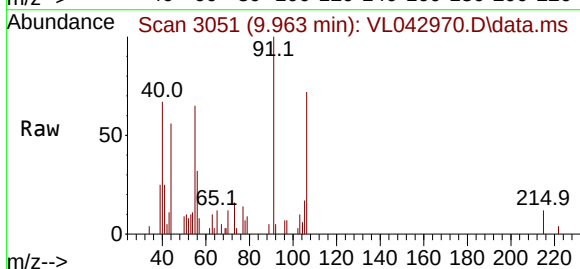




#61
Styrene
Concen: 0.069 ppbv
RT: 9.879 min Scan# 3021
Delta R.T. 0.013 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48




Instrument :
MSVOA_L
ClientSampleId :
131-1A-2DUP


Tgt Ion:104 Resp: 1637
Ion Ratio Lower Upper
104 100
78 45.4 39.9 59.9
103 37.3 36.9 55.3

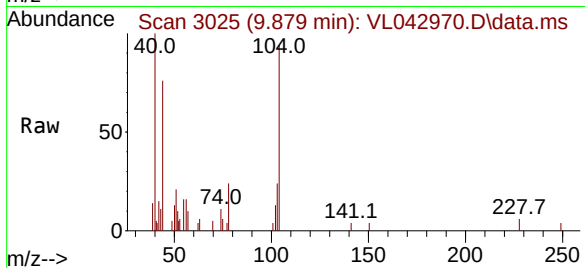

#68
1-Bromo-4-Fluorobenzene
Concen: 10.185 ppbv
RT: 10.377 min Scan# 3179
Delta R.T. 0.007 min
Lab File: VL042970.D
Acq: 22 Sep 2025 22:48

Tgt Ion: 95 Resp: 296189
Ion Ratio Lower Upper
95 100
174 62.6 51.4 77.2
175 4.6 4.0 6.0


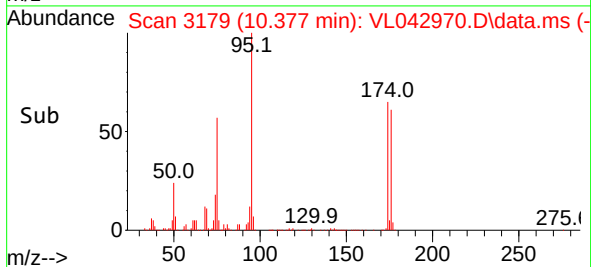

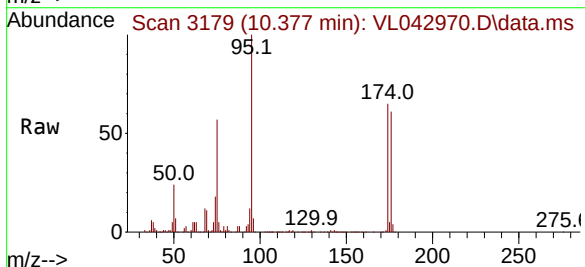




#73
 1,3,5-Trimethylbenzene
 Concen: 0.034 ppbv
 RT: 11.202 min Scan# 3434
 Delta R.T. 0.003 min
 Lab File: VL042970.D
 Acq: 22 Sep 2025 22:48




Instrument :
 MSVOA_L
 ClientSampleId :
 131-1A-2DUP


Tgt Ion:105 Resp: 1741
 Ion Ratio Lower Upper
 105 100
 120 34.7 38.0 57.0#



#74
 1,2,4-Trimethylbenzene
 Concen: 0.091 ppbv
 RT: 11.536 min Scan# 3537
 Delta R.T. 0.003 min
 Lab File: VL042970.D
 Acq: 22 Sep 2025 22:48

Tgt Ion:105 Resp: 5151
 Ion Ratio Lower Upper
 105 100
 120 47.0 40.9 61.3
 91 16.3 51.2 76.8#
 77 19.4 18.4 27.6

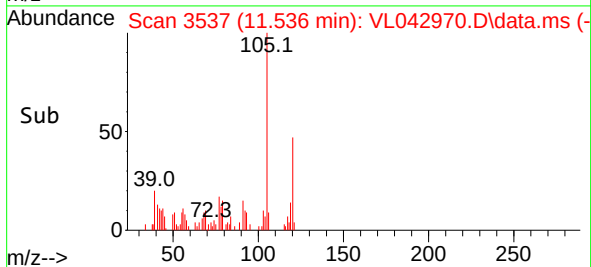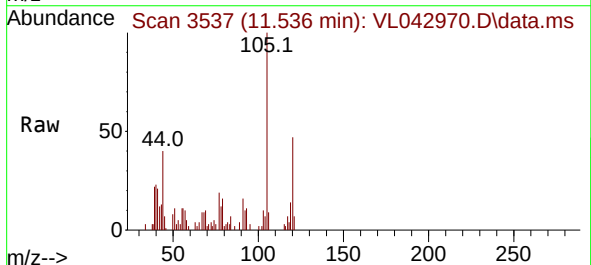



#79

Naphthalene

Concen: 0.142 ppbv

RT: 13.513 min Scan# 4147

Delta R.T. 0.003 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Instrument :

MSVOA_L

ClientSampleId :

131-1A-2DUP





Tgt Ion:128 Resp: 7088

Ion Ratio Lower Upper

128 100

127 12.4 10.6 15.8

129 9.4 9.0 13.6

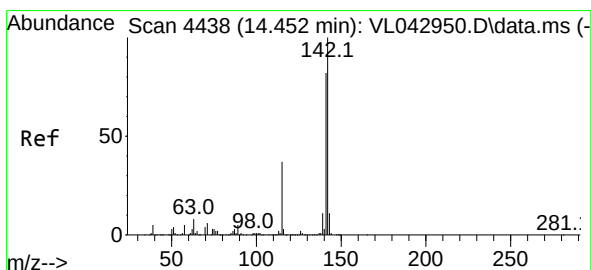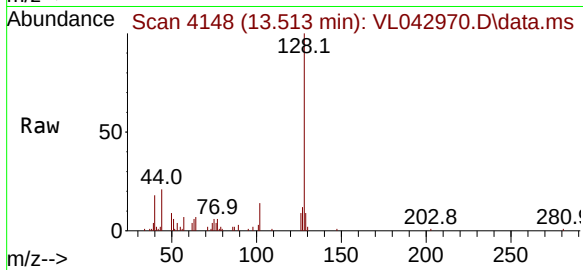

#80

Naphthalene,2-methyl-

Concen: 0.239 ppbv

RT: 14.459 min Scan# 4440

Delta R.T. 0.007 min

Lab File: VL042970.D

Acq: 22 Sep 2025 22:48

Tgt Ion:142 Resp: 3693

Ion Ratio Lower Upper

142 100

141 74.9 65.1 97.7

115 34.1 28.9 43.3

