

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL092321\
Data File : VL037668.D
Acq On : 23 Sep 2021 18:30
Operator : SY/AP
Sample : CAN 10024
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10024

Quant Time: Sep 24 09:54:24 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Sep 16 13:42:46 2021
QLast Update : Thu Sep 16 13:42:46 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.68	49	1539541	10.00	ppbv	0.03
33) 1,4-Difluorobenzene	7.18	114	4450385	10.00	ppbv	0.02
55) Chlorobenzene-d5	12.09	117	3713864	10.00	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.42	95	2691130	10.03	ppbv	0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.30%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL092321\
Data File : VL037668.D
Acq On : 23 Sep 2021 18:30
Operator : SY/AP
Sample : CAN 10024
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10024

Quant Time: Sep 24 09:54:24 2021
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL091621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Sep 16 13:42:46 2021
QLast Update : Thu Sep 16 13:42:46 2021
Response via : Initial Calibration

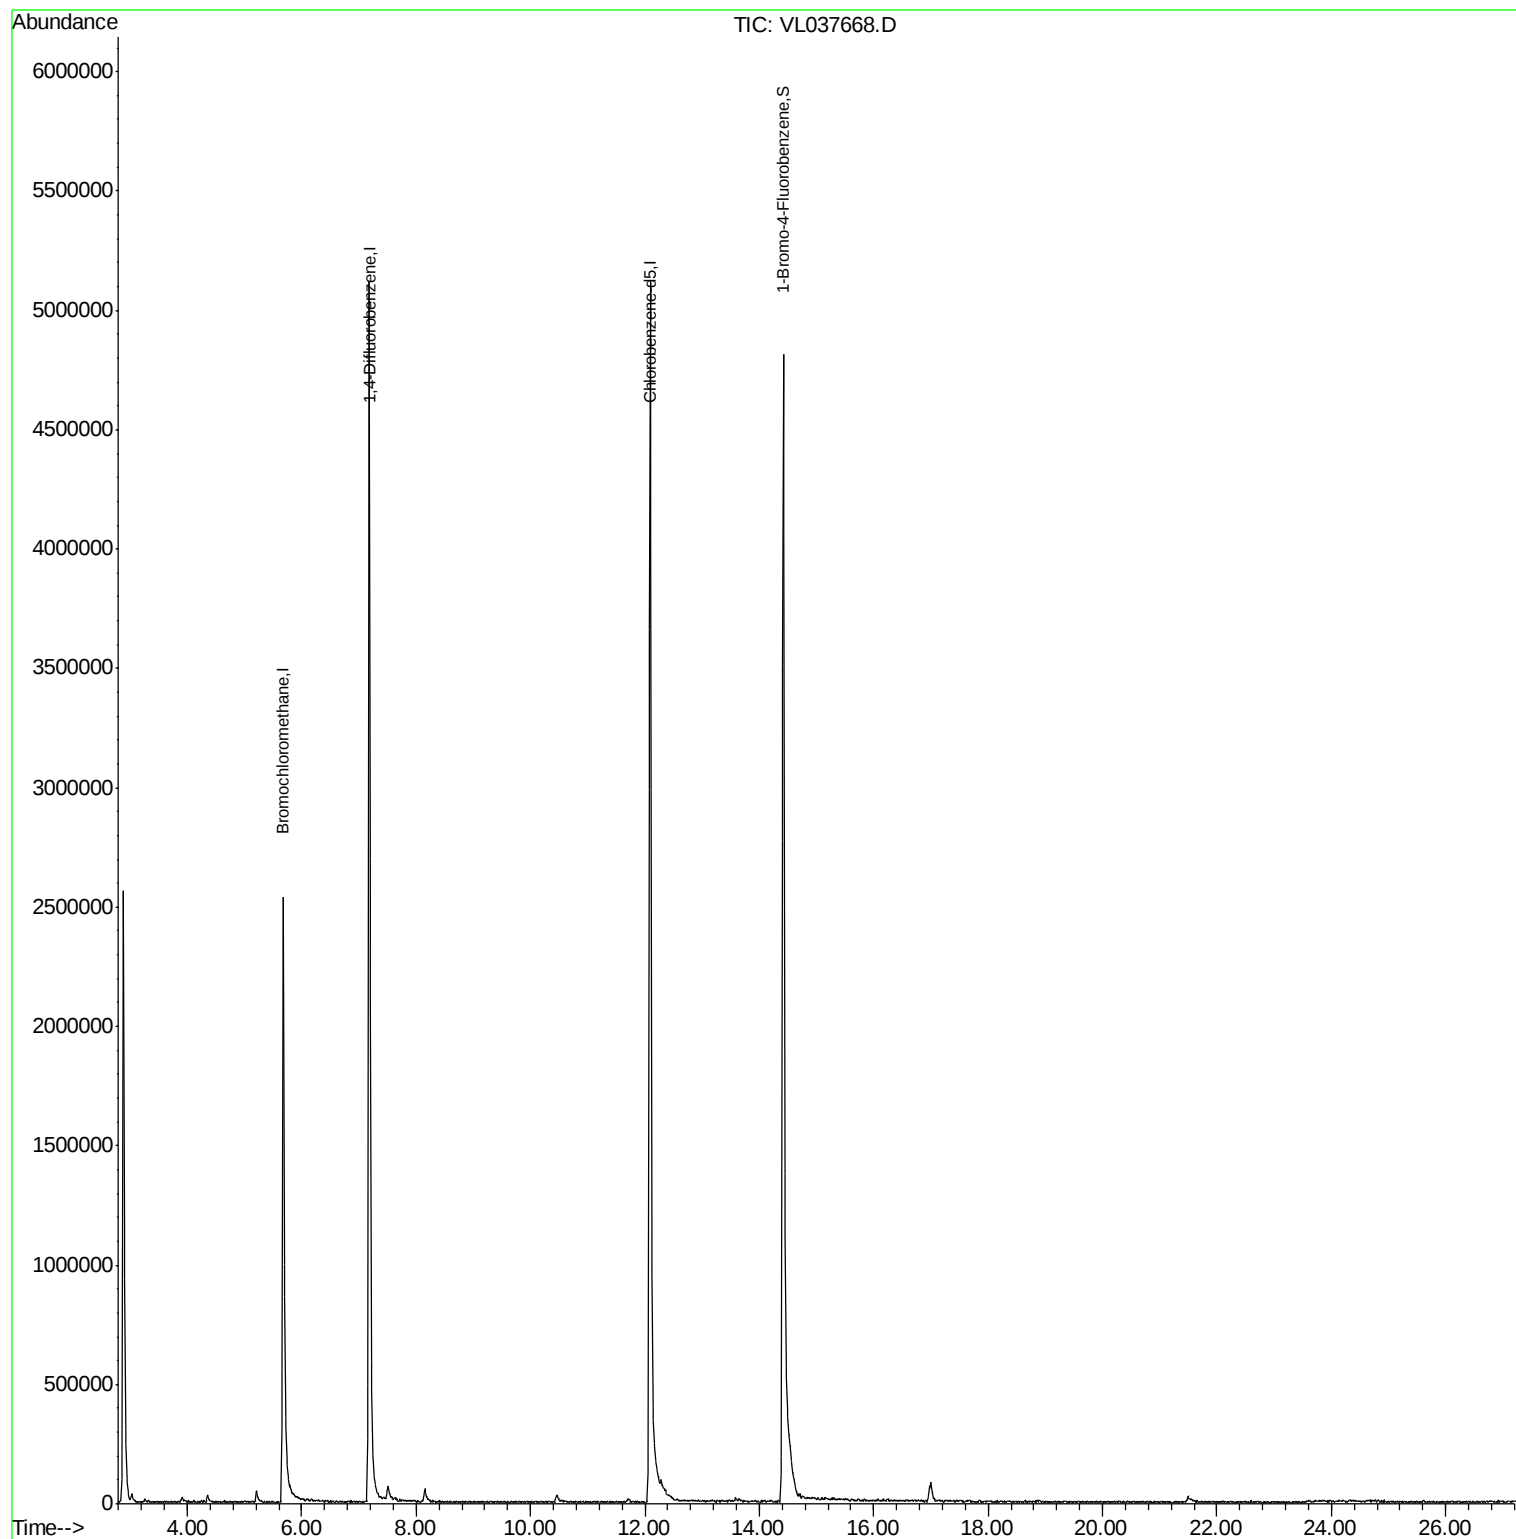

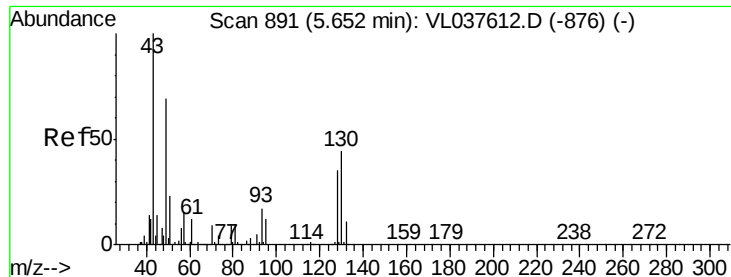

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.68 min Scan# 899

Delta R.T. 0.03 min

Lab File: VL037668.D

Acq: 23 Sep 2021 18:30

Instrument :

MSVOA_L

ClientSampleId :

CAN 10024


Tgt Ion: 49 Resp: 1539541

Ion Ratio Lower Upper

49 100

128 53.6 27.9 83.6




130 69.9 33.9 101.7

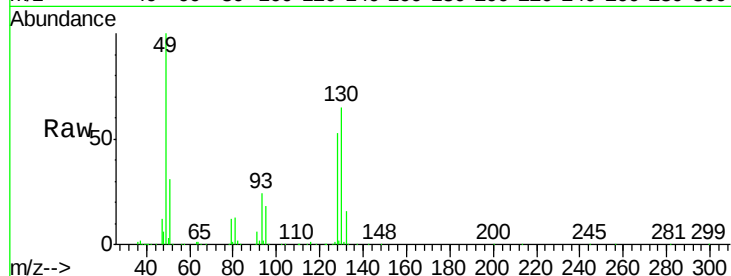

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

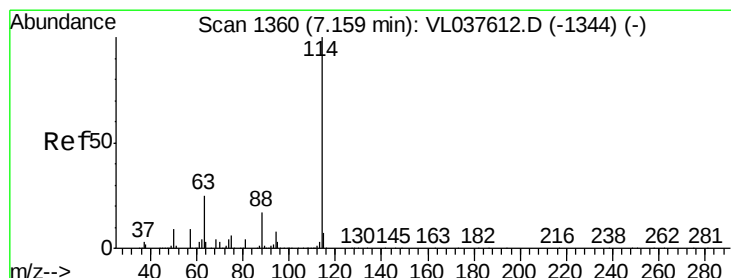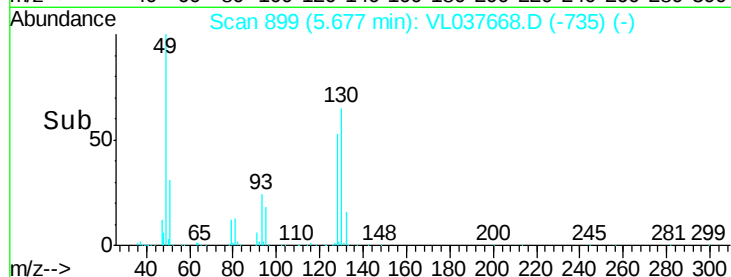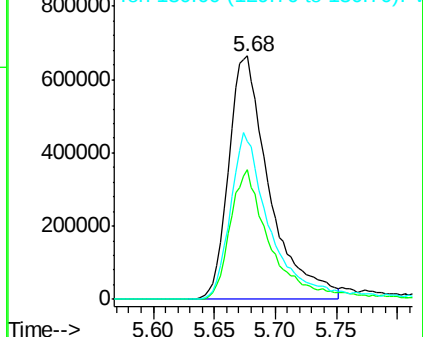

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.18 min Scan# 1367

Delta R.T. 0.02 min

Lab File: VL037668.D

Acq: 23 Sep 2021 18:30


Tgt Ion: 114 Resp: 4450385

Ion Ratio Lower Upper

114 100

63 24.5 19.6 29.4



88 18.2 14.2 21.4

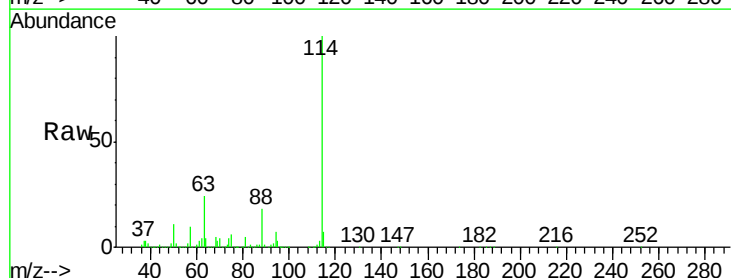


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



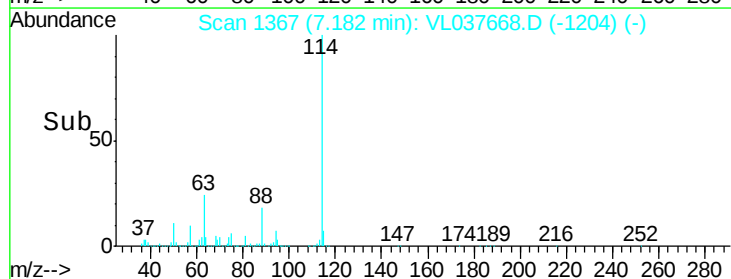
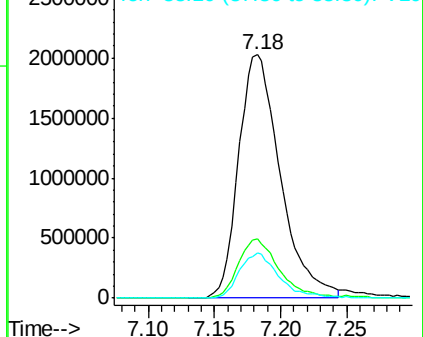


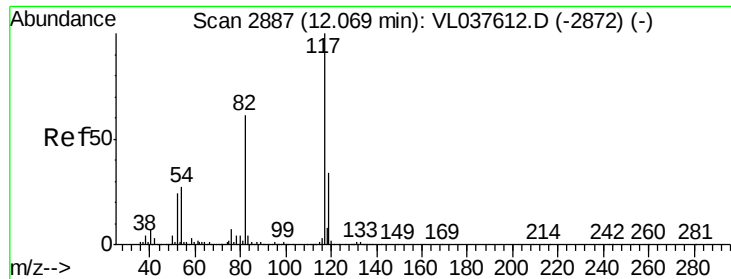

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.09 min Scan# 2894
Delta R.T. 0.02 min
Lab File: VL037668.D
Acq: 23 Sep 2021 18:30

Instrument :
MSVOA_L
ClientSampleId :
CAN 10024

Tgt Ion: 117 Resp: 3713864
Ion Ratio Lower Upper
117 100
82 68.2 50.6 75.8
119 35.2 26.2 39.2

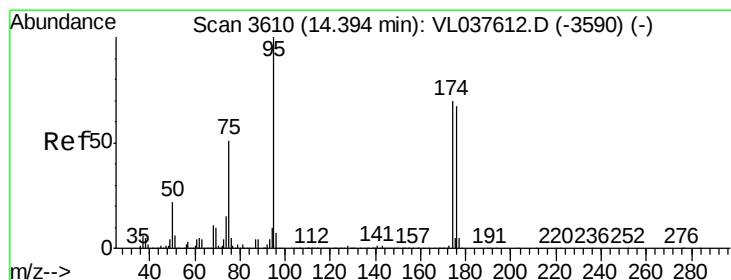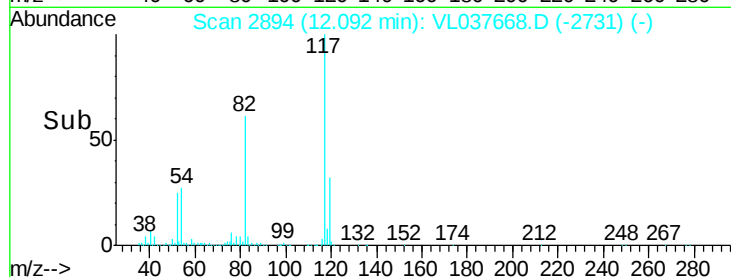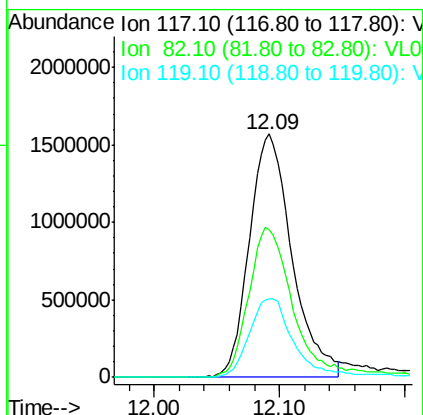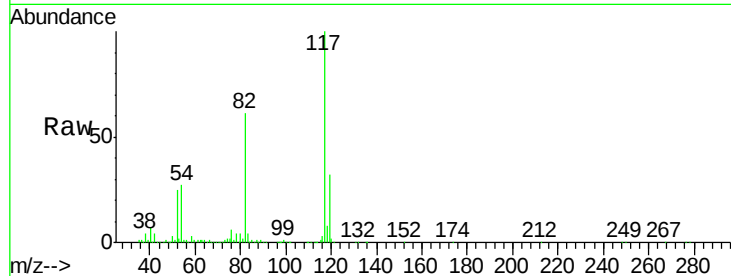

#68
1-Bromo-4-Fluorobenzene
Concen: 10.027 ppbv
RT: 14.42 min Scan# 3618
Delta R.T. 0.03 min
Lab File: VL037668.D
Acq: 23 Sep 2021 18:30

Tgt Ion: 95 Resp: 2691130
Ion Ratio Lower Upper
95 100
174 77.6 56.3 84.5
175 5.5 4.4 6.6

