


Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_L\DATA\VL092321\  
 Data File : VL037653.D  
 Acq On : 23 Sep 2021 8:13  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 400mL/MSVOA\_L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL091621AIR.M  
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Thu Sep 16 13:42:46 2021  
 Last Update : Thu Sep 16 13:42:46 2021

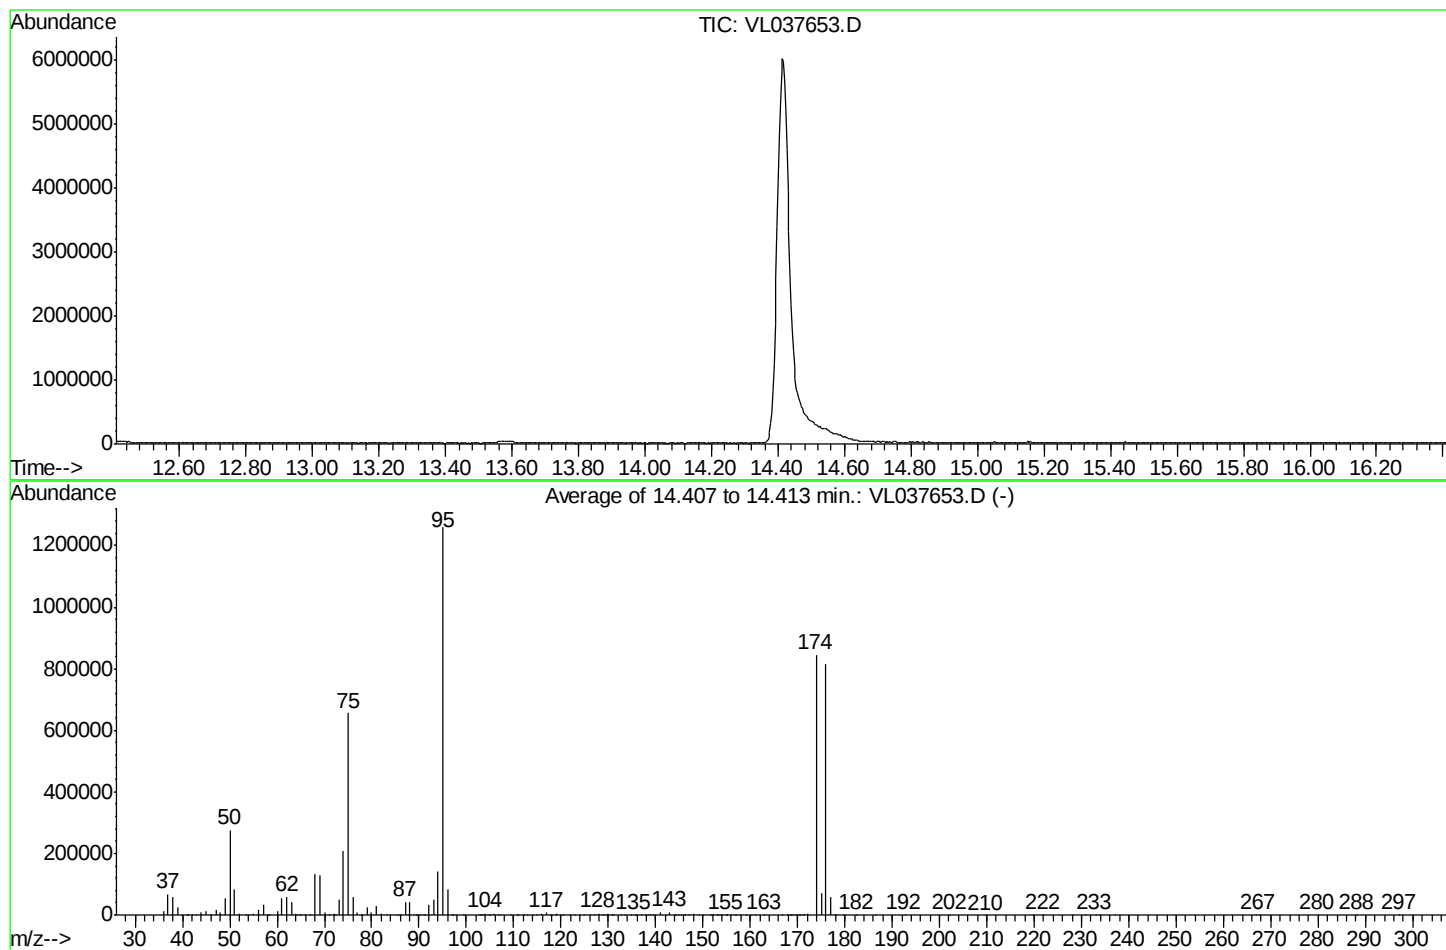

AutoFind: Scans 3614, 3615, 3616; Background Corrected with Scan 3591

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 21.8      | 274901  | PASS             |
| 75          | 95           | 30           | 66           | 52.1      | 656170  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 1259178 | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 83141   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 120          | 67.2      | 845994  | PASS             |
| 175         | 174          | 4            | 9            | 8.4       | 70986   | PASS             |
| 176         | 174          | 93           | 101          | 96.6      | 817045  | PASS             |
| 177         | 176          | 5            | 9            | 7.1       | 58408   | PASS             |